


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN032020\
 Data File : BN010312.D
 Acq On : 20 Mar 2020 20:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:26:45 2020

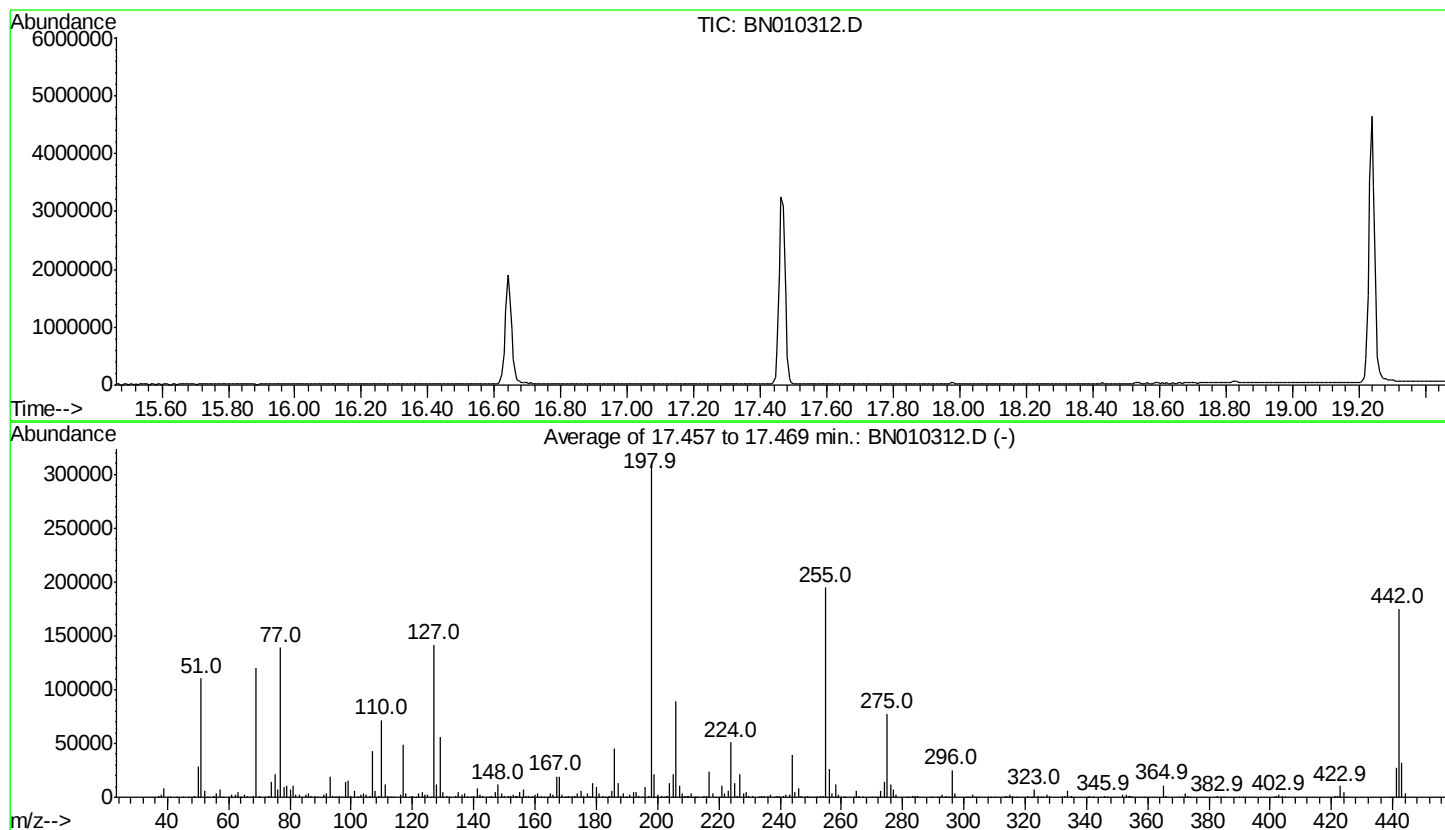

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	110266	PASS
68	69	0.00	2	1.4	1684	PASS
69	198	0.00	100	38.9	119696	PASS
70	69	0.00	2	0.6	771	PASS
127	198	10	80	46.1	141890	PASS
197	198	0.00	2	0.6	1808	PASS
198	198	100	100	100.0	308010	PASS
199	198	5	9	6.9	21289	PASS
275	198	10	60	25.3	77864	PASS
365	198	1	100	3.6	11155	PASS
441	198	0.01	100	8.8	27047	PASS
442	198	50	100	56.9	175293	PASS
443	442	15	24	18.5	32396	PASS