

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032021\
 Data File : BN013999.D
 Acq On : 19 Mar 2021 14:52
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN032021

Quant Time: Mar 19 15:28:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 19 14:40:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	5850	0.40	ng	0.00
7) Naphthalene-d8	10.479	136	21271	0.40	ng	# 0.00
13) Acenaphthene-d10	14.333	164	11604	0.40	ng	0.00
19) Phenanthrene-d10	17.067	188	25364	0.40	ng	0.00
29) Chrysene-d12	21.250	240	25513	0.40	ng	# 0.00
36) Perylene-d12	23.465	264	22341	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.292	112	5861	0.44	ng	0.00
5) Phenol-d6	6.862	99	7294	0.43	ng	0.00
8) Nitrobenzene-d5	8.844	82	5519	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	12.066	152	13600	0.41	ng	0.00
14) 2,4,6-Tribromophenol	15.818	330	1196	0.32	ng	0.00
15) 2-Fluorobiphenyl	12.950	172	18221	0.42	ng	0.00
27) Fluoranthene-d10	19.099	212	28282	0.40	ng	0.00
31) Terphenyl-d14	19.699	244	22728	0.41	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.238	88	3314	0.43	ng	94
3) n-Nitrosodimethylamine	3.569	42	2147	0.42	ng	96
6) bis(2-Chloroethyl)ether	7.128	93	6446	0.43	ng	97
9) Naphthalene	10.517	128	21951	0.42	ng	99
10) Hexachlorobutadiene	10.809	225	4151	0.42	ng	# 99
12) 2-Methylnaphthalene	12.142	142	14507	0.41	ng	100
16) Acenaphthylene	14.041	152	17299	0.39	ng	100
17) Acenaphthene	14.397	154	13438	0.41	ng	99
18) Fluorene	15.374	166	16537	0.40	ng	100
20) 4,6-Dinitro-2-methylph...	15.450	198	1078	0.38	ng	# 79
21) 4-Bromophenyl-phenylether	16.264	248	4898	0.38	ng	92
22) Hexachlorobenzene	16.386	284	6261	0.42	ng	100
23) Atrazine	16.532	200	3265	0.37	ng	# 91
24) Pentachlorophenol	16.727	266	1245	0.35	ng	97
25) Phenanthrene	17.104	178	28244	0.41	ng	99
26) Anthracene	17.201	178	22265	0.39	ng	100
28) Fluoranthene	19.129	202	31101	0.40	ng	99
30) Pyrene	19.491	202	31597	0.40	ng	100
32) Benzo(a)anthracene	21.239	228	29937	0.41	ng	100
33) Chrysene	21.282	228	33143	0.42	ng	99
34) Bis(2-ethylhexyl)phtha...	21.175	149	11840	0.44	ng	97
35) Indeno(1,2,3-cd)pyrene	25.680	276	36597	0.43	ng	99
37) Benzo(b)fluoranthene	22.801	252	32663	0.40	ng	98
38) Benzo(k)fluoranthene	22.801	252	32663	0.41	ng	97
39) Benzo(a)pyrene	23.369	252	29346	0.42	ng	96
40) Dibenzo(a,h)anthracene	25.693	278	30947	0.42	ng	98
41) Benzo(g,h,i)perylene	26.357	276	32404	0.42	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032021\
Data File : BN013999.D
Acq On : 19 Mar 2021 14:52
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Quant Time: Mar 19 15:28:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 19 14:40:09 2021
Response via : Initial Calibration









1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. 0.000 min
 Lab File: BN013999.D
 Acq: 19 Mar 2021 14:52




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN032021


Tgt Ion:	152	Resp:	5850
Ion	Ratio	Lower	Upper
152	100		
150	152.9	121.8	182.8
115	58.3	46.6	69.8



1,4-Dioxane
 Concen: 0.43 ng
 RT: 3.238 min Scan# 57
 Delta R.T. -0.008 min
 Lab File: BN013999.D
 Acq: 19 Mar 2021 14:52

Tgt Ion:	88	Resp:	3314
Ion	Ratio	Lower	Upper
88	100		
58	74.6	64.6	96.8
43	31.6	26.6	40.0









n-Nitrosodimethylamine
Concen: 0.42 ng
RT: 3.569 min Scan# 98
Delta R.T. -0.008 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Tgt Ion: 42 Resp: 2147




Ion	Ratio	Lower	Upper
42	100		
74	113.9	95.0	142.6
44	6.3	5.8	8.8




2-Fluorophenol
Concen: 0.44 ng
RT: 5.292 min Scan# 312
Delta R.T. -0.008 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion: 112 Resp: 5861

Ion	Ratio	Lower	Upper
112	100		
64	60.1	44.3	66.5
63	31.3	23.0	34.6









Phenol-d6
Concen: 0.43 ng
RT: 6.862 min Scan# 507
Delta R.T. -0.008 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52




Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Tgt Ion:	99	Resp:	7294
Ion	Ratio	Lower	Upper
99	100		
42	22.4	15.2	22.8
71	33.1	26.1	39.1




bis(2-Chloroethyl)ether
Concen: 0.43 ng
RT: 7.128 min Scan# 540
Delta R.T. -0.008 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	93	Resp:	6446
Ion	Ratio	Lower	Upper
93	100		
63	79.9	60.8	91.2
95	33.0	26.0	39.0





Abundance Scan 858 (10.480 min): BN013994.D\data.ms (-85#7-)




Naphthalene-d8
Concen: 0.40 ng
RT: 10.479 min Scan# 858
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021


Tgt Ion:	136	Resp:	21271
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.6
54	5.8	6.4	9.6#
68	4.5	4.5	6.7



Abundance Scan 858 (10.479 min): BN013999.D\data.ms (-842) (-)





Abundance Scan 729 (8.845 min): BN013994.D\data.ms (-726#8)




Nitrobenzene-d5
Concen: 0.39 ng
RT: 8.844 min Scan# 729
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52


Tgt Ion:	82	Resp:	5519
Ion	Ratio	Lower	Upper
82	100		
128	43.0	39.2	58.8
54	49.3	40.1	60.1



Abundance Scan 729 (8.844 min): BN013999.D\data.ms (-713) (-)






Abundance Scan 862 (10.530 min): BN013994.D\data.ms (-855) (-)




Naphthalene
Concen: 0.42 ng
RT: 10.517 min Scan# 861
Delta R.T. -0.013 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Tgt Ion:	128	Resp:	21951
Ion	Ratio	Lower	Upper
128	100		
129	11.3	9.0	13.4
127	13.5	10.4	15.6






Abundance Scan 885 (10.822 min): BN013994.D\data.ms (-880) (-)




Hexachlorobutadiene
Concen: 0.42 ng
RT: 10.809 min Scan# 884
Delta R.T. -0.013 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	225	Resp:	4151
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.6	51.2	76.8





Abundance Scan 1066 (12.071 min): BN013994.D\data.ms (-1015) (-)




2-Methylnaphthalene-d10
Concen: 0.41 ng
RT: 12.066 min Scan# 1065
Delta R.T. -0.005 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021


Tgt Ion:152 Resp: 13600
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2



Abundance Scan 1065 (12.066 min): BN013999.D\data.ms (-1021) (-)





Abundance Scan 1082 (12.142 min): BN013994.D\data.ms (-1010) (-)




2-Methylnaphthalene
Concen: 0.41 ng
RT: 12.142 min Scan# 1082
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:142 Resp: 14507
Ion Ratio Lower Upper
142 100
141 88.0 70.5 105.7
115 34.9 27.4 41.0




Abundance Scan 1082 (12.142 min): BN013999.D\data.ms (-1060) (-)






Abundance Scan 1308 (14.334 min): BN013994.D\data.ms (-1308) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.333 min Scan# 1308
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021




Tgt Ion:	164	Resp:	11604
Ion Ratio	Lower	Upper	
164	100		
162	98.6	79.6	119.4
160	43.9	36.0	54.0






Abundance Scan 1425 (15.818 min): BN013994.D\data.ms (-1419) (-)


2,4,6-Tribromophenol
Concen: 0.32 ng
RT: 15.818 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52



Tgt Ion:	330	Resp:	1196
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	39.6	26.8	40.2





Abundance Scan 1199 (12.951 min): BN013994.D\data.ms (-1191) (-)




2-Fluorobiphenyl
Concen: 0.42 ng
RT: 12.950 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021


Tgt Ion:	172	Resp:	18221
Ion	Ratio	Lower	Upper
172	100		
171	34.3	28.6	42.8
170	23.0	18.9	28.3



Abundance Scan 1199 (12.950 min): BN013999.D\data.ms (-1191) (-)





Abundance Scan 1285 (14.042 min): BN013994.D\data.ms (-1269) (-)




Acenaphthylene
Concen: 0.39 ng
RT: 14.041 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52


Tgt Ion:	152	Resp:	17299
Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.7	23.5
153	13.1	10.5	15.7



Abundance Scan 1285 (14.041 min): BN013999.D\data.ms (-1269) (-)





Abundance Scan 1312 (14.384 min): BN013994.D\data.ms (-1304) (-)




Acenaphthene
Concen: 0.41 ng
RT: 14.397 min Scan# 1313
Delta R.T. 0.012 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021


Tgt Ion:	154	Resp:	13438
Ion Ratio	Lower	Upper	
154	100		
153	110.2	88.4	132.6
152	54.5	43.0	64.4



Abundance Scan 1313 (14.397 min): BN013999.D\data.ms (-1304) (-)





Abundance Scan 1390 (15.374 min): BN013994.D\data.ms (-1304) (-)





Fluorene
Concen: 0.40 ng
RT: 15.374 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	166	Resp:	16537
Ion Ratio	Lower	Upper	
166	100		
165	97.6	77.8	116.8
167	13.5	10.6	16.0



Abundance Scan 1390 (15.374 min): BN013999.D\data.ms (-1374) (-)









Scan 1527 (17.068 min): BN013994.D\data.ms (-1527) (-)
 Phenanthrene-d10
 Concen: 0.40 ng
 RT: 17.067 min Scan# 1527
 Delta R.T. -0.000 min
 Lab File: BN013999.D
 Acq: 19 Mar 2021 14:52




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN032021

Tgt Ion:	188	Resp:	25364
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	9.4	9.0	13.6




Scan 1396 (15.450 min): BN013994.D\data.ms (-1396) (-)
 4,6-Dinitro-2-methylphenol
 Concen: 0.38 ng
 RT: 15.450 min Scan# 1396
 Delta R.T. -0.000 min
 Lab File: BN013999.D
 Acq: 19 Mar 2021 14:52

Tgt Ion:	198	Resp:	1078
Ion Ratio	Lower	Upper	
198	100		
51	93.8	61.7	92.5#
105	56.4	33.0	49.6#






Abundance Scan 1461 (16.264 min): BN013999.D\data.ms (-1453) (-)




4-Bromophenyl-phenylether
Concen: 0.38 ng
RT: 16.264 min Scan# 1461
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Tgt Ion:	248	Resp:	4898
Ion	Ratio	Lower	Upper
248	100		
250	88.9	75.5	113.3
141	77.3	53.8	80.8







Abundance Scan 1471 (16.386 min): BN013999.D\data.ms (-1463) (-)



Hexachlorobenzene
Concen: 0.42 ng
RT: 16.386 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	284	Resp:	6261
Ion	Ratio	Lower	Upper
284	100		
142	35.0	27.9	41.9
249	30.2	24.2	36.2









#23 (-)
 Atrazine
 Concen: 0.37 ng
 RT: 16.532 min Scan# 1483
 Delta R.T. -0.000 min
 Lab File: BN013999.D
 Acq: 19 Mar 2021 14:52




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN032021

Tgt Ion:	200	Resp:	3265
Ion Ratio	Lower	Upper	
200	100		
173	30.9	18.6	28.0#
215	47.5	41.0	61.6



#24 (-)
 Pentachlorophenol
 Concen: 0.35 ng
 RT: 16.727 min Scan# 1499
 Delta R.T. -0.000 min
 Lab File: BN013999.D
 Acq: 19 Mar 2021 14:52


Tgt Ion:	266	Resp:	1245
Ion Ratio	Lower	Upper	
266	100		
264	62.7	51.6	77.4
268	65.3	54.6	82.0






Abundance Scan 1530 (17.104 min): BN013994.D\data.ms (-1525) (-)

Phenanthrene
Concen: 0.41 ng
RT: 17.104 min Scan# 1530
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021




Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.0	22.4
179	15.4	12.3	18.5






Abundance Scan 1538 (17.201 min): BN013994.D\data.ms (-1526) (-)


Anthracene
Concen: 0.39 ng
RT: 17.201 min Scan# 1538
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52



Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.4	14.6	21.8
179	15.3	12.2	18.2






Abundance Scan 1823 (19.099 min): BN013999.D\data.ms (-1823) (-)




Fluoranthene-d10
Concen: 0.40 ng
RT: 19.099 min Scan# 1823
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Tgt Ion:	212	Resp:	28282
Ion	Ratio	Lower	Upper
212	100		
106	12.6	9.7	14.5
104	7.0	5.5	8.3






Abundance Scan 1829 (19.129 min): BN013999.D\data.ms (-1829) (-)




Fluoranthene
Concen: 0.40 ng
RT: 19.129 min Scan# 1829
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	202	Resp:	31101
Ion	Ratio	Lower	Upper
202	100		
101	10.9	8.1	12.1
203	17.2	13.9	20.9





Abundance Scan 2123 (21.250 min): BN013994.D\data.ms (-2123) (-)




Chrysene-d12
Concen: 0.40 ng
RT: 21.250 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021


Tgt Ion:	240	Resp:	25513
Ion	Ratio	Lower	Upper
240	100		
120	10.2	10.2	15.4#
236	26.3	21.3	31.9



Abundance Scan 2123 (21.250 min): BN013999.D\data.ms (-2104) (-)





Abundance Scan 1902 (19.491 min): BN013994.D\data.ms (-1890) (-)




Pyrene
Concen: 0.40 ng
RT: 19.491 min Scan# 1902
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	202	Resp:	31597
Ion	Ratio	Lower	Upper
202	100		
200	20.2	16.3	24.5
203	17.6	14.0	21.0




Abundance Scan 1902 (19.491 min): BN013999.D\data.ms (-1862) (-)






Abundance Scan 1944 (19.700 min): BN013994.D\data.ms (-1935) (-)

Terphenyl-d14
Concen: 0.41 ng
RT: 19.699 min Scan# 1944
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

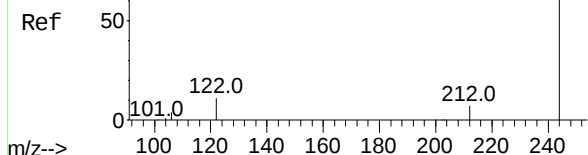


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.9	6.1	9.1
122	12.2	9.8	14.8






Abundance Scan 2121 (21.229 min): BN013994.D\data.ms (-2132) (-)


Benzo(a)anthracene
Concen: 0.41 ng
RT: 21.239 min Scan# 2122
Delta R.T. 0.010 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52



Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.5	20.5	30.7
229	20.0	16.2	24.4






Abundance Scan 2126 (21.282 min): BN013999.D\data.ms (-2126) (-)




Chrysene
Concen: 0.42 ng
RT: 21.282 min Scan# 2126
Delta R.T. -0.000 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Tgt Ion:	228	Resp:	33143
Ion Ratio	Lower	Upper	
228	100		
226	30.1	24.3	36.5
229	19.3	15.1	22.7






Abundance Scan 2115 (21.165 min): BN013999.D\data.ms (-2115) (-)




Bis(2-ethylhexyl)phthalate
Concen: 0.44 ng
RT: 21.175 min Scan# 2116
Delta R.T. 0.010 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	149	Resp:	11840
Ion Ratio	Lower	Upper	
149	100		
167	25.7	22.1	33.1
279	4.0	3.5	5.3





Abundance Scan 3186 (25.673 min): BN013994.D\data.ms (-3186) (-)




Indeno(1,2,3-cd)pyrene
Concen: 0.43 ng
RT: 25.680 min Scan# 3188
Delta R.T. 0.007 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021


Tgt Ion:	276	Resp:	36597
Ion Ratio	Lower	Upper	
276	100		
138	23.6	19.8	29.6
277	24.8	19.9	29.9



Abundance Scan 3188 (25.680 min): BN013999.D\data.ms (-3157) (-)





Abundance Scan 2539 (23.458 min): BN013994.D\data.ms (-2539) (-)




Perylene-d12
Concen: 0.40 ng
RT: 23.465 min Scan# 2541
Delta R.T. 0.007 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52


Tgt Ion:	264	Resp:	22341
Ion Ratio	Lower	Upper	
264	100		
260	24.9	19.3	28.9
265	34.5	66.2	99.4#



Abundance Scan 2541 (23.465 min): BN013999.D\data.ms (-2495) (-)





Abundance Scan 2345 (22.794 min): BN013994.D\data.ms (-2345) (-)




Benzo(b)fluoranthene
Concen: 0.40 ng
RT: 22.801 min Scan# 2347
Delta R.T. 0.007 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52


Tgt Ion:	252	Resp:	32663
Ion	Ratio	Lower	Upper
252	100		
253	24.6	20.4	30.6
125	13.1	11.6	17.4



Abundance Scan 2347 (22.801 min): BN013999.D\data.ms (-2287) (-)





Abundance Scan 2358 (22.839 min): BN013994.D\data.ms (-2358) (-)




Benzo(k)fluoranthene
Concen: 0.41 ng
RT: 22.801 min Scan# 2347
Delta R.T. -0.038 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Tgt Ion:	252	Resp:	32663
Ion	Ratio	Lower	Upper
252	100		
253	24.6	20.5	30.7
125	13.1	12.3	18.5




Abundance Scan 2347 (22.801 min): BN013999.D\data.ms (-2270) (-)





Abundance Scan 2511 (23.363 min): BN013994.D\data.ms (-2453) (-)

Benzo(a)pyrene
Concen: 0.42 ng
RT: 23.369 min Scan# 2513
Delta R.T. 0.007 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52


Instrument :
BNA_N
ClientSampleId :
ICVBN032021



Tgt Ion:	252	Resp:	29346
Ion Ratio	Lower	Upper	
252	100		
253	25.4	21.8	32.6
125	16.6	14.6	21.8




Abundance Scan 2513 (23.369 min): BN013999.D\data.ms (-2453) (-)





Abundance Scan 3190 (25.687 min): BN013994.D\data.ms (-3174) (-)


Dibenzo(a,h)anthracene
Concen: 0.42 ng
RT: 25.693 min Scan# 3192
Delta R.T. 0.007 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52




Tgt Ion:	278	Resp:	30947
Ion Ratio	Lower	Upper	
278	100		
139	16.5	13.1	19.7
279	25.2	21.4	32.0



Abundance Scan 3192 (25.693 min): BN013999.D\data.ms (-3167) (-)




Abundance Scan 3384 (26.351 min): BN013994.D\data.ms (-3384) (-)




Benzo(g,h,i)perylene
Concen: 0.42 ng
RT: 26.357 min Scan# 3386
Delta R.T. 0.007 min
Lab File: BN013999.D
Acq: 19 Mar 2021 14:52

Instrument :
BNA_N
ClientSampleId :
ICVBN032021

Abundance Scan 3386 (26.357 min): BN013999.D\data.ms



Tgt Ion:	276	Resp:	32404
Ion	Ratio	Lower	Upper
276	100		
277	24.4	20.0	30.0
138	21.4	17.8	26.8



Abundance Scan 3386 (26.357 min): BN013999.D\data.ms (-3326) (-)

