
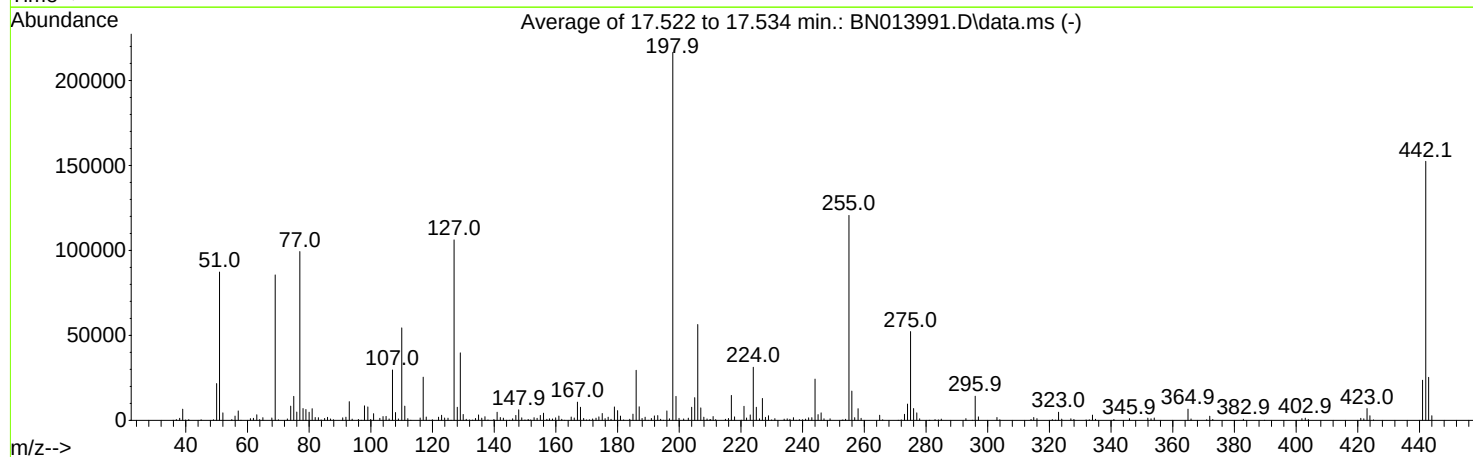


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032021\
 Data File : BN013991.D
 Acq On : 19 Mar 2021 09:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 19 14:40:09 2021

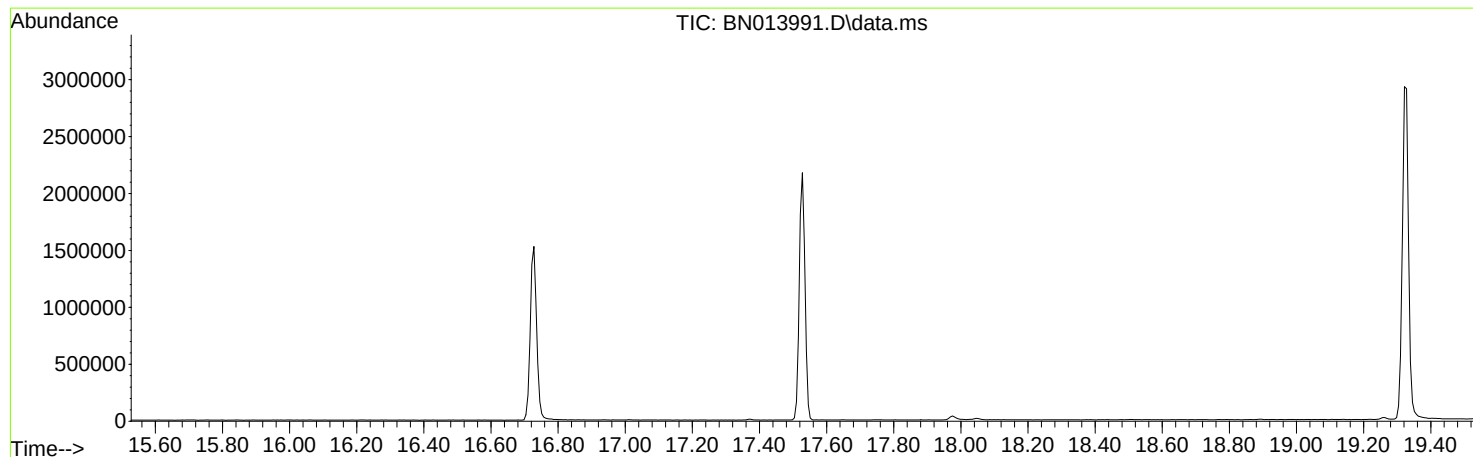

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	87257	PASS
68	69	0.00	2	1.7	1442	PASS
69	198	0.00	100	39.5	85579	PASS
70	69	0.00	2	0.5	427	PASS
127	198	10	80	49.1	106232	PASS
197	198	0.00	2	0.4	911	PASS
198	198	100	100	100.0	216448	PASS
199	198	5	9	6.5	14164	PASS
275	198	10	60	24.2	52293	PASS
365	198	1	100	3.0	6597	PASS
441	198	0.01	100	10.9	23627	PASS
442	442	50	100	100.0	152413	PASS
443	442	15	24	16.6	25349	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/20/2021	BNA_N	<u>BN013991.D</u>
Compound Name	Response	Retention Time
DDT	723605	20.56
DDD	1012	20.12
DDE	674	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1686	725291	0.23

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032021\
Data File : BN013991.D
Acq On : 19 Mar 2021 09:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 19 11:10:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

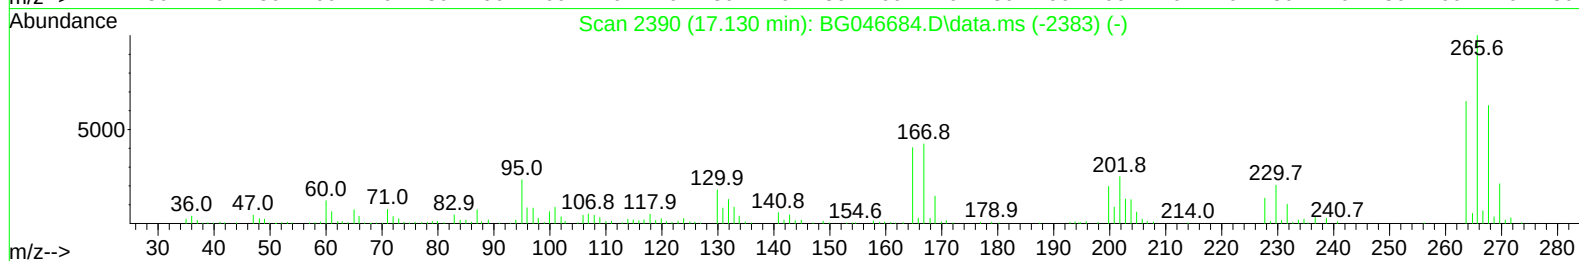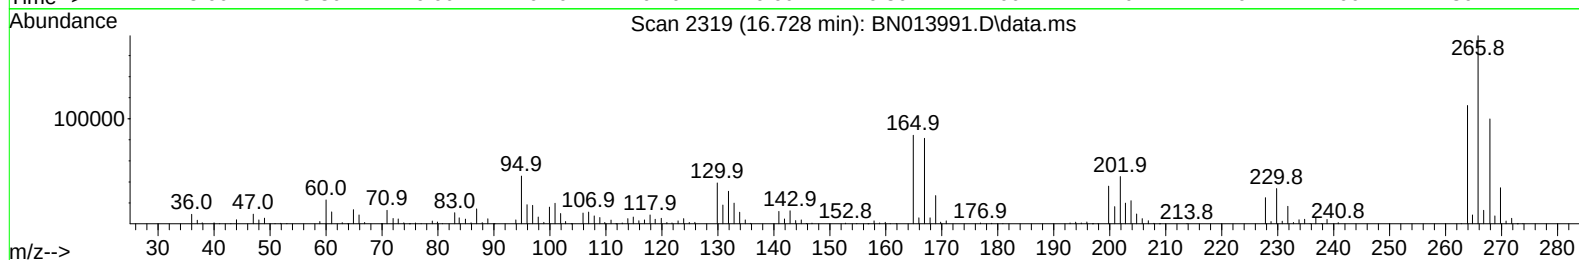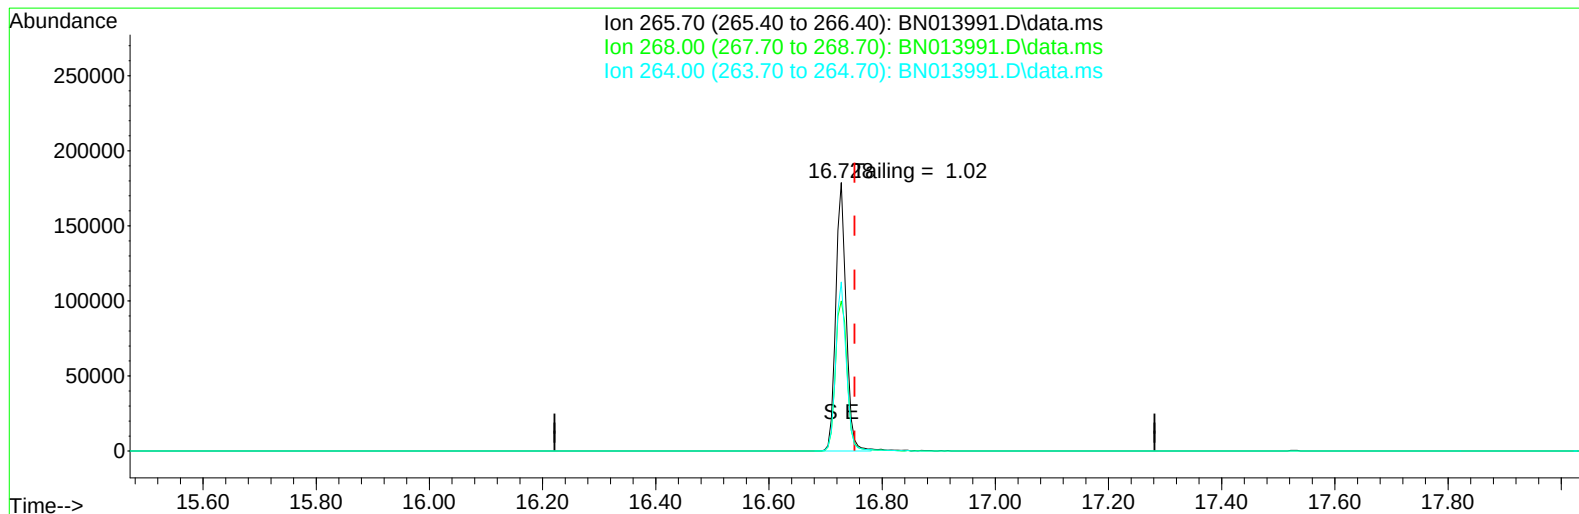

TIC: BN013991.D\data.ms

(70) Pentachlorophenol (C)

16.728min (-0.023) 19721.95 ng




response 229683

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	55.85
264.00	61.60	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032021\
Data File : BN013991.D
Acq On : 19 Mar 2021 09:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 19 11:10:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

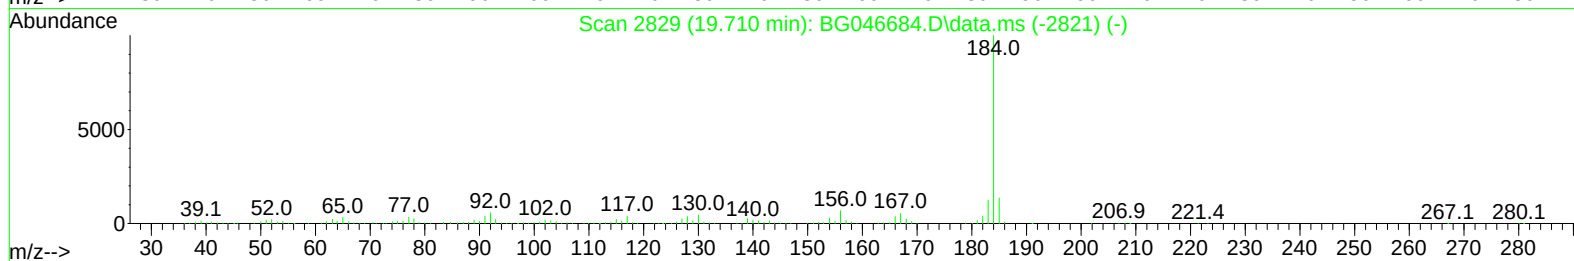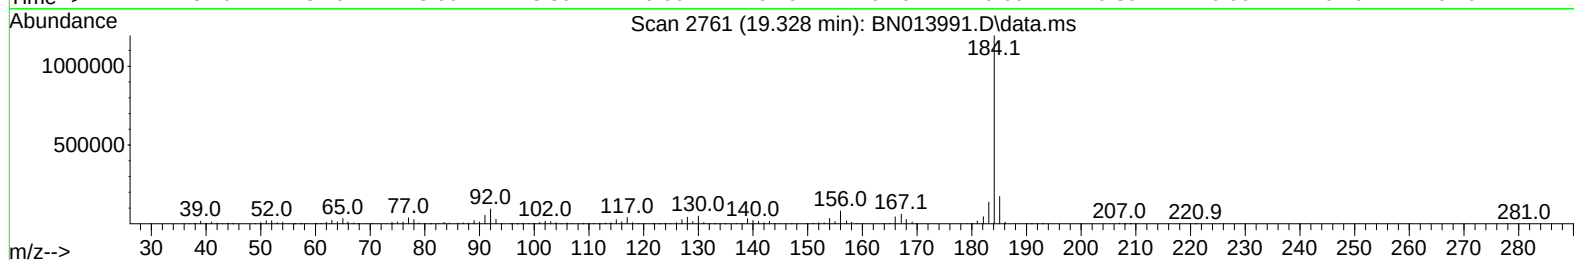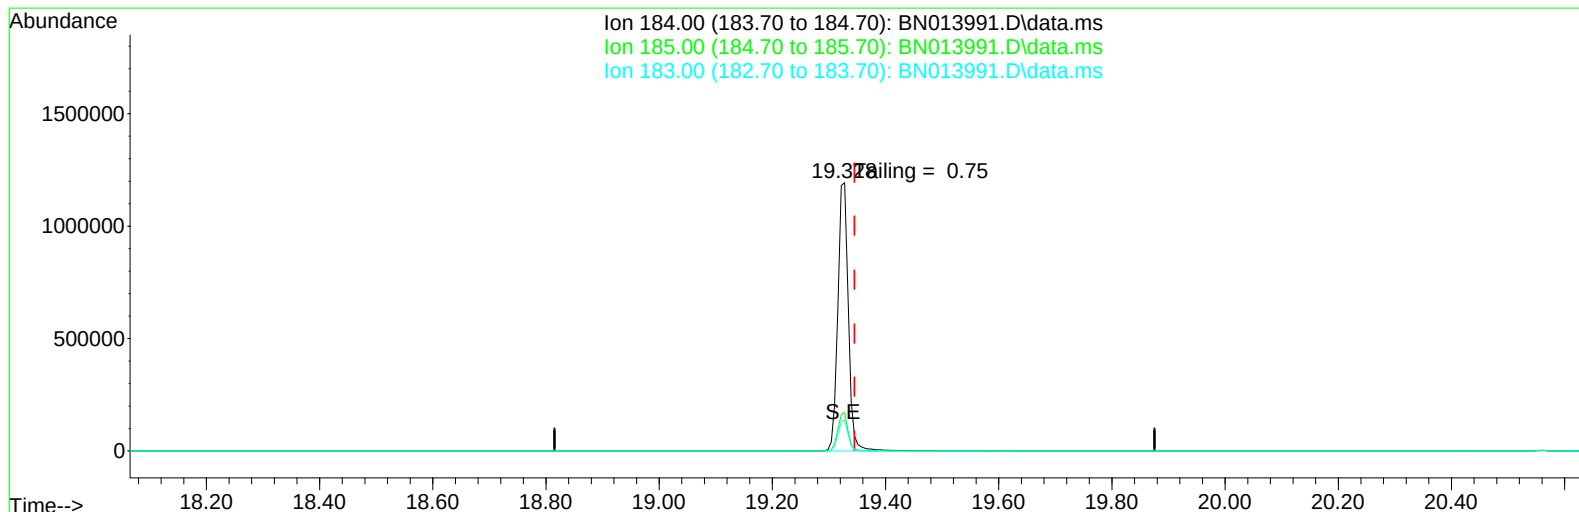

TIC: BN013991.D\data.ms

(77) Benzidine

19.328min (-0.017) 0.00 ng

response 1545872

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.47
183.00	13.20	11.52
0.00	0.00	0.00