

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032124\
 Data File : BN030441.D
 Acq On : 21 Mar 2024 11:00
 Operator : MA/JU
 Sample : PB159692BL 10X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK692

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	19	23	32	rVB	128329	186531	1.73%	0.171%
2	3.617	86	90	112	rBV	1733790	2615772	24.25%	2.393%
3	3.952	143	147	152	rVB	20576	26940	0.25%	0.025%
4	6.881	638	645	657	rBV	1975665	3061225	28.38%	2.801%
5	7.064	670	676	687	rVB	1619636	2572550	23.85%	2.354%
6	7.258	701	709	724	rBV	1868491	2986789	27.69%	2.733%
7	7.722	781	788	796	rBV	1185664	1883075	17.46%	1.723%
8	8.422	899	907	924	rBV	2392429	3827928	35.49%	3.502%
9	8.881	975	985	997	rBV	1857194	2996822	27.79%	2.742%
10	9.599	1098	1107	1117	rBV	1312814	2089820	19.38%	1.912%
11	10.128	1189	1197	1214	rBV	2255392	3722995	34.52%	3.406%
12	10.511	1254	1262	1273	rVB	1709612	2852693	26.45%	2.610%
13	10.646	1277	1285	1294	rBV	2570578	4257246	39.47%	3.895%
14	12.105	1528	1533	1540	rVB	46805	75570	0.70%	0.069%
15	12.752	1637	1643	1645	rBV4	7737	11466	0.11%	0.010%
16	13.275	1727	1732	1738	rBV	24278	40263	0.37%	0.037%
17	13.787	1812	1819	1832	rBV	4339373	6004871	55.68%	5.494%
18	14.057	1857	1865	1873	rBV	4960163	7260854	67.32%	6.643%
19	14.369	1911	1918	1924	rBV	2609984	3941255	36.54%	3.606%
20	14.551	1942	1949	1968	rBV	2077568	2930307	27.17%	2.681%
21	14.787	1985	1989	1994	rVB8	8502	11958	0.11%	0.011%
22	15.363	2080	2087	2097	rBV	6157843	8738038	81.02%	7.994%
23	15.475	2098	2106	2123	rVV	1233308	1745067	16.18%	1.597%
24	15.604	2123	2128	2134	rVB2	27918	45632	0.42%	0.042%
25	16.145	2216	2220	2225	rVB4	21054	30064	0.28%	0.028%
26	16.793	2327	2330	2336	rVB6	10922	15273	0.14%	0.014%
27	16.898	2344	2348	2355	rBV4	7477	11936	0.11%	0.011%
28	17.116	2378	2385	2393	rBV	3355135	4694921	43.53%	4.295%
29	17.216	2395	2402	2415	rVV2	6458589	9527813	88.34%	8.717%
30	19.075	2713	2718	2725	rBV	80209	108864	1.01%	0.100%
31	19.145	2725	2730	2735	rBV	74868	102031	0.95%	0.093%
32	19.510	2786	2792	2805	rVB2	7785319	10785169	100.00%	9.867%
33	21.357	3100	3106	3116	rBV	3501854	4772292	44.25%	4.366%
34	24.127	3567	3577	3590	rBV2	4526596	10553874	97.86%	9.656%
35	24.327	3602	3611	3623	rVB	1999655	4816208	44.66%	4.406%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032124\
Data File : BN030441.D
Acq On : 21 Mar 2024 11:00
Operator : MA/JU
Sample : PB159692BL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK692

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032024.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 109304112

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032124\
Data File : BN030441.D
Acq On : 21 Mar 2024 11:00
Operator : MA/JU
Sample : PB159692BL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK692

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

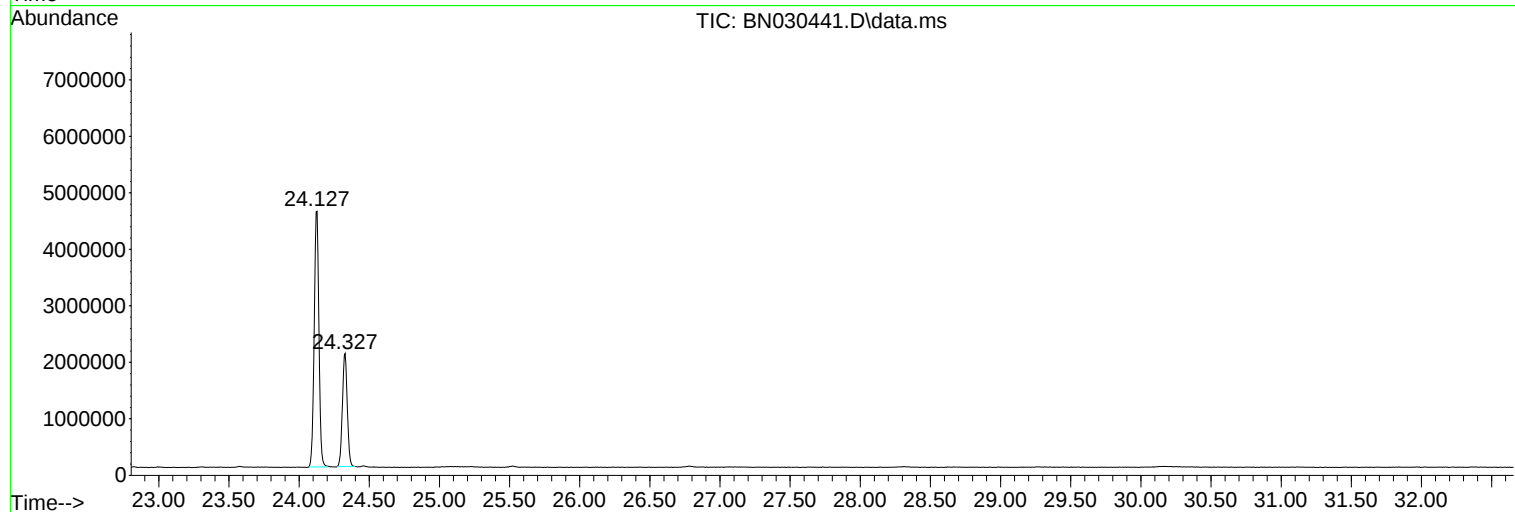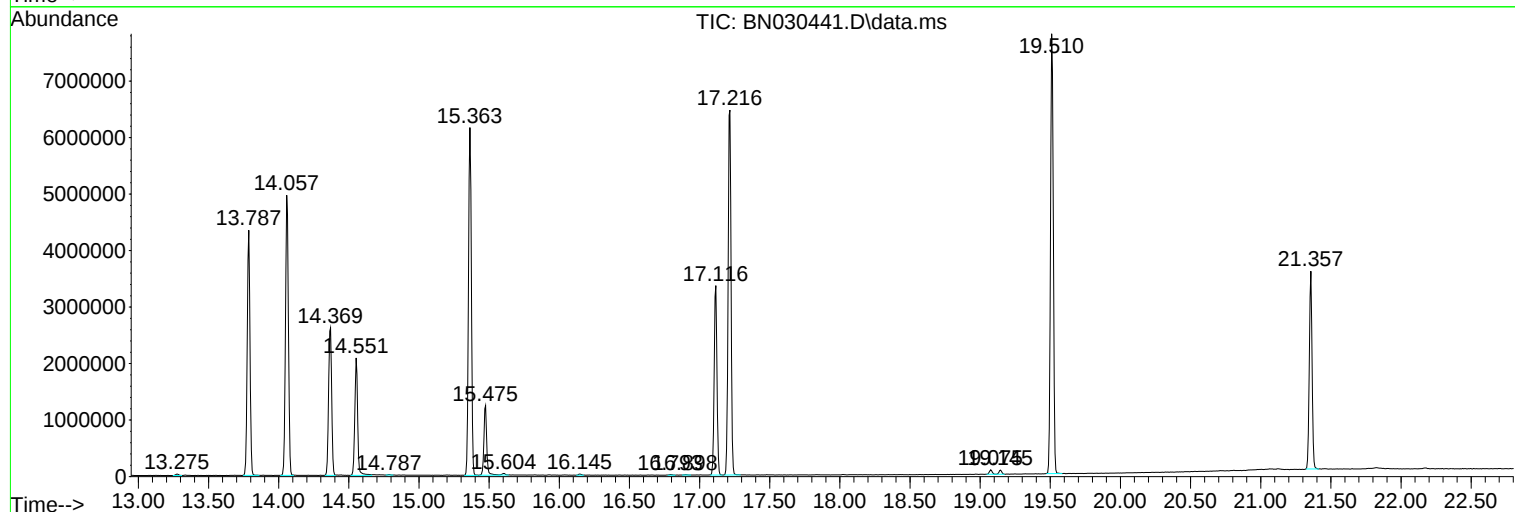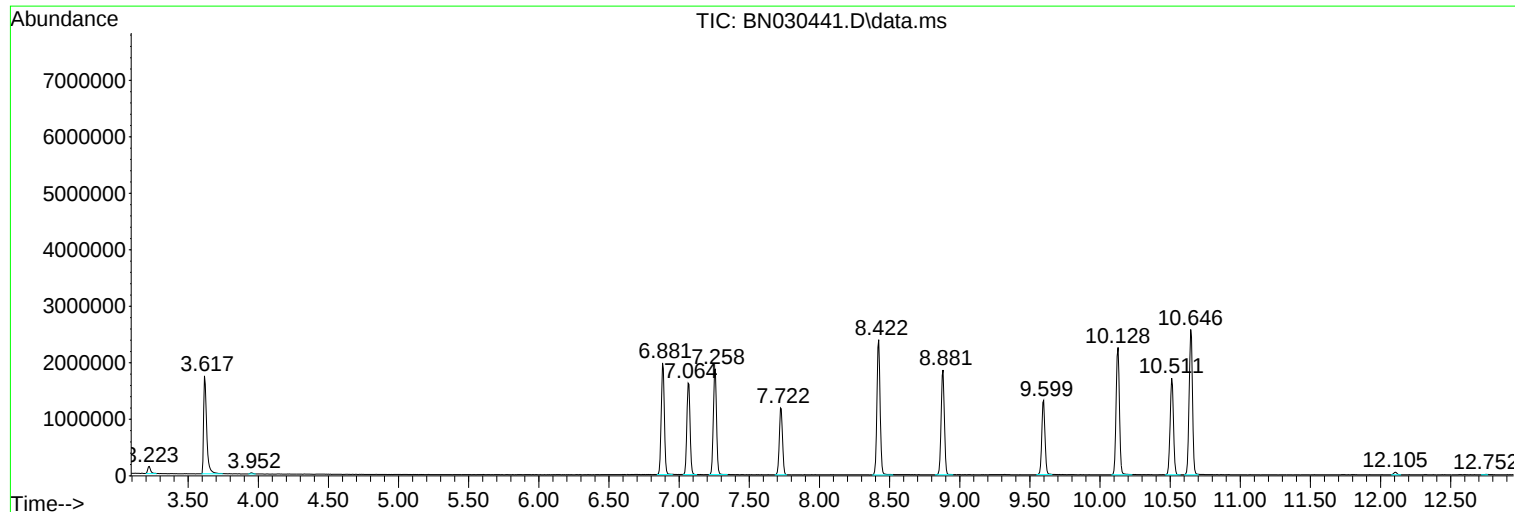

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032124\
Data File : BN030441.D
Acq On : 21 Mar 2024 11:00
Operator : MA/JU
Sample : PB159692BL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK692

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032124\
Data File : BN030441.D
Acq On : 21 Mar 2024 11:00
Operator : MA/JU
Sample : PB159692BL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK692

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------