

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032218\
 Data File : BN000536.D
 Acq On : 22 Mar 2018 12:45
 Operator : JU/SJ
 Sample : J1922-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 23 02:22:36 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 23 02:22:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	183551	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	808444	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.04	164	447595	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.76	188	951752	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	871842	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	708188	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.59	96	29259	5.69	ng/uL	0.00
5) Phenol-d5	7.56	99	173556	10.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.72	67	368057	37.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.94	132	414118	31.98	ng/ul	0.00
13) 4-Methylphenol-d8	9.13	113	306550	22.98	ng/ul	0.00
19) Nitrobenzene-d5	9.60	128	239389	36.46	ng/ul	0.00
22) 2-Nitrophenol-d4	10.33	143	260425	38.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.87	165	447047	36.66	ng/ul	0.00
29) 4-Chloroaniline-d4	11.39	131	7590	0.61	ng/ul	0.00
43) Dimethylphthalate-d6	14.42	166	1380254	39.03	ng/ul	0.00
46) Acenaphthylene-d8	14.74	160	1732604	37.14	ng/ul	0.00
51) 4-Nitrophenol-d4	15.22	143	58392	8.89	ng/ul	0.00
57) Fluorene-d10	16.02	176	1131065	37.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.13	200	149043	27.34	ng/ul	0.00
70) Anthracene-d10	17.86	188	1682640	36.78	ng/ul	0.00
76) Pyrene-d10	20.12	212	1768439	36.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	1305418	39.05	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	9.14	70	16008	1.544	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032218\
Data File : BN000536.D
Acq On : 22 Mar 2018 12:45
Operator : JU/SJ
Sample : J1922-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 23 02:22:36 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 23 02:22:02 2018
Response via : Initial Calibration

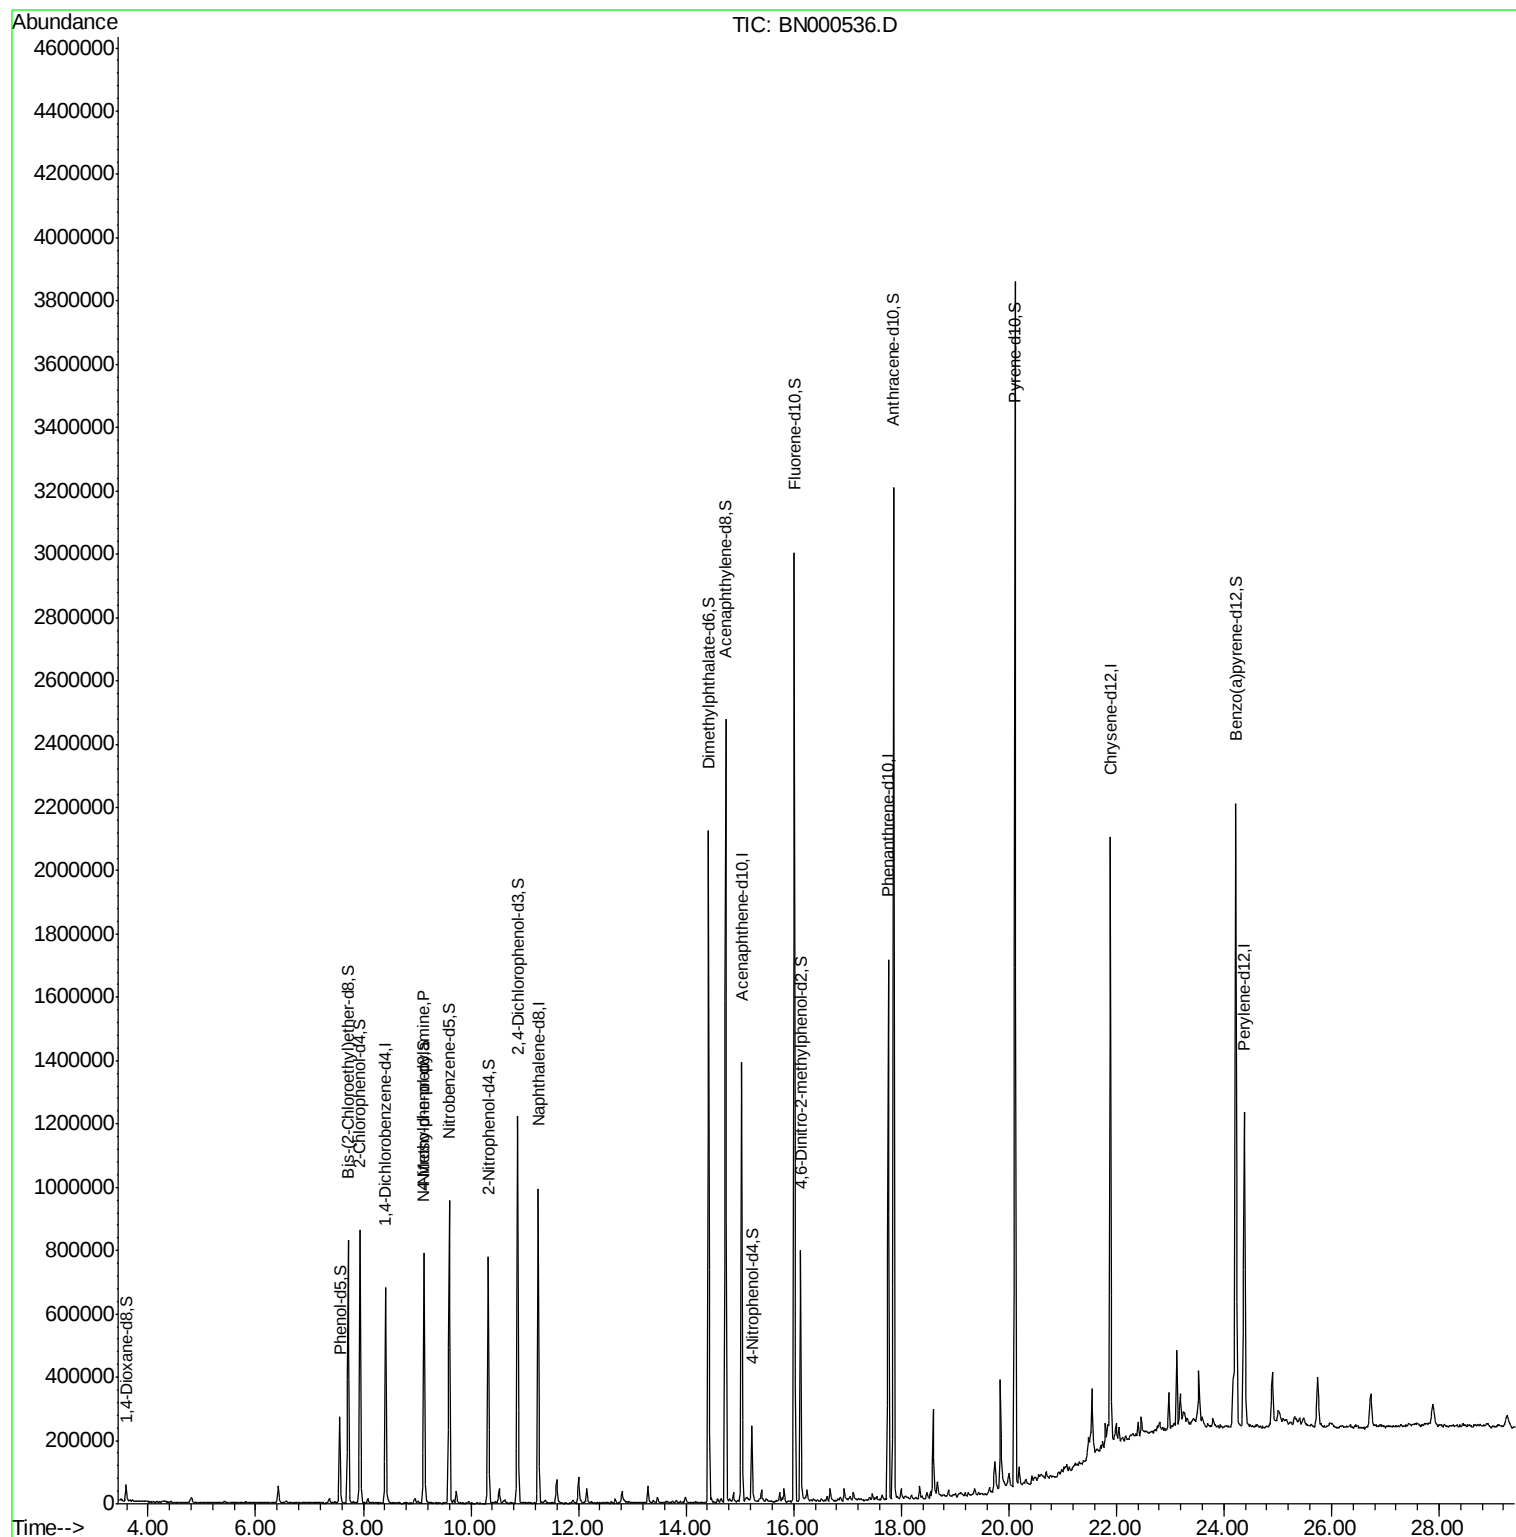

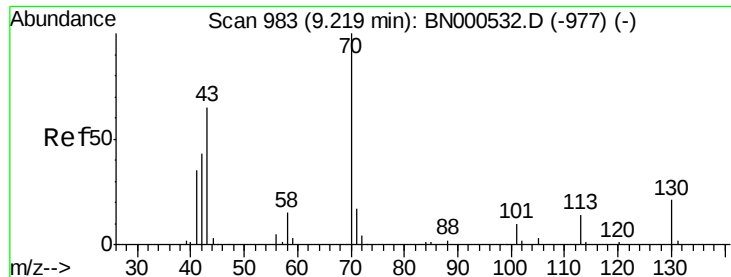

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.544 ng/ul
 RT: 9.14 min Scan# 969
 Delta R.T. -0.08 min
 Lab File: BN000536.D
 Acq: 22 Mar 2018 12:45

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 16008
 Ion Ratio Lower Upper
 70 100
 42 145.8 40.2 60.4#
 101 0.0 7.7 11.5#
 130 0.0 17.8 26.6#

