

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_N\DATA\BN032218\
 Data File : BN000554.D
 Acq On : 22 Mar 2018 23:20
 Operator : JU/SJ
 Sample : J1905-09DL 100X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM44DL

Quant Time: Mar 23 08:26:14 2018
 Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 23 02:22:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	177866	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	766046	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.03	164	422804	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.76	188	887123	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	674847	20.00	ng/ul	-0.01
83) Perylene-d12	24.36	264	545607	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.56	99	2072	0.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.72	67	4875	0.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.94	132	4078	0.33	ng/ul	0.00
13) 4-Methylphenol-d8	9.13	113	3069	0.24	ng/ul	0.00
19) Nitrobenzene-d5	9.60	128	2164	0.35	ng/ul	0.00
22) 2-Nitrophenol-d4	10.32	143	2000	0.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.87	165	3947	0.34	ng/ul	0.00
29) 4-Chloroaniline-d4	11.34	131	1686	0.14	ng/ul	-0.05
43) Dimethylphthalate-d6	14.42	166	14671	0.44	ng/ul	0.00
46) Acenaphthylene-d8	14.73	160	17205	0.39	ng/ul	0.00
51) 4-Nitrophenol-d4	15.23	143	1164	0.19	ng/ul	0.00
57) Fluorene-d10	16.01	176	14676	0.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.14	200	3516	0.69	ng/ul	0.00
70) Anthracene-d10	17.86	188	19414	0.46	ng/ul	0.00
76) Pyrene-d10	20.11	212	17006	0.46	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.20	264	10922	0.42	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
55) 2,3,4,6-Tetrachlorophenol	15.65	232	268527	39.142	ng/ul#	93
68) Pentachlorophenol	17.42	266	2484399	492.880	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_N\DATA\BN032218\
Data File : BN000554.D
Acq On : 22 Mar 2018 23:20
Operator : JU/SJ
Sample : J1905-09DL 100X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM44DL

Quant Time: Mar 23 08:26:14 2018
Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 23 02:22:02 2018
Response via : Initial Calibration

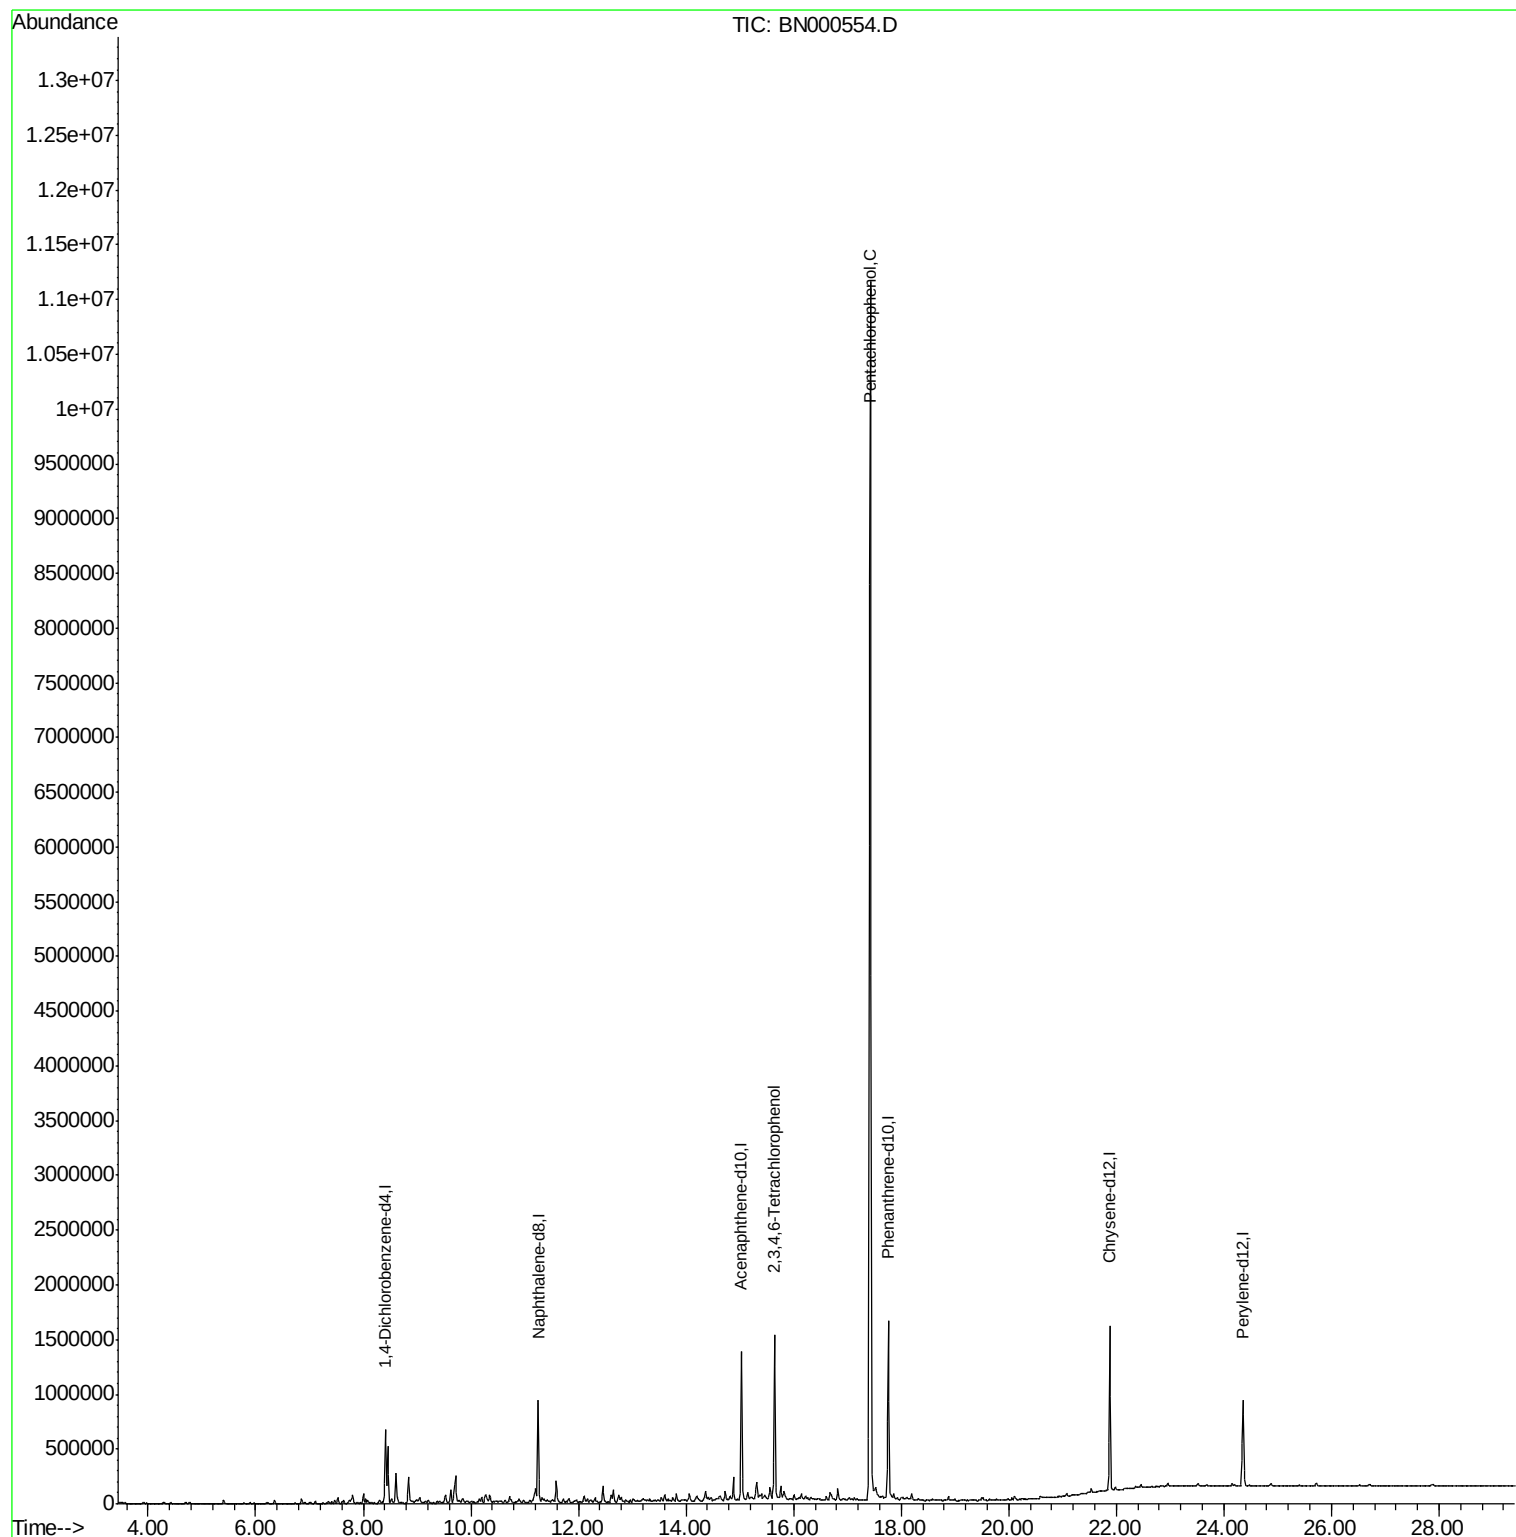

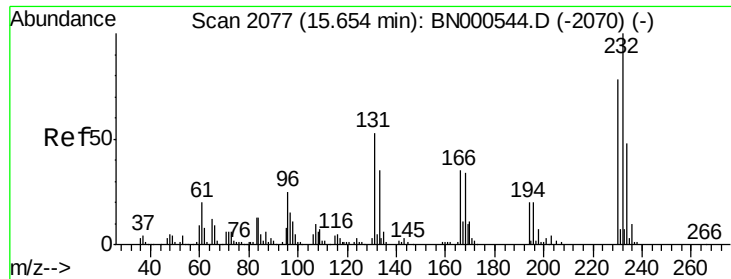

#55

2,3,4,6-Tetrachlorophenol

Concen: 39.142 ng/ul

RT: 15.65 min Scan# 2076

Delta R.T. -0.01 min

Lab File: BN000554.D

Acq: 22 Mar 2018 23:20

Instrument :

BNA_N

ClientSampled :

DAM44DL

Tgt Ion:232 Resp: 268527


Ion Ratio Lower Upper

232 100

131 54.7 48.0 72.0

130 2.9 4.0 6.0#

166 35.7 32.0 48.0



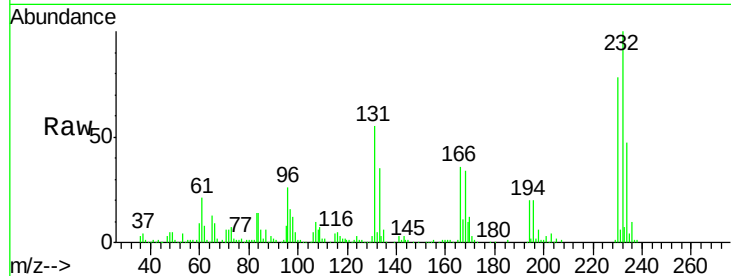


Abundance Ion 232.00 (231.70 to 232.70): E

Ion 131.00 (130.70 to 131.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 166.00 (165.70 to 166.70): E

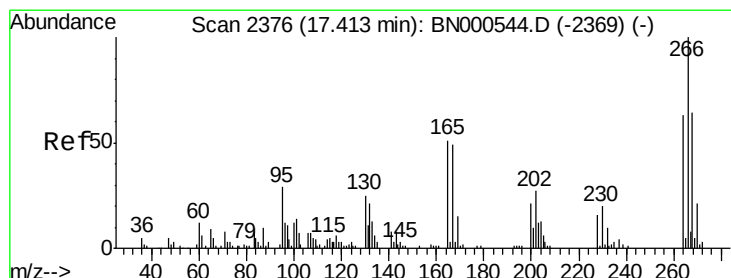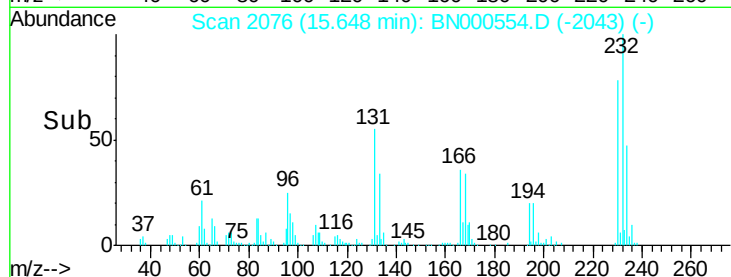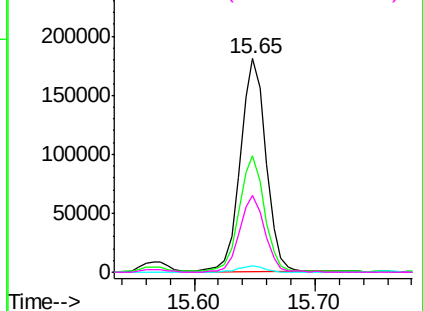

#68

Pentachlorophenol

Concen: 492.880 ng/ul

RT: 17.42 min Scan# 2378

Delta R.T. 0.01 min

Lab File: BN000554.D

Acq: 22 Mar 2018 23:20


Tgt Ion:266 Resp: 2484399

Ion Ratio Lower Upper

266 100

264 64.0 48.2 72.4

268 64.1 52.3 78.5

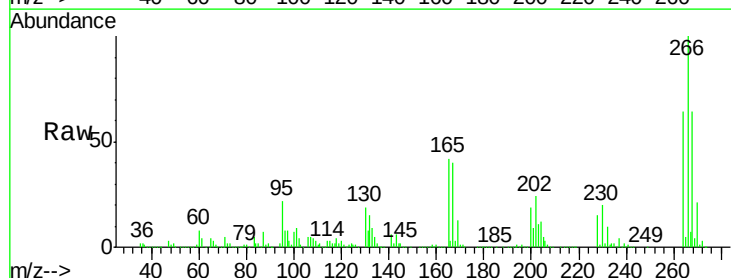

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

