

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019089.D
 Acq On : 23 Mar 2022 13:32
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Mar 23 16:45:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 13:18:23 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.854	152	4101	0.400	ng	0.00
7) Naphthalene-d8	10.658	136	10590	0.400	ng	# 0.00
13) Acenaphthene-d10	14.485	164	6124	0.400	ng	-0.01
19) Phenanthrene-d10	17.226	188	12299	0.400	ng	-0.01
29) Chrysene-d12	21.422	240	9232	0.400	ng	# 0.00
35) Perylene-d12	23.788	264	8257	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.406	112	3360	0.366	ng	0.00
5) Phenol-d6	7.010	99	3232	0.335	ng	0.00
8) Nitrobenzene-d5	9.004	82	2508	0.328	ng	-0.01
11) 2-Methylnaphthalene-d10	12.250	152	6106	0.348	ng	0.00
14) 2,4,6-Tribromophenol	15.985	330	781	0.264	ng	0.00
15) 2-Fluorobiphenyl	13.116	172	9499	0.387	ng	-0.01
27) Fluoranthene-d10	19.261	212	14005	0.384	ng	0.00
31) Terphenyl-d14	19.860	244	7676	0.339	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.247	88	2093	0.413	ng	99
3) n-Nitrosodimethylamine	3.579	42	1950	0.330	ng	# 96
6) bis(2-Chloroethyl)ether	7.269	93	4155	0.362	ng	97
9) Naphthalene	10.701	128	11647	0.387	ng	99
10) Hexachlorobutadiene	11.000	225	2787	0.378	ng	# 99
12) 2-Methylnaphthalene	12.322	142	7318	0.357	ng	97
16) Acenaphthylene	14.207	152	9925	0.349	ng	100
17) Acenaphthene	14.549	154	7428	0.373	ng	98
18) Fluorene	15.532	166	9215	0.367	ng	99
20) 4,6-Dinitro-2-methylph...	15.629	198	416	0.289	ng	# 56
21) 4-Bromophenyl-phenylether	16.426	248	2934	0.378	ng	94
22) Hexachlorobenzene	16.549	284	4148	0.415	ng	100
23) Atrazine	16.682	200	1734	0.299	ng	96
24) Pentachlorophenol	16.887	266	553	0.180	ng	97
25) Phenanthrene	17.267	178	14579	0.379	ng	100
26) Anthracene	17.359	178	10891	0.335	ng	99
28) Fluoranthene	19.291	202	17467	0.387	ng	99
30) Pyrene	19.653	202	17770	0.386	ng	99
32) Benzo(a)anthracene	21.405	228	9790	0.344	ng	99
33) Chrysene	21.458	228	15222	0.397	ng	100
34) Bis(2-ethylhexyl)phtha...	21.333	149	6052	0.321	ng	99
36) Indeno(1,2,3-cd)pyrene	26.238	276	10894	0.366	ng	96
37) Benzo(b)fluoranthene	23.112	252	15589	0.518	ng	96
38) Benzo(k)fluoranthene	23.112	252	15322	0.371	ng	95
39) Benzo(a)pyrene	23.688	252	10552	0.385	ng	# 68
40) Dibenzo(a,h)anthracene	26.264	278	6212	0.268	ng	# 92
41) Benzo(g,h,i)perylene	26.986	276	12582	0.430	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019089.D
Acq On : 23 Mar 2022 13:32
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Mar 23 16:45:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 13:18:23 2022
Response via : Initial Calibration




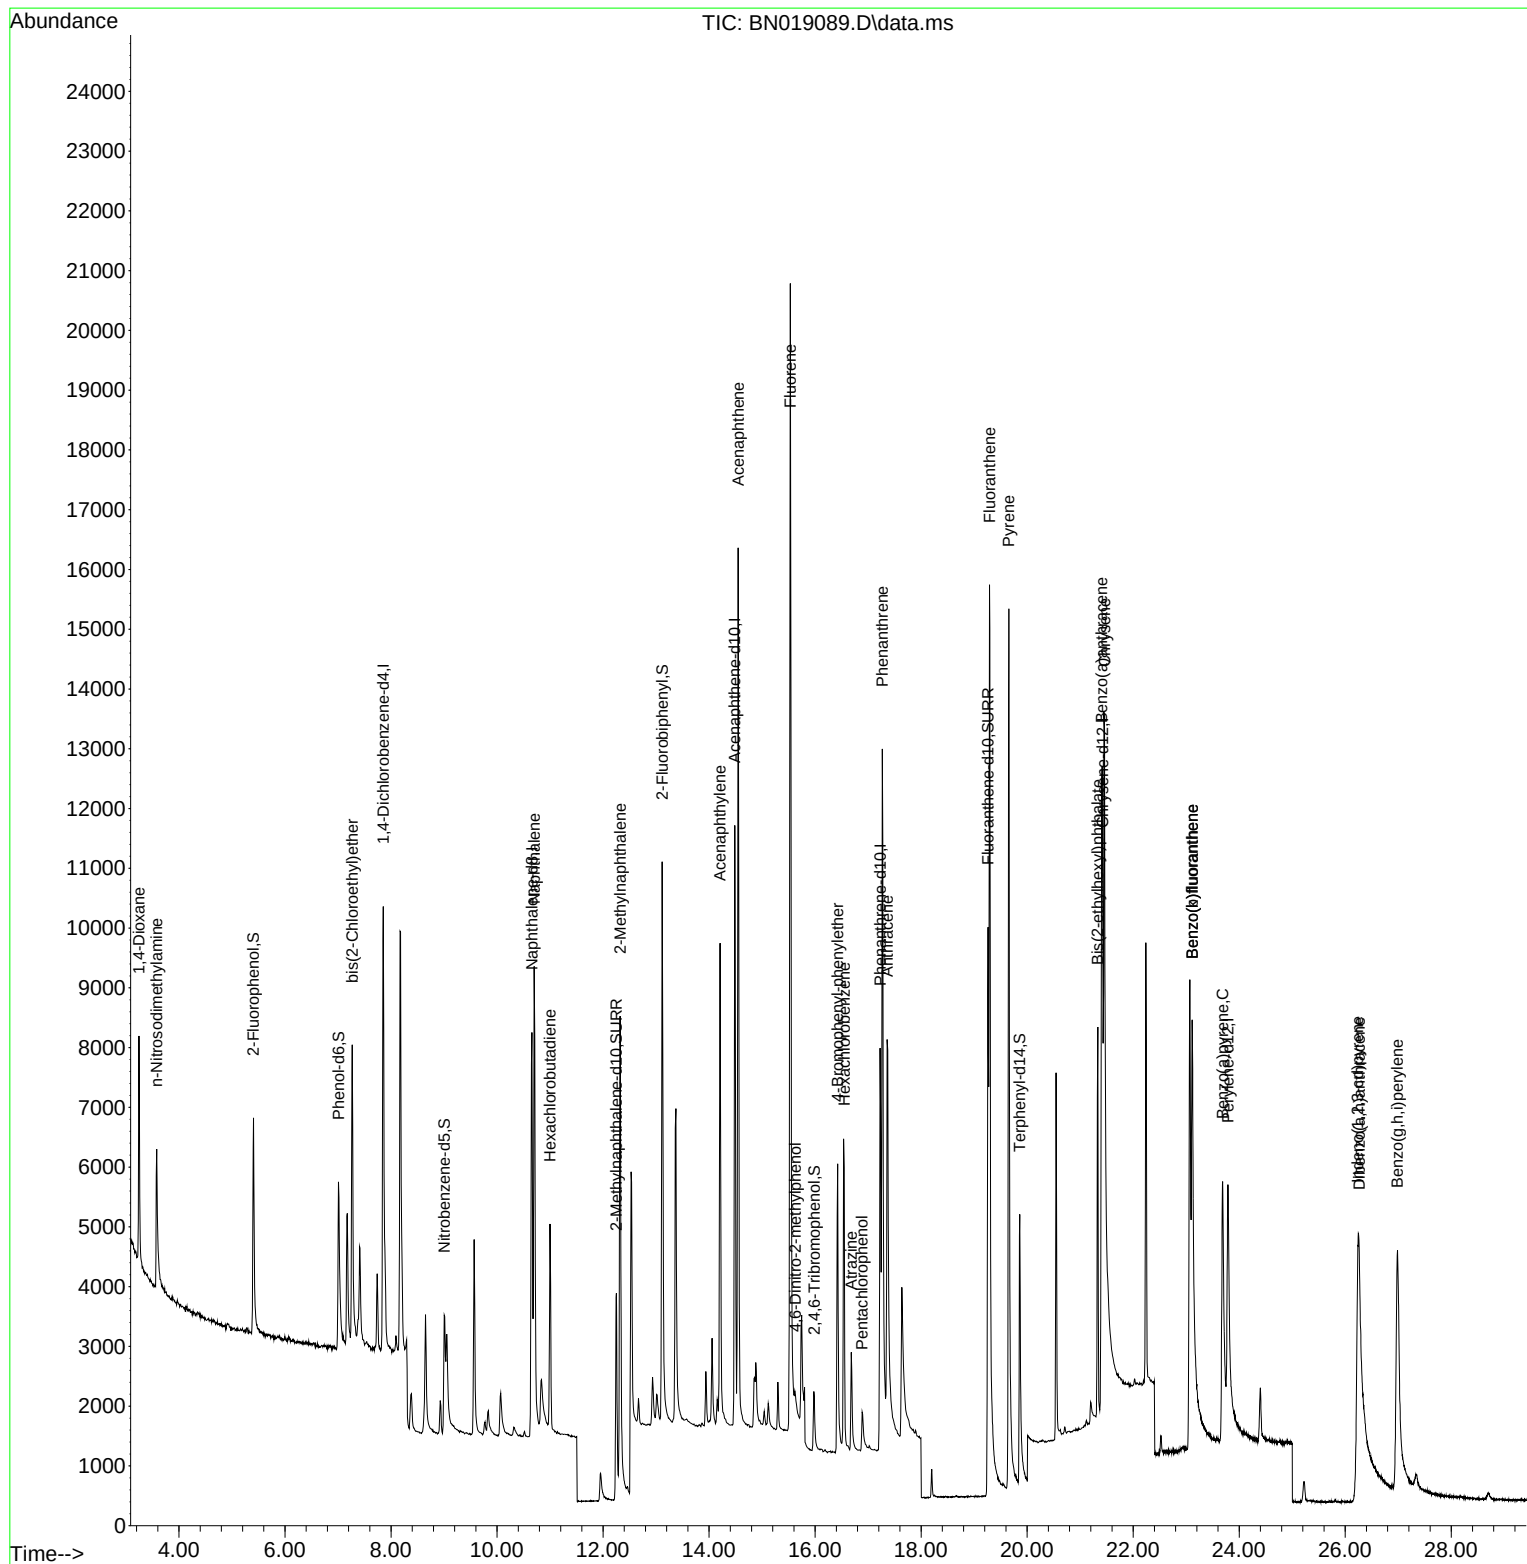




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.854 min Scan# 661
 Delta R.T. 0.000 min
 Lab File: BN019089.D
 Acq: 23 Mar 2022 13:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:152 Resp: 4101
 Ion Ratio Lower Upper
 152 100
 150 153.1 123.9 185.9
 115 61.0 48.2 72.4

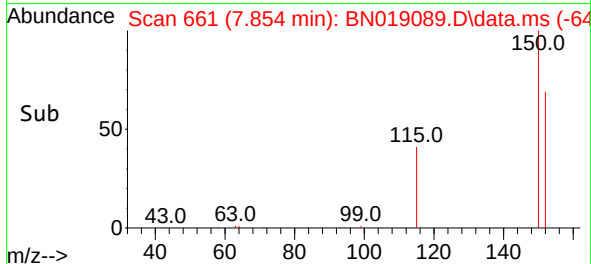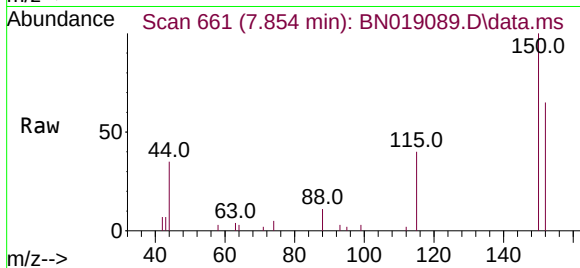

#2
 1,4-Dioxane
 Concen: 0.413 ng
 RT: 3.247 min Scan# 23
 Delta R.T. 0.000 min
 Lab File: BN019089.D
 Acq: 23 Mar 2022 13:32

Tgt Ion: 88 Resp: 2093
 Ion Ratio Lower Upper
 88 100
 43 32.3 24.6 37.0
 58 82.2 65.4 98.2




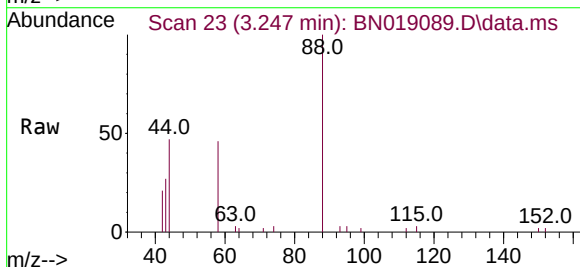


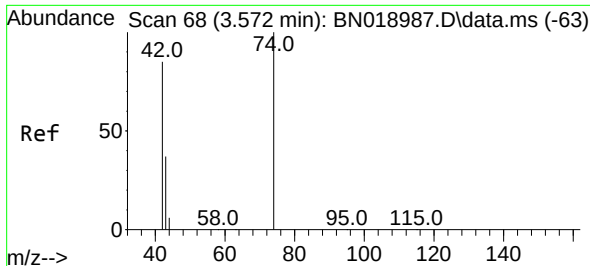

#3
n-Nitrosodimethylamine
Concen: 0.330 ng
RT: 3.579 min Scan# 61
Delta R.T. 0.007 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 1950
Ion Ratio Lower Upper
42 100
74 116.9 96.9 145.3
44 6.8 7.3 10.9#

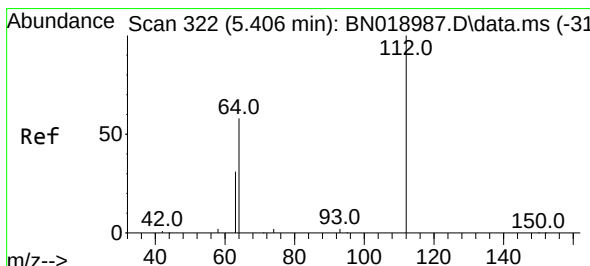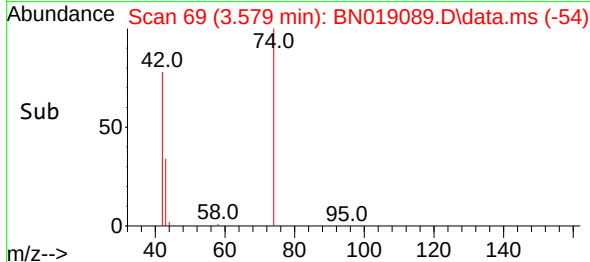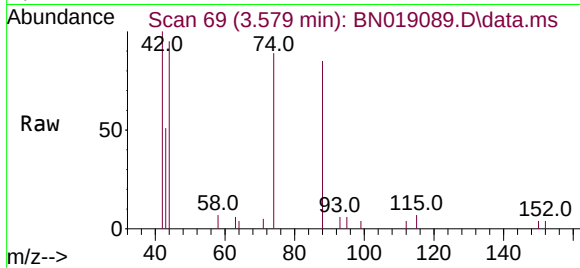

#4
2-Fluorophenol
Concen: 0.366 ng
RT: 5.406 min Scan# 322
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion: 112 Resp: 3360
Ion Ratio Lower Upper
112 100
64 62.9 47.8 71.8
63 31.8 25.7 38.5


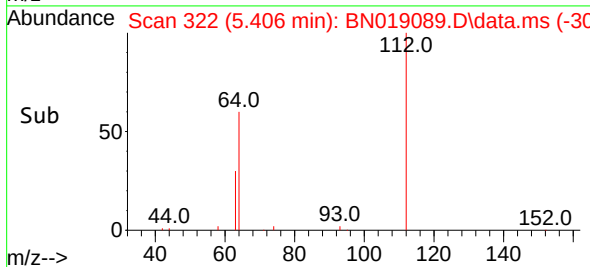

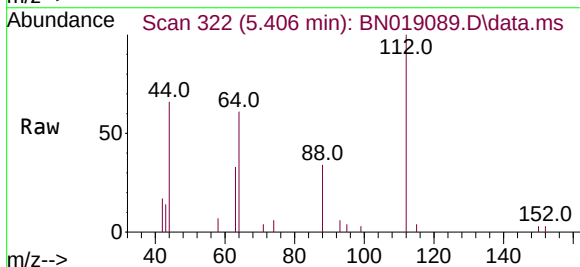




#5
Phenol-d6
Concen: 0.335 ng
RT: 7.010 min Scan# 544
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 3232
Ion Ratio Lower Upper
99 100
42 21.8 16.2 24.4
71 35.1 27.7 41.5

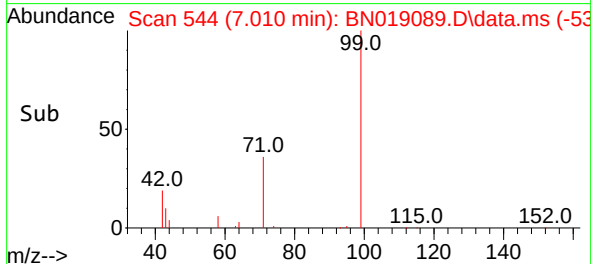

#6
bis(2-Chloroethyl)ether
Concen: 0.362 ng
RT: 7.269 min Scan# 580
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion: 93 Resp: 4155
Ion Ratio Lower Upper
93 100
63 81.9 62.8 94.2
95 33.0 26.2 39.4









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.658 min Scan# 944
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	10590
Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.0	13.4
54	8.9	5.8	8.6
68	6.7	4.6	7.0

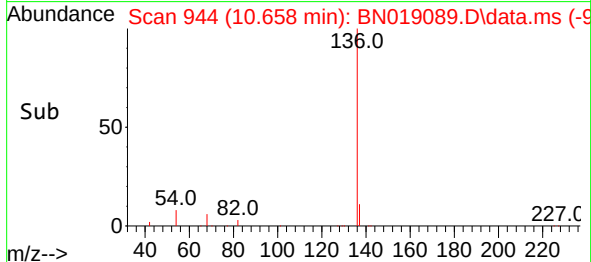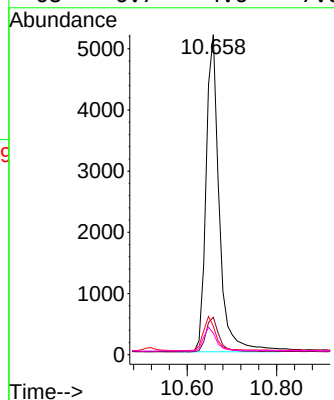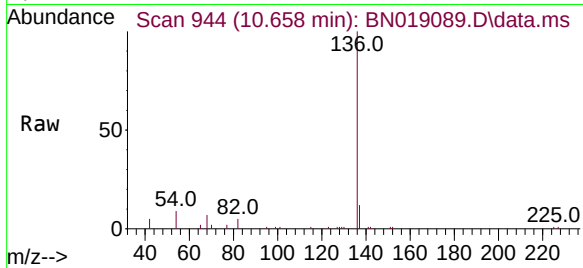

#8
Nitrobenzene-d5
Concen: 0.328 ng
RT: 9.004 min Scan# 789
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:	82	Resp:	2508
Ion	Ratio	Lower	Upper
82	100		
128	36.4	33.0	49.6
54	61.8	42.5	63.7



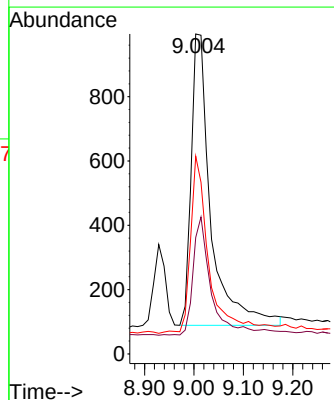
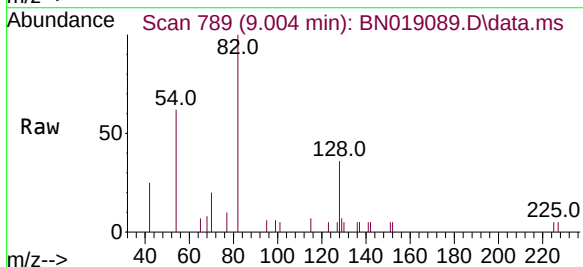


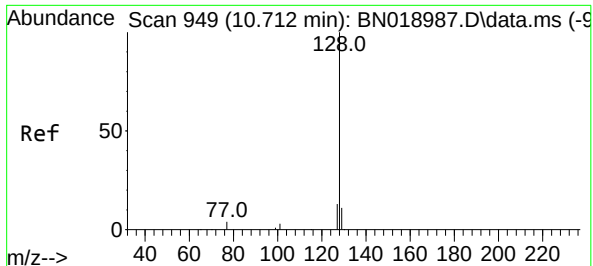

#9
Naphthalene
Concen: 0.387 ng
RT: 10.701 min Scan# 949
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	11647
Ion Ratio	Lower	Upper	
128	100		
129	11.4	9.0	13.4
127	13.6	10.7	16.1

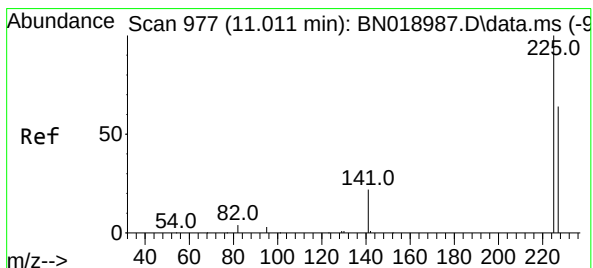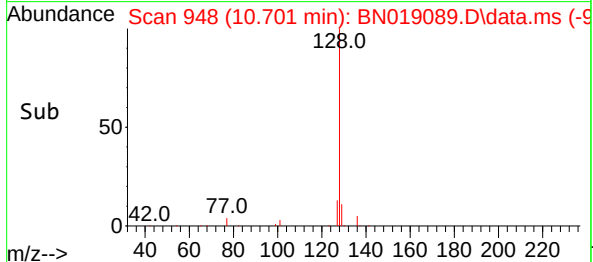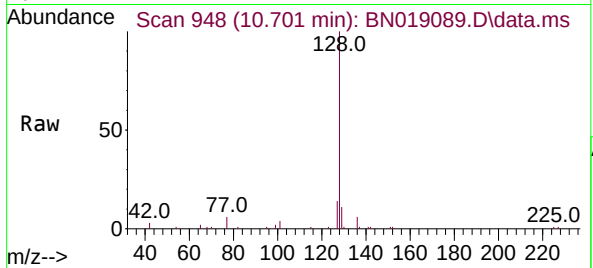

#10
Hexachlorobutadiene
Concen: 0.378 ng
RT: 11.000 min Scan# 976
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:	225	Resp:	2787
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.2	51.0	76.6


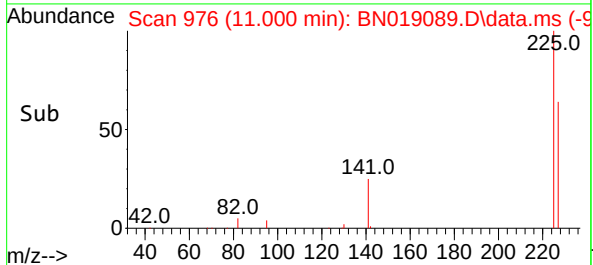

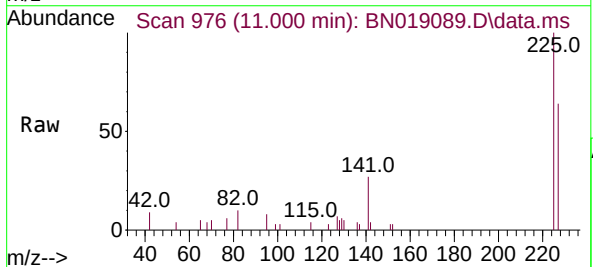




#11
2-Methylnaphthalene-d10
Concen: 0.348 ng
RT: 12.250 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 6106
Ion Ratio Lower Upper
152 100
151 20.4 16.5 24.7

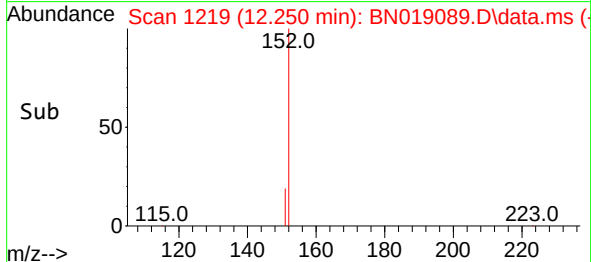

#12
2-Methylnaphthalene
Concen: 0.357 ng
RT: 12.322 min Scan# 1238
Delta R.T. -0.004 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:142 Resp: 7318
Ion Ratio Lower Upper
142 100
141 89.8 70.0 105.0
115 38.8 29.8 44.8




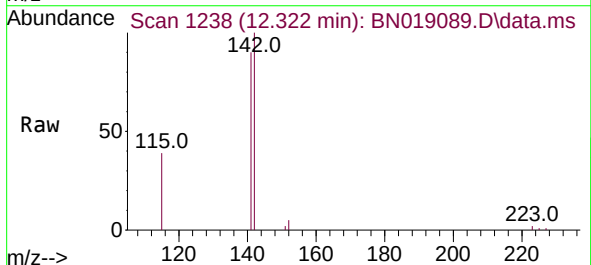




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.485 min Scan# 1473
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 6124
Ion Ratio Lower Upper
164 100
162 106.6 85.2 127.8
160 50.6 41.5 62.3

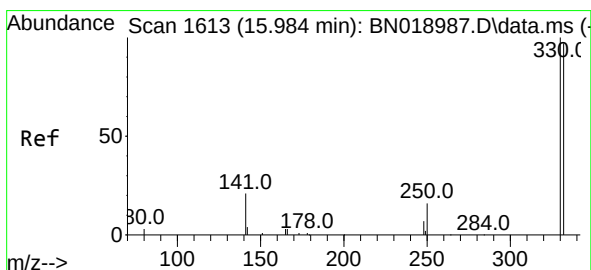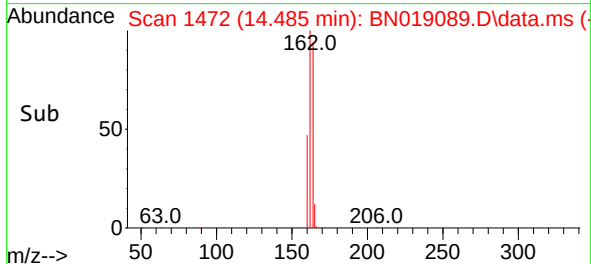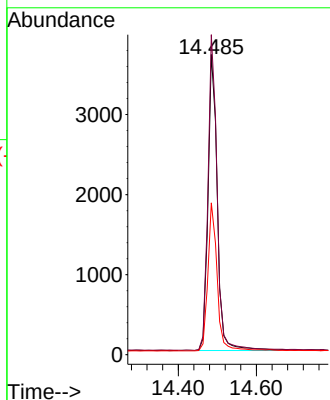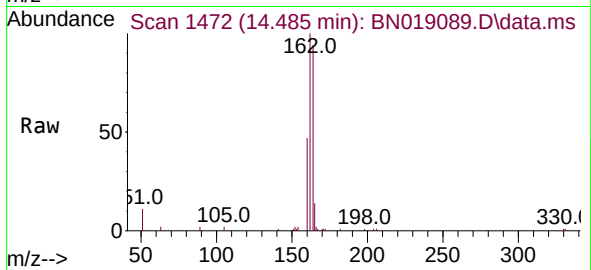

#14
2,4,6-Tribromophenol
Concen: 0.264 ng
RT: 15.985 min Scan# 1613
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:330 Resp: 781
Ion Ratio Lower Upper
330 100
332 96.9 76.8 115.2
141 0.0 32.2 48.2#



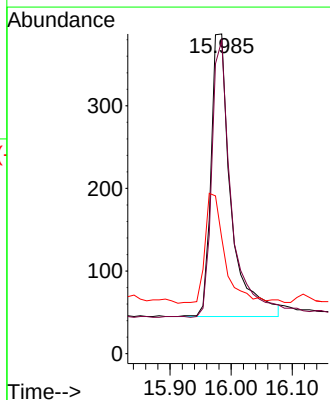





#15
2-Fluorobiphenyl
Concen: 0.387 ng
RT: 13.116 min Scan# 1344
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 9499
Ion Ratio Lower Upper
172 100
171 35.7 28.2 42.2
170 24.3 18.7 28.1

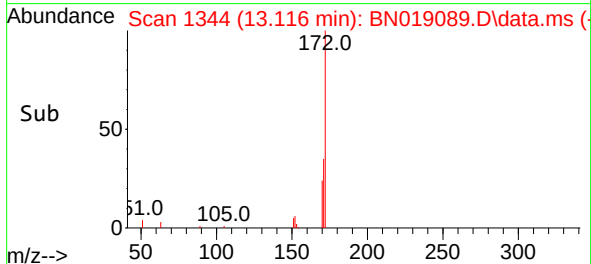

#16
Acenaphthylene
Concen: 0.349 ng
RT: 14.207 min Scan# 1446
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:152 Resp: 9925
Ion Ratio Lower Upper
152 100
151 19.8 15.9 23.9
153 13.2 10.6 15.8


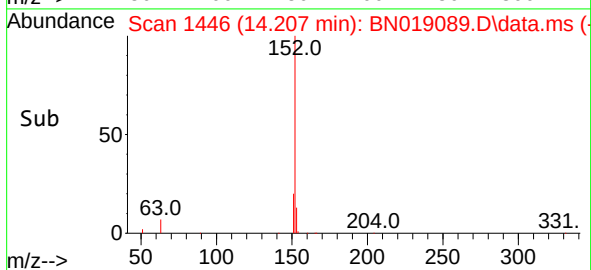




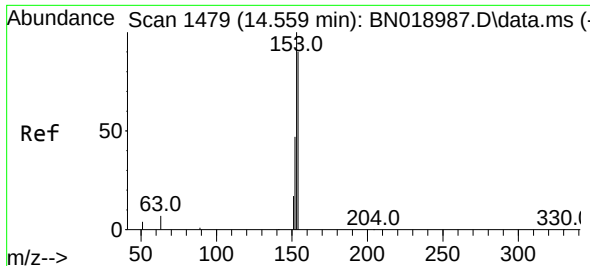

#17
Acenaphthene
Concen: 0.373 ng
RT: 14.549 min Scan# 1479
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 7428
Ion Ratio Lower Upper
154 100
153 114.5 89.7 134.5
152 57.2 44.7 67.1

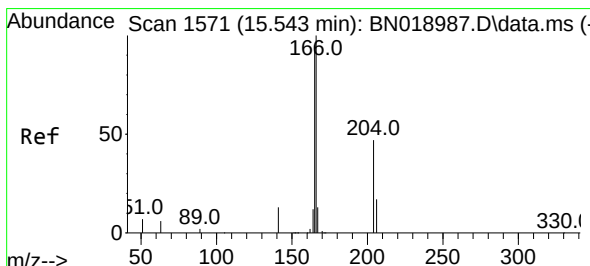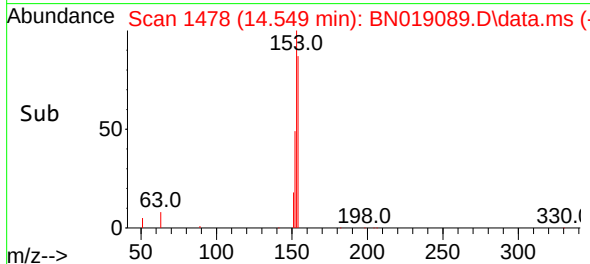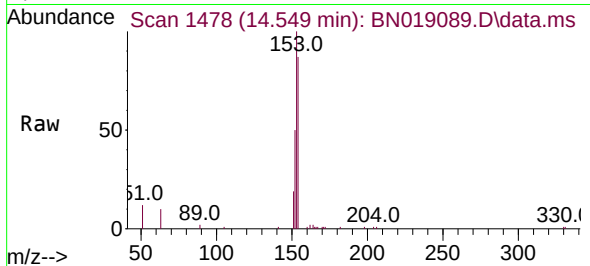

#18
Fluorene
Concen: 0.367 ng
RT: 15.532 min Scan# 1570
Delta R.T. -0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:166 Resp: 9215
Ion Ratio Lower Upper
166 100
165 99.6 79.2 118.8
167 13.5 10.7 16.1


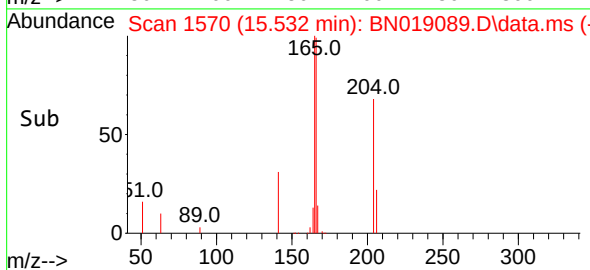

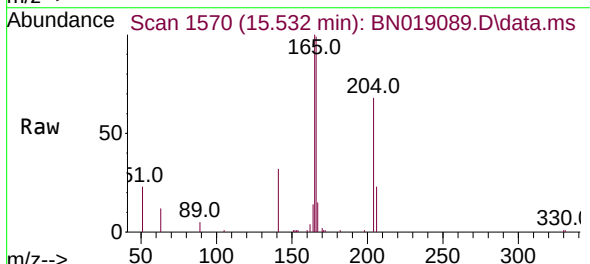




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.226 min Scan# 1734
Delta R.T. -0.010 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 12299
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.2 11.8 17.8

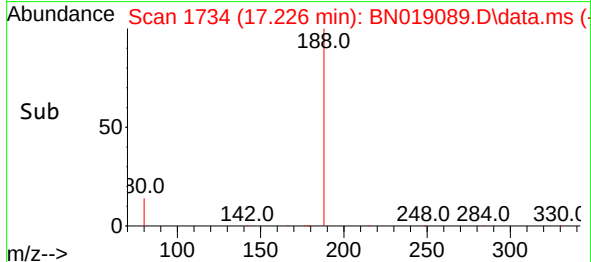

#20
4,6-Dinitro-2-methylphenol
Concen: 0.289 ng
RT: 15.629 min Scan# 1579
Delta R.T. 0.011 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:198 Resp: 416
Ion Ratio Lower Upper
198 100
182 34.8 13.0 19.4#
77 0.0 0.0 0.0


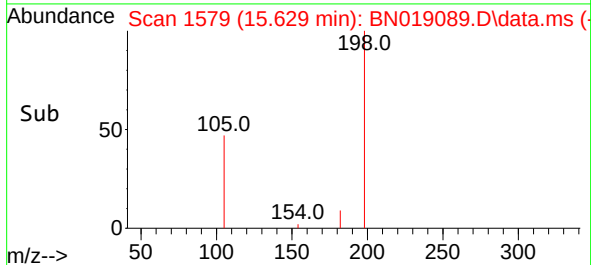






#21
4-Bromophenyl-phenylether
Concen: 0.378 ng
RT: 16.426 min Scan# 1656
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 2934
Ion Ratio Lower Upper
248 100
250 98.1 80.7 121.1
141 58.4 39.6 59.4

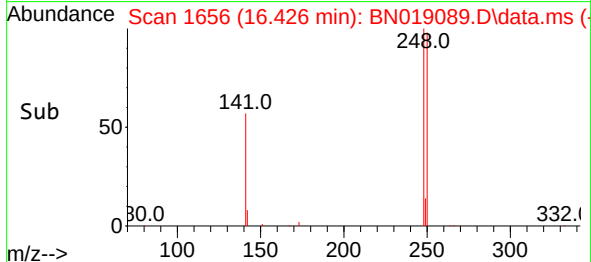

#22
Hexachlorobenzene
Concen: 0.415 ng
RT: 16.549 min Scan# 1668
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:284 Resp: 4148
Ion Ratio Lower Upper
284 100
142 37.4 29.8 44.8
249 32.8 26.2 39.2




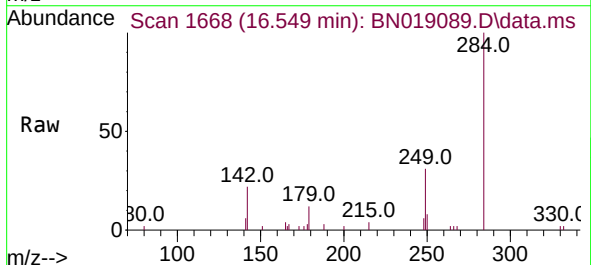


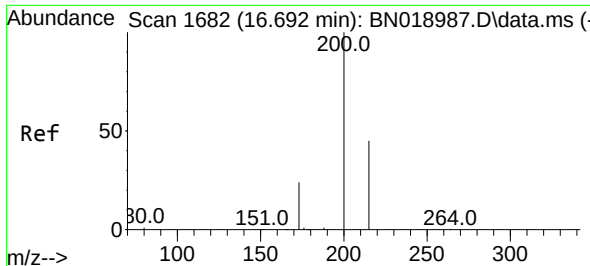

#23
Atrazine
Concen: 0.299 ng
RT: 16.682 min Scan# 1681
Delta R.T. -0.010 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 1734
Ion Ratio Lower Upper
200 100
173 33.3 23.9 35.9
215 46.8 36.6 54.8

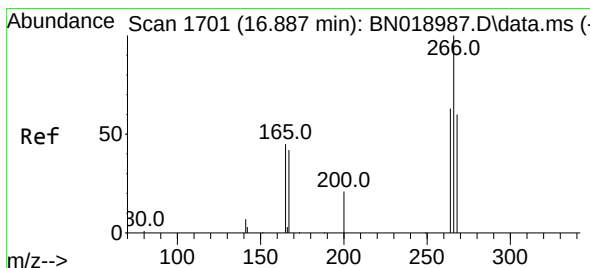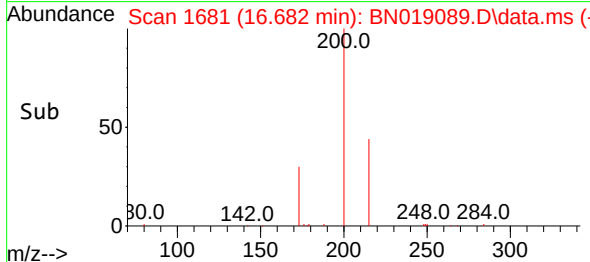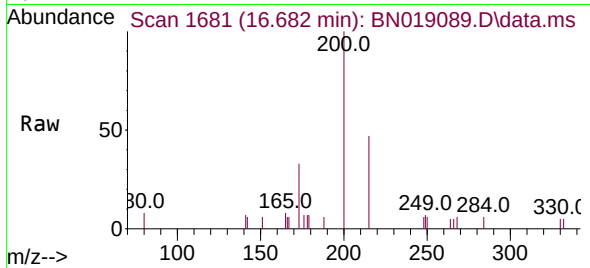

#24
Pentachlorophenol
Concen: 0.180 ng
RT: 16.887 min Scan# 1701
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:266 Resp: 553
Ion Ratio Lower Upper
266 100
264 67.1 50.2 75.4
268 66.0 51.9 77.9


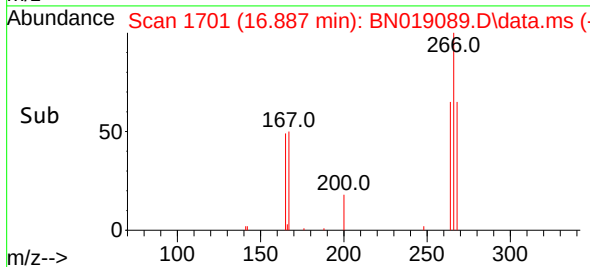

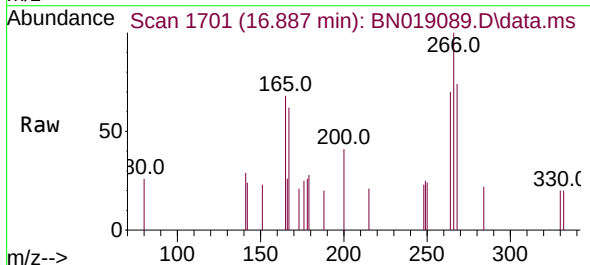


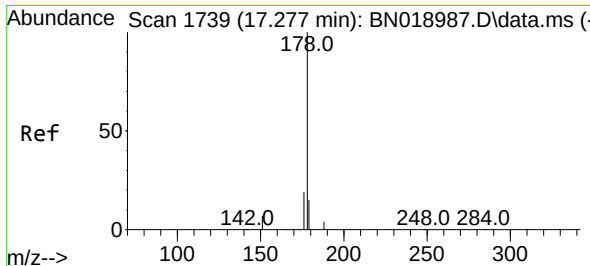

#25
Phenanthrene
Concen: 0.379 ng
RT: 17.267 min Scan# 1738
Delta R.T. -0.010 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 14579
Ion Ratio Lower Upper
178 100
176 19.1 15.4 23.0
179 15.2 12.2 18.2

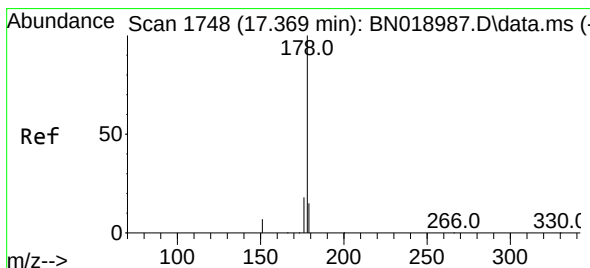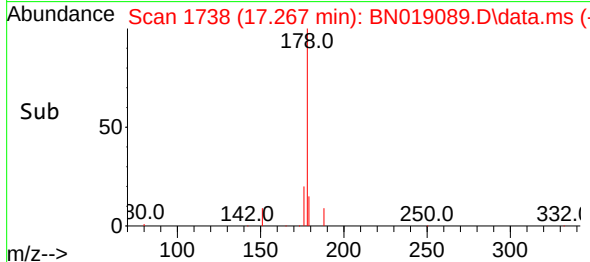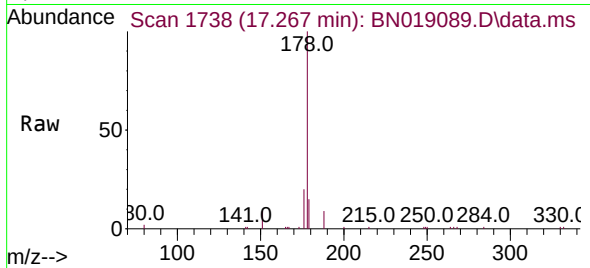

#26
Anthracene
Concen: 0.335 ng
RT: 17.359 min Scan# 1747
Delta R.T. -0.010 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:178 Resp: 10891
Ion Ratio Lower Upper
178 100
176 19.0 14.8 22.2
179 14.7 12.2 18.4


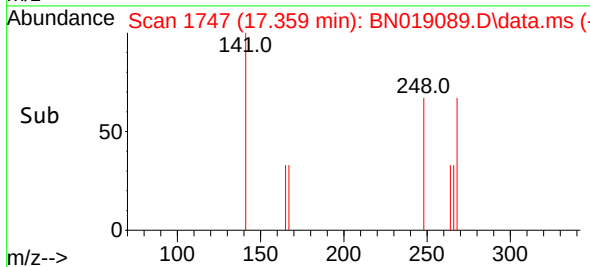

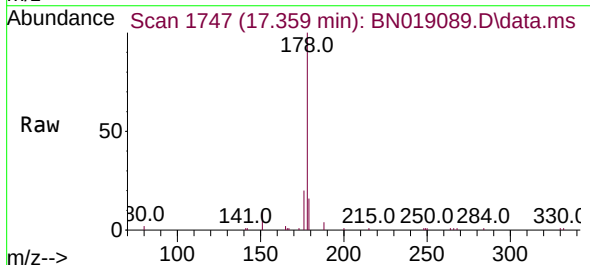


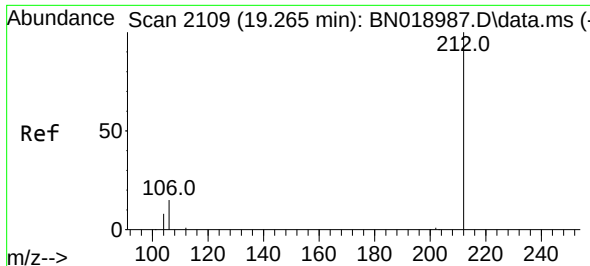

#27
Fluoranthene-d10
Concen: 0.384 ng
RT: 19.261 min Scan# 2108
Delta R.T. -0.004 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 14005
Ion Ratio Lower Upper
212 100
106 15.2 12.7 19.1
104 8.7 7.1 10.7

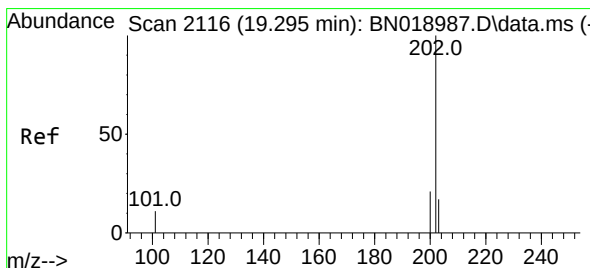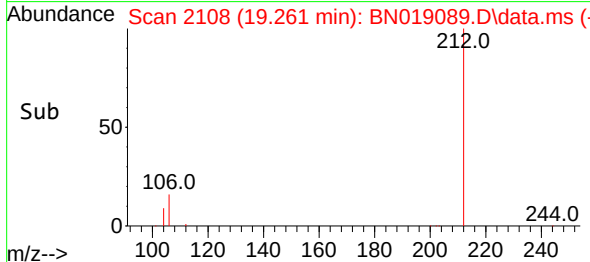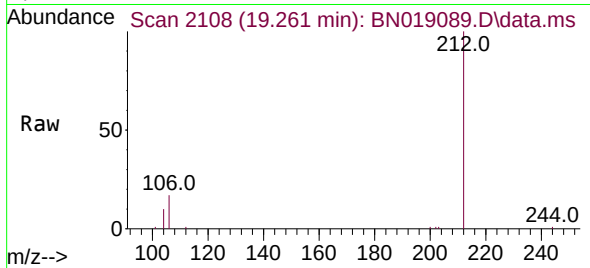

#28
Fluoranthene
Concen: 0.387 ng
RT: 19.291 min Scan# 2115
Delta R.T. -0.004 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:202 Resp: 17467
Ion Ratio Lower Upper
202 100
101 11.8 9.8 14.6
203 16.5 13.7 20.5


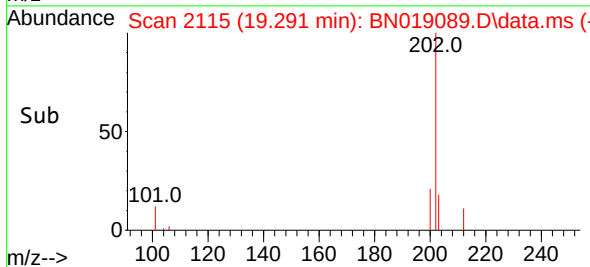

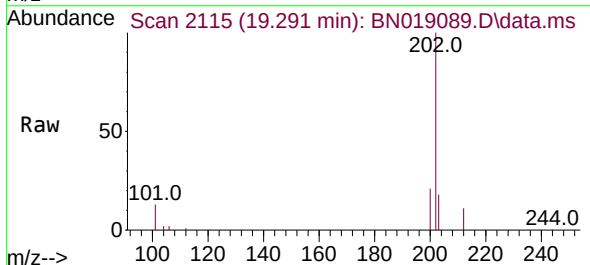




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.422 min Scan# 2443
Delta R.T. 0.000 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 9232
Ion Ratio Lower Upper
240 100
120 16.3 8.5 12.7#
236 29.5 22.4 33.6

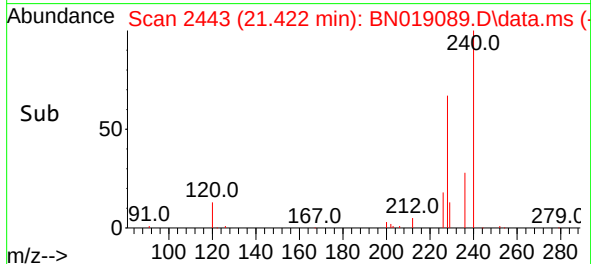

#30
Pyrene
Concen: 0.386 ng
RT: 19.653 min Scan# 2201
Delta R.T. -0.004 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:202 Resp: 17770
Ion Ratio Lower Upper
202 100
200 21.2 16.9 25.3
203 17.2 14.2 21.2


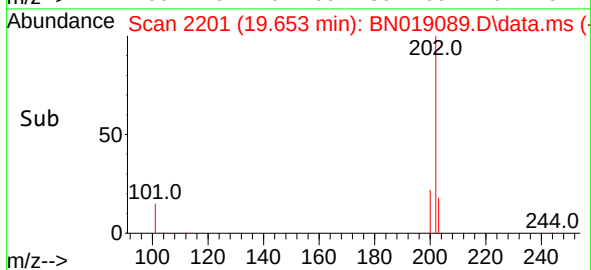

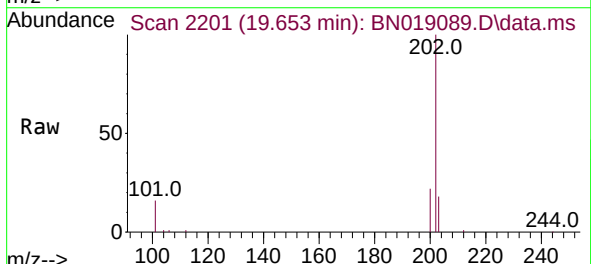




#31
 Terphenyl-d14
 Concen: 0.339 ng
 RT: 19.860 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN019089.D
 Acq: 23 Mar 2022 13:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 7676
 Ion Ratio Lower Upper
 244 100
 212 11.2 8.2 12.4
 122 0.0 0.0 0.0

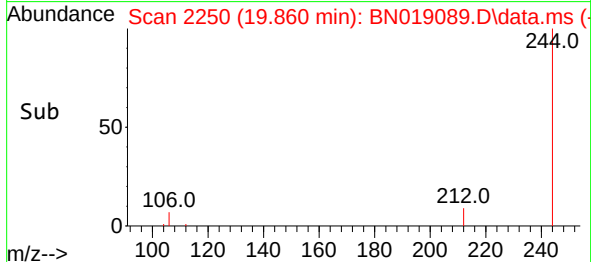

#32
 Benzo(a)anthracene
 Concen: 0.344 ng
 RT: 21.405 min Scan# 2441
 Delta R.T. 0.000 min
 Lab File: BN019089.D
 Acq: 23 Mar 2022 13:32

Tgt Ion:228 Resp: 9790
 Ion Ratio Lower Upper
 228 100
 226 28.1 21.9 32.9
 229 20.3 16.0 24.0

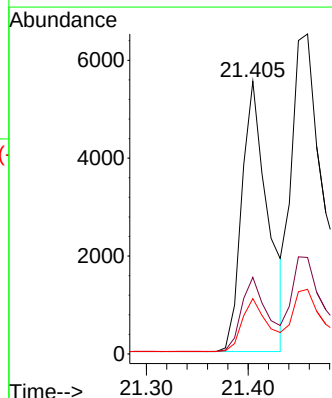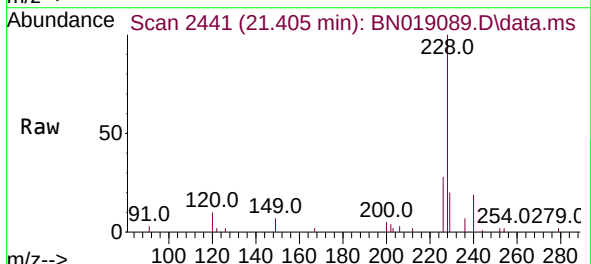

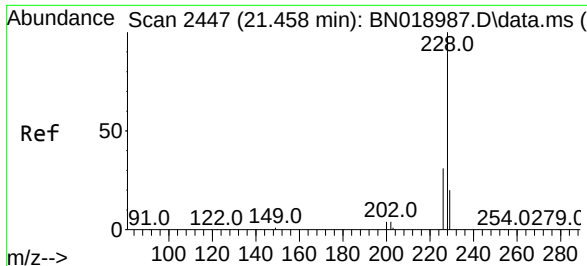

#33

Chrysene

Concen: 0.397 ng

RT: 21.458 min Scan# 2447

Delta R.T. 0.000 min

Lab File: BN019089.D

Acq: 23 Mar 2022 13:32

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 15222

Ion Ratio Lower Upper

228 100

226 30.2 24.0 36.0

229 20.2 15.9 23.9

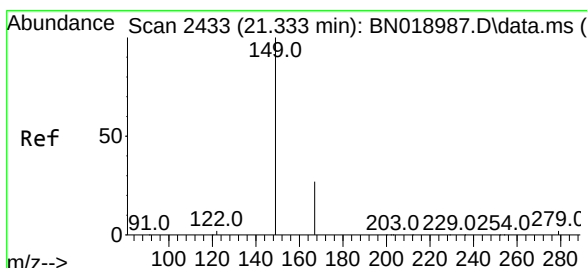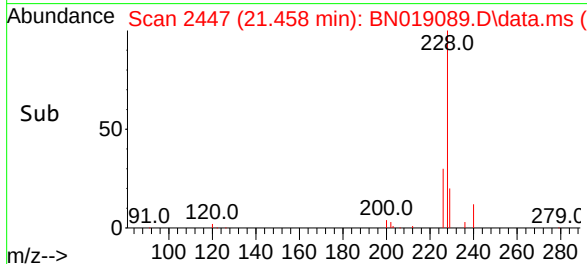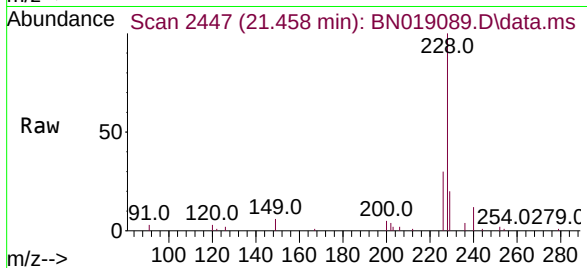

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.321 ng

RT: 21.333 min Scan# 2433

Delta R.T. 0.000 min

Lab File: BN019089.D

Acq: 23 Mar 2022 13:32




Tgt Ion:149 Resp: 6052


Ion Ratio Lower Upper

149 100

167 27.7 21.8 32.8

279 2.9 2.0 3.0


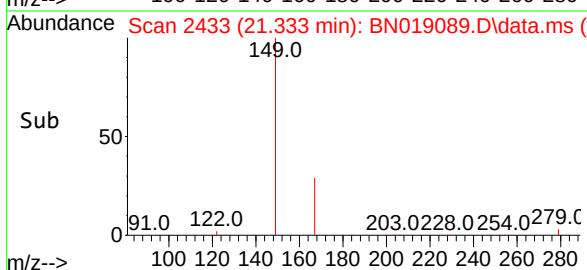
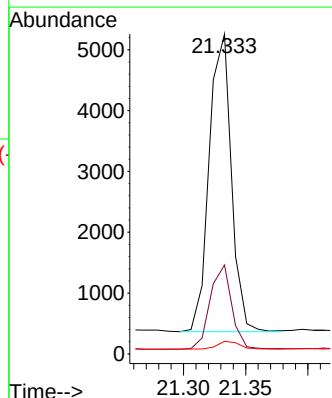
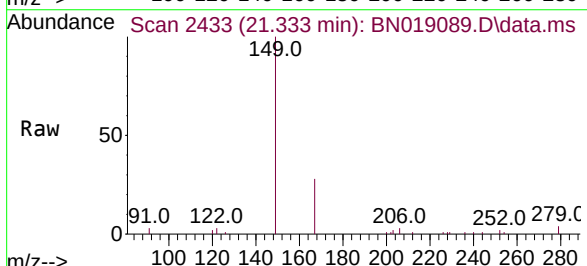




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.788 min Scan# 30
Delta R.T. -0.003 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:264 Resp: 8257
Ion Ratio Lower Upper
264 100
260 28.8 22.4 33.6
265 42.9 25.3 37.9#

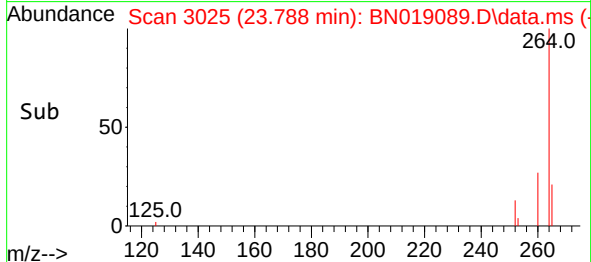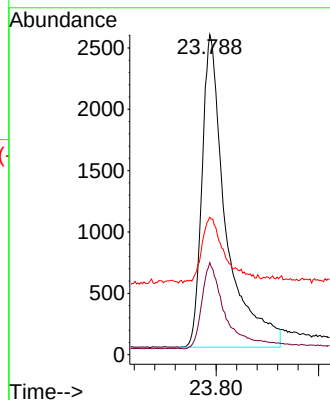

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.366 ng
RT: 26.238 min Scan# 3863
Delta R.T. -0.012 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:276 Resp: 10894
Ion Ratio Lower Upper
276 100
138 27.2 24.5 36.7
277 24.3 19.8 29.8



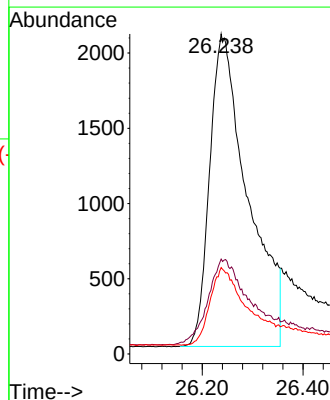
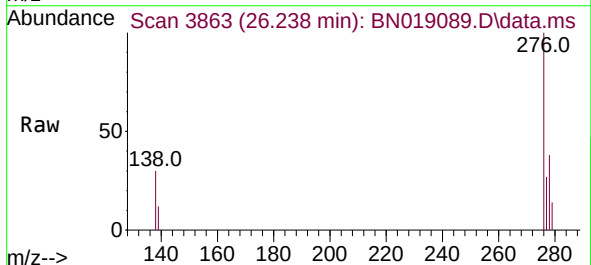




#37
Benzo(b)fluoranthene
Concen: 0.518 ng
RT: 23.112 min Scan# 2794
Delta R.T. 0.038 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 15589
Ion Ratio Lower Upper
252 100
253 26.3 18.9 28.3
125 14.0 12.1 18.1

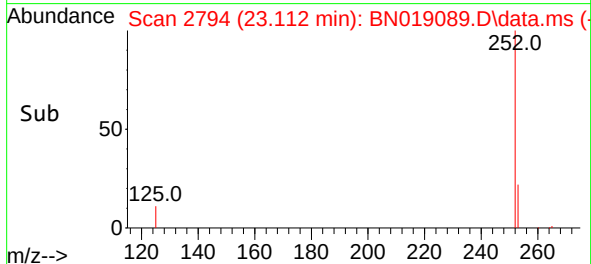

#38
Benzo(k)fluoranthene
Concen: 0.371 ng
RT: 23.112 min Scan# 2794
Delta R.T. -0.006 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:252 Resp: 15322
Ion Ratio Lower Upper
252 100
253 26.3 18.9 28.3
125 14.0 10.3 15.5


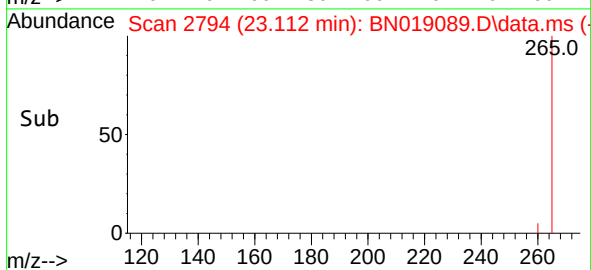






#39
Benzo(a)pyrene
Concen: 0.385 ng
RT: 23.688 min Scan# 2991
Delta R.T. -0.003 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 10552
Ion Ratio Lower Upper
252 100
253 32.8 20.1 30.1#
125 42.9 15.2 22.8#

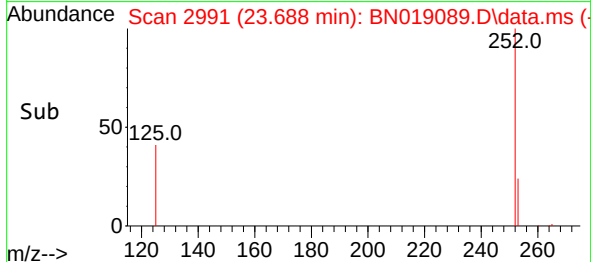

#40
Dibenzo(a,h)anthracene
Concen: 0.268 ng
RT: 26.264 min Scan# 3872
Delta R.T. -0.012 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Tgt Ion:278 Resp: 6212
Ion Ratio Lower Upper
278 100
139 23.6 17.2 25.8
279 30.5 19.9 29.9#

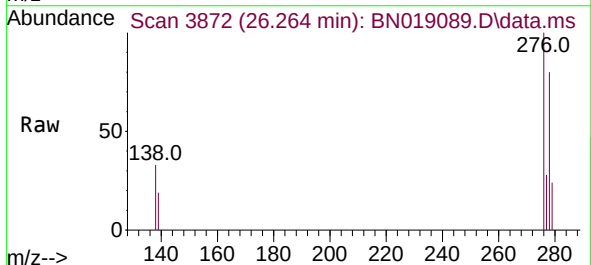

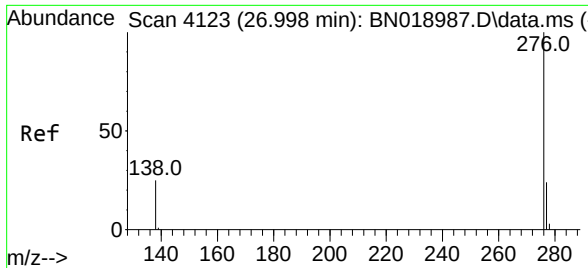

#41
Benzo(g,h,i)perylene
Concen: 0.430 ng
RT: 26.986 min Scan# 41
Delta R.T. -0.012 min
Lab File: BN019089.D
Acq: 23 Mar 2022 13:32

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 12582
Ion Ratio Lower Upper
276 100
277 25.3 19.4 29.0
138 28.0 21.0 31.6

