
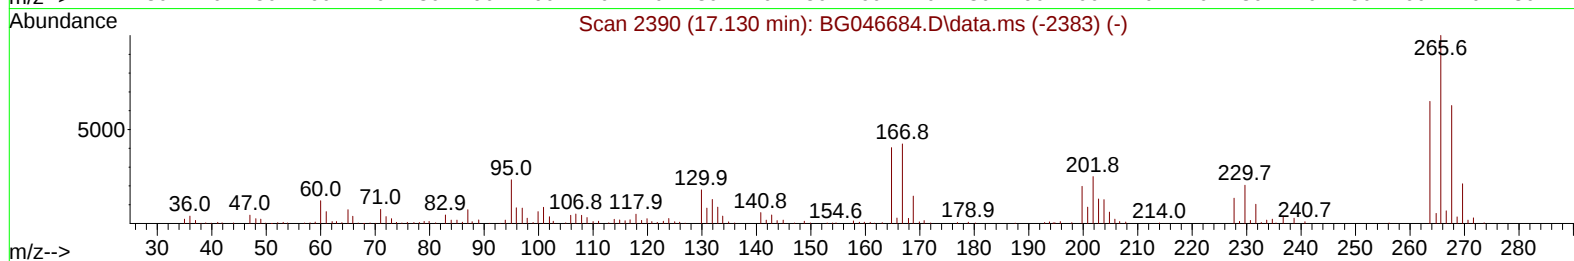
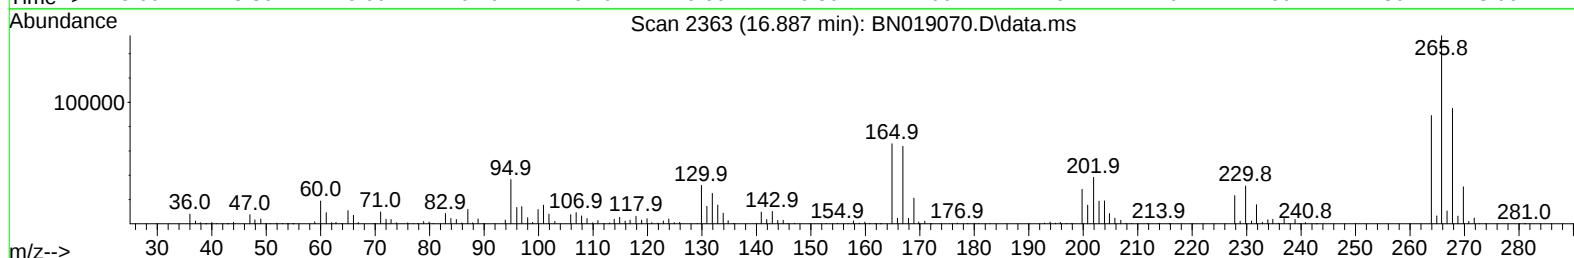


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019070.D
Acq On : 23 Mar 2022 00:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 06:13:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

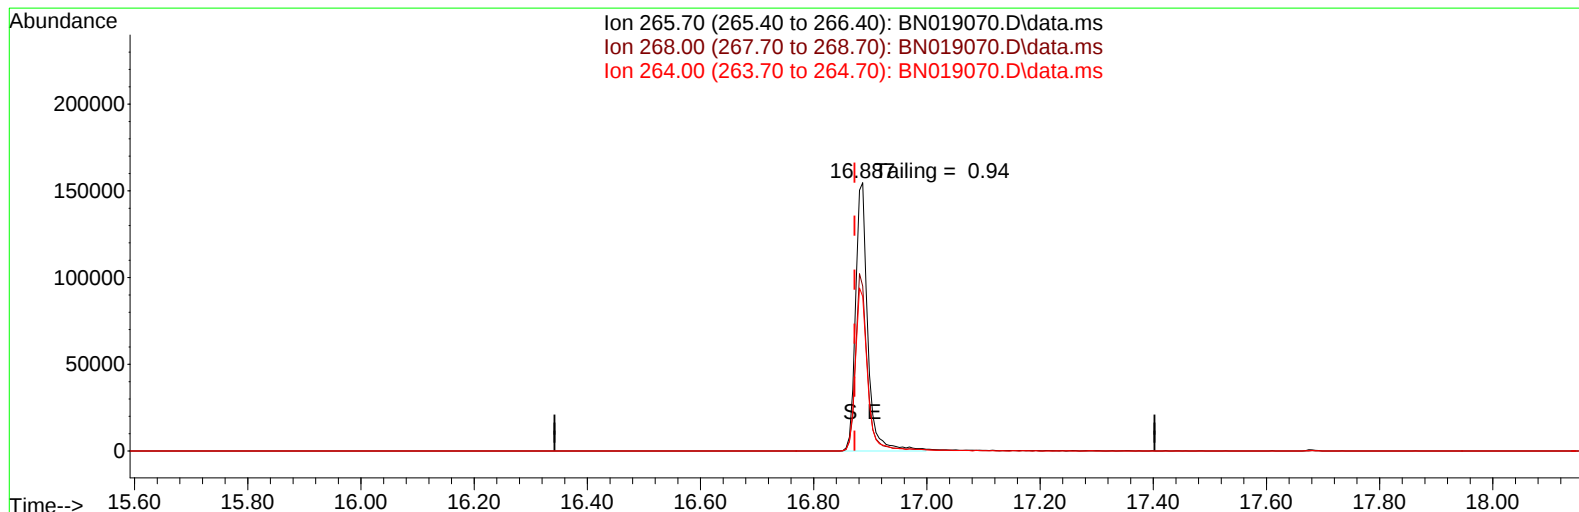

TIC: BN019070.D\data.ms

(70) Pentachlorophenol (C)




16.887min (+ 0.015) 16800.81 ng

response 234163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.42
264.00	61.60	57.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019070.D
Acq On : 23 Mar 2022 00:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 06:13:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

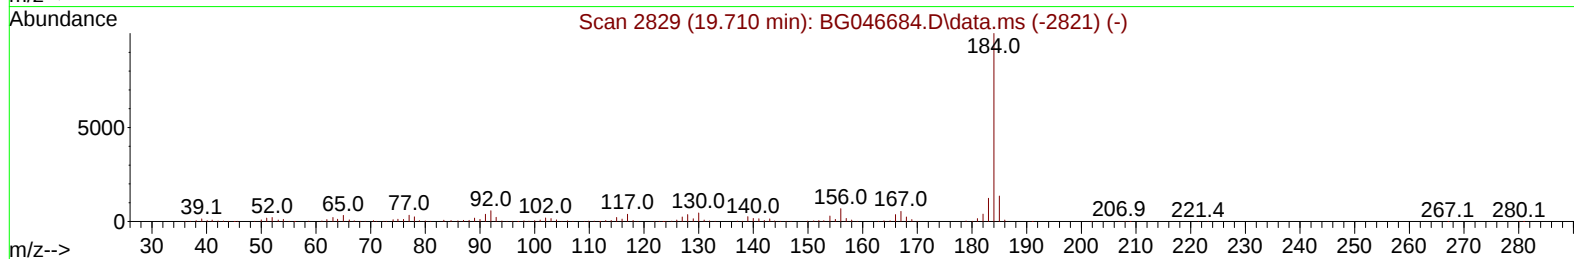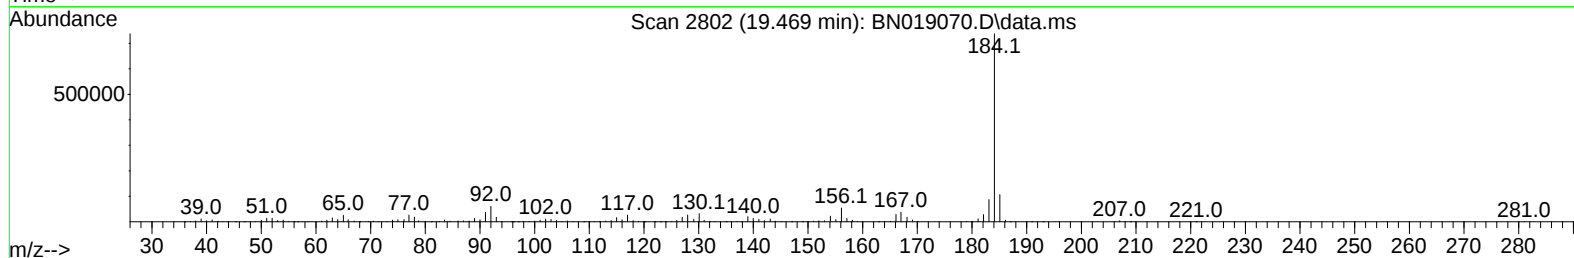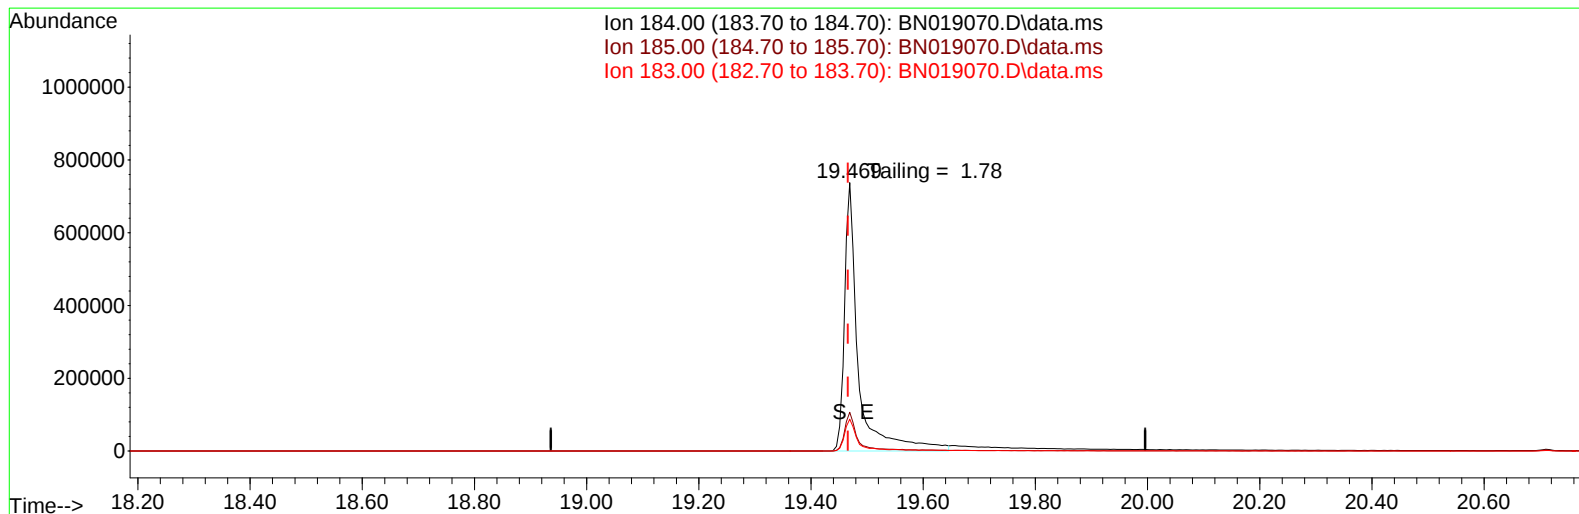

TIC: BN019070.D\data.ms

(77) Benzidine**19.469min (+ 0.003) 0.00 ng****response 1349801**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	11.89
0.00	0.00	0.00