
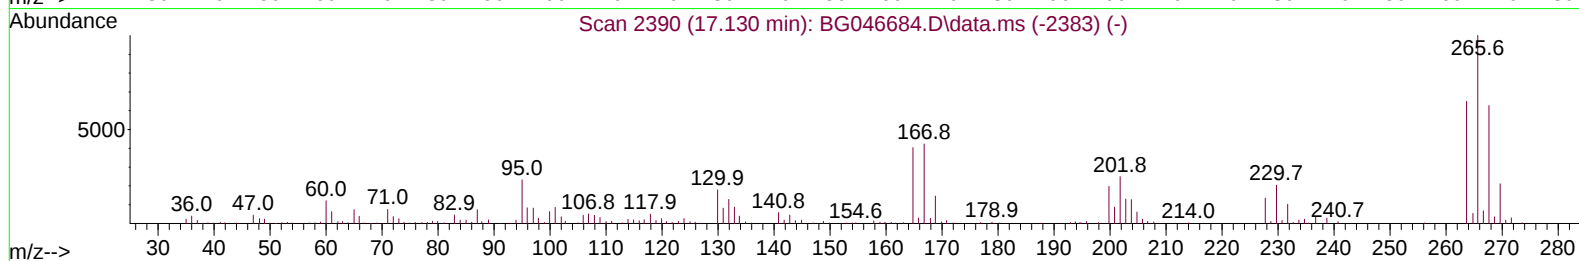
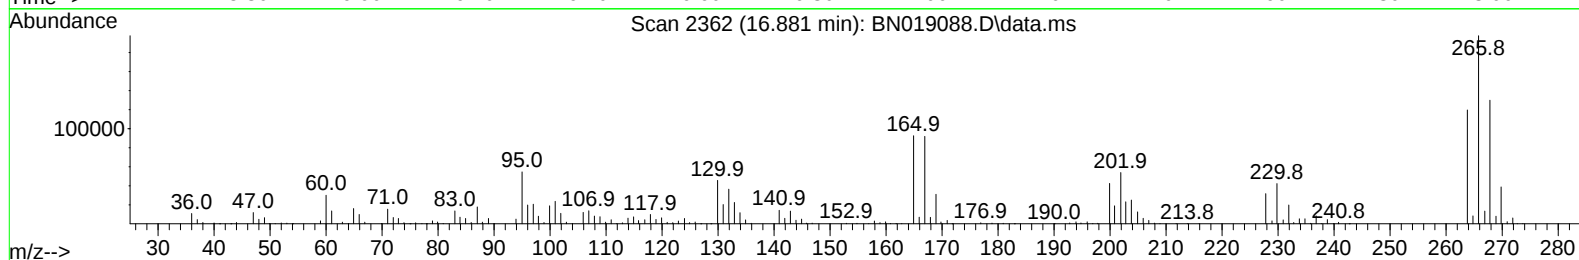


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019088.D
Acq On : 23 Mar 2022 12:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 16:56:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:36 2022
Response via : Initial Calibration

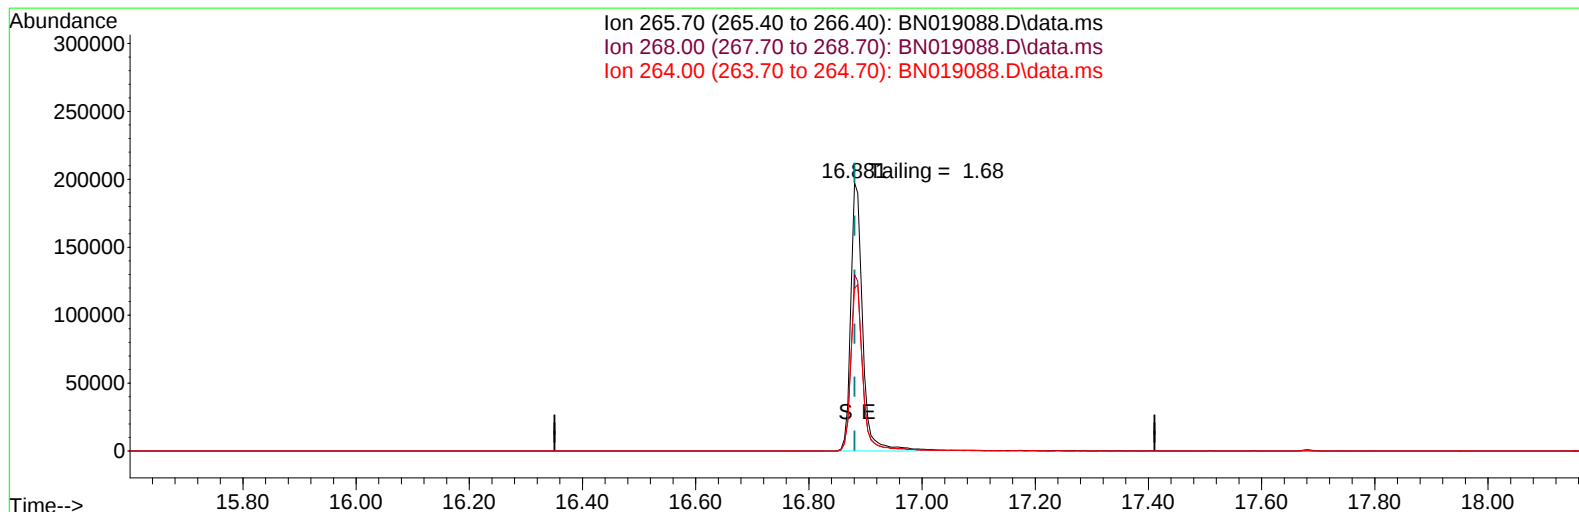

TIC: BN019088.D\data.ms




(70) Pentachlorophenol (C)

16.881min (0.000) 16148.70 ng

response 289707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.69
264.00	61.60	60.58
0.00	0.00	0.00

Quant Time: Mar 23 16:56:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:36 2022
Response via : Initial Calibration

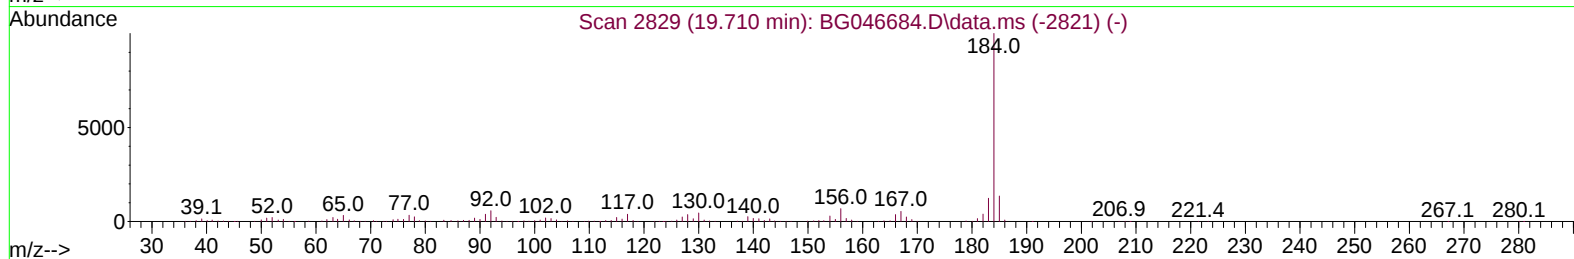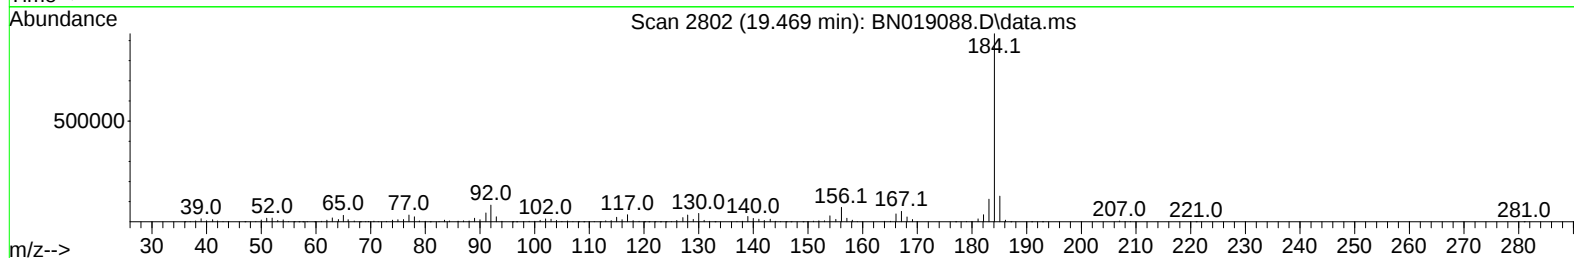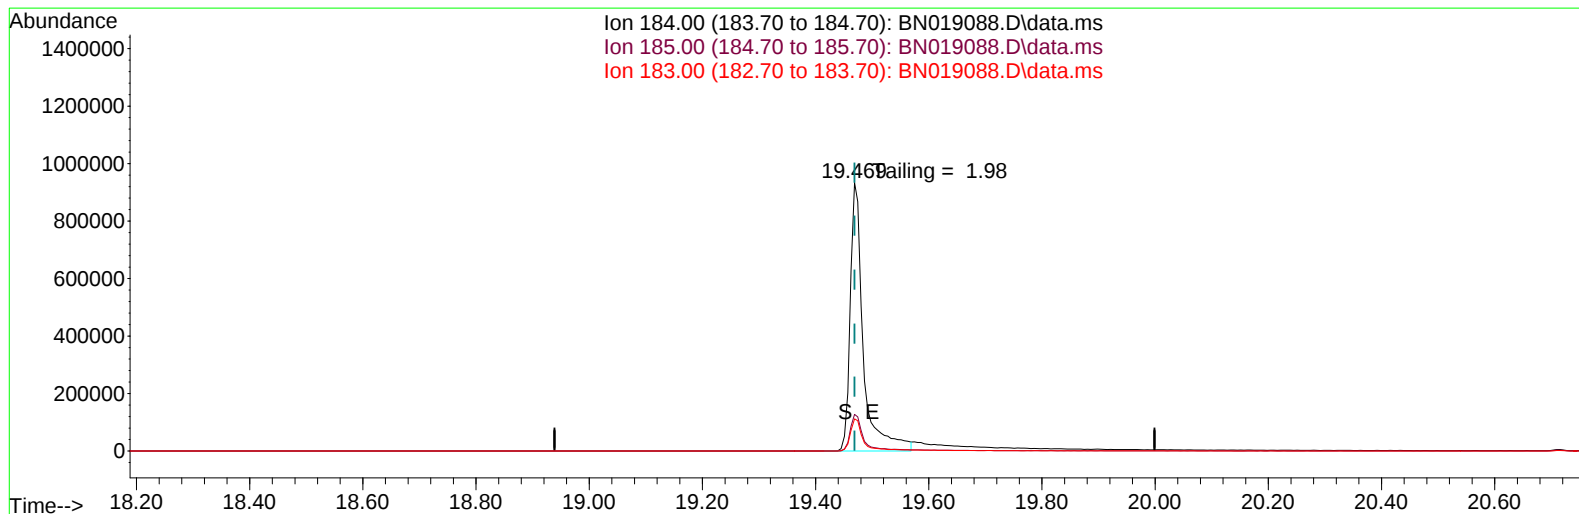

TIC: BN019088.D\data.ms

(77) Benzidine

19.469min (0.000) 0.00 ng

response **1679282**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.67
183.00	13.20	12.03
0.00	0.00	0.00