

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019118.D
 Acq On : 24 Mar 2022 08:43
 Operator : CG/JU
 Sample : N2074-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE122D2-20220321

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 03/24/2022
 Supervised By : Jagrut Upadhyay 03/24/2022

Quant Time: Mar 24 09:13:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 13:18:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.854	152	3821	0.400	ng	0.00
7) Naphthalene-d8	10.658	136	9695	0.400	ng	# 0.00
13) Acenaphthene-d10	14.484	164	5906	0.400	ng	-0.01
19) Phenanthrene-d10	17.236	188	11556	0.400	ng	0.00
29) Chrysene-d12	21.422	240	8758	0.400	ng	# 0.00
35) Perylene-d12	23.790	264	7003	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.406	112	900	0.105	ng	0.00
5) Phenol-d6	7.024	99	385	0.043	ng	0.01
8) Nitrobenzene-d5	9.025	82	1511m	0.216	ng	0.01
11) 2-Methylnaphthalene-d10	12.250	152	4451	0.277	ng	0.00
14) 2,4,6-Tribromophenol	15.984	330	548	0.192	ng	0.00
15) 2-Fluorobiphenyl	13.116	172	6333	0.267	ng	-0.01
27) Fluoranthene-d10	19.261	212	15603	0.455	ng	0.00
31) Terphenyl-d14	19.860	244	8885	0.413	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.247	88	19611m	4.153	ng	Qvalue
34) Bis(2-ethylhexyl)phtha...	21.324	149	1738	0.097	ng	# 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019118.D
Acq On : 24 Mar 2022 08:43
Operator : CG/JU
Sample : N2074-17
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321

Quant Time: Mar 24 09:13:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 13:18:23 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 03/24/2022
Supervised By : Jagrut Upadhyay 03/24/2022

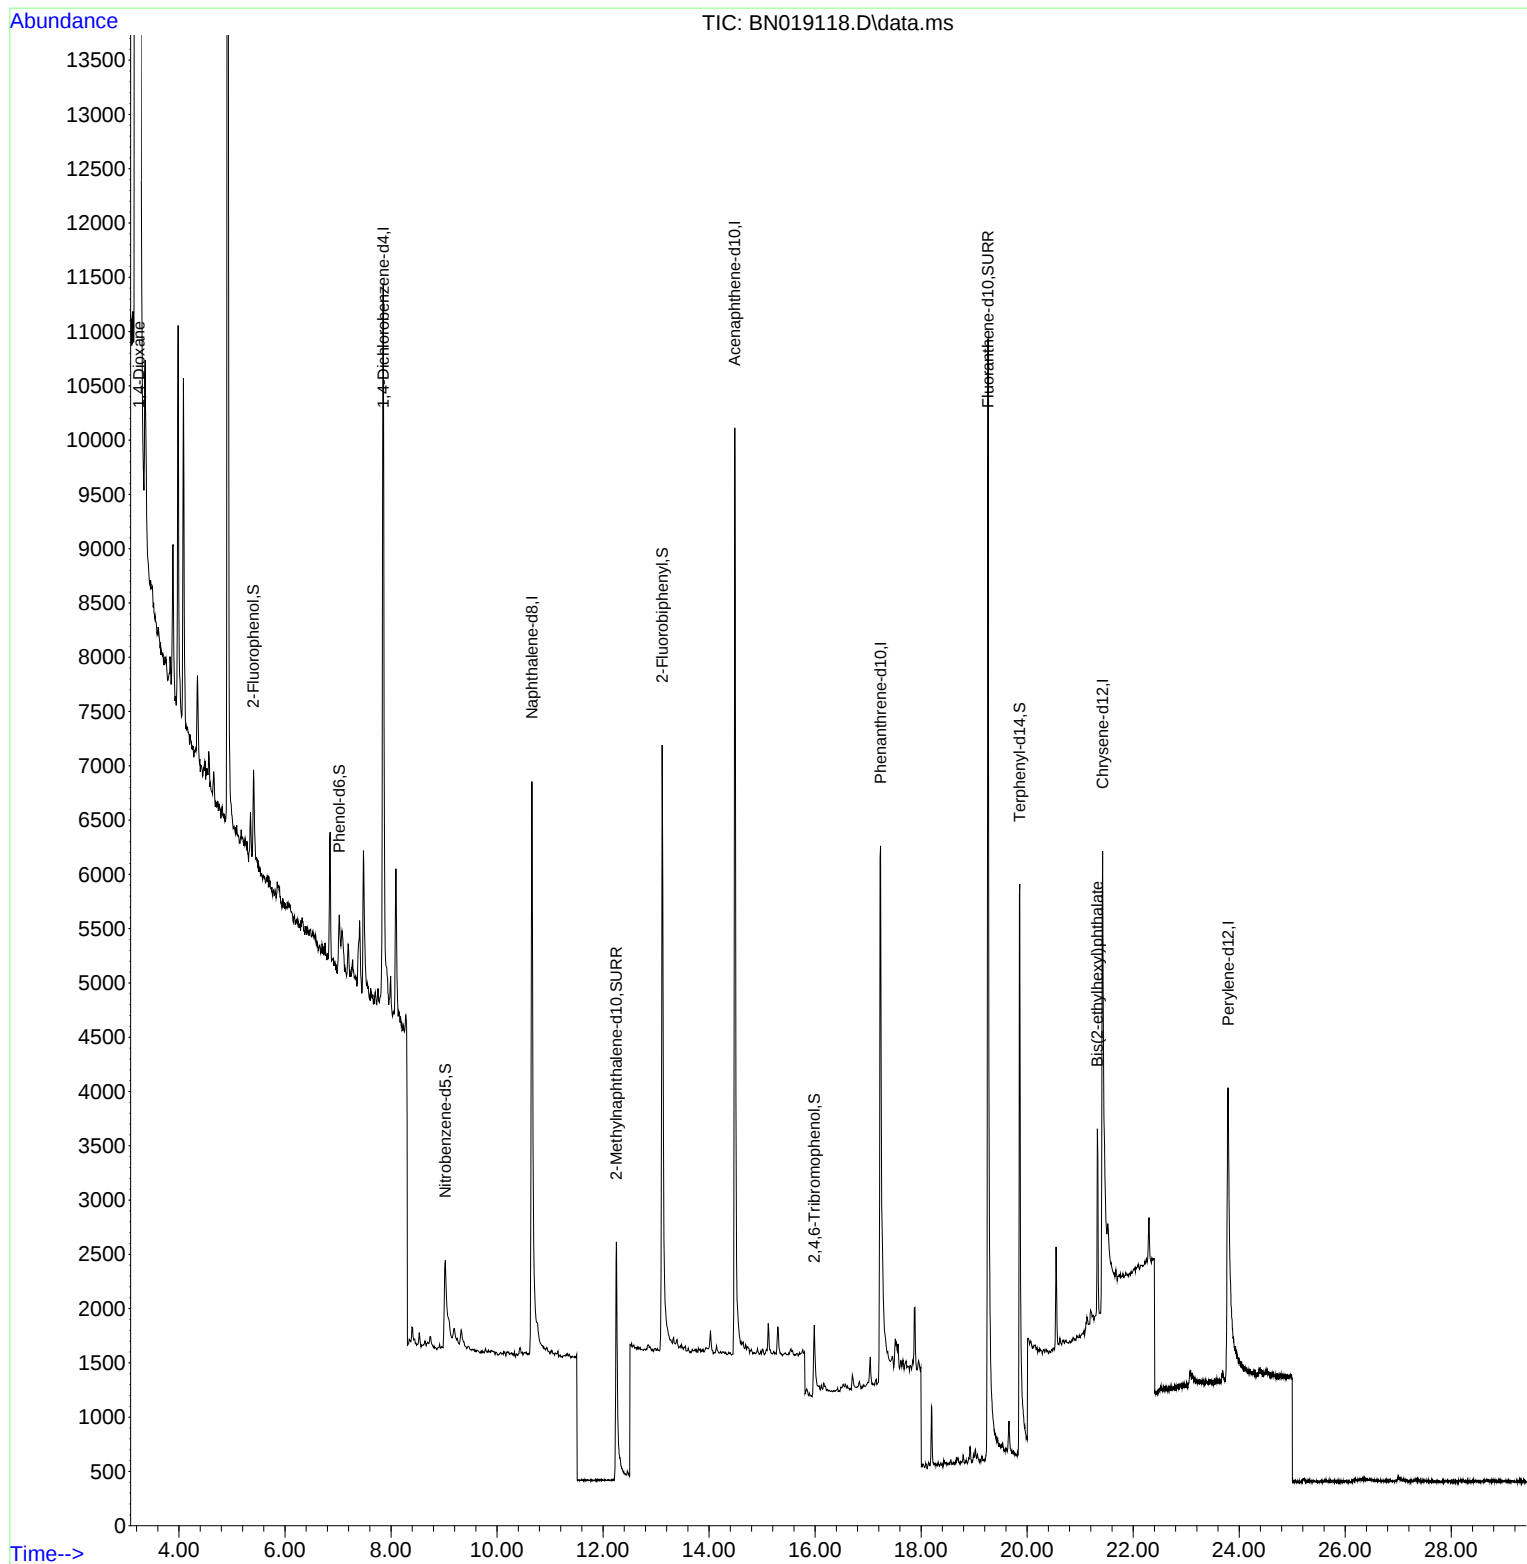

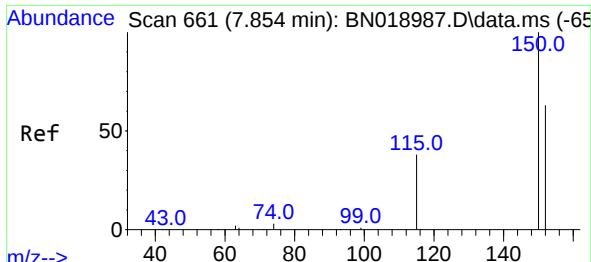

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.854 min Scan# 661
Delta R.T. 0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321

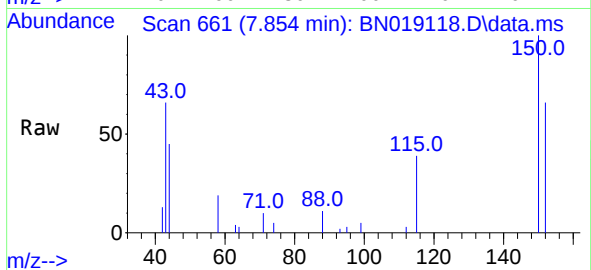


Tgt Ion: 152 Resp: 382
Ion Ratio Lower Upper
152 100
150 150.8 123.9 185.9
115 59.3 48.2 72.4

Manual Integrations
APPROVED



Reviewed By : Christian Giraldo 03/24/2022
Supervised By : Jagrut Upadhyay 03/24/2022

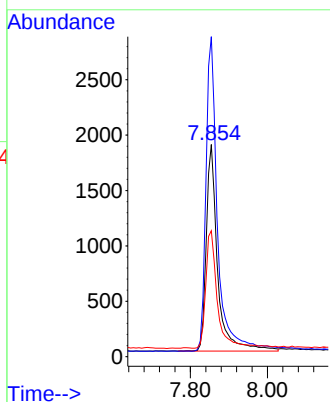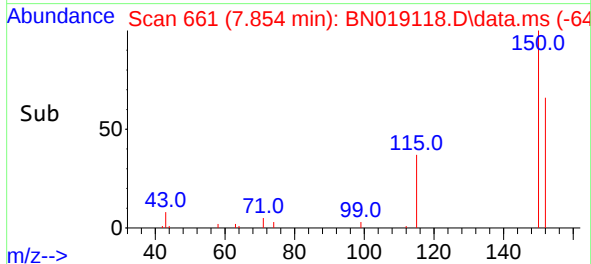


#2
1,4-Dioxane
Concen: 4.153 ng m
RT: 3.247 min Scan# 23
Delta R.T. -0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43

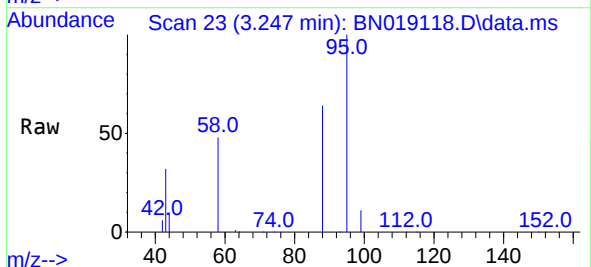


Tgt Ion: 88 Resp: 19611
Ion Ratio Lower Upper
88 100
43 72.6 24.6 37.0#
58 77.1 65.4 98.2

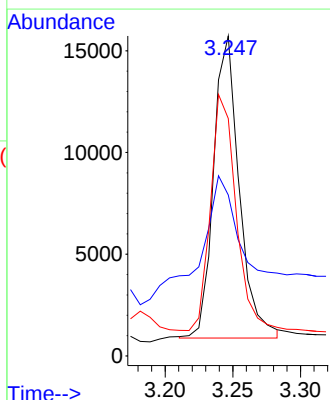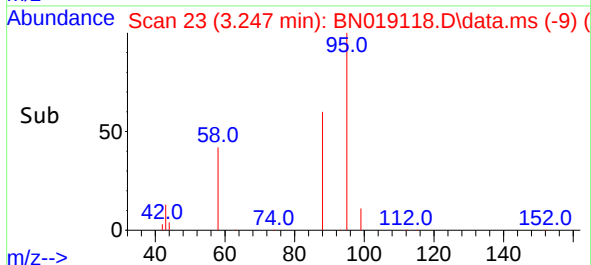



#4
2-Fluorophenol
Concen: 0.105 ng
RT: 5.406 min Scan# 311
Delta R.T. -0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321

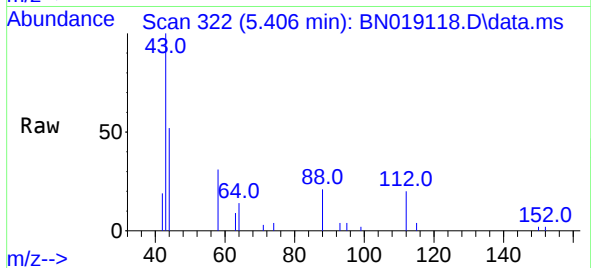


Tgt Ion: 112 Resp: 900
Ion Ratio Lower Upper
112 100
64 63.2 47.8 71.8
63 33.7 25.7 38.5

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/24/2022
Supervised By :Jagrut Upadhyay 03/24/2022

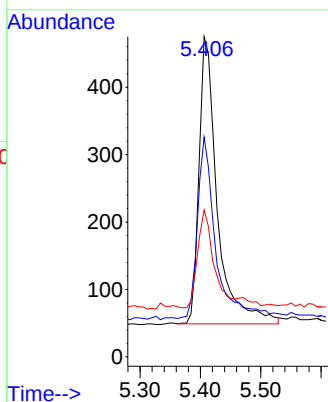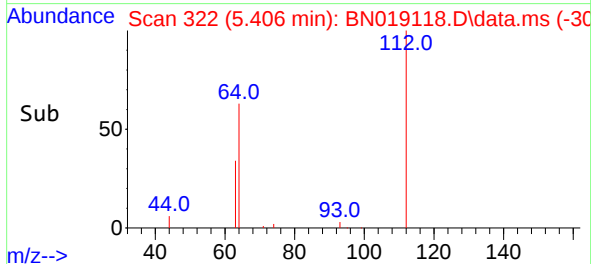


#5
Phenol-d6
Concen: 0.043 ng
RT: 7.024 min Scan# 546
Delta R.T. 0.014 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43

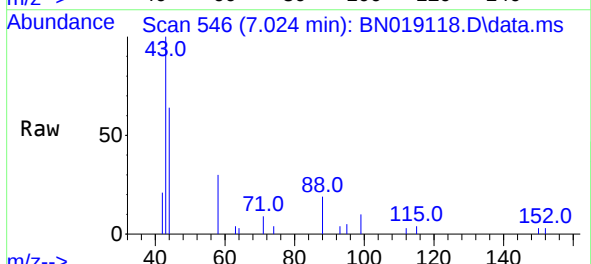


Tgt Ion: 99 Resp: 385
Ion Ratio Lower Upper
99 100
42 40.0 16.2 24.4#
71 64.9 27.7 41.5#

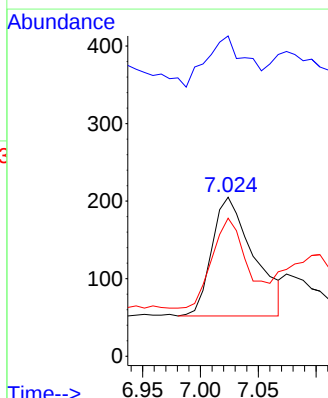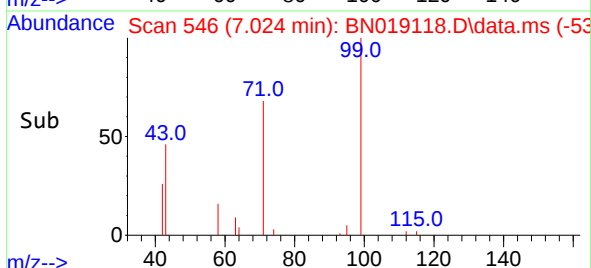



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.658 min Scan# 944
Delta R.T. 0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321



Tgt Ion:	136	Resp:	969
Ion	Ratio	Lower	Upper
136	100		
137	12.1	9.0	13.4
54	10.8	5.8	8.6
68	8.4	4.6	7.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/24/2022
Supervised By :Jagrut Upadhyay 03/24/2022

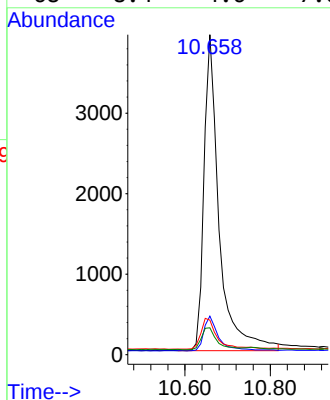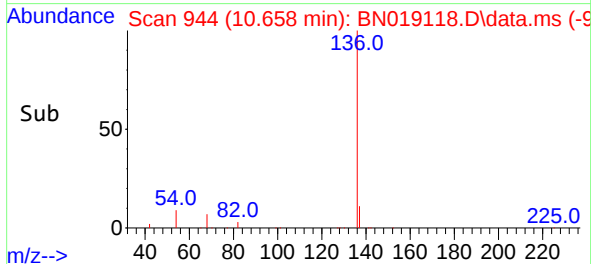

#8
Nitrobenzene-d5
Concen: 0.216 ng m
RT: 9.025 min Scan# 791
Delta R.T. 0.011 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43


Tgt Ion:	82	Resp:	1511
Ion	Ratio	Lower	Upper
82	100		
128	45.4	33.0	49.6
54	60.3	42.5	63.7

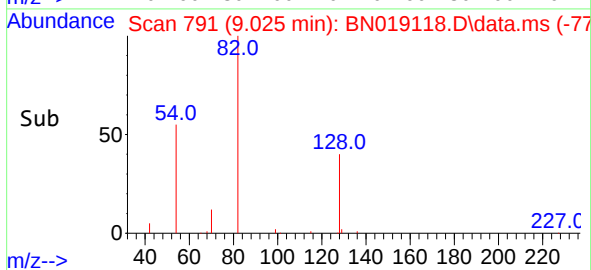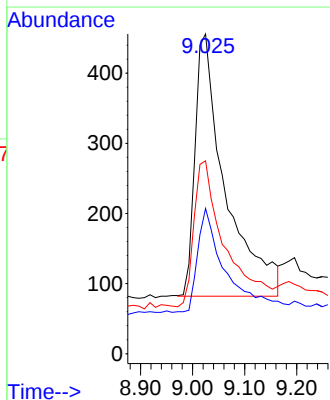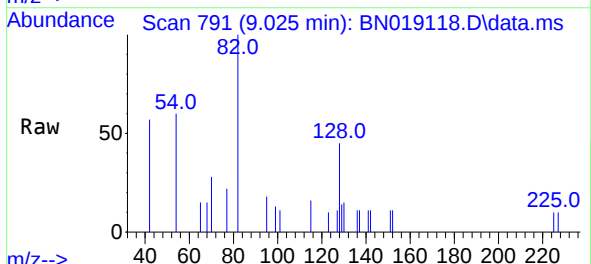



#11
2-Methylnaphthalene-d10
Concen: 0.277 ng
RT: 12.250 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43



Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321



Tgt Ion:152 Resp: 445
Ion Ratio Lower Upper
152 100
151 19.7 16.5 24.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/24/2022
Supervised By :Jagrut Upadhyay 03/24/2022

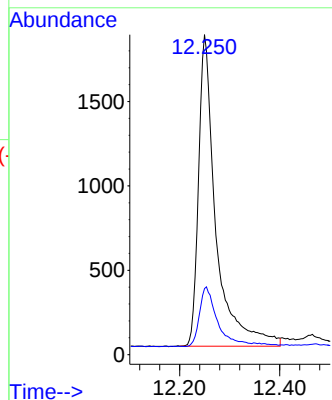

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.484 min Scan# 1472
Delta R.T. -0.011 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43


Tgt Ion:164 Resp: 5906
Ion Ratio Lower Upper
164 100
162 104.9 85.2 127.8
160 50.1 41.5 62.3

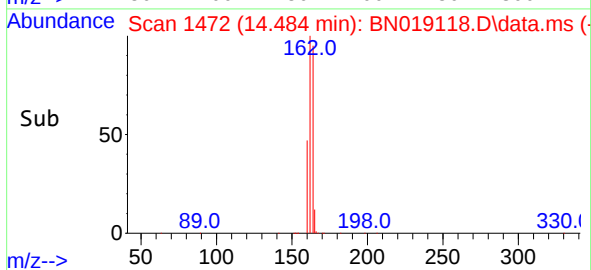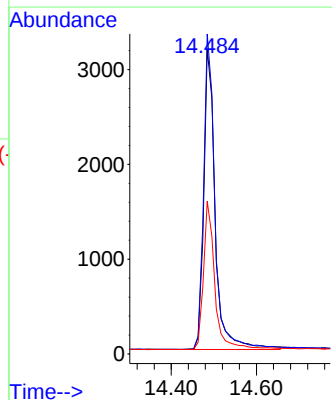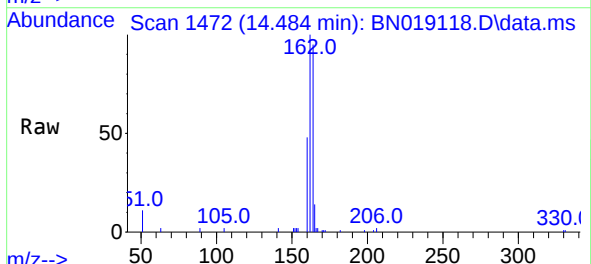



#14
2,4,6-Tribromophenol
Concen: 0.192 ng
RT: 15.984 min Scan# 1613
Delta R.T. 0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321

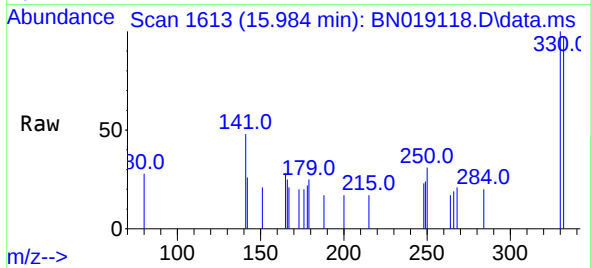


Tgt Ion: 330 Resp: 548
Ion Ratio Lower Upper
330 100
332 98.0 76.8 115.2
141 41.1 32.2 48.2

Manual Integrations
APPROVED



Reviewed By : Christian Giraldo 03/24/2022
Supervised By : Jagrut Upadhyay 03/24/2022

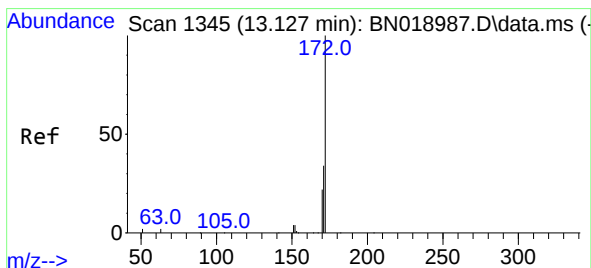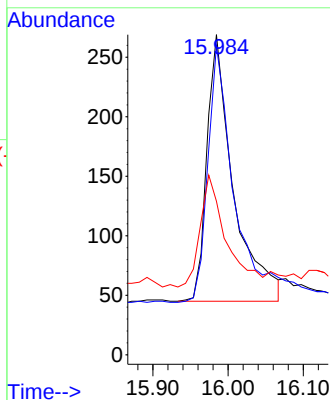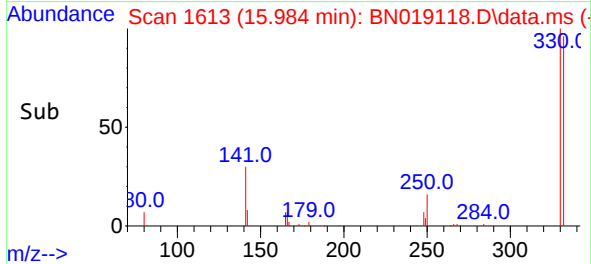


#15
2-Fluorobiphenyl
Concen: 0.267 ng
RT: 13.116 min Scan# 1344
Delta R.T. -0.011 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43

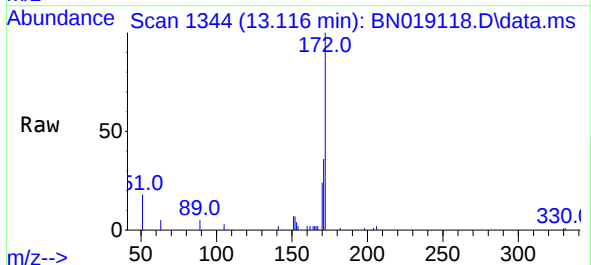


Tgt Ion: 172 Resp: 6333
Ion Ratio Lower Upper
172 100
171 36.1 28.2 42.2
170 24.4 18.7 28.1

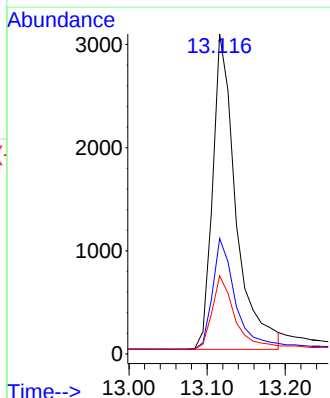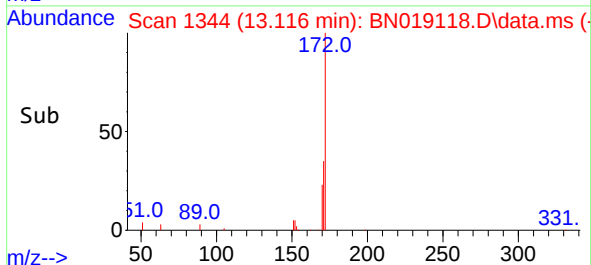

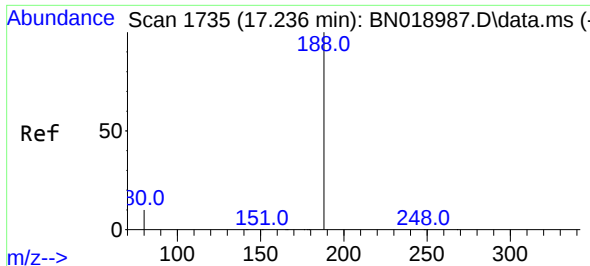

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.236 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321

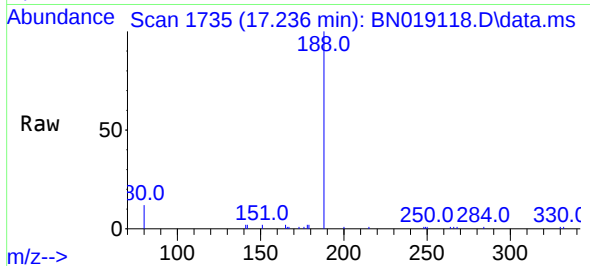

Tgt Ion:188 Resp: 11550
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.9 11.8 17.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/24/2022
Supervised By :Jagrut Upadhyay 03/24/2022

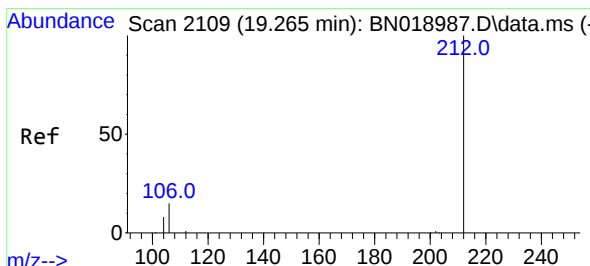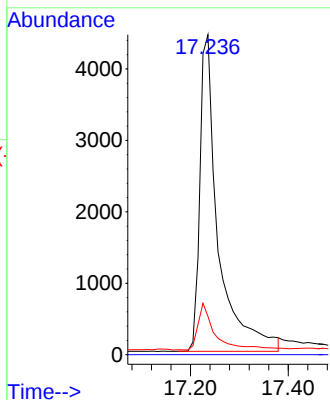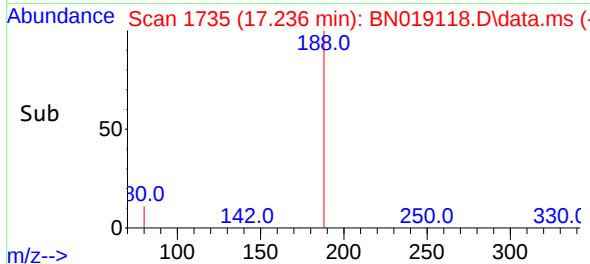

#27
Fluoranthene-d10
Concen: 0.455 ng
RT: 19.261 min Scan# 2108
Delta R.T. -0.004 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43


Tgt Ion:212 Resp: 15603
Ion Ratio Lower Upper
212 100
106 16.0 12.7 19.1
104 9.3 7.1 10.7

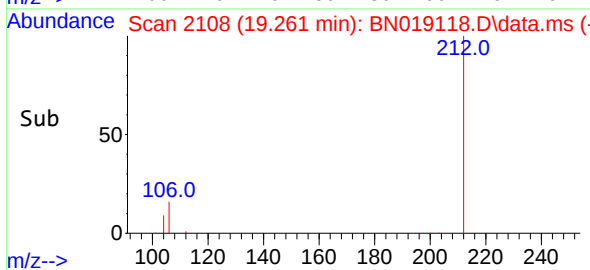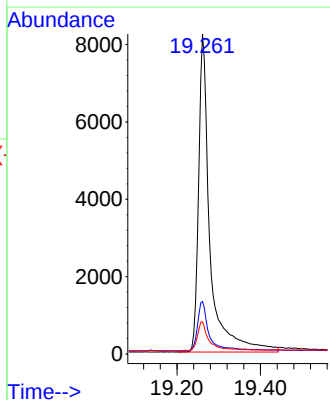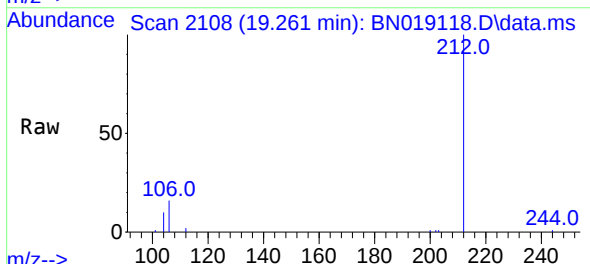



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.422 min Scan# 2443
Delta R.T. -0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321




Tgt Ion:240 Resp: 8758
Ion Ratio Lower Upper
240 100
120 17.9 8.5 12.7
236 29.1 22.4 33.6

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/24/2022
Supervised By :Jagrut Upadhyay 03/24/2022

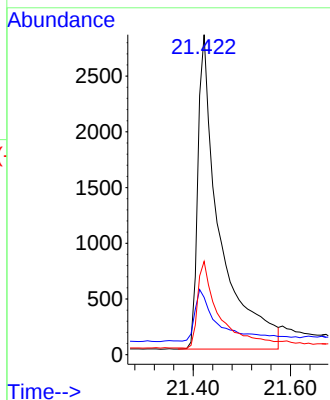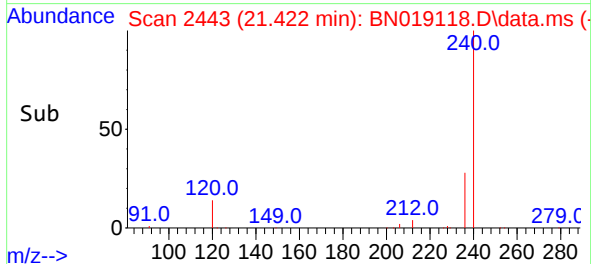


#31
Terphenyl-d14
Concen: 0.413 ng
RT: 19.860 min Scan# 2250
Delta R.T. -0.004 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43

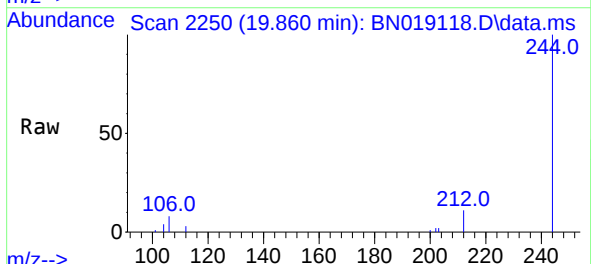


Tgt Ion:244 Resp: 8885
Ion Ratio Lower Upper
244 100
212 11.2 8.2 12.4
122 0.0 0.0 0.0

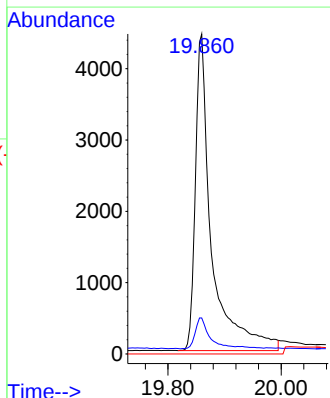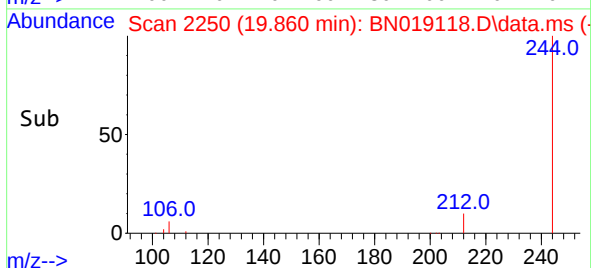

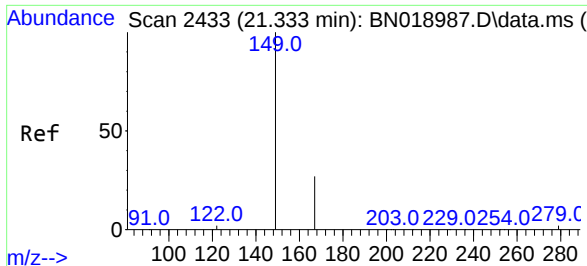

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.097 ng
RT: 21.324 min Scan# 2432
Delta R.T. -0.009 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43




Instrument :
BNA_N
ClientSampleId :
RE122D2-20220321

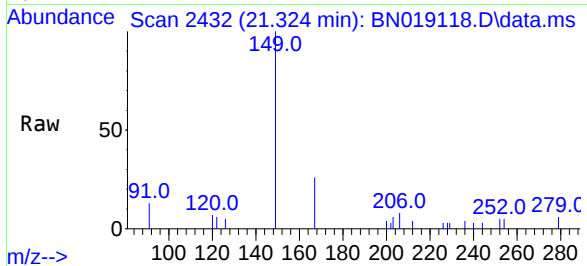

Tgt Ion:149 Resp: 1738
Ion Ratio Lower Upper
149 100
167 27.2 21.8 32.8
279 3.3 2.0 3.0

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 03/24/2022
Supervised By :Jagrut Upadhyay 03/24/2022

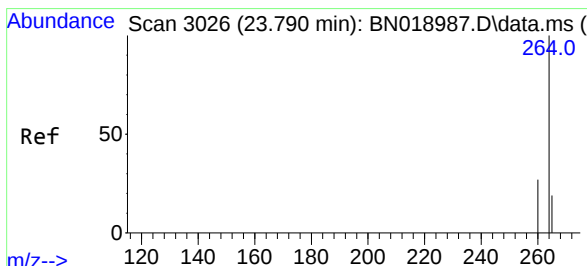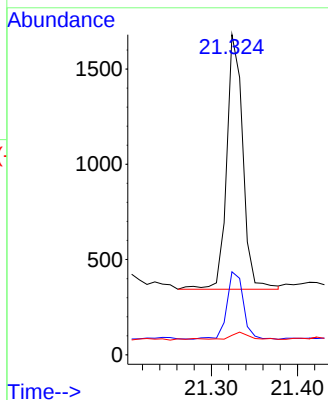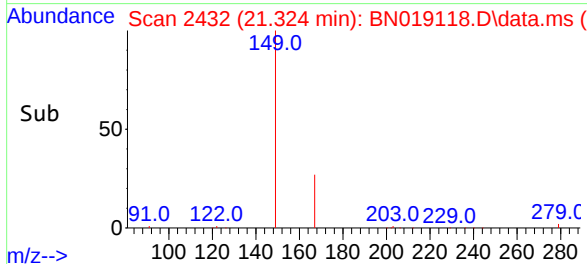

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.790 min Scan# 3026
Delta R.T. 0.000 min
Lab File: BN019118.D
Acq: 24 Mar 2022 08:43

Tgt Ion:264 Resp: 7003
Ion Ratio Lower Upper
264 100
260 29.9 22.4 33.6
265 52.5 25.3 37.9

