
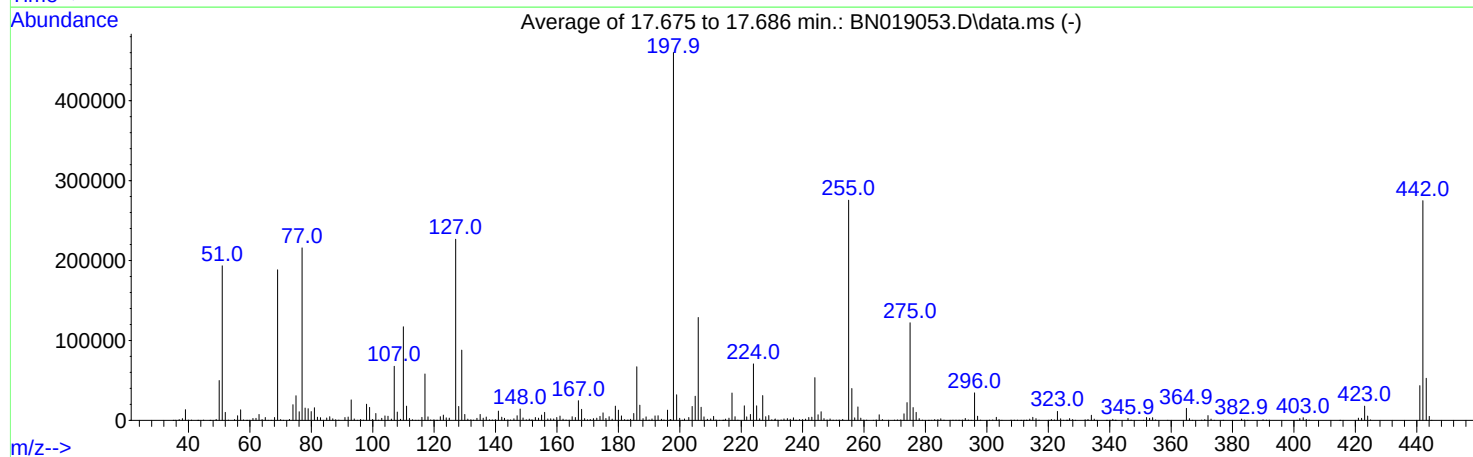


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019053.D
 Acq On : 22 Mar 2022 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

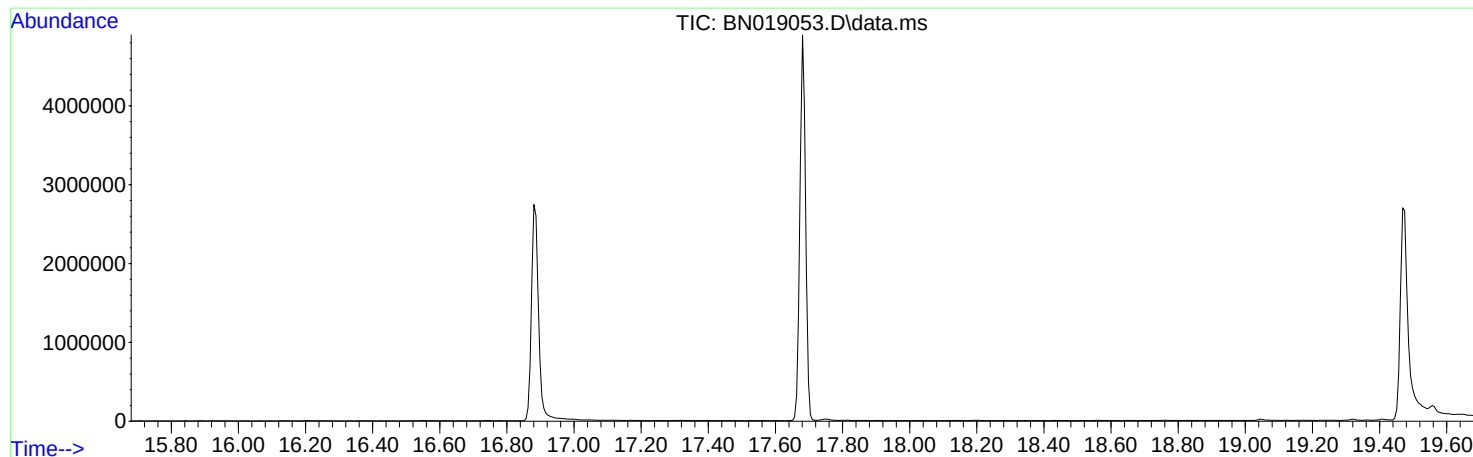




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	193344	PASS
68	69	0.00	2	1.9	3609	PASS
69	198	0.00	100	40.9	188416	PASS
70	69	0.00	2	0.6	1099	PASS
127	198	10	80	49.3	226731	PASS
197	198	0.00	2	0.3	1187	PASS
198	198	100	100	100.0	460288	PASS
199	198	5	9	7.0	32099	PASS
275	198	10	60	26.5	122096	PASS
365	198	1	100	3.3	14985	PASS
441	198	0.01	100	9.4	43365	PASS
442	442	50	100	100.0	274837	PASS
443	442	15	24	19.2	52691	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019053.D
 Acq On : 22 Mar 2022 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 06:01:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 14 15:11:57 2022
 Response via : Initial Calibration

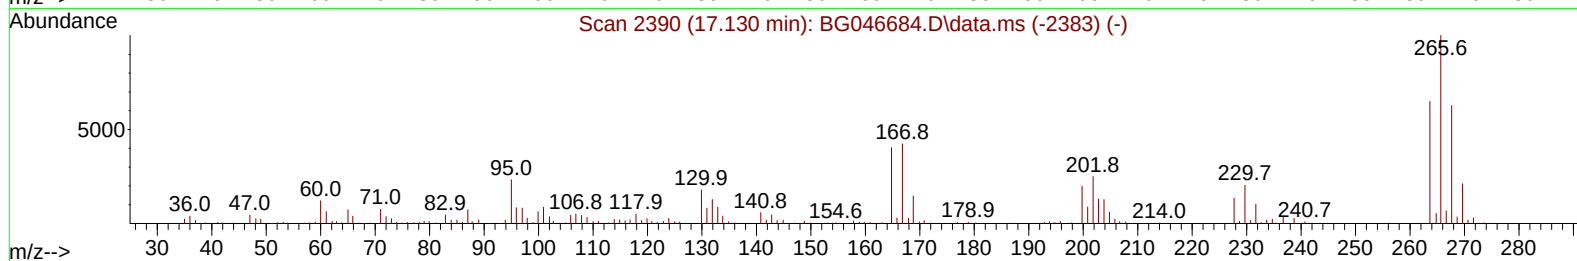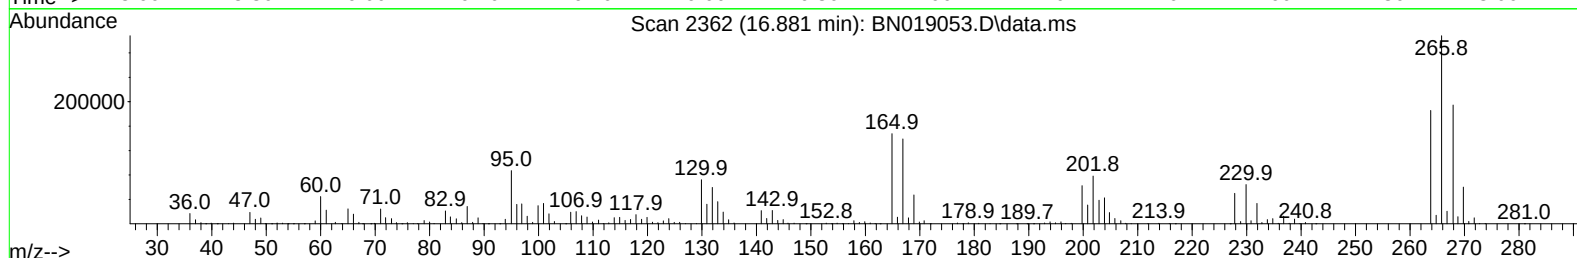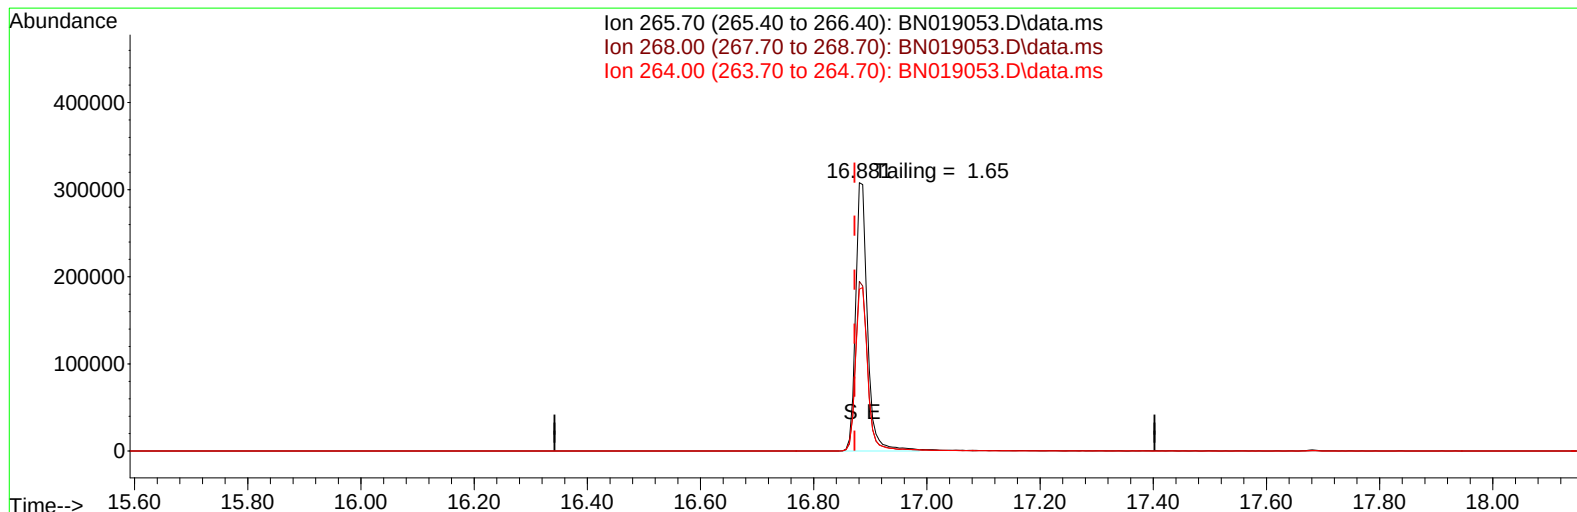

TIC: BN019053.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.009) 18260.03 ng




response 452685

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.21
264.00	61.60	60.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019053.D
Acq On : 22 Mar 2022 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 06:01:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

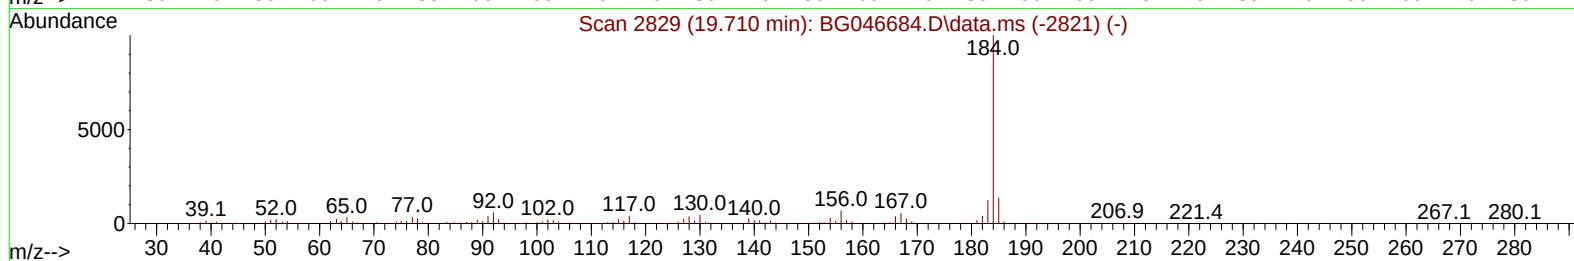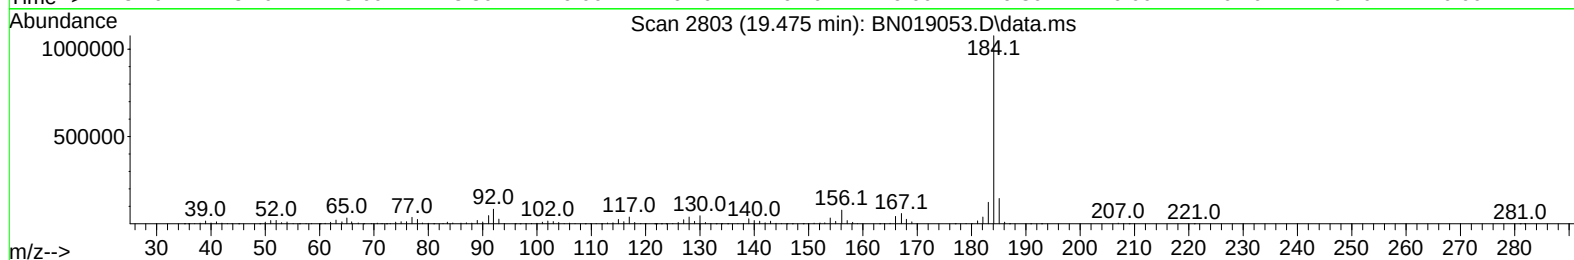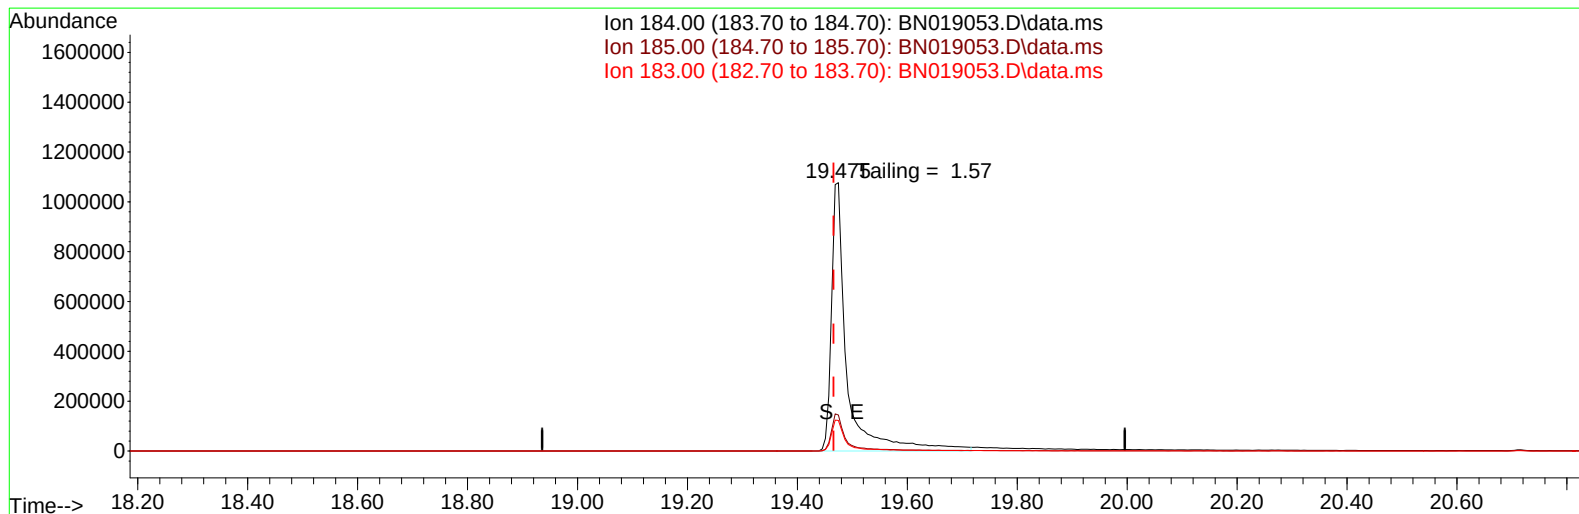

TIC: BN019053.D\data.ms

(77) Benzidine

19.475min (+ 0.009) 0.00 ng

response 2195158

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.45
183.00	13.20	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_N	<u>BN019053.D</u>
Compound Name	Response	Retention Time
DDT	890373	20.716
DDD	290906	20.275
DDE	1117	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
292023	1182396	24.70

Instrument :
BNA_N
ClientSampleId :
DFTPP