
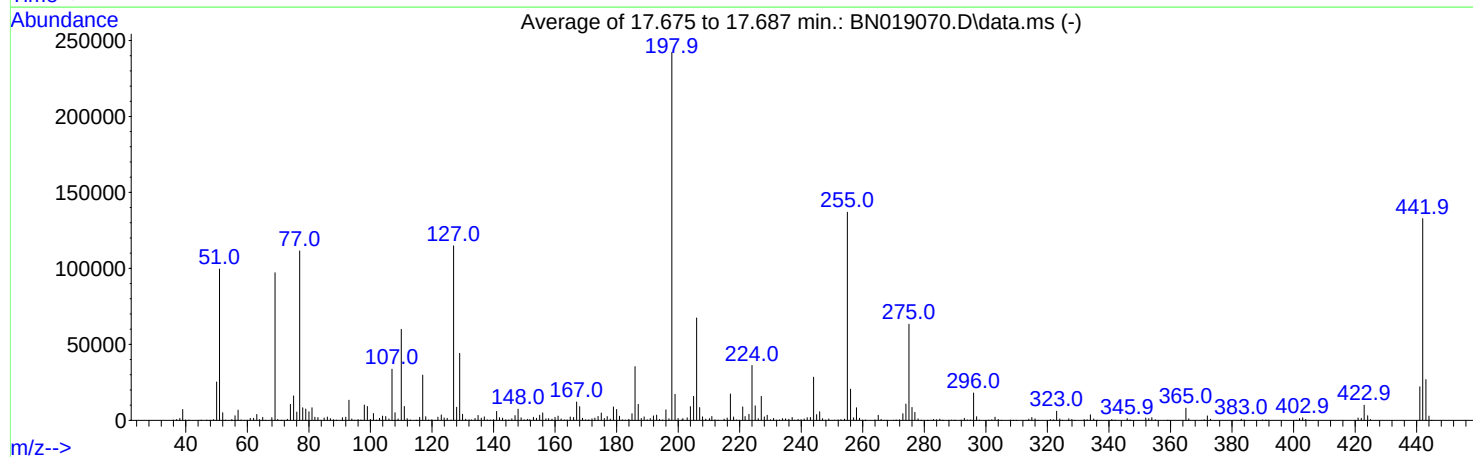


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019070.D
 Acq On : 23 Mar 2022 00:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

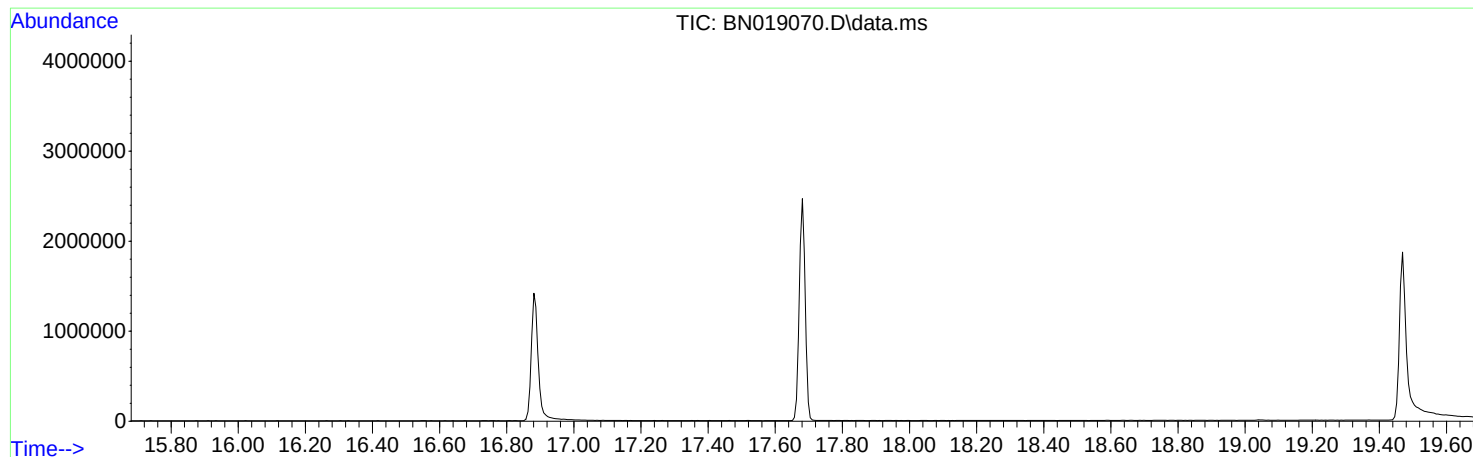




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	99614	PASS
68	69	0.00	2	1.8	1745	PASS
69	198	0.00	100	40.1	97144	PASS
70	69	0.00	2	0.6	590	PASS
127	198	10	80	47.5	114885	PASS
197	198	0.00	2	0.4	1032	PASS
198	198	100	100	100.0	242069	PASS
199	198	5	9	7.1	17160	PASS
275	198	10	60	26.2	63323	PASS
365	198	1	100	3.3	8025	PASS
441	198	0.01	100	9.1	22090	PASS
442	442	50	100	100.0	132781	PASS
443	442	15	24	20.2	26859	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019070.D
Acq On : 23 Mar 2022 00:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 06:13:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 14 15:11:57 2022
Response via : Initial Calibration

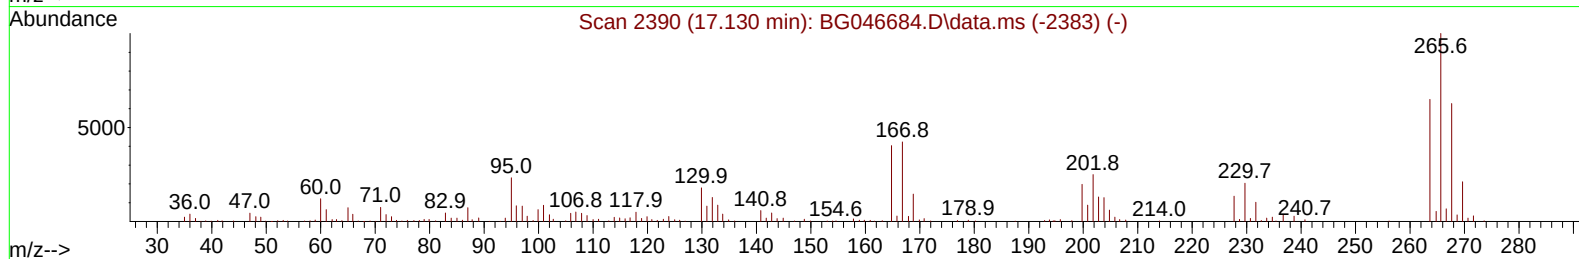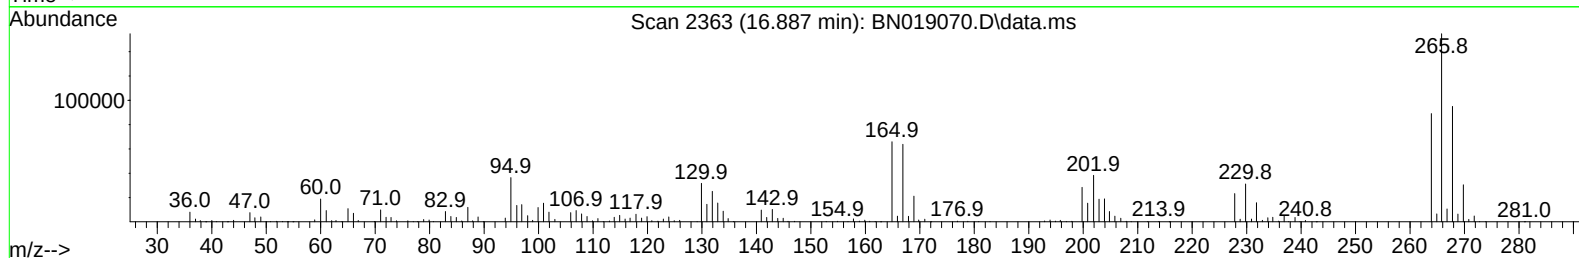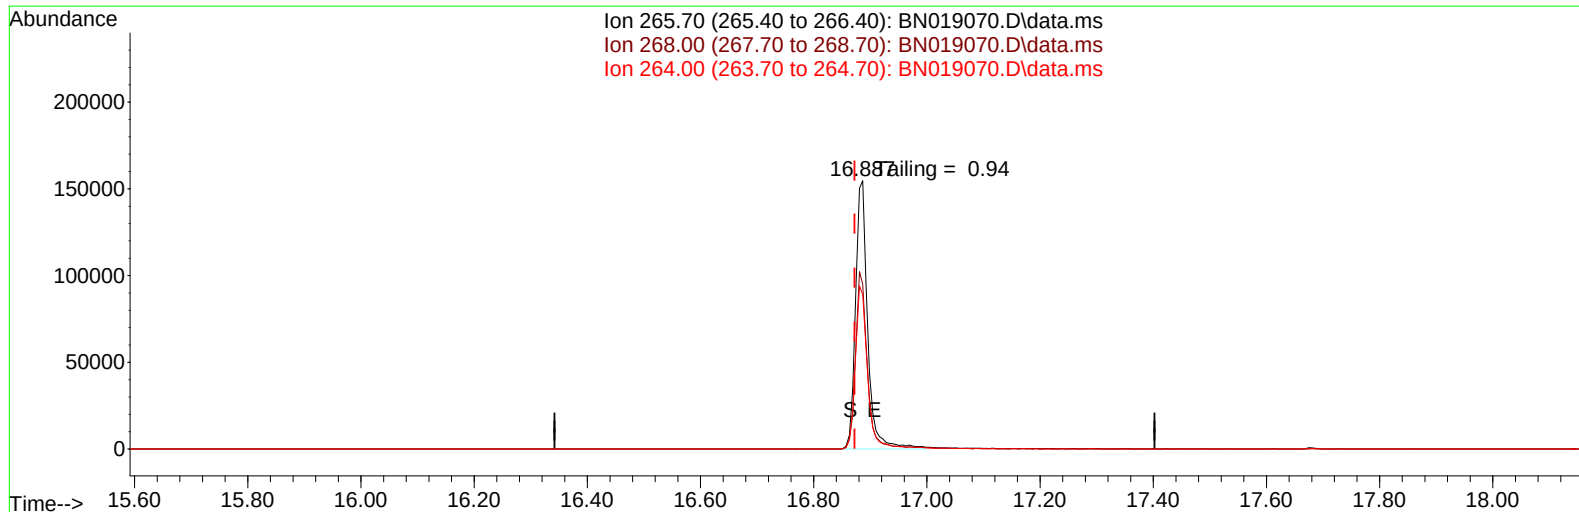

TIC: BN019070.D\data.ms

(70) Pentachlorophenol (C)

16.887min (+ 0.015) 16800.81 ng




response 234163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.42
264.00	61.60	57.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019070.D
 Acq On : 23 Mar 2022 00:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 06:13:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 14 15:11:57 2022
 Response via : Initial Calibration

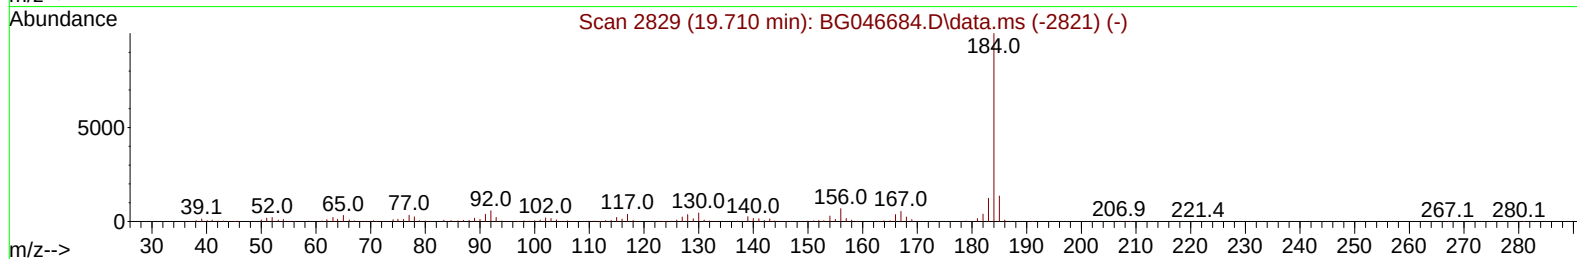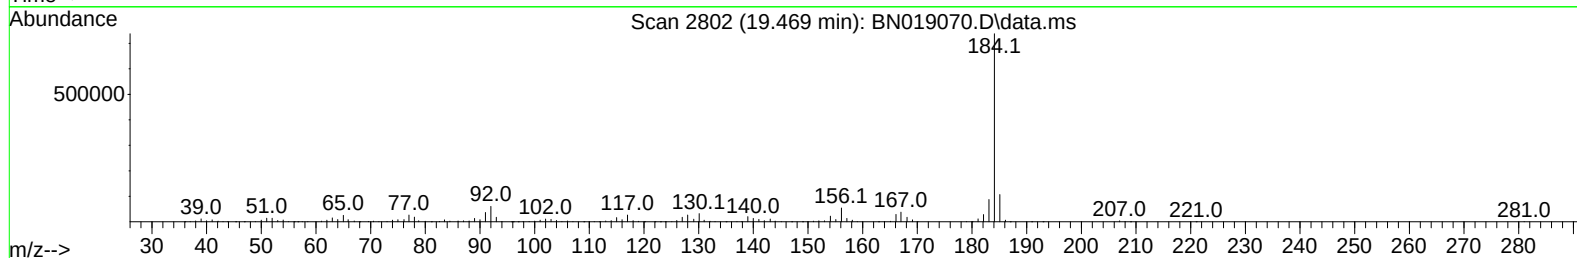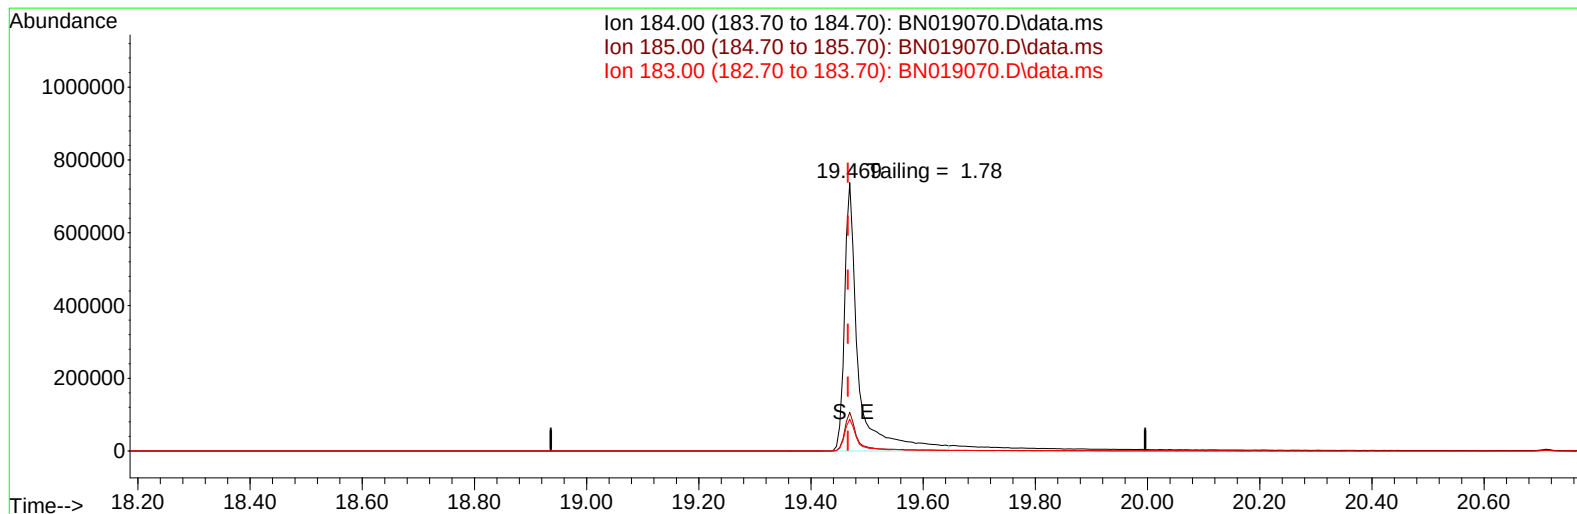

TIC: BN019070.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng

response 1349801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_N	<u>BN019070.D</u>
Compound Name	Response	Retention Time
DDT	896464	20.716
DDD	7542	20.275
DDE	318	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7860	904324	0.87

Instrument :
BNA_N
ClientSampleId :
DFTPP