
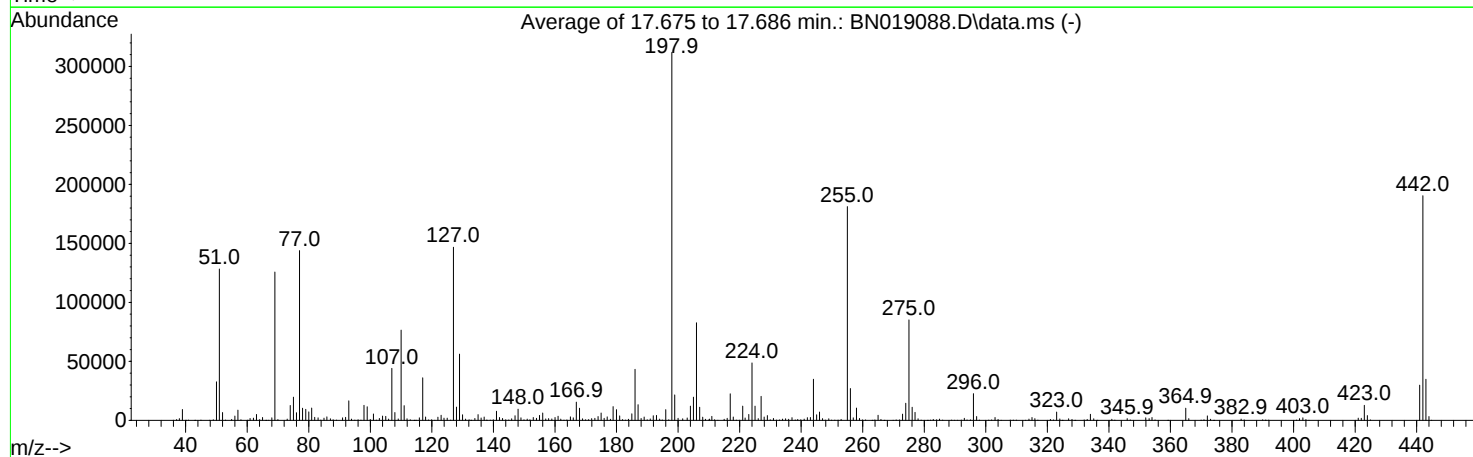


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019088.D
 Acq On : 23 Mar 2022 12:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

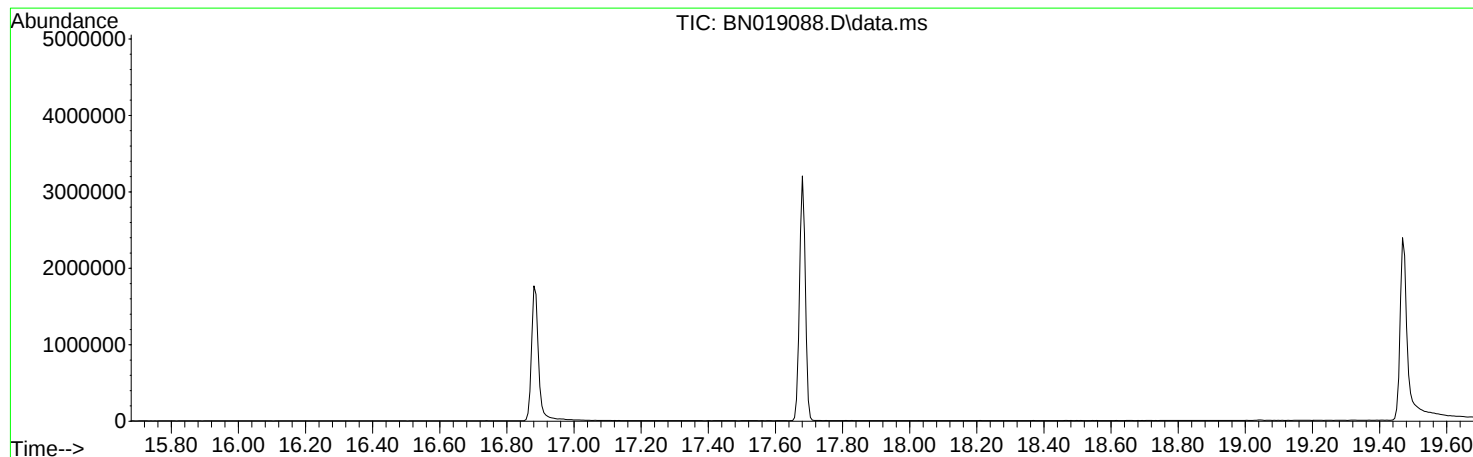




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	128243	PASS
68	69	0.00	2	1.8	2221	PASS
69	198	0.00	100	40.3	125736	PASS
70	69	0.00	2	0.6	709	PASS
127	198	10	80	47.1	146757	PASS
197	198	0.00	2	0.2	611	PASS
198	198	100	100	100.0	311808	PASS
199	198	5	9	6.9	21632	PASS
275	198	10	60	27.3	85163	PASS
365	198	1	100	3.3	10381	PASS
441	198	0.01	100	9.6	29904	PASS
442	442	50	100	100.0	190480	PASS
443	442	15	24	18.3	34885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019088.D
Acq On : 23 Mar 2022 12:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 16:56:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:36 2022
Response via : Initial Calibration

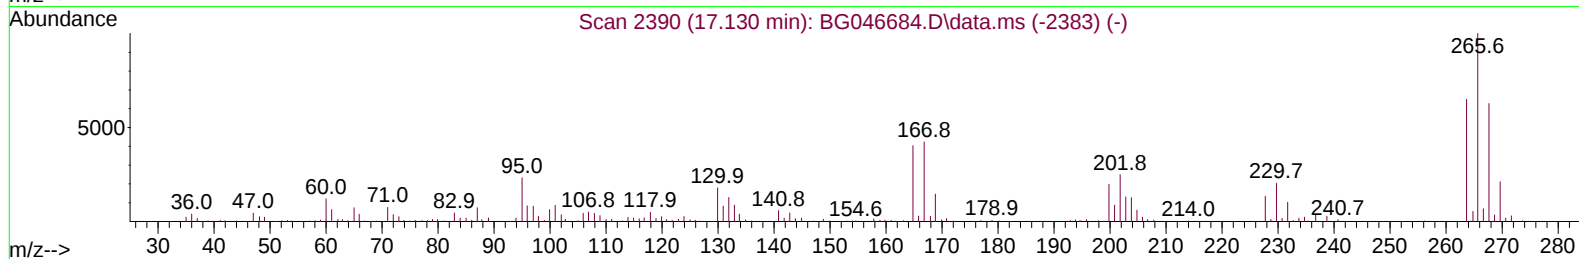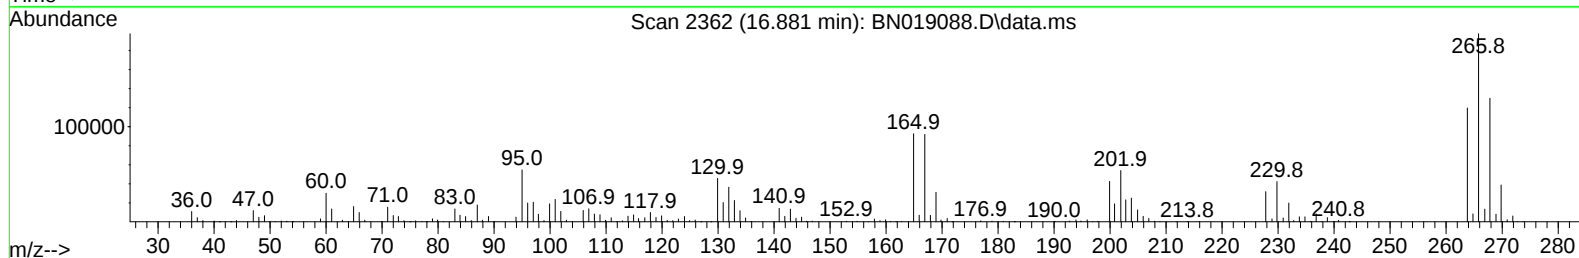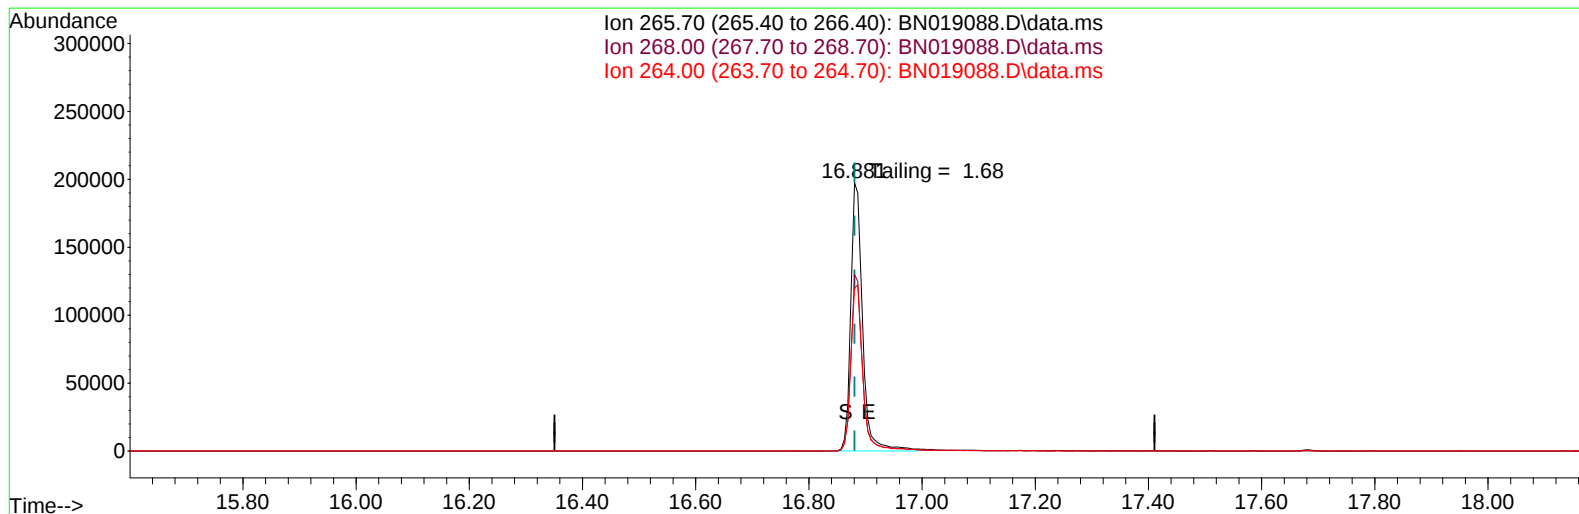

TIC: BN019088.D\data.ms

(70) Pentachlorophenol (C)

16.881min (0.000) 16148.70 ng

response 289707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.69
264.00	61.60	60.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2022	BNA_N	<u>BN019088.D</u>
Compound Name	Response	Retention Time
DDT	1100613	20.71
DDD	8058	20.27
DDE	375	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8433	1109046	0.76

Instrument :
BNA_N
ClientSampleId :
DFTPP