
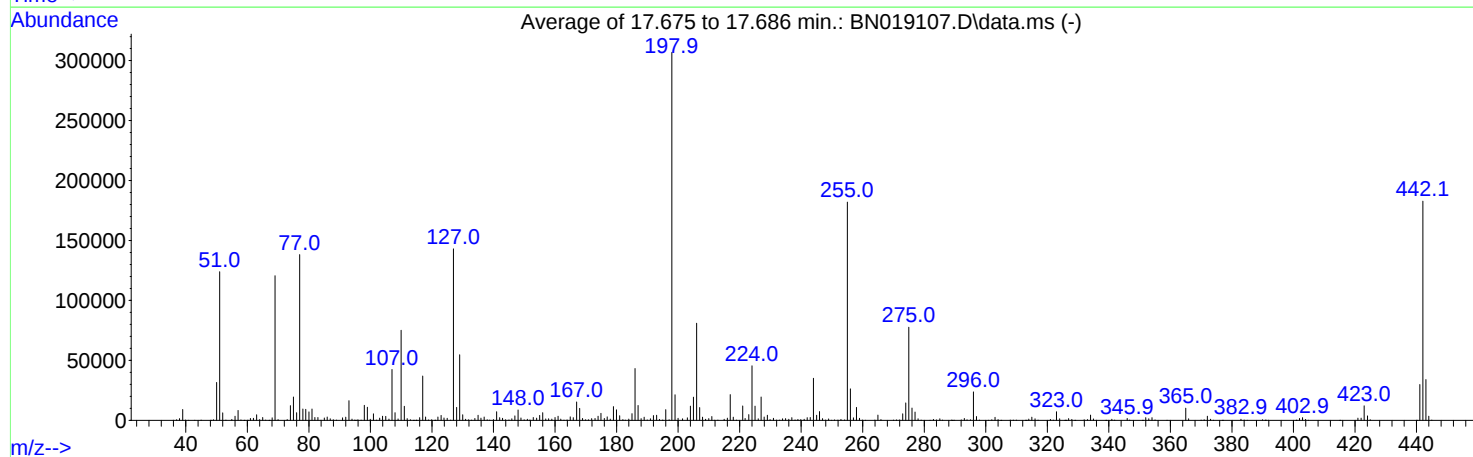


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
 Data File : BN019107.D
 Acq On : 24 Mar 2022 02:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

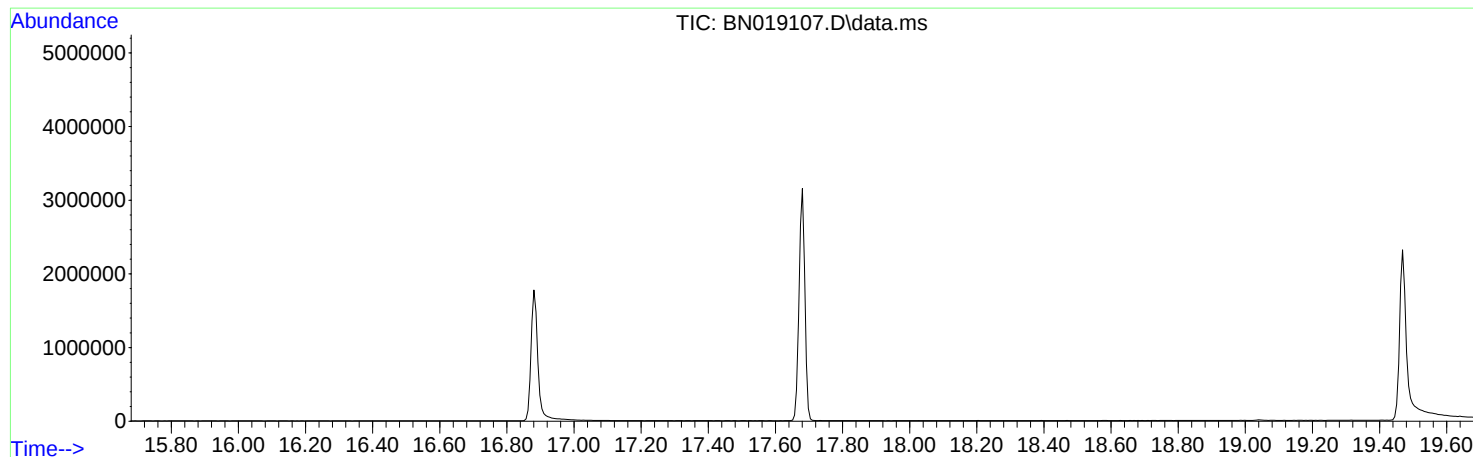




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	123932	PASS
68	69	0.00	2	1.8	2182	PASS
69	198	0.00	100	39.3	120592	PASS
70	69	0.00	2	0.6	684	PASS
127	198	10	80	46.6	143013	PASS
197	198	0.00	2	0.2	540	PASS
198	198	100	100	100.0	306731	PASS
199	198	5	9	7.0	21398	PASS
275	198	10	60	25.3	77603	PASS
365	198	1	100	3.3	10083	PASS
441	198	0.01	100	9.7	29843	PASS
442	442	50	100	100.0	182848	PASS
443	442	15	24	18.6	34040	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019107.D
Acq On : 24 Mar 2022 02:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 24 06:30:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

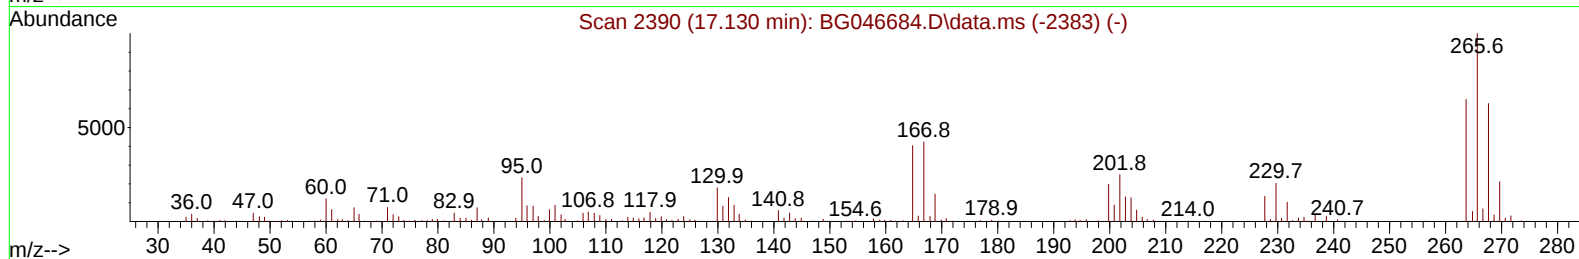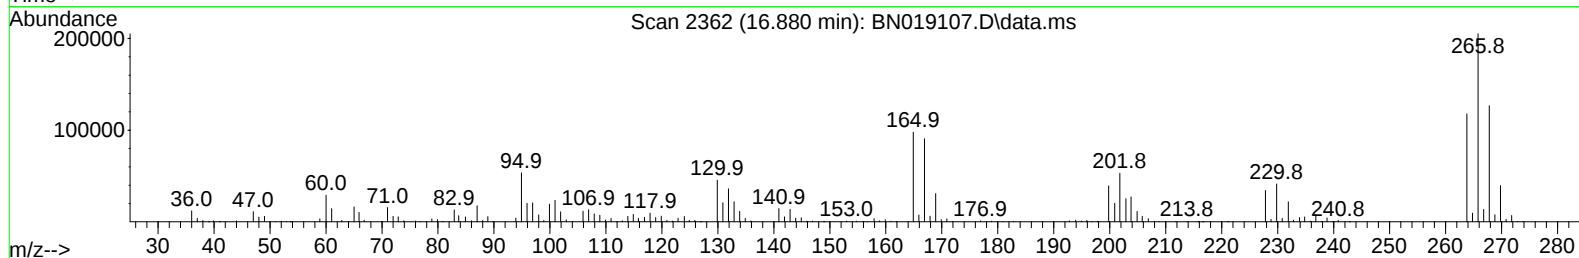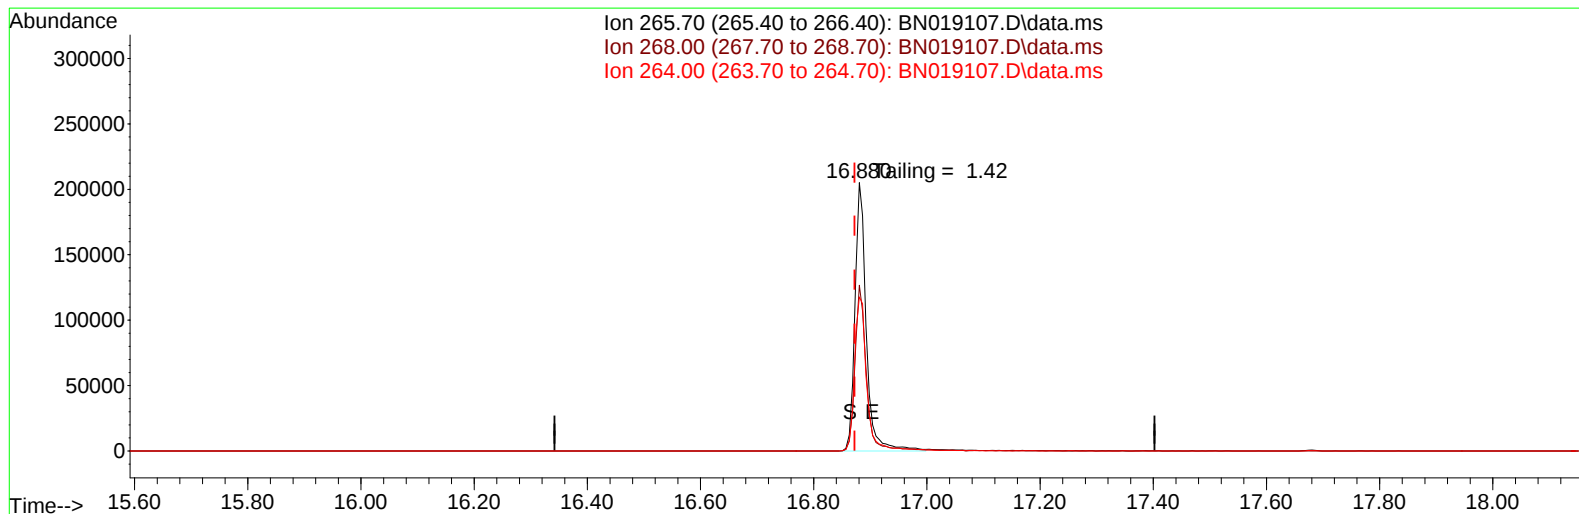

TIC: BN019107.D\data.ms

(70) Pentachlorophenol (C)

16.880min (+ 0.009) 16004.92 ng




response 288886

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.77
264.00	61.60	57.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032222\
Data File : BN019107.D
Acq On : 24 Mar 2022 02:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 24 06:30:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

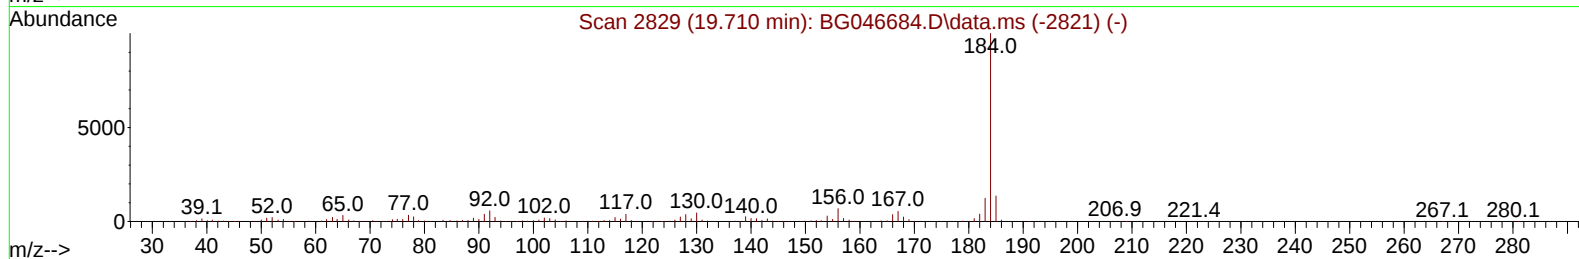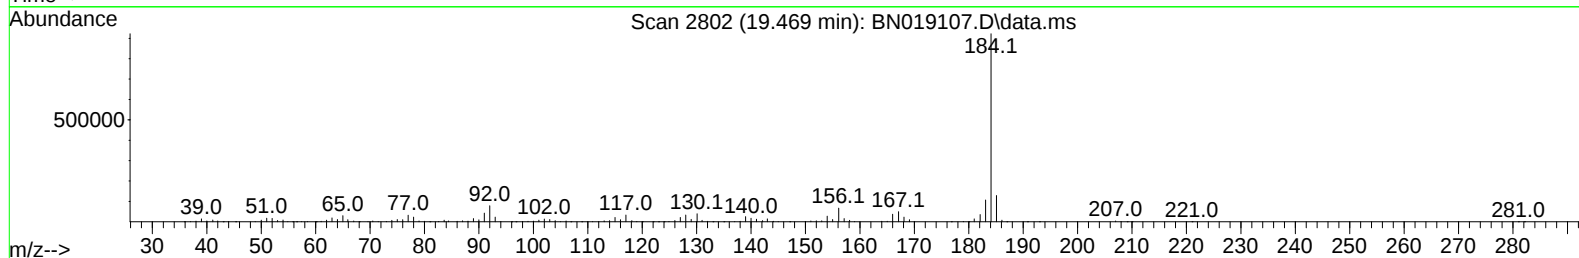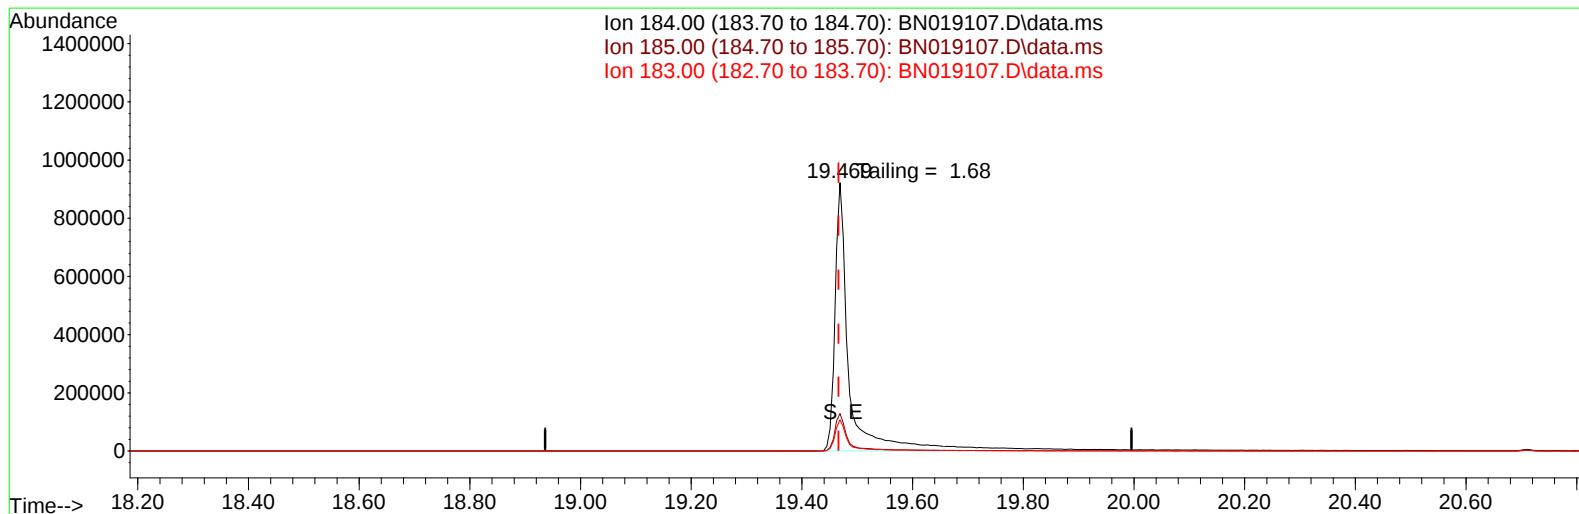

TIC: BN019107.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng

response 1671856

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_N	<u>BN019107.D</u>
Compound Name	Response	Retention Time
DDT	1085996	20.71
DDD	11230	20.269
DDE	704	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11934	1097930	1.09

Instrument :
BNA_N
ClientSampleId :
DFTPP