

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
 Data File : BN024482.D
 Acq On : 22 Mar 2023 16:33
 Operator : CG/JU
 Sample : PB151553BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK553

Quant Time: Mar 23 03:10:24 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 22 14:57:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	8804	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	25585	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	13394	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.409	188	27239	0.400	ng/ul	0.00
17) Chrysene-d12	21.597	240	19559	0.400	ng/ul	0.00
23) Perylene-d12	24.102	264	15651	0.400	ng/ul	# 0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	56059	5.786	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	10375	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	19972	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.656	166	3394	0.071	ng/ul#	14
20) Pyrene	19.798	202	3229	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.933	252	6421	0.125	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
Data File : BN024482.D
Acq On : 22 Mar 2023 16:33
Operator : CG/JU
Sample : PB151553BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK553

Quant Time: Mar 23 03:10:24 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 14:57:36 2023
Response via : Initial Calibration




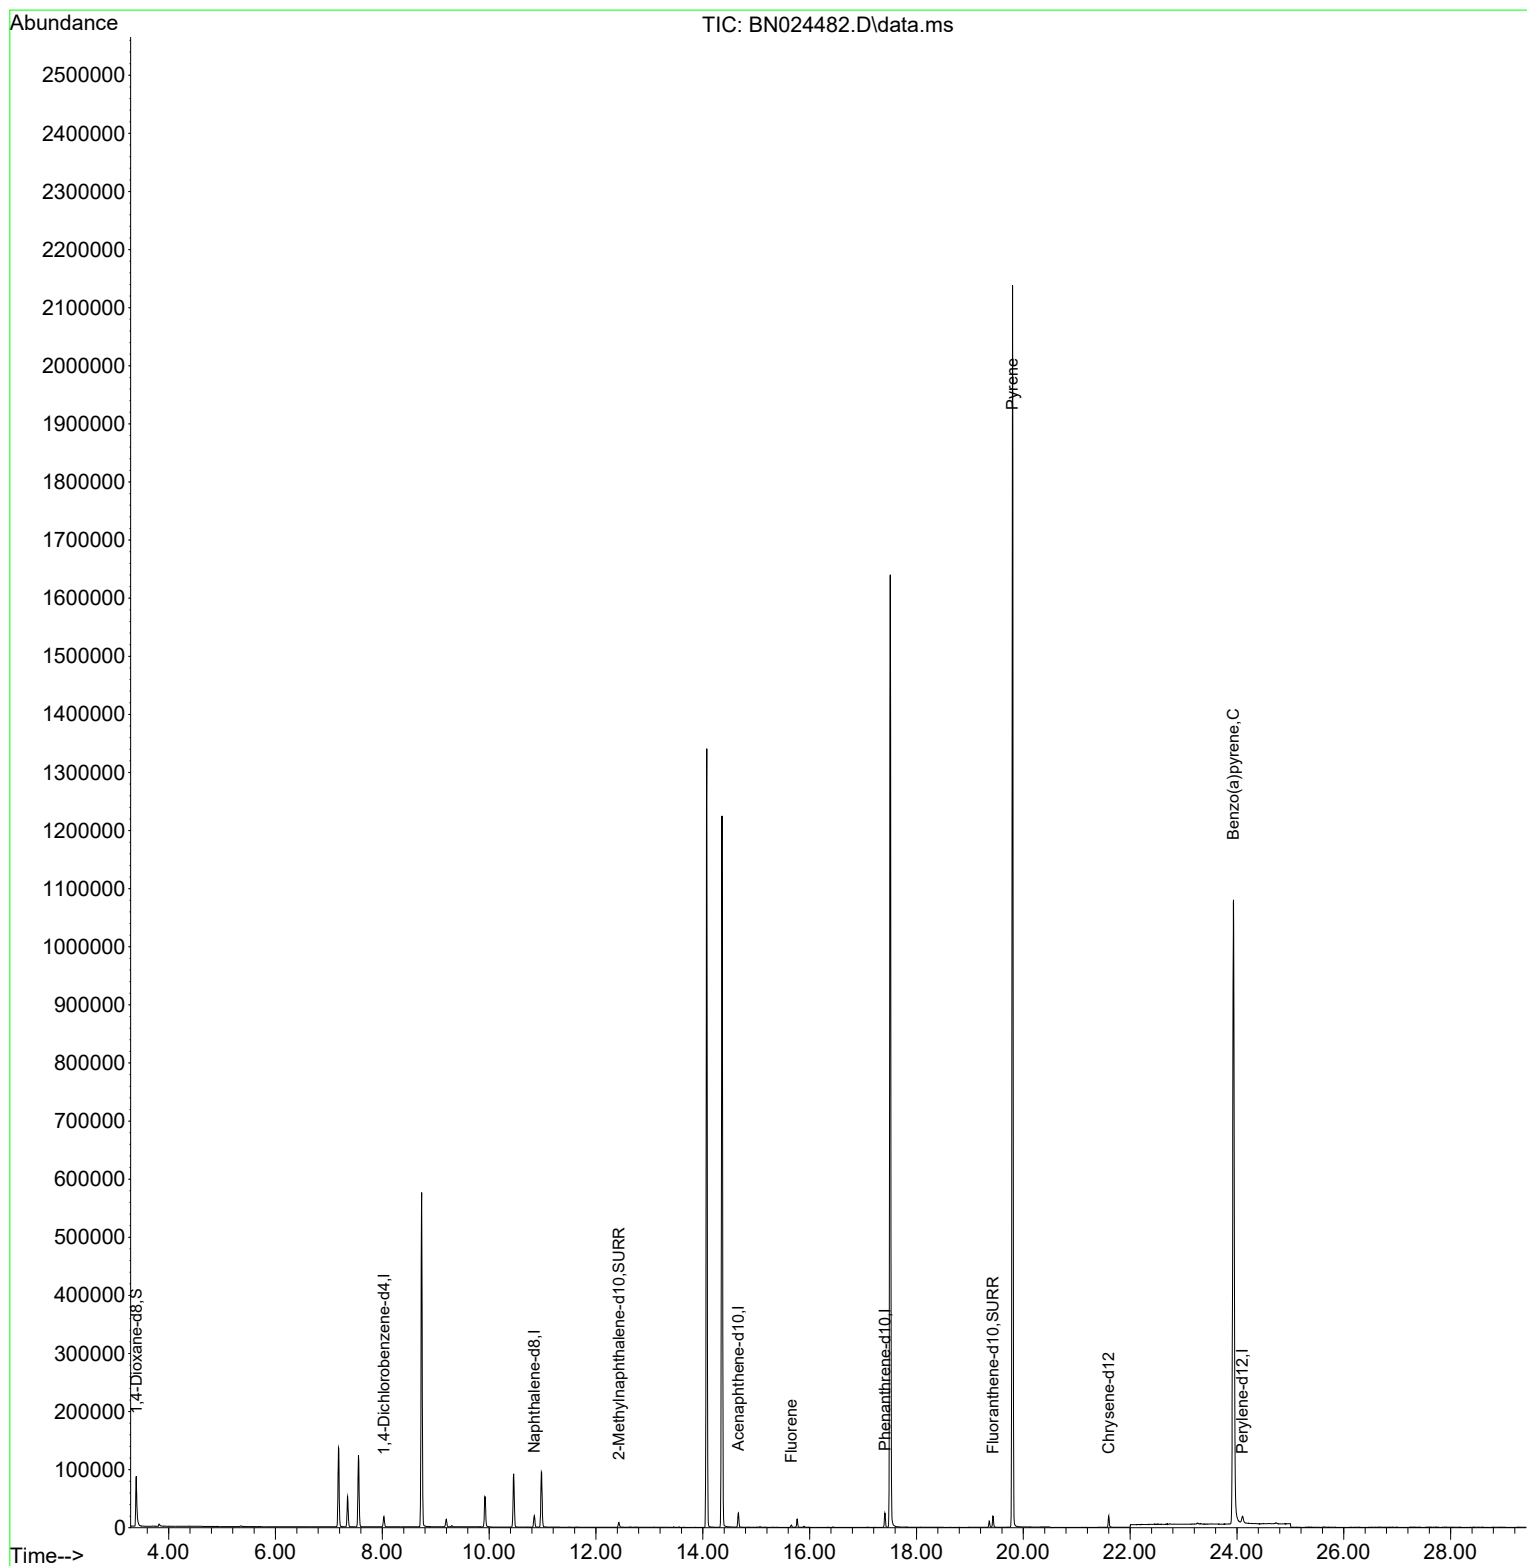


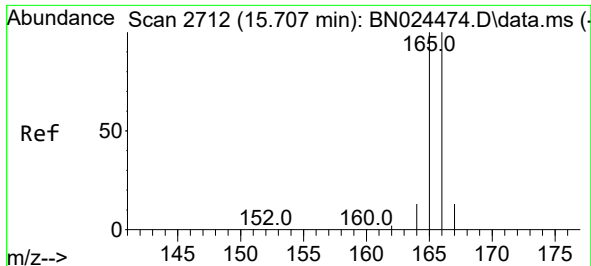

#12
Fluorene
Concen: 0.071 ng/ul
RT: 15.656 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN024482.D
Acq: 22 Mar 2023 16:33




Instrument :
BNA_N
ClientSampleId :
SBLK553


Tgt Ion:166 Resp: 3394
Ion Ratio Lower Upper
166 100
165 7.4 77.4 116.0#
167 32.9 10.9 16.3#

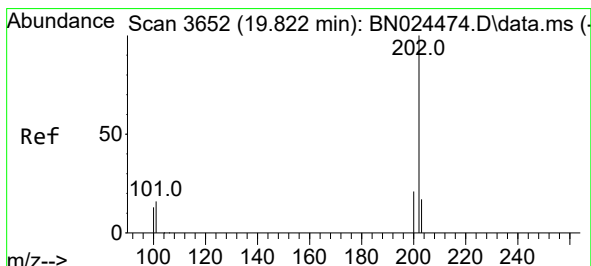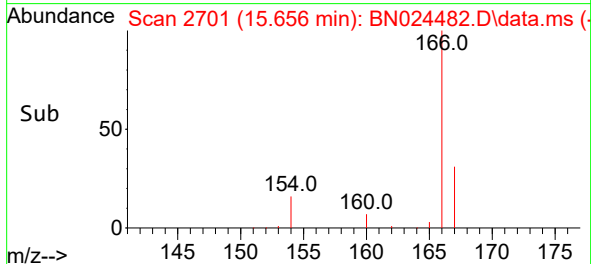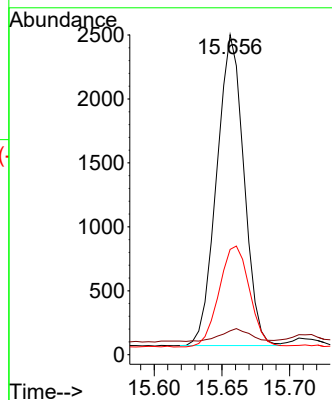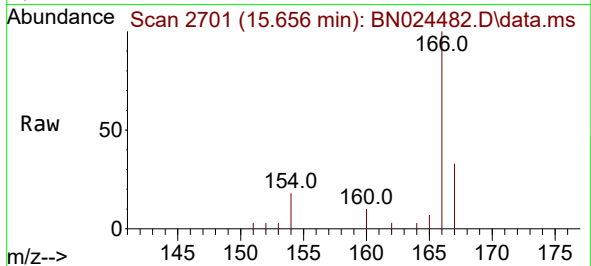

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.798 min Scan# 3647
Delta R.T. -0.024 min
Lab File: BN024482.D
Acq: 22 Mar 2023 16:33


Tgt Ion:202 Resp: 3229
Ion Ratio Lower Upper
202 100
101 166.6 12.1 18.1#
100 1227.2 9.4 14.0#

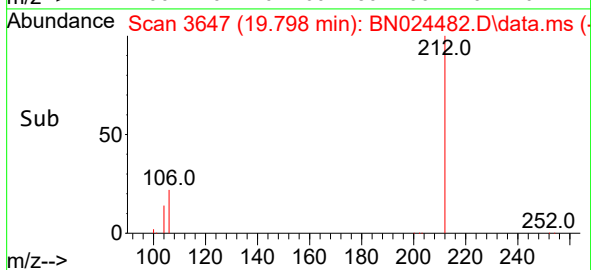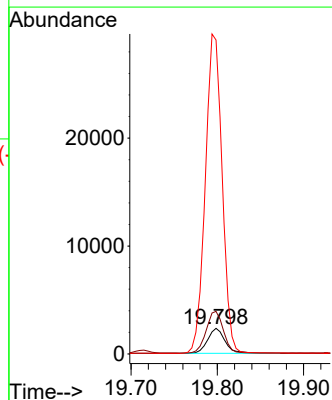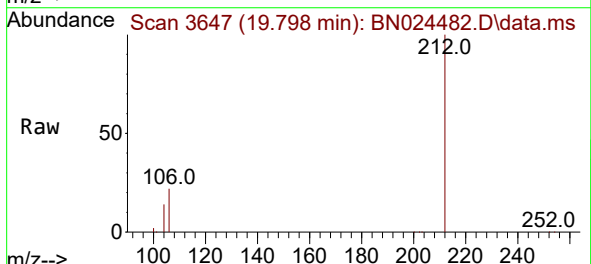

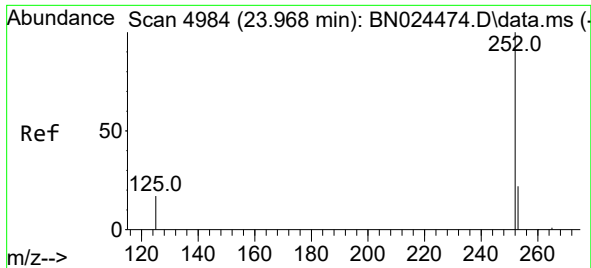

#26
 Benzo(a)pyrene
 Concen: 0.125 ng/ul
 RT: 23.933 min Scan# 49
 Delta R.T. -0.035 min
 Lab File: BN024482.D
 Acq: 22 Mar 2023 16:33

Instrument :
 BNA_N
 ClientSampleId :
 SBLK553

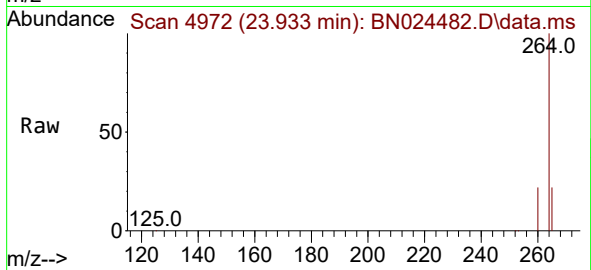

Tgt Ion:252 Resp: 6421
 Ion Ratio Lower Upper
 252 100
 253 48.4 19.2 28.8#
 125 49.3 15.8 23.6#

