

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
 Data File : BN024492.D
 Acq On : 22 Mar 2023 23:22
 Operator : CG/JU
 Sample : PB151557BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK557

Quant Time: Mar 23 03:33:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 23 03:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.025	152	10402	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	30660	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	16809	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.409	188	35237	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	27570	0.400	ng/ul	0.00
23) Perylene-d12	24.076	264	28835	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	63362	5.535	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	12784	0.351	ng/ul	0.00
18) Fluoranthene-d10	19.432	212	26618	0.363	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.794	202	3924	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.916	252	8242	0.087	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
Data File : BN024492.D
Acq On : 22 Mar 2023 23:22
Operator : CG/JU
Sample : PB151557BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK557

Quant Time: Mar 23 03:33:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 03:32:22 2023
Response via : Initial Calibration




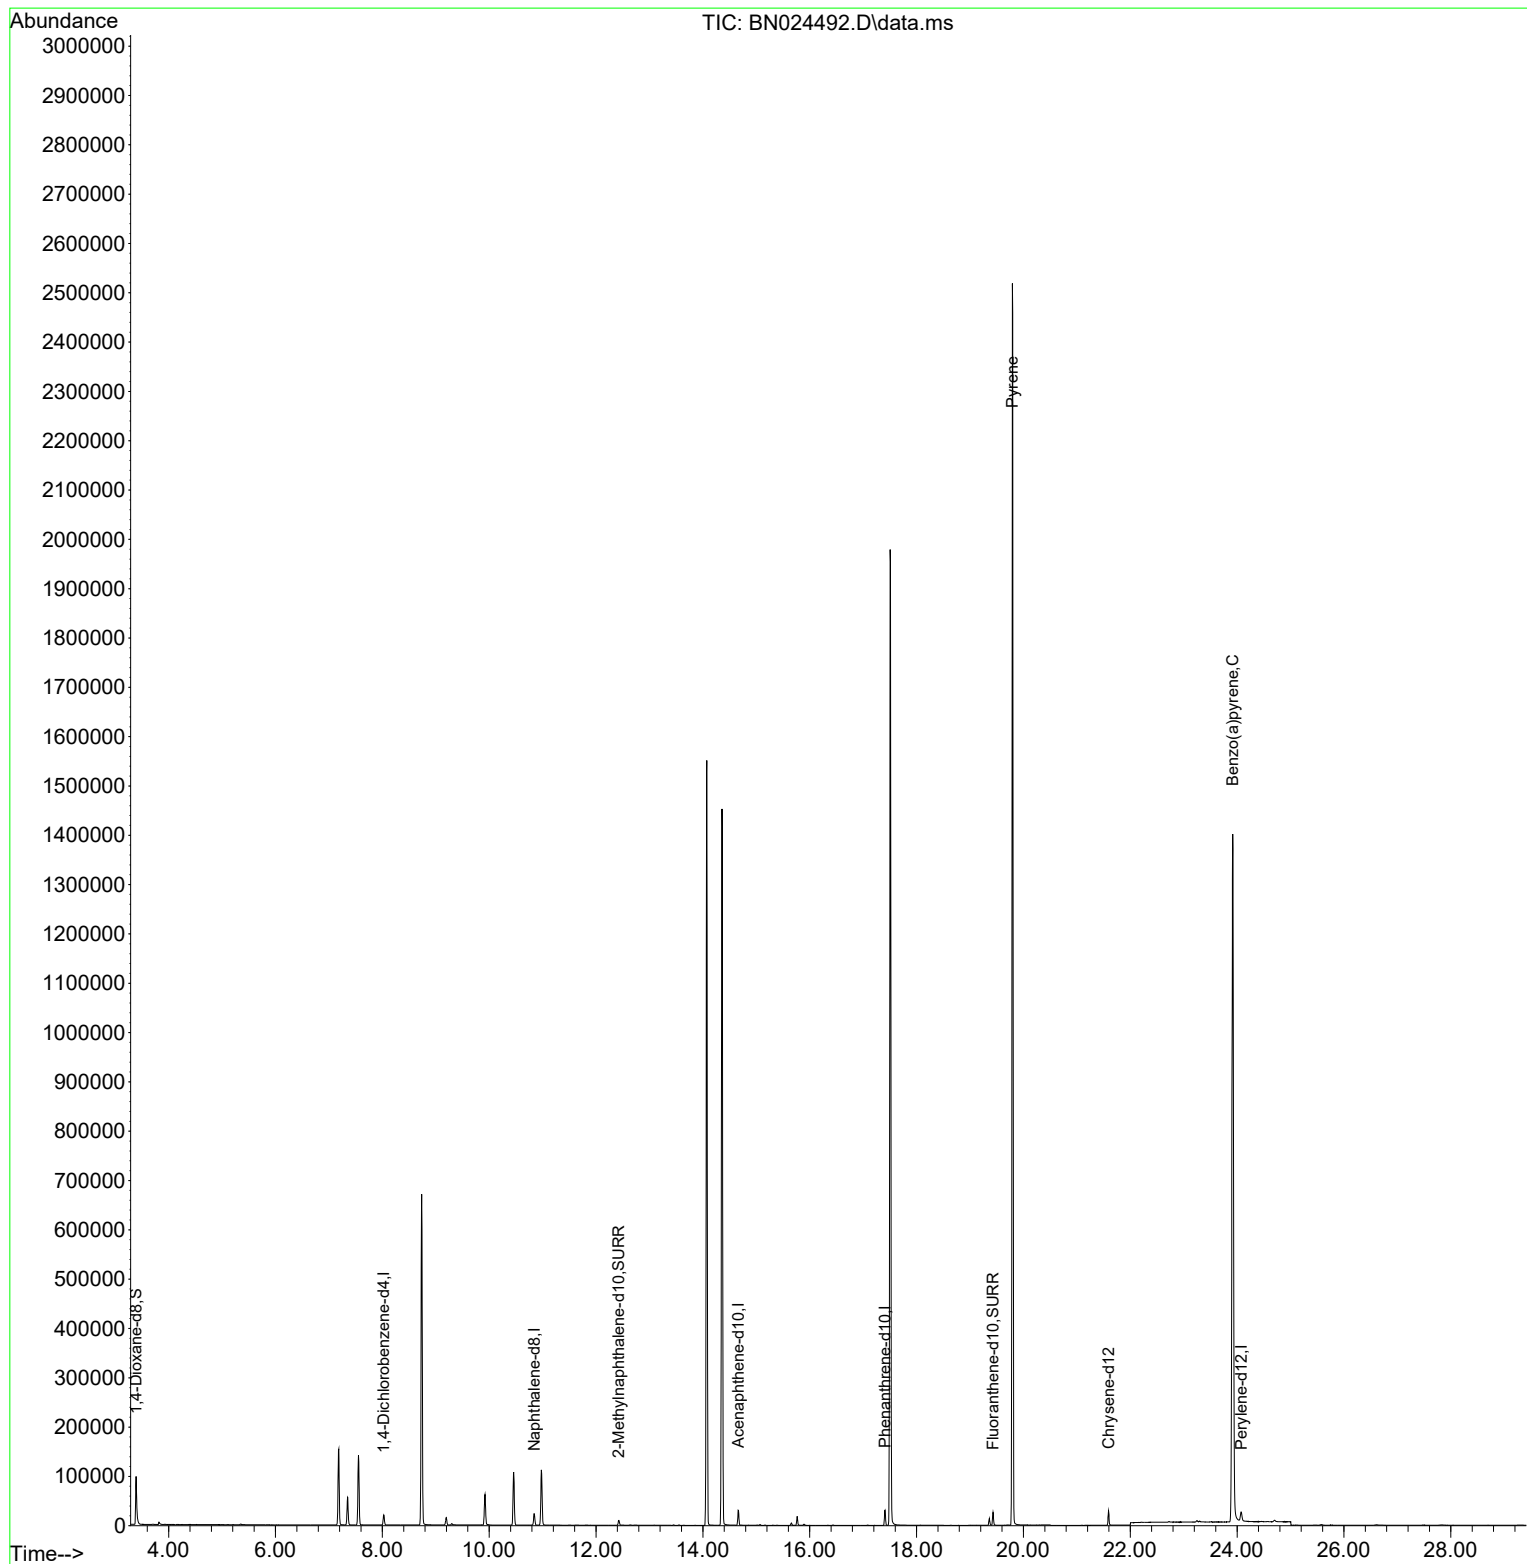


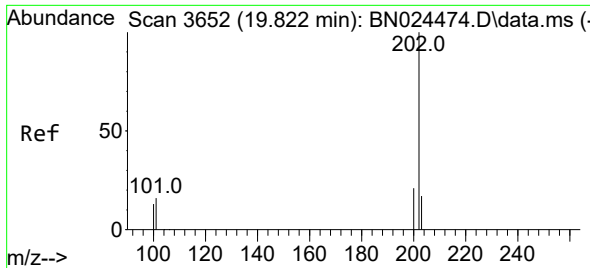

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.794 min Scan# 3646
Delta R.T. -0.028 min
Lab File: BN024492.D
Acq: 22 Mar 2023 23:22

Instrument :
BNA_N
ClientSampleId :
SBLK557

Tgt Ion:202 Resp: 3924
Ion Ratio Lower Upper
202 100
101 163.7 12.1 18.1#
100 1254.6 9.4 14.0#

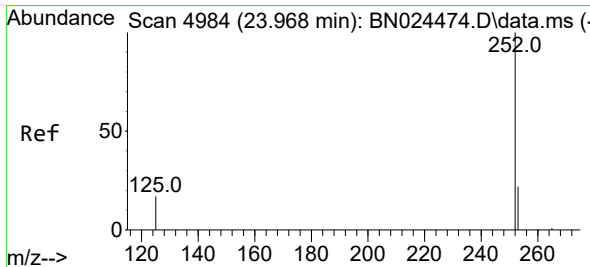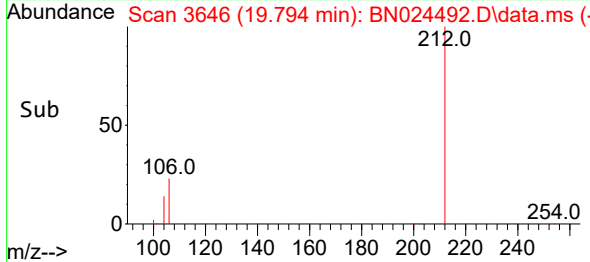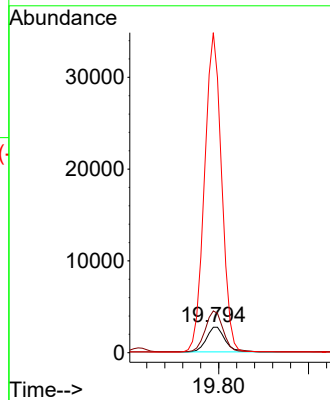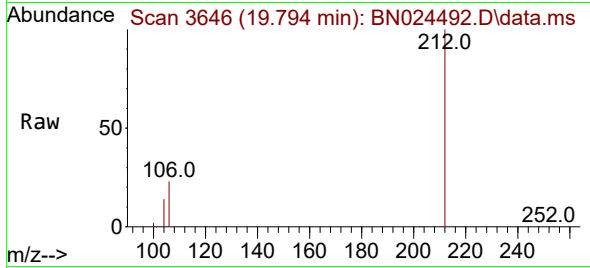

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.916 min Scan# 4966
Delta R.T. -0.061 min
Lab File: BN024492.D
Acq: 22 Mar 2023 23:22

Tgt Ion:252 Resp: 8242
Ion Ratio Lower Upper
252 100
253 46.6 19.2 28.8#
125 46.7 15.8 23.6#

