

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
 Data File : BN024478.D
 Acq On : 22 Mar 2023 12:05
 Operator : CG/JU
 Sample : 01810-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAF7

Quant Time: Mar 22 13:32:00 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 17:57:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.025	152	9259	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	27199	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	14535	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.409	188	30023	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	22412	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	19031	0.400	ng/ul	# 0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	46008	4.515	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.429	152	13370	0.414	ng/ul	0.00
18) Fluoranthene-d10	19.432	212	30033	0.504	ng/ul	0.00
Target Compounds						
						Qvalue
11) Acenaphthene	14.726	153	1399	0.030	ng/ul	98
16) Anthracene	17.540	178	1917	0.025	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
Data File : BN024478.D
Acq On : 22 Mar 2023 12:05
Operator : CG/JU
Sample : 01810-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAF7

Quant Time: Mar 22 13:32:00 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 17:57:40 2023
Response via : Initial Calibration




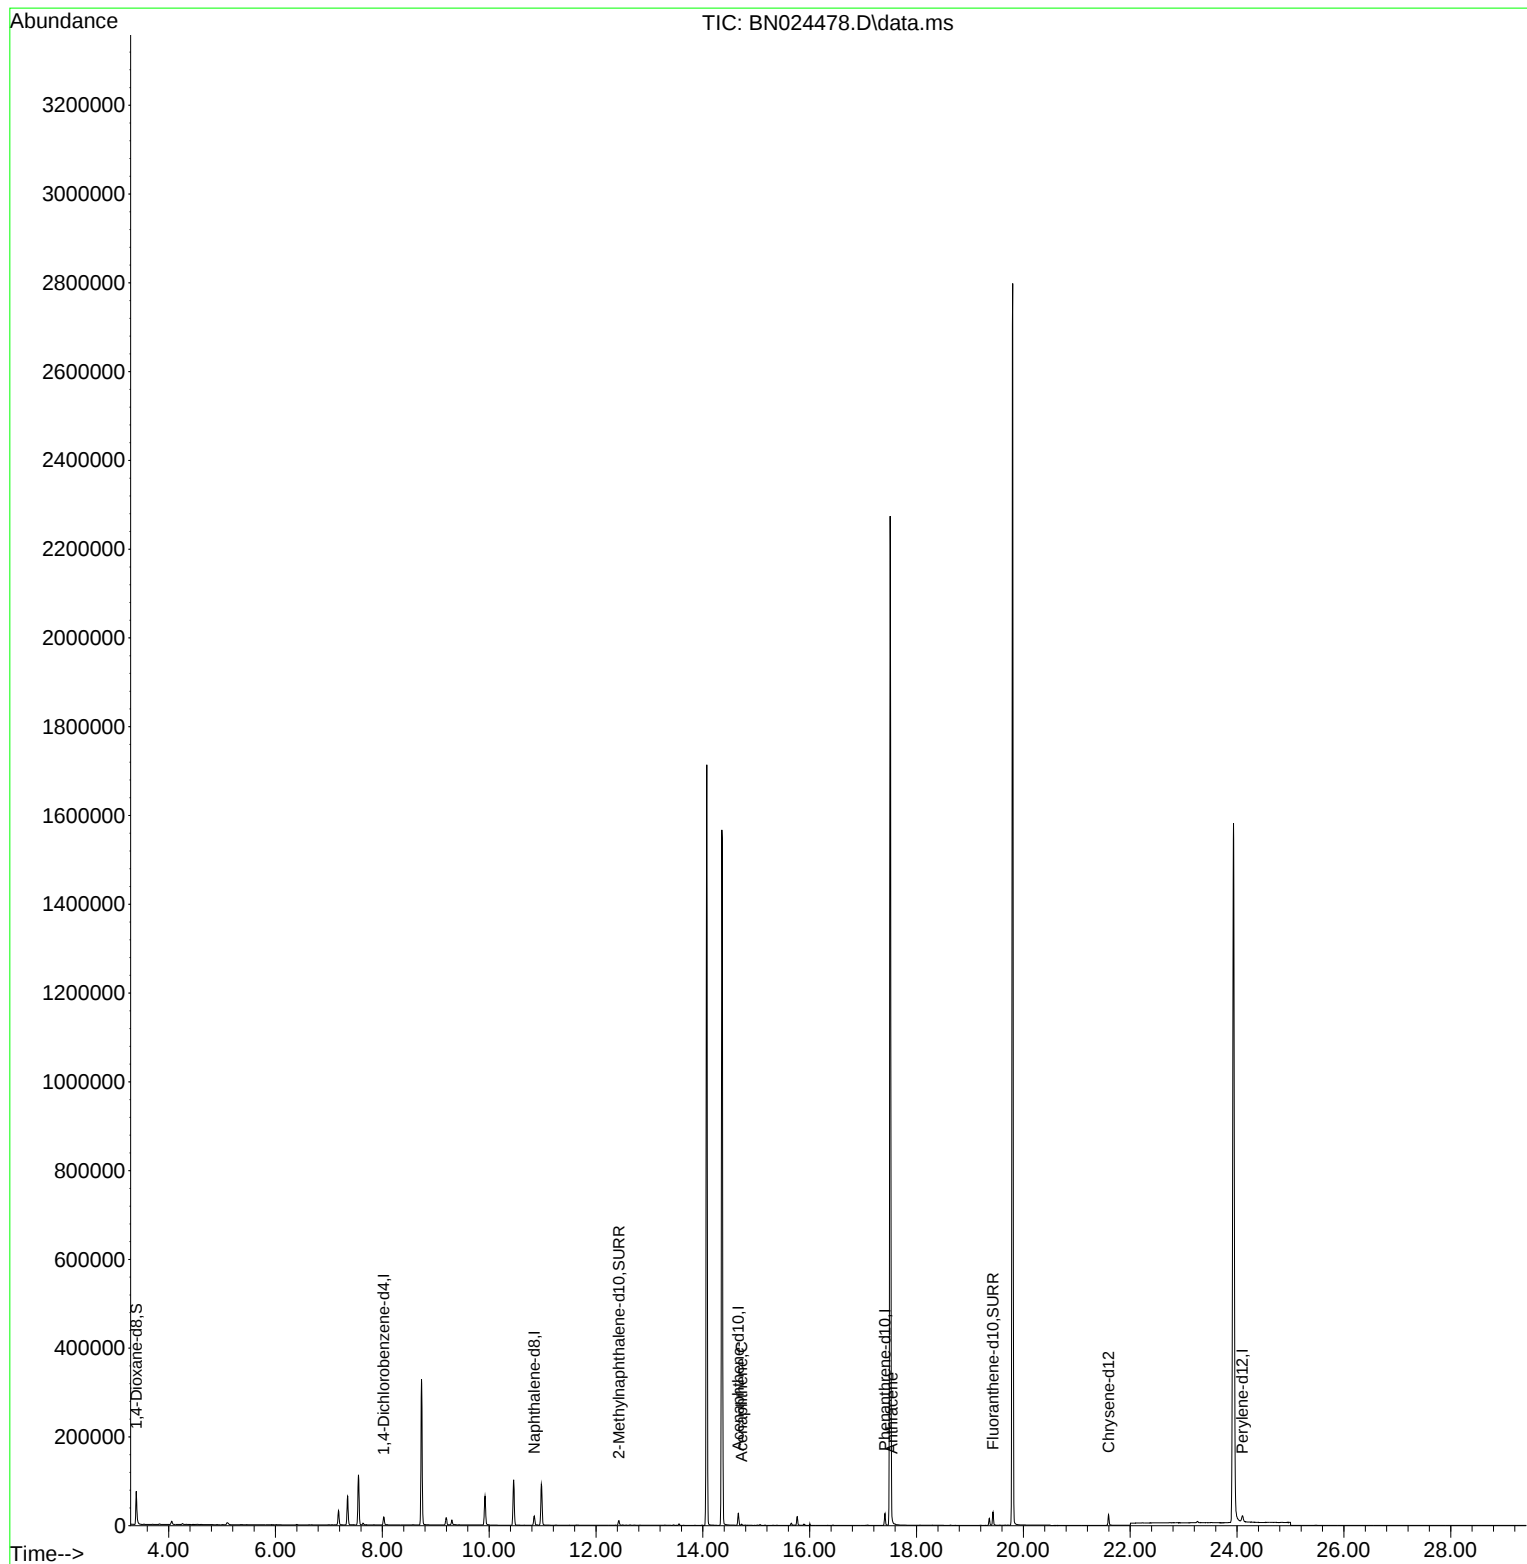


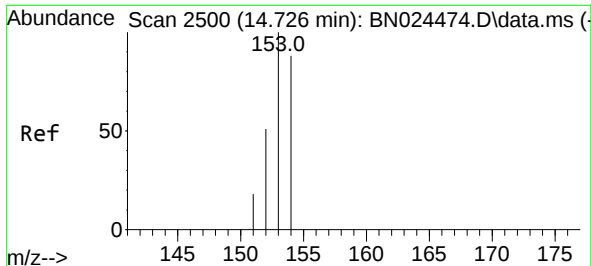

#11
Acenaphthene
Concen: 0.030 ng/ul
RT: 14.726 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN024478.D
Acq: 22 Mar 2023 12:05

Instrument :
BNA_N
ClientSampleId :
DCAF7

Tgt Ion:153 Resp: 1399
Ion Ratio Lower Upper
153 100
152 52.9 42.6 64.0
154 85.3 70.6 105.8

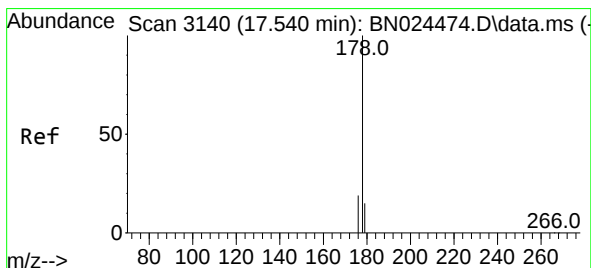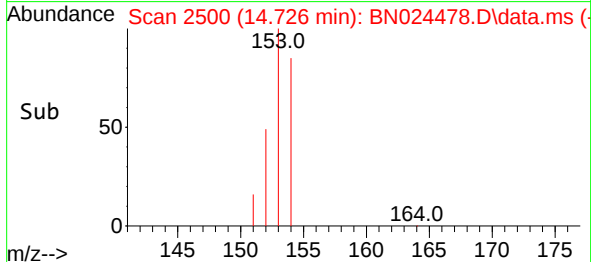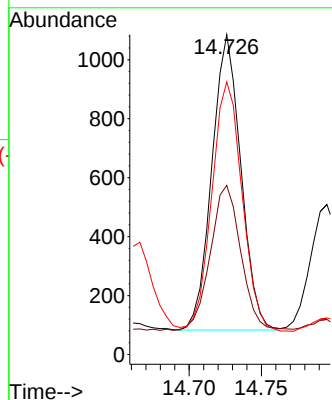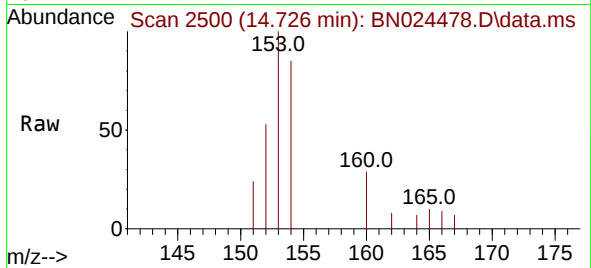

#16
Anthracene
Concen: 0.025 ng/ul
RT: 17.540 min Scan# 3140
Delta R.T. -0.004 min
Lab File: BN024478.D
Acq: 22 Mar 2023 12:05

Tgt Ion:178 Resp: 1917
Ion Ratio Lower Upper
178 100
179 25.6 12.3 18.5#
176 24.6 15.3 22.9#

