

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032223\  
 Data File : BN024486.D  
 Acq On : 22 Mar 2023 19:02  
 Operator : CG/JU  
 Sample : 01949-05  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 CB937

Quant Time: Mar 23 03:10:57 2023  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN030923.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 22 14:57:36 2023  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	9312	0.400	ng/u1	0.00
4) Naphthalene-d8	10.845	136	27171	0.400	ng/u1 #	0.00
9) Acenaphthene-d10	14.666	164	16222	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.409	188	33354	0.400	ng/u1 #	0.00
17) Chrysene-d12	21.592	240	26367	0.400	ng/u1 #	0.00
23) Perylene-d12	24.073	264	28321	0.400	ng/u1 #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	51583	5.034	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.429	152	14367	0.445	ng/u1	0.00
18) Fluoranthene-d10	19.436	212	36075	0.514	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.431	88	15451	1.386	ng/u1#	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032223\  
 Data File : BN024486.D  
 Acq On : 22 Mar 2023 19:02  
 Operator : CG/JU  
 Sample : 01949-05  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 CB937

Quant Time: Mar 23 03:10:57 2023  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN030923.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 22 14:57:36 2023  
 Response via : Initial Calibration

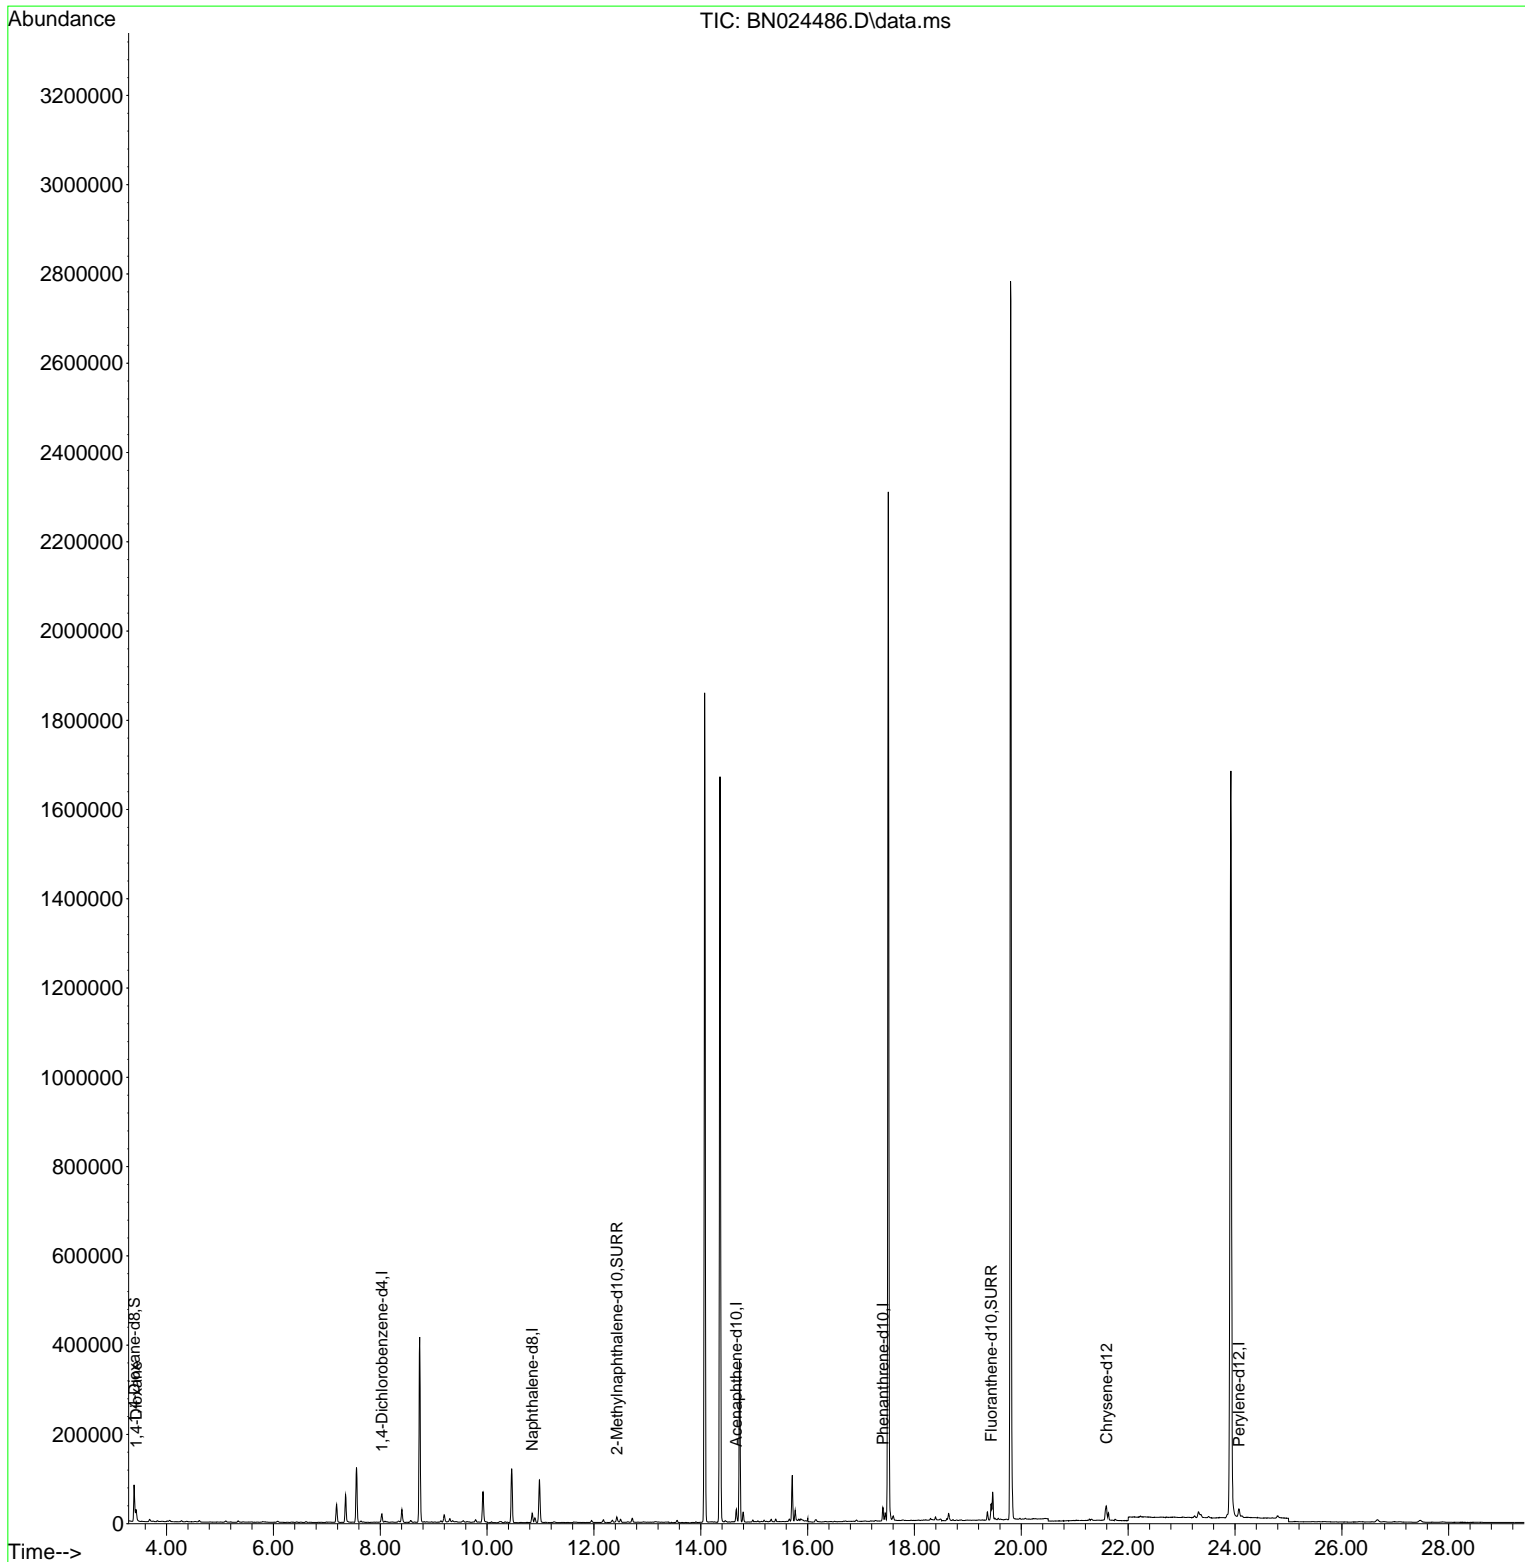

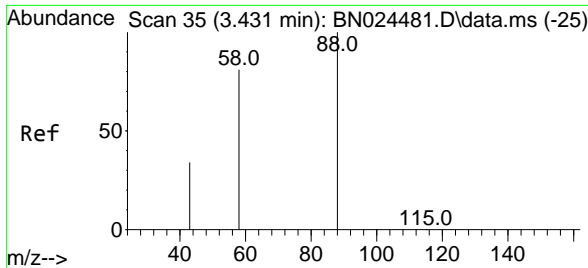

#2  
 1,4-Dioxane  
 Concen: 1.386 ng/ul  
 RT: 3.431 min Scan# 31  
 Delta R.T. -0.004 min  
 Lab File: BN024486.D  
 Acq: 22 Mar 2023 19:02

Instrument :  
 BNA\_N  
 ClientSampleId :  
 CB937

Tgt Ion: 88 Resp: 15451

Ion	Ratio	Lower	Upper
88	100		
43	53.9	32.1	48.1#
58	78.6	55.1	82.7

