

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
 Data File : BN024490.D
 Acq On : 22 Mar 2023 21:31
 Operator : CG/JU
 Sample : 01947-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB933

Quant Time: Mar 23 03:11:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 22 14:57:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	9743	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	28979	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	16521	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.409	188	35315	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	28588	0.400	ng/ul	0.00
23) Perylene-d12	24.076	264	29366	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	51397	4.794	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	13280	0.386	ng/ul	0.00
18) Fluoranthene-d10	19.431	212	36756	0.483	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.451	178	2472	0.024	ng/ul#	81
16) Anthracene	17.540	178	2306	0.026	ng/ul#	77
19) Fluoranthene	19.459	202	2944	0.026	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
Data File : BN024490.D
Acq On : 22 Mar 2023 21:31
Operator : CG/JU
Sample : 01947-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB933

Quant Time: Mar 23 03:11:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 14:57:36 2023
Response via : Initial Calibration




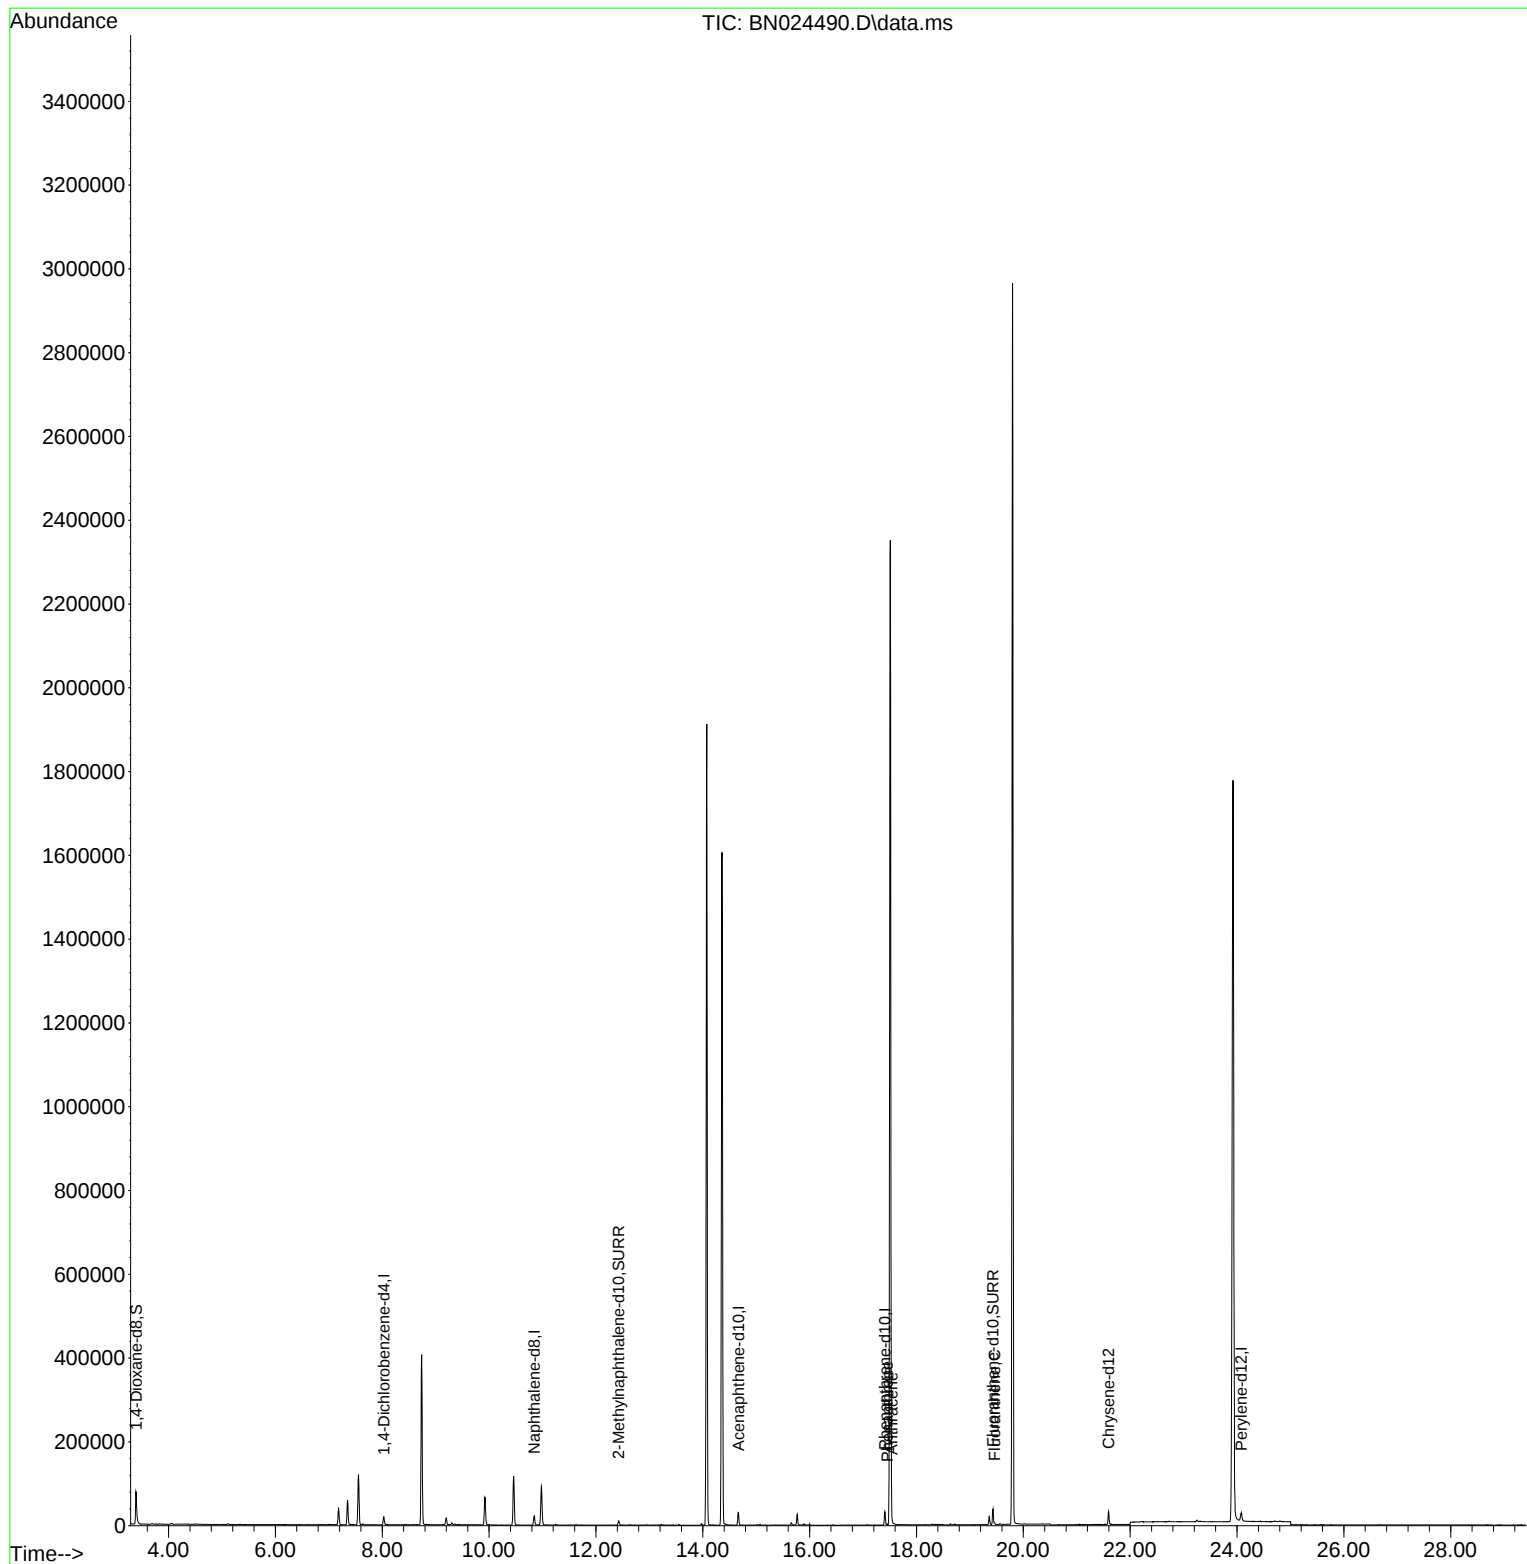


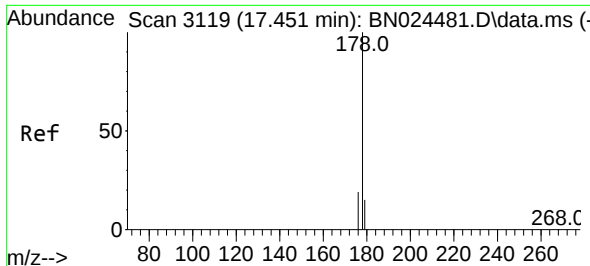

#15
Phenanthrene
Concen: 0.024 ng/ul
RT: 17.451 min Scan# 3119
Delta R.T. 0.004 min
Lab File: BN024490.D
Acq: 22 Mar 2023 21:31




Instrument :
BNA_N
ClientSampleId :
CB933


Tgt Ion:178 Resp: 2472
Ion Ratio Lower Upper
178 100
179 26.4 12.2 18.2#
176 25.7 15.7 23.5#

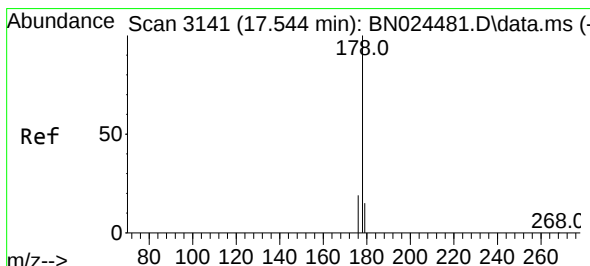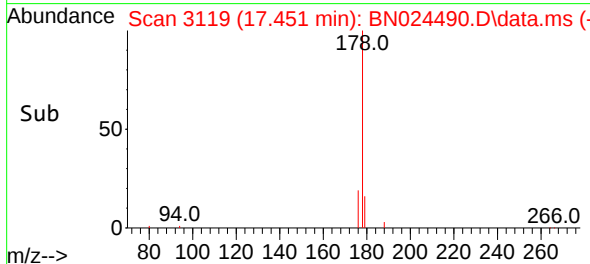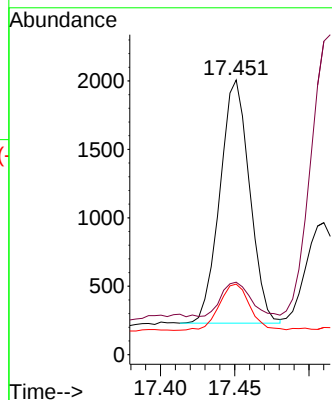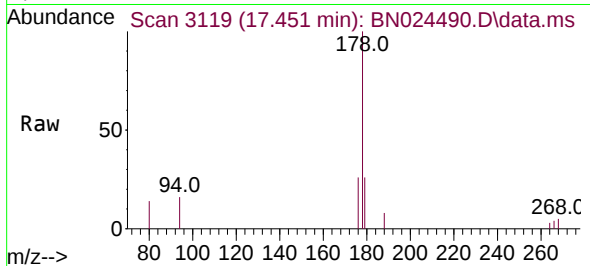

#16
Anthracene
Concen: 0.026 ng/ul
RT: 17.540 min Scan# 3140
Delta R.T. -0.000 min
Lab File: BN024490.D
Acq: 22 Mar 2023 21:31


Tgt Ion:178 Resp: 2306
Ion Ratio Lower Upper
178 100
179 29.0 12.3 18.5#
176 26.1 15.3 22.9#

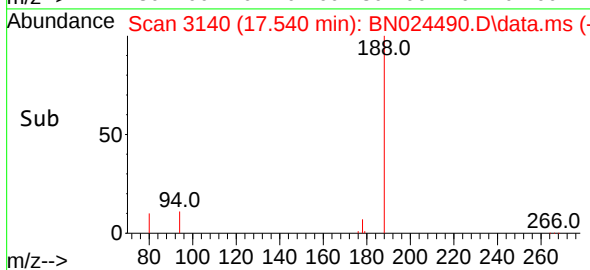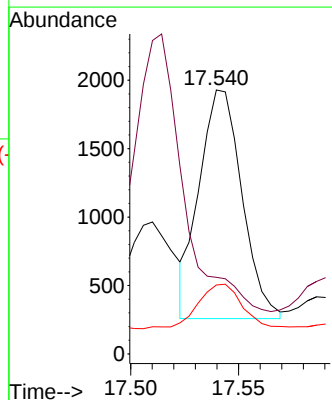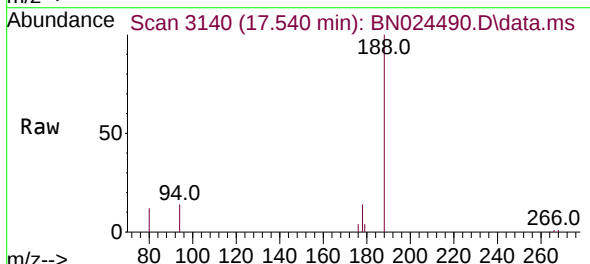

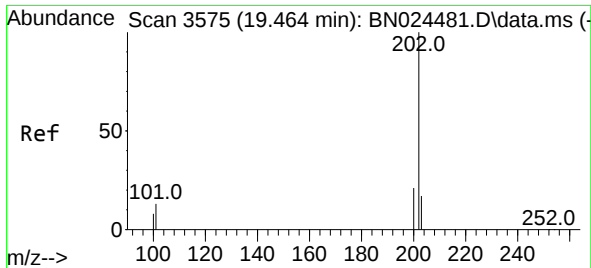

#19
 Fluoranthene
 Concen: 0.026 ng/ul
 RT: 19.459 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN024490.D
 Acq: 22 Mar 2023 21:31

Instrument :
 BNA_N
 ClientSampleId :
 CB933

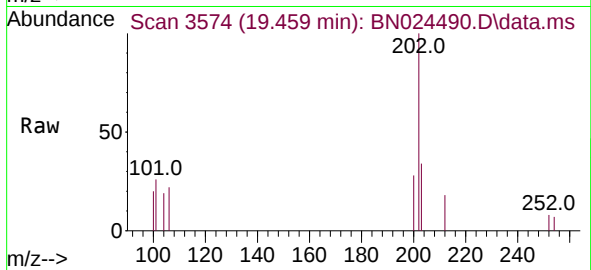

Tgt Ion:202 Resp: 2944
 Ion Ratio Lower Upper
 202 100
 101 26.5 10.4 15.6#
 100 19.7 7.7 11.5#

