

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
 Data File : BN024495.D
 Acq On : 23 Mar 2023 01:12
 Operator : CG/JU
 Sample : 01947-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB935

Quant Time: Mar 23 03:33:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 23 03:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.025	152	10501	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	31115	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.661	164	17951	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.405	188	38664	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.589	240	31538	0.400	ng/ul	0.00
23) Perylene-d12	24.082	264	32758	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	45607	3.947	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.423	152	12761	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.432	212	34580	0.412	ng/ul	0.00
Target Compounds						
						Qvalue
16) Anthracene	17.540	178	2774	0.029	ng/ul#	49
19) Fluoranthene	19.459	202	2723	0.022	ng/ul#	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
Data File : BN024495.D
Acq On : 23 Mar 2023 01:12
Operator : CG/JU
Sample : 01947-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB935

Quant Time: Mar 23 03:33:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 03:32:22 2023
Response via : Initial Calibration




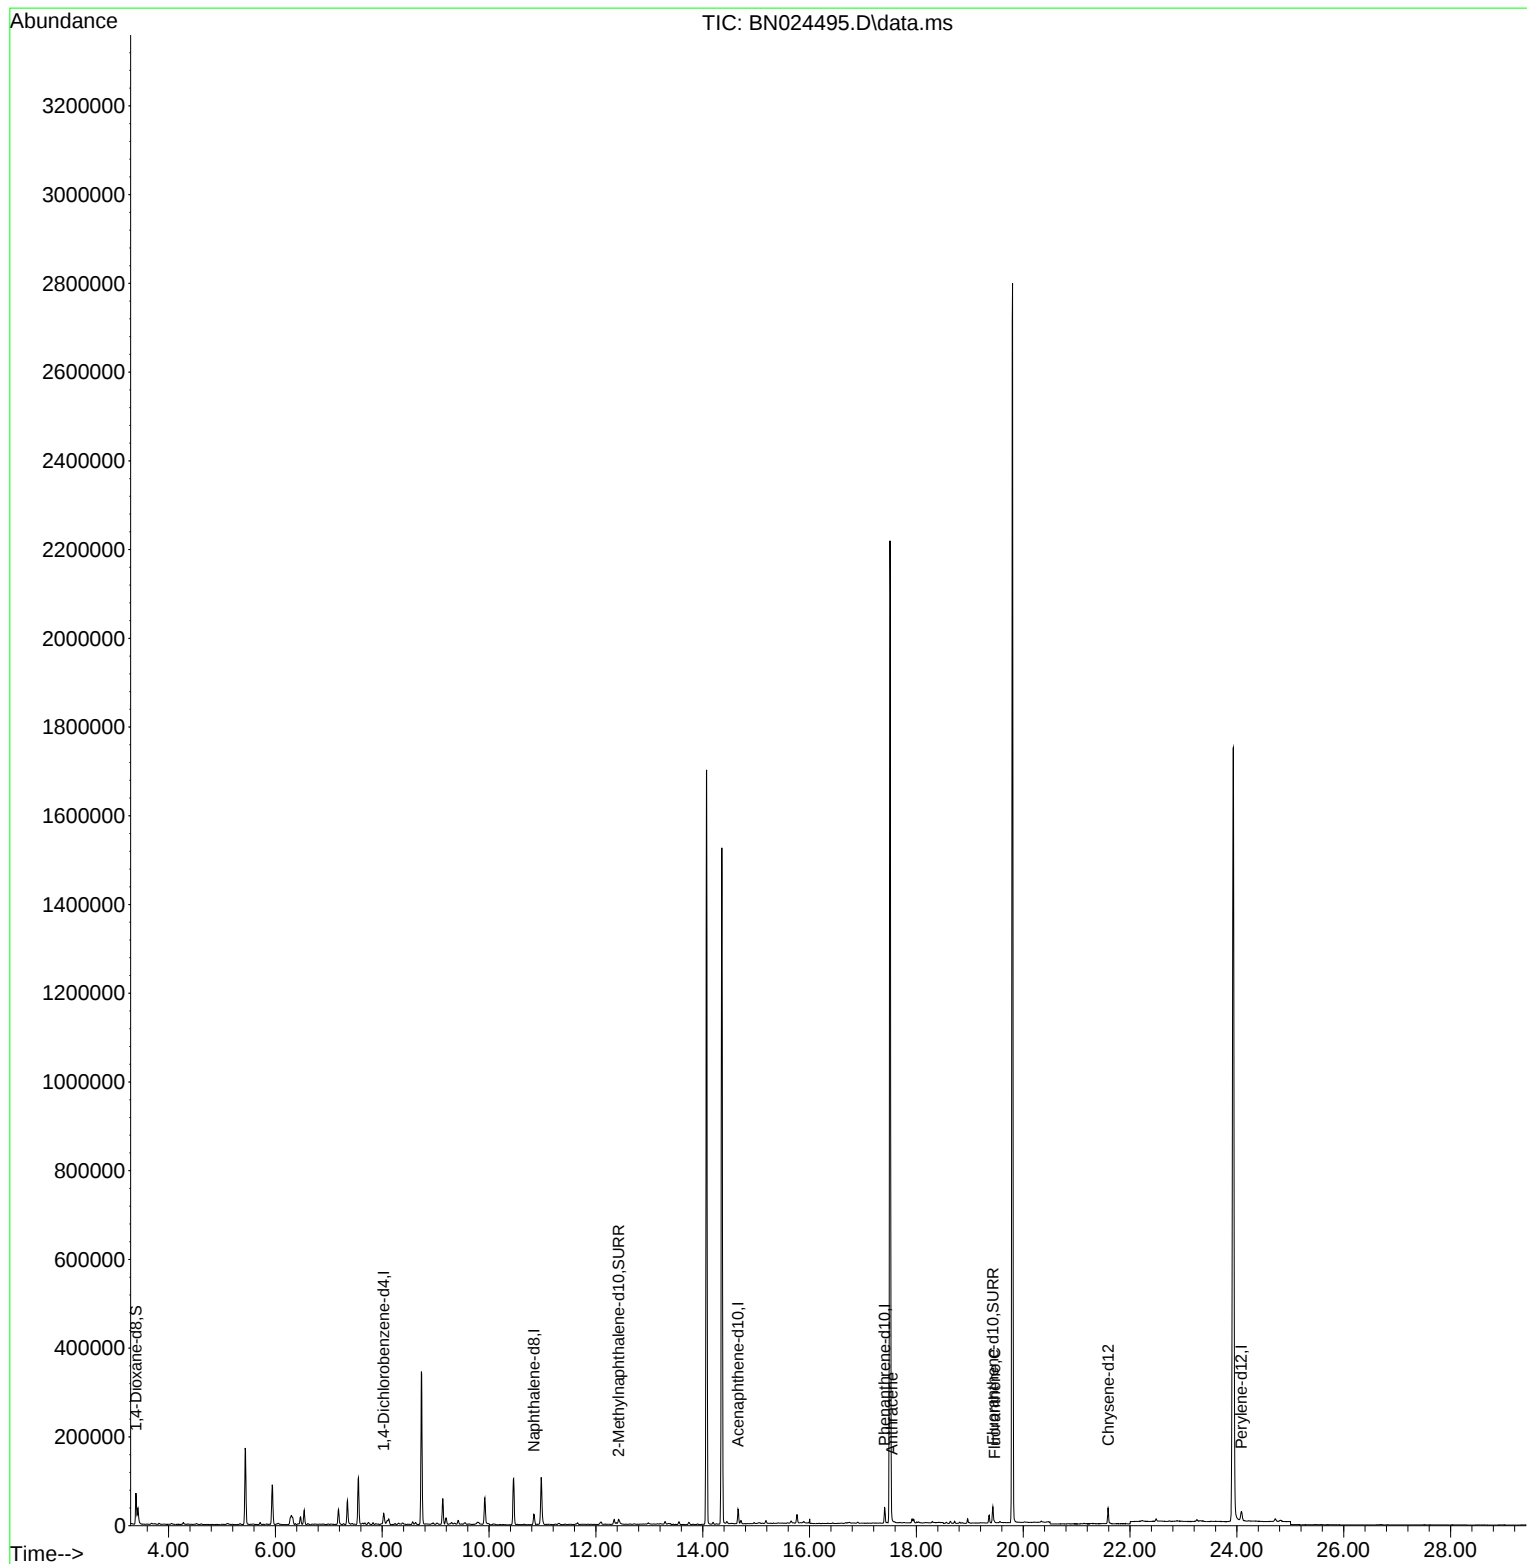


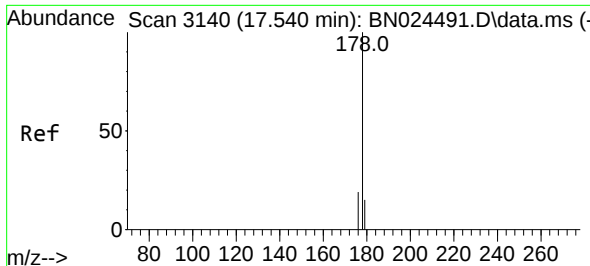

#16
 Anthracene
 Concen: 0.029 ng/ul
 RT: 17.540 min Scan# 3140
 Delta R.T. 0.000 min
 Lab File: BN024495.D
 Acq: 23 Mar 2023 01:12

Instrument :
 BNA_N
 ClientSampleId :
 CB935

Tgt Ion:178 Resp: 2774
 Ion Ratio Lower Upper
 178 100
 179 39.3 12.3 18.5#
 176 40.2 15.3 22.9#

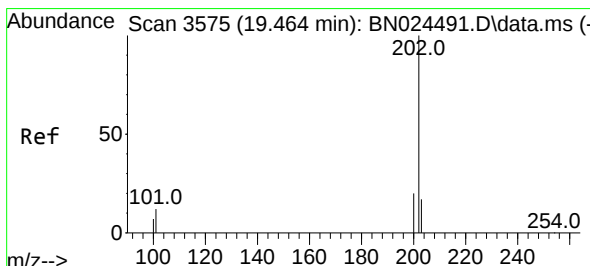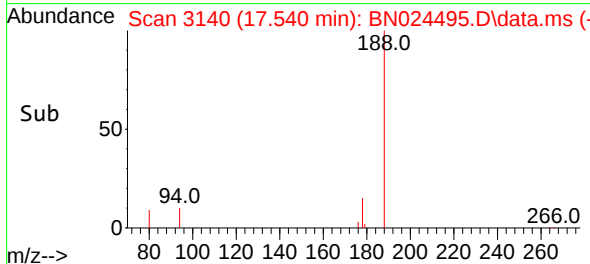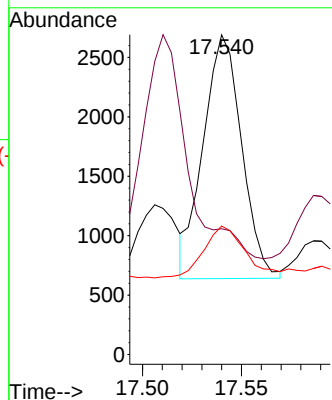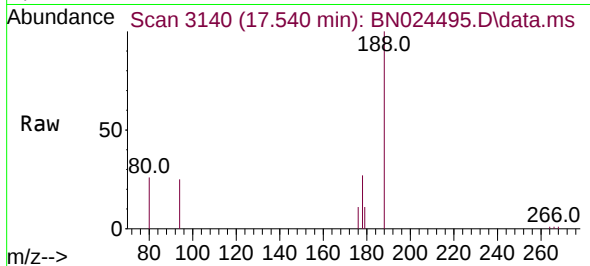

#19
 Fluoranthene
 Concen: 0.022 ng/ul
 RT: 19.459 min Scan# 3574
 Delta R.T. -0.004 min
 Lab File: BN024495.D
 Acq: 23 Mar 2023 01:12

Tgt Ion:202 Resp: 2723
 Ion Ratio Lower Upper
 202 100
 101 51.3 10.4 15.6#
 100 38.1 7.7 11.5#

