

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
 Data File : BN024496.D
 Acq On : 23 Mar 2023 01:48
 Operator : CG/JU
 Sample : 01949-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB935

Quant Time: Mar 23 03:34:04 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 23 03:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.025	152	9848	0.400	ng/u1	0.00
4) Naphthalene-d8	10.839	136	28971	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.661	164	17009	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.409	188	35572	0.400	ng/u1	# 0.00
17) Chrysene-d12	21.589	240	27970	0.400	ng/u1	0.00
23) Perylene-d12	24.082	264	28781	0.400	ng/u1	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	44699	4.124	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.423	152	13351	0.388	ng/u1	0.00
18) Fluoranthene-d10	19.432	212	35172	0.473	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.427	88	23636	2.005	ng/u1	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032223\
Data File : BN024496.D
Acq On : 23 Mar 2023 01:48
Operator : CG/JU
Sample : 01949-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB935


Quant Time: Mar 23 03:34:04 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 03:32:22 2023
Response via : Initial Calibration

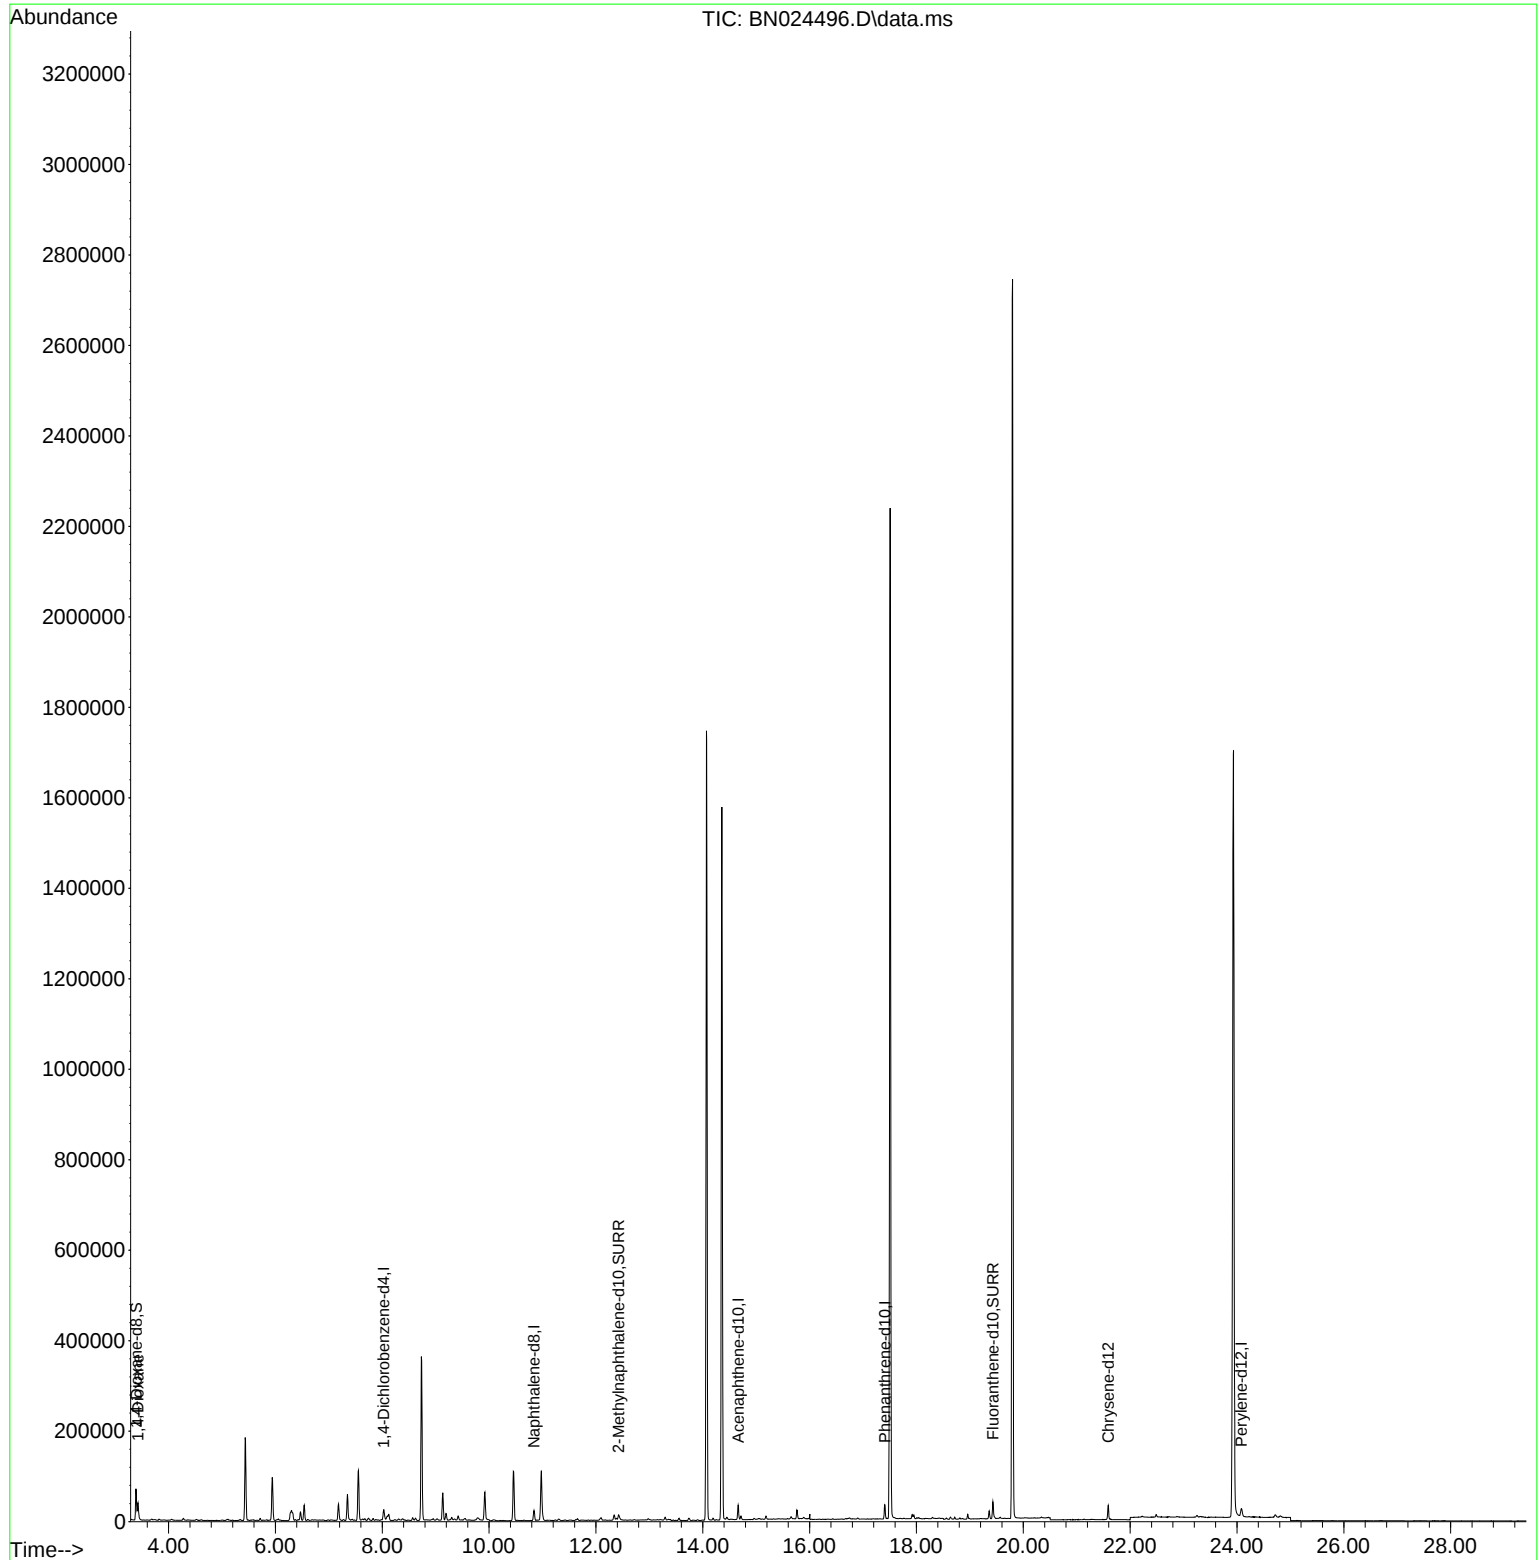

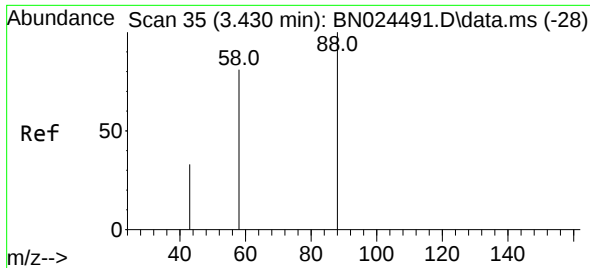

#2
 1,4-Dioxane
 Concen: 2.005 ng/ul
 RT: 3.427 min Scan# 34
 Delta R.T. -0.004 min
 Lab File: BN024496.D
 Acq: 23 Mar 2023 01:48

Instrument :
 BNA_N
 ClientSampleId :
 CB935

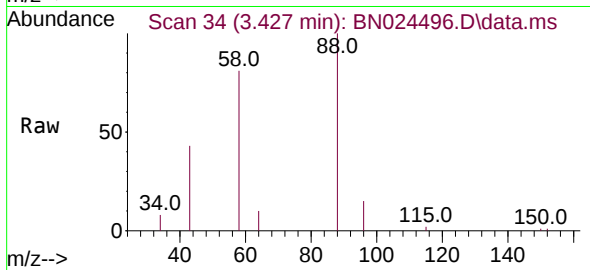

Tgt Ion: 88 Resp: 23636

Ion	Ratio	Lower	Upper
88	100		
43	43.4	32.1	48.1
58	81.4	55.1	82.7

