


Abundance

Ion 265.70 (265.40 to 266.40): BN030449.D\data.ms
 Ion 268.00 (267.70 to 268.70): BN030449.D\data.ms
 Ion 264.00 (263.70 to 264.70): BN030449.D\data.ms

16.757 Tailing = 1.30

S E

Time-->

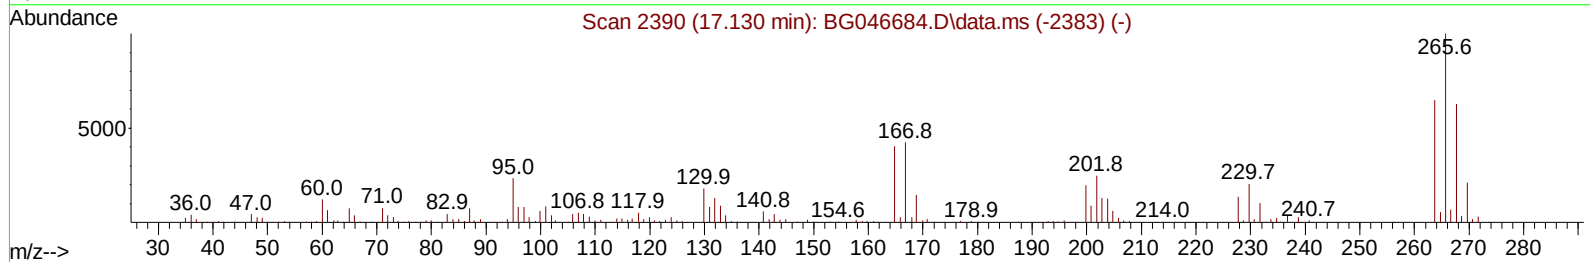

TIC: BN030449.D\data.ms

(70) Pentachlorophenol (C)




16.757min (0.000) 27905.41 ng

response **771518**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.47
264.00	61.60	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032224\
Data File : BN030449.D
Acq On : 21 Mar 2024 16:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 02:28:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 22 02:28:35 2024
Response via : Initial Calibration

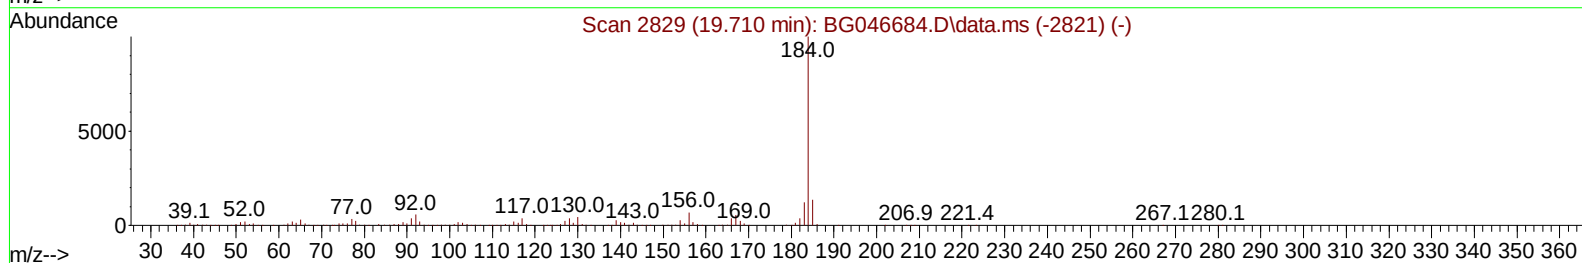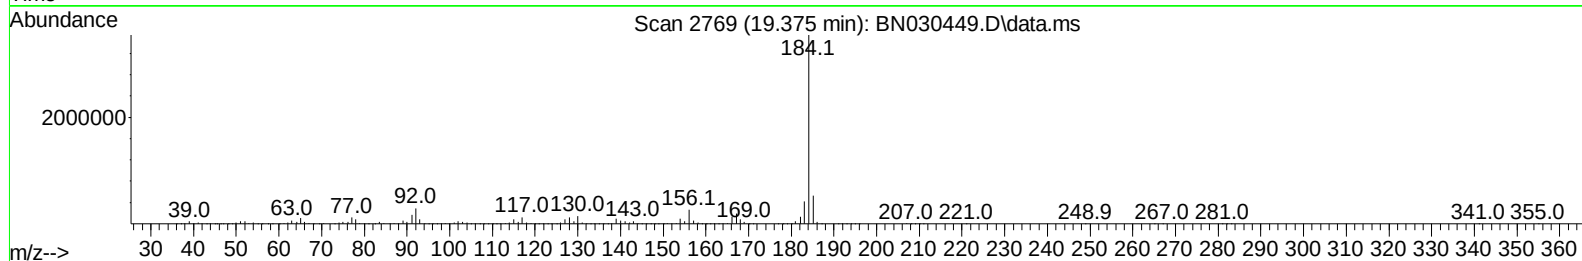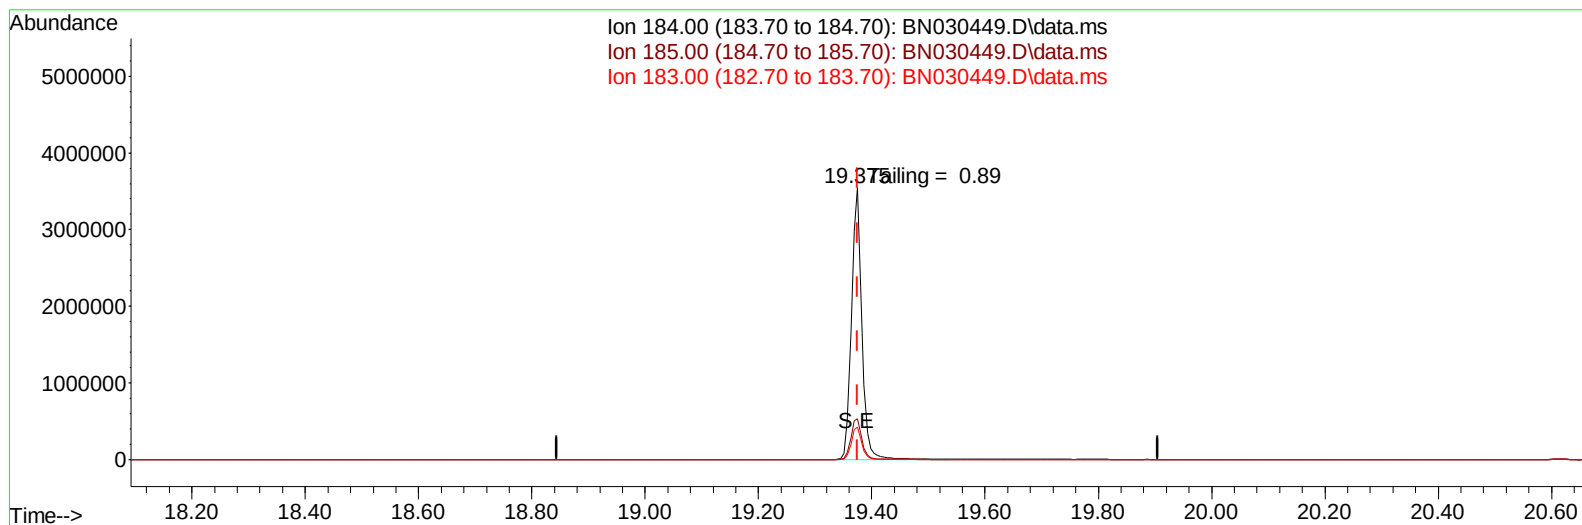

TIC: BN030449.D\data.ms

(77) Benzidine

19.375min (0.000) 0.00 ng

response 4549837

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.05
183.00	13.20	11.89
0.00	0.00	0.00