

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032224\
 Data File : BN030453.D
 Acq On : 21 Mar 2024 19:03
 Operator : MA/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Mar 21 23:57:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN032224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 21 23:54:14 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.732	152	10014	0.400	ng	0.00
7) Naphthalene-d8	10.509	136	27805	0.400	ng	0.00
13) Acenaphthene-d10	14.361	164	14639	0.400	ng	0.00
19) Phenanthrene-d10	17.107	188	32194	0.400	ng	0.00
29) Chrysene-d12	21.304	240	23233	0.400	ng	0.00
35) Perylene-d12	23.560	264	21271	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.312	112	19153	0.774	ng	0.00
5) Phenol-d6	6.887	99	24991	0.773	ng	0.00
8) Nitrobenzene-d5	8.875	82	16558	0.773	ng	0.00
11) 2-Methylnaphthalene-d10	12.106	152	31916	0.788	ng	0.00
14) 2,4,6-Tribromophenol	15.853	330	4048	0.759	ng	0.00
15) 2-Fluorobiphenyl	12.993	172	49120	0.777	ng	0.00
27) Fluoranthene-d10	19.146	212	63588	0.792	ng	0.00
31) Terphenyl-d14	19.754	244	41501	0.797	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.254	88	9688	0.749	ng	97
3) n-Nitrosodimethylamine	3.564	42	10002	0.803	ng	99
6) bis(2-Chloroethyl)ether	7.161	93	24500	0.791	ng	100
9) Naphthalene	10.562	128	62926	0.783	ng	99
10) Hexachlorobutadiene	10.851	225	11855	0.792	ng	# 98
12) 2-Methylnaphthalene	12.182	142	40570	0.790	ng	99
16) Acenaphthylene	14.083	152	58216	0.774	ng	100
17) Acenaphthene	14.426	154	39664	0.787	ng	100
18) Fluorene	15.420	166	53589	0.797	ng	99
20) 4,6-Dinitro-2-methylph...	15.484	198	2197	0.756	ng	# 73
21) 4-Bromophenyl-phenylether	16.312	248	16256	0.780	ng	97
22) Hexachlorobenzene	16.411	284	19818	0.788	ng	100
23) Atrazine	16.585	200	11649	0.776	ng	99
24) Pentachlorophenol	16.759	266	5399	0.730	ng	97
25) Phenanthrene	17.156	178	81082	0.787	ng	100
26) Anthracene	17.243	178	70988	0.782	ng	100
28) Fluoranthene	19.178	202	91886	0.789	ng	100
30) Pyrene	19.540	202	92136	0.793	ng	100
32) Benzo(a)anthracene	21.295	228	73175	0.778	ng	100
33) Chrysene	21.340	228	79534	0.797	ng	99
34) Bis(2-ethylhexyl)phtha...	21.250	149	29758	0.746	ng	99
36) Indeno(1,2,3-cd)pyrene	25.850	276	65260	0.758	ng	98
37) Benzo(b)fluoranthene	22.885	252	71527	0.766	ng	98
38) Benzo(k)fluoranthene	22.929	252	72339	0.778	ng	97
39) Benzo(a)pyrene	23.464	252	56697	0.786	ng	96
40) Dibenzo(a,h)anthracene	25.870	278	53658	0.776	ng	98
41) Benzo(g,h,i)perylene	26.543	276	58503	0.768	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032224\
Data File : BN030453.D
Acq On : 21 Mar 2024 19:03
Operator : MA/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Mar 21 23:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN032224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 21 23:54:14 2024
Response via : Initial Calibration




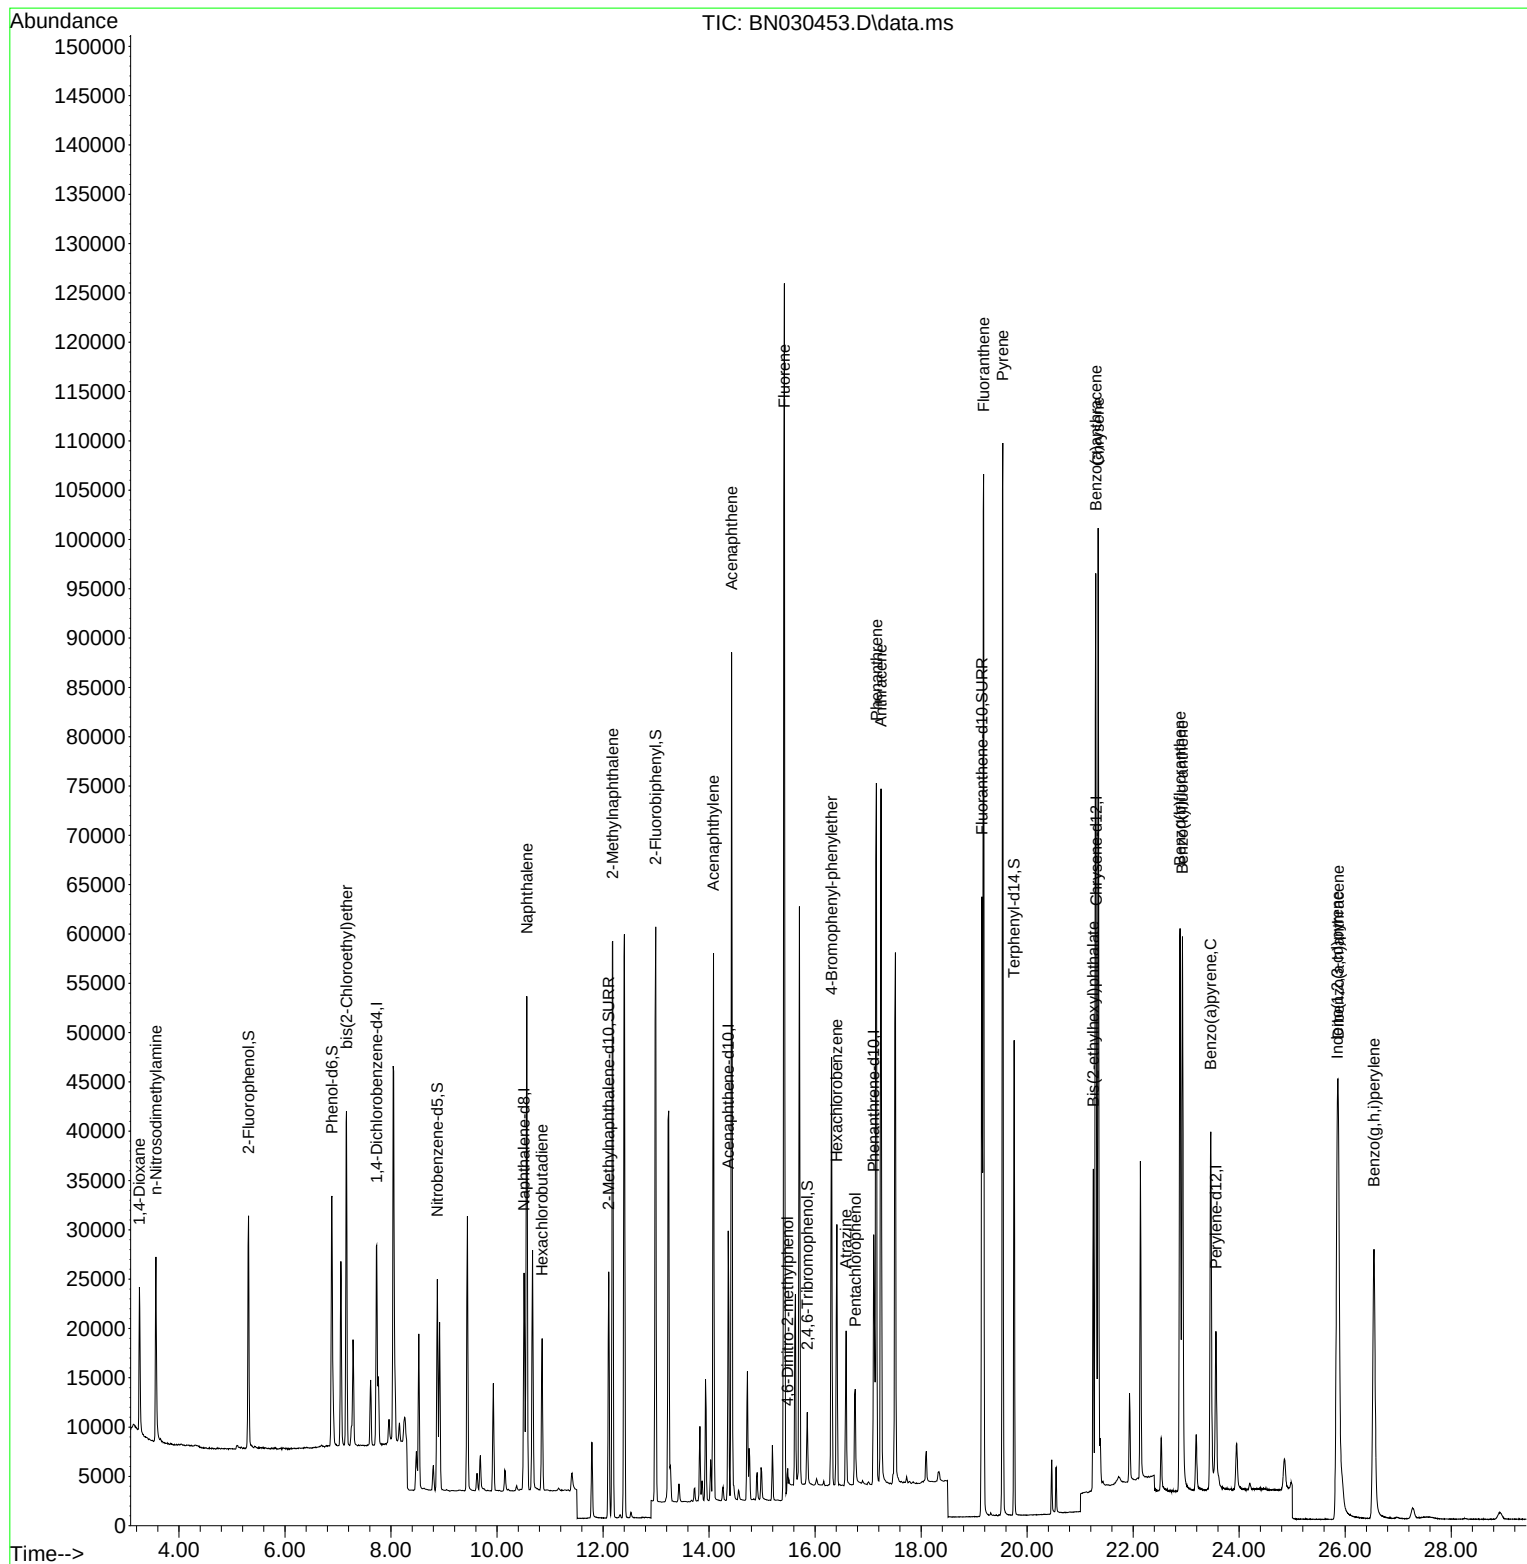




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.732 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:152 Resp: 10014
 Ion Ratio Lower Upper
 152 100
 150 154.7 122.2 183.4
 115 61.1 48.2 72.4

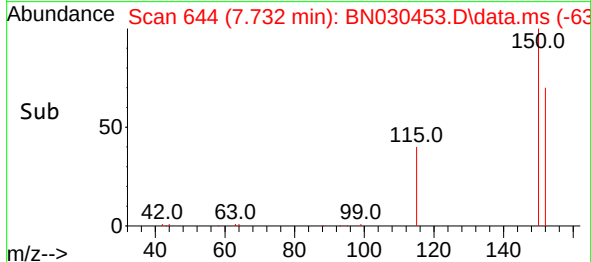

#2
 1,4-Dioxane
 Concen: 0.749 ng
 RT: 3.254 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03

Tgt Ion: 88 Resp: 9688
 Ion Ratio Lower Upper
 88 100
 43 27.6 21.8 32.6
 58 70.8 53.9 80.9




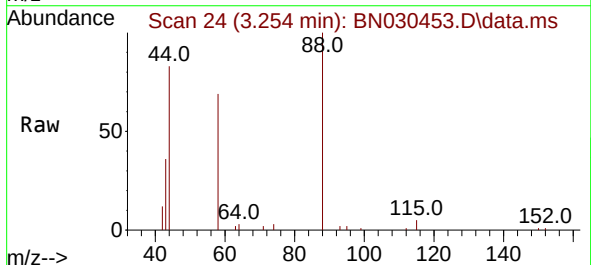


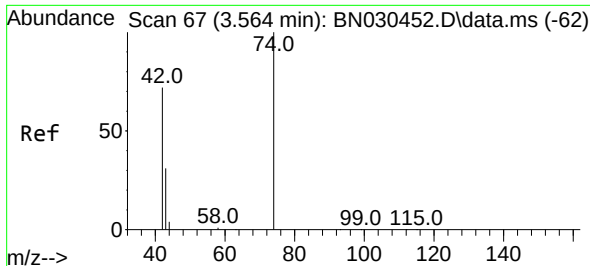

#3
 n-Nitrosodimethylamine
 Concen: 0.803 ng
 RT: 3.564 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion: 42 Resp: 10002
 Ion Ratio Lower Upper
 42 100
 74 140.0 112.6 169.0
 44 10.4 9.9 14.9

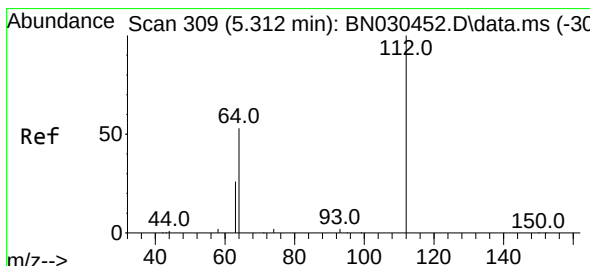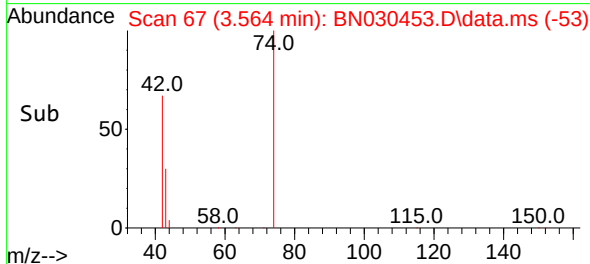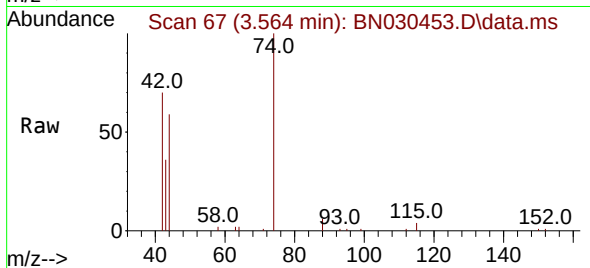

#4
 2-Fluorophenol
 Concen: 0.774 ng
 RT: 5.312 min Scan# 309
 Delta R.T. -0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03

Tgt Ion: 112 Resp: 19153
 Ion Ratio Lower Upper
 112 100
 64 55.1 44.2 66.2
 63 28.1 23.0 34.4


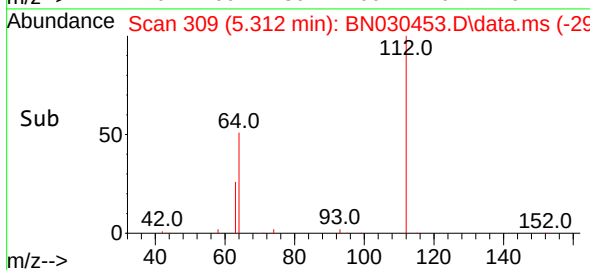

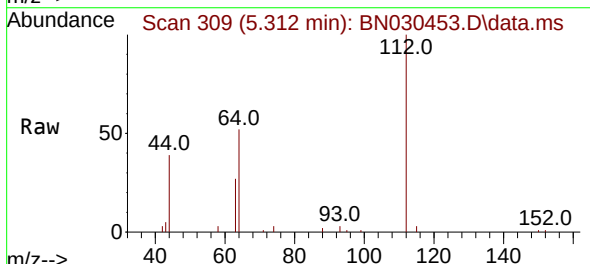




#5
Phenol-d6
Concen: 0.773 ng
RT: 6.887 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 99 Resp: 24991
Ion Ratio Lower Upper
99 100
42 17.7 13.9 20.9
71 31.7 25.4 38.0

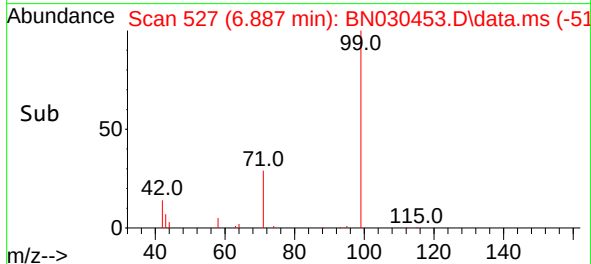

#6
bis(2-Chloroethyl)ether
Concen: 0.791 ng
RT: 7.161 min Scan# 565
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion: 93 Resp: 24500
Ion Ratio Lower Upper
93 100
63 73.6 58.6 87.8
95 32.6 26.3 39.5









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.509 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:136	Resp:	27805
Ion Ratio	Lower	Upper
136	100	
137	11.2	8.9 13.3
54	9.3	7.4 11.0
68	8.2	6.5 9.7

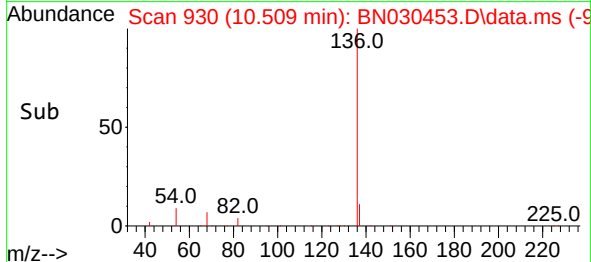

#8
Nitrobenzene-d5
Concen: 0.773 ng
RT: 8.875 min Scan# 777
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion: 82	Resp:	16558
Ion Ratio	Lower	Upper
82	100	
128	39.7	31.8 47.8
54	46.2	38.8 58.2




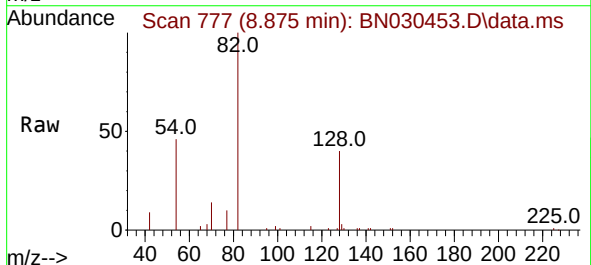




#9
Naphthalene
Concen: 0.783 ng
RT: 10.562 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:128 Resp: 62926
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 12.9 10.4 15.6

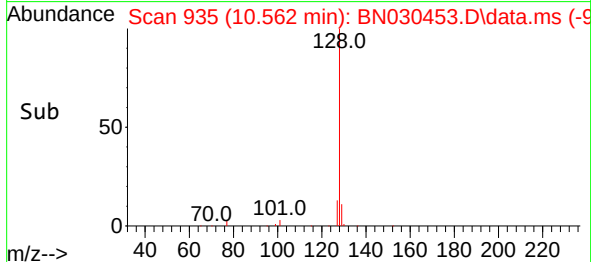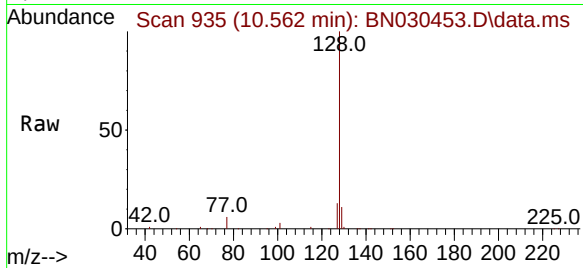

#10
Hexachlorobutadiene
Concen: 0.792 ng
RT: 10.851 min Scan# 962
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:225 Resp: 11855
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.6 51.8 77.8




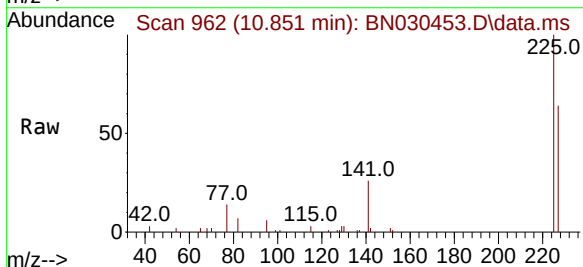




#11
2-Methylnaphthalene-d10
Concen: 0.788 ng
RT: 12.106 min Scan# 1181
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 31916
Ion Ratio Lower Upper
152 100
151 21.0 17.0 25.6

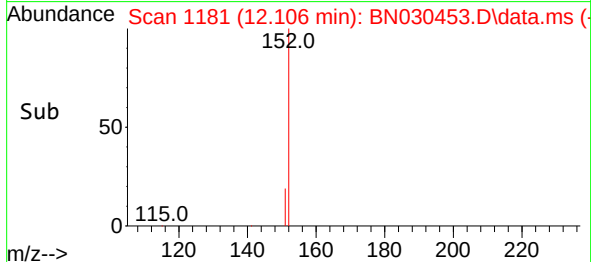

#12
2-Methylnaphthalene
Concen: 0.790 ng
RT: 12.182 min Scan# 1201
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:142 Resp: 40570
Ion Ratio Lower Upper
142 100
141 88.3 70.5 105.7
115 35.7 29.2 43.8




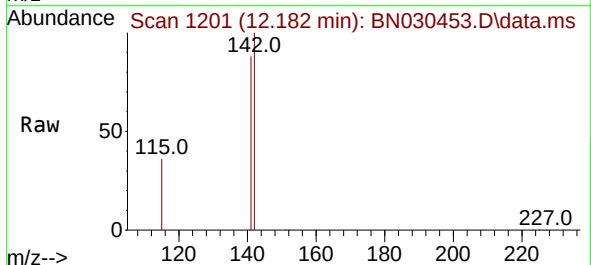




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.361 min Scan# 1529
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 14639
Ion Ratio Lower Upper
164 100
162 107.3 85.4 128.2
160 54.6 43.4 65.2

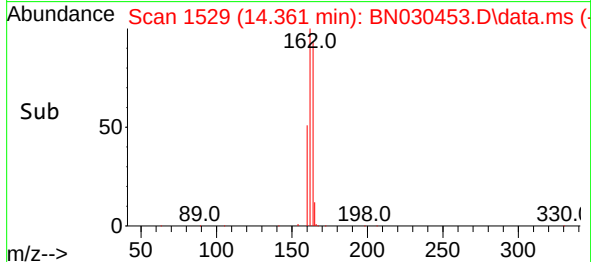

#14
2,4,6-Tribromophenol
Concen: 0.759 ng
RT: 15.853 min Scan# 1664
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:330 Resp: 4048
Ion Ratio Lower Upper
330 100
332 95.6 77.4 116.0
141 46.0 36.2 54.4


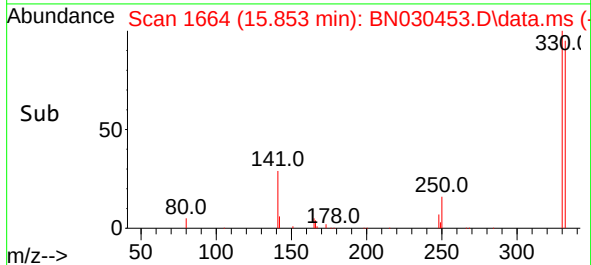




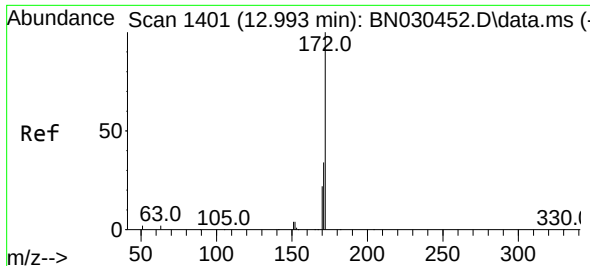

#15
2-Fluorobiphenyl
Concen: 0.777 ng
RT: 12.993 min Scan# 1401
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172 Resp: 49120
Ion Ratio Lower Upper
172 100
171 34.0 27.4 41.2
170 22.7 18.1 27.1

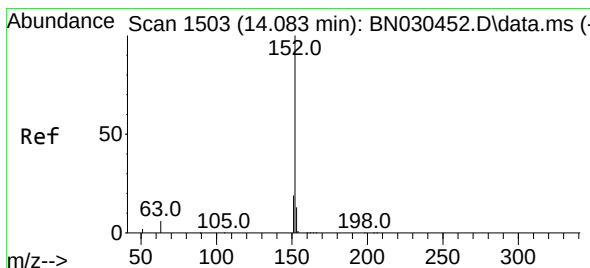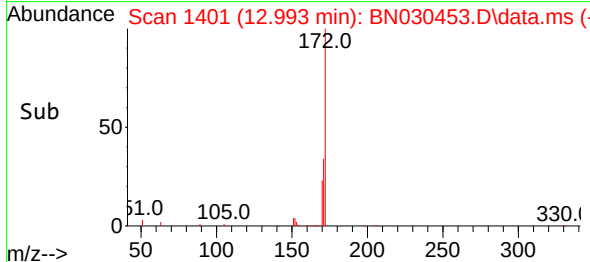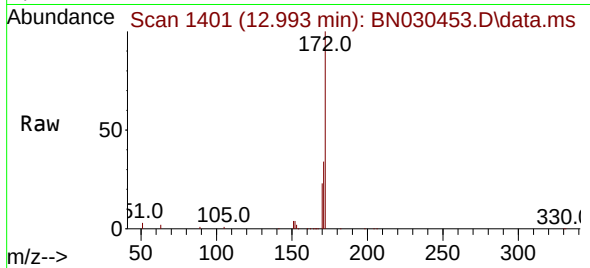

#16
Acenaphthylene
Concen: 0.774 ng
RT: 14.083 min Scan# 1503
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:152 Resp: 58216
Ion Ratio Lower Upper
152 100
151 19.5 15.5 23.3
153 13.0 10.3 15.5


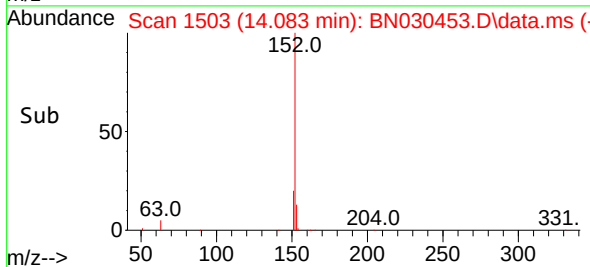

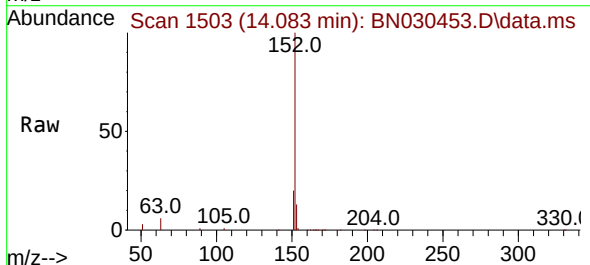


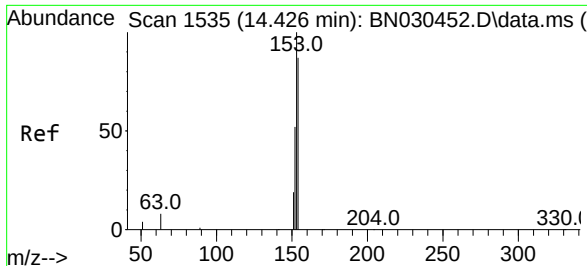

#17
Acenaphthene
Concen: 0.787 ng
RT: 14.426 min Scan# 1535
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:154 Resp: 39664
Ion Ratio Lower Upper
154 100
153 111.6 89.3 133.9
152 58.5 47.4 71.2

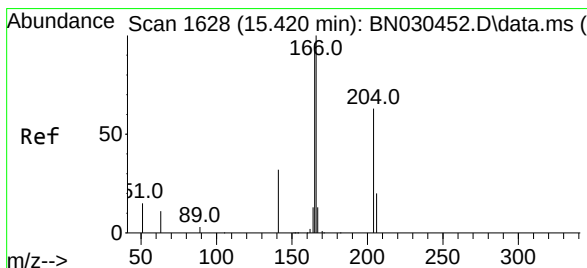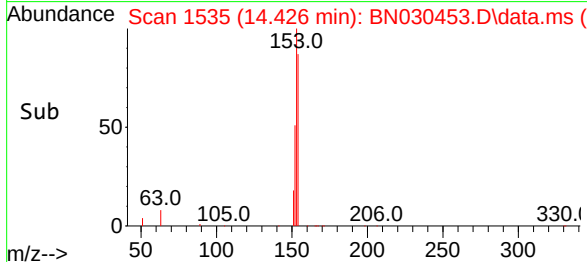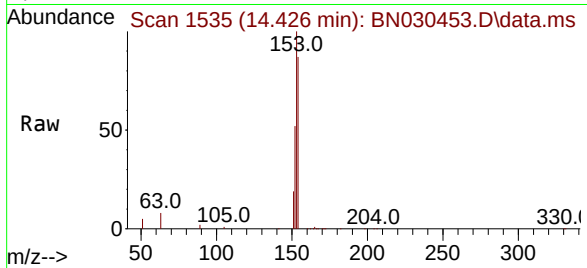

#18
Fluorene
Concen: 0.797 ng
RT: 15.420 min Scan# 1628
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:166 Resp: 53589
Ion Ratio Lower Upper
166 100
165 97.8 77.8 116.6
167 13.3 10.6 16.0


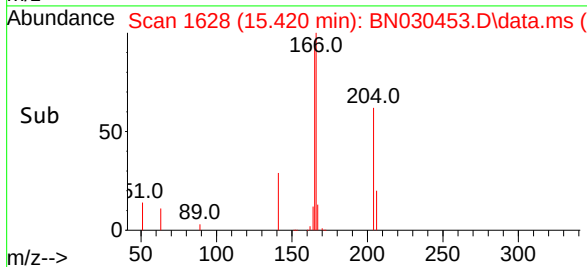

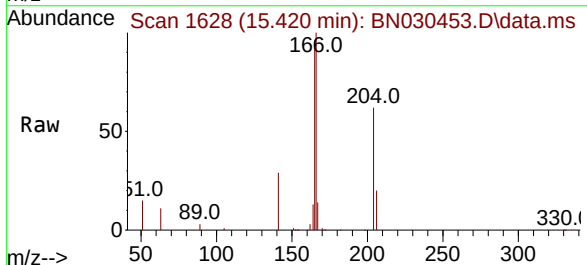


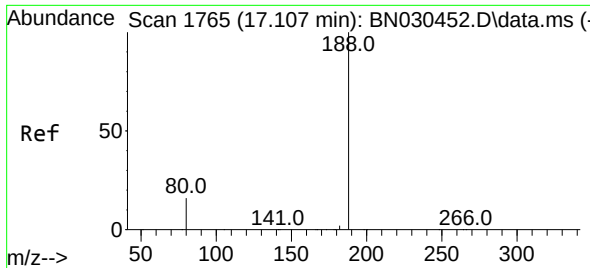

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.107 min Scan# 1765
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:188 Resp: 32194
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 16.3 13.6 20.4

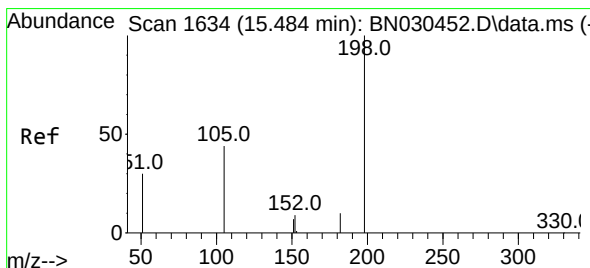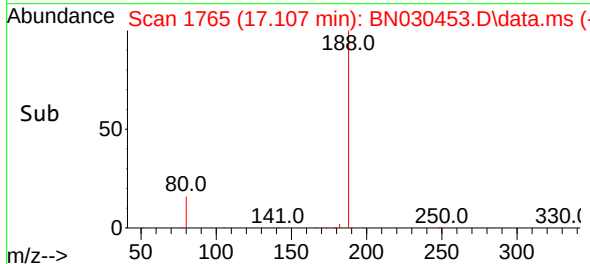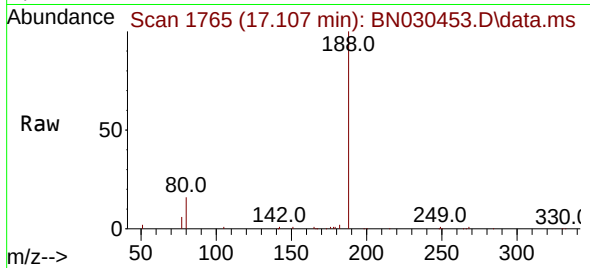

#20
4,6-Dinitro-2-methylphenol
Concen: 0.756 ng
RT: 15.484 min Scan# 1634
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:198 Resp: 2197
Ion Ratio Lower Upper
198 100
51 61.0 72.6 108.8#
105 57.7 60.3 90.5#


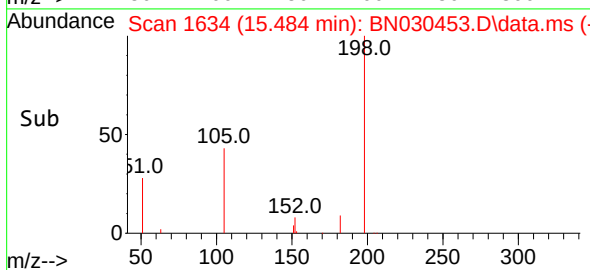

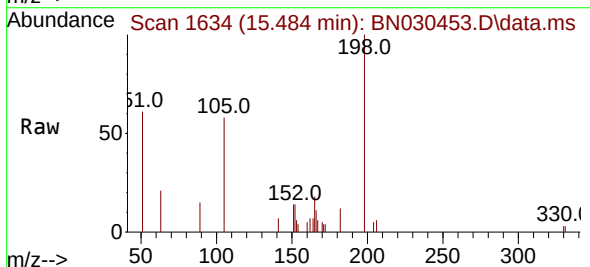


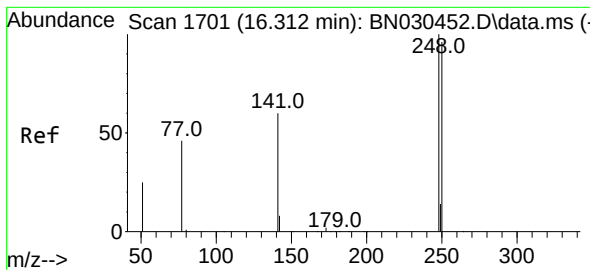

#21
4-Bromophenyl-phenylether
Concen: 0.780 ng
RT: 16.312 min Scan# 1701
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 16256
Ion Ratio Lower Upper
248 100
250 98.0 77.0 115.6
141 57.5 49.2 73.8

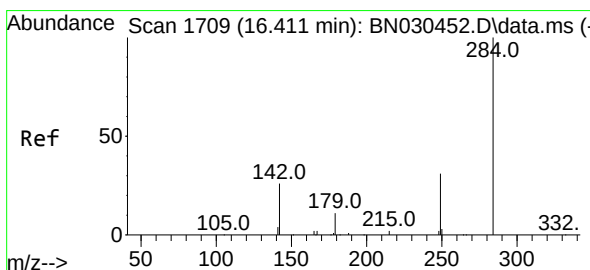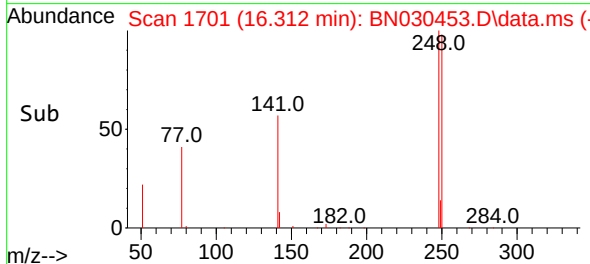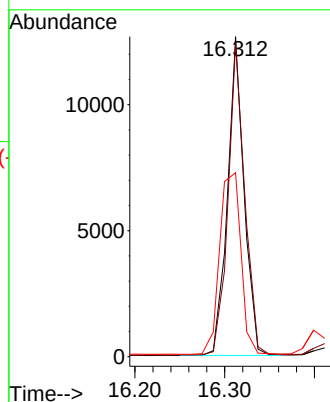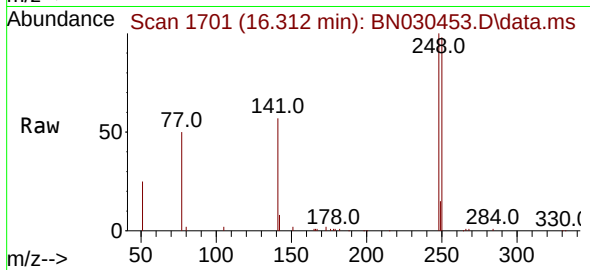

#22
Hexachlorobenzene
Concen: 0.788 ng
RT: 16.411 min Scan# 1709
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:284 Resp: 19818
Ion Ratio Lower Upper
284 100
142 39.9 31.8 47.8
249 31.3 25.2 37.8


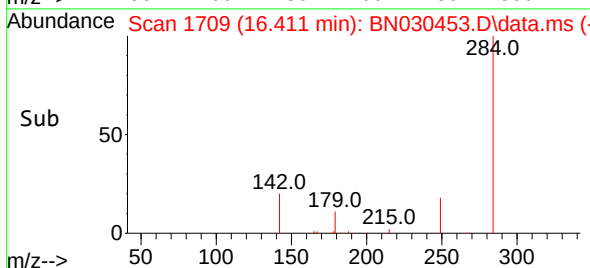

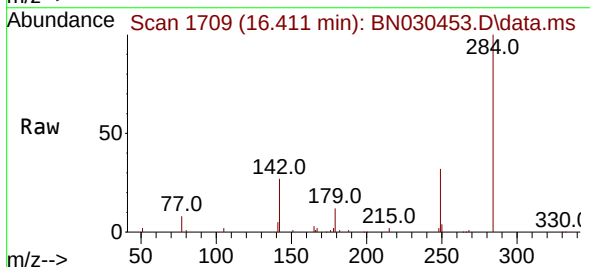




#23
 Atrazine
 Concen: 0.776 ng
 RT: 16.585 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:200 Resp: 11649
 Ion Ratio Lower Upper
 200 100
 173 25.1 20.6 31.0
 215 45.9 37.1 55.7

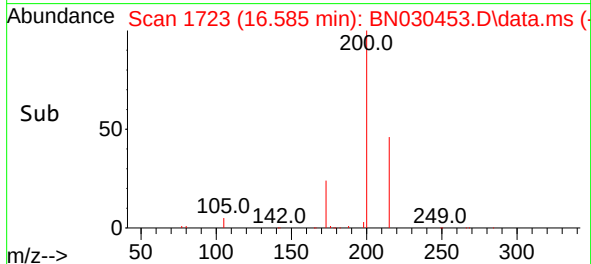

#24
 Pentachlorophenol
 Concen: 0.730 ng
 RT: 16.759 min Scan# 1737
 Delta R.T. -0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03

Tgt Ion:266 Resp: 5399
 Ion Ratio Lower Upper
 266 100
 264 62.9 49.8 74.6
 268 65.1 49.3 73.9


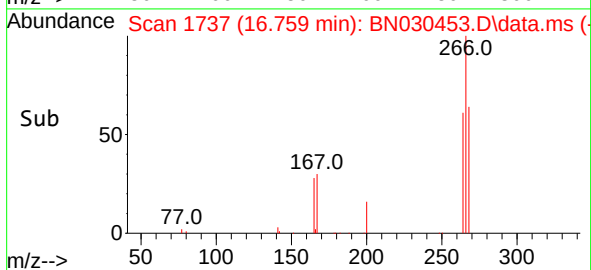




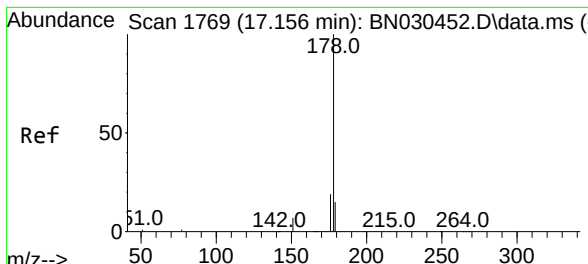

#25
 Phenanthrene
 Concen: 0.787 ng
 RT: 17.156 min Scan# 1769
 Delta R.T. 0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:	178	Resp:	81082
Ion Ratio	Lower	Upper	
178	100		
176	19.3	15.4	23.2
179	15.2	12.3	18.5

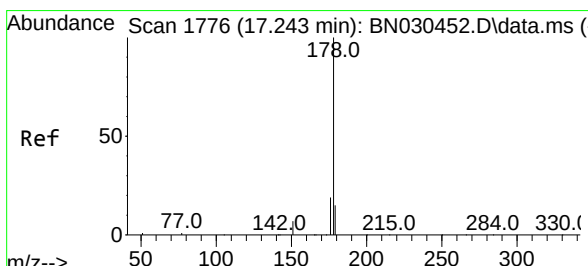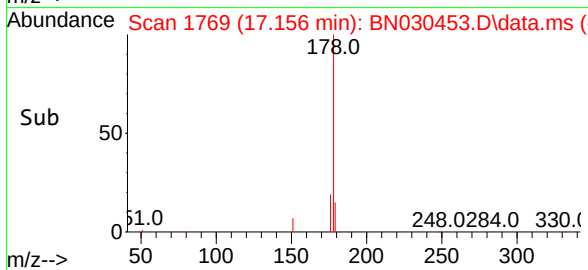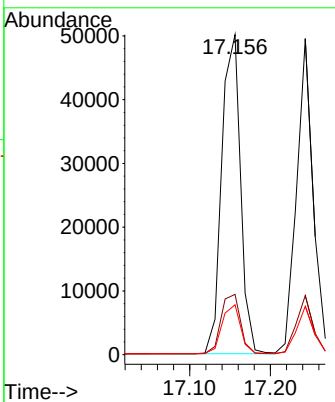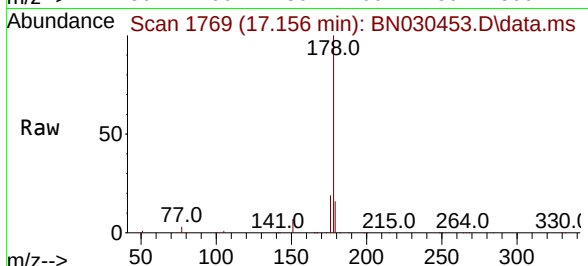

#26
 Anthracene
 Concen: 0.782 ng
 RT: 17.243 min Scan# 1776
 Delta R.T. -0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03

Tgt Ion:	178	Resp:	70988
Ion Ratio	Lower	Upper	
178	100		
176	18.7	15.0	22.4
179	15.1	12.2	18.2


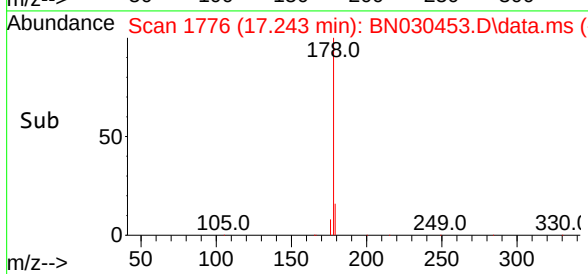
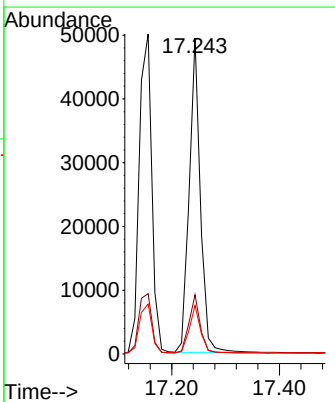
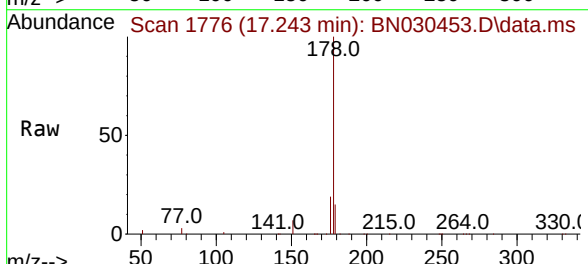


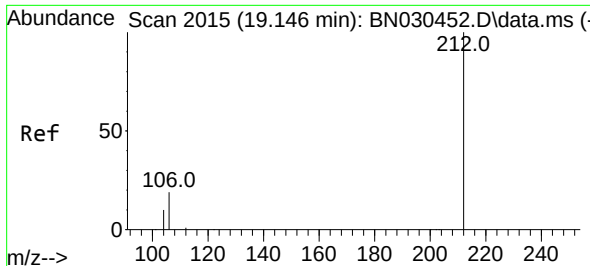

#27
Fluoranthene-d10
Concen: 0.792 ng
RT: 19.146 min Scan# 2015
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 63588
Ion Ratio Lower Upper
212 100
106 18.5 14.7 22.1
104 10.4 8.3 12.5

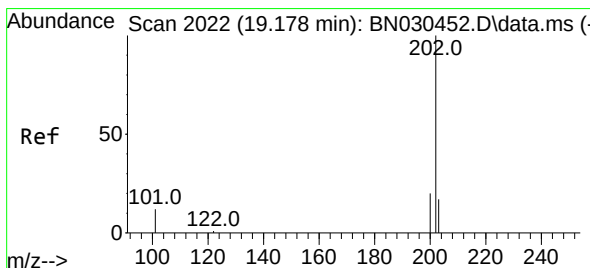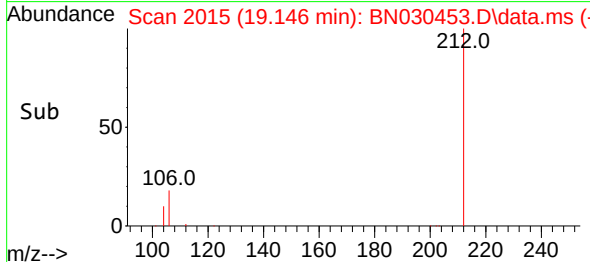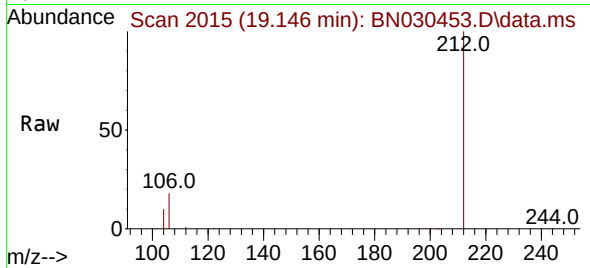

#28
Fluoranthene
Concen: 0.789 ng
RT: 19.178 min Scan# 2022
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:202 Resp: 91886
Ion Ratio Lower Upper
202 100
101 13.4 10.7 16.1
203 17.3 13.6 20.4

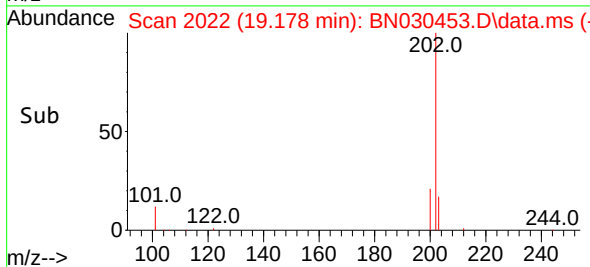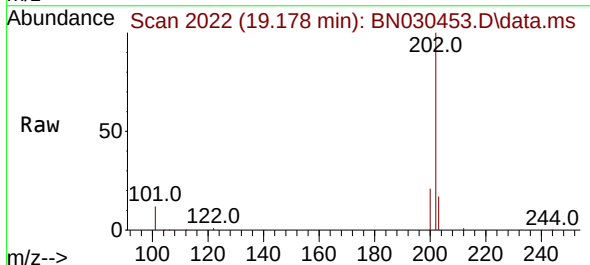

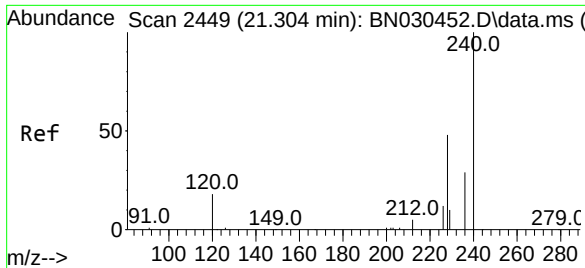

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.304 min Scan# 2449

Delta R.T. -0.000 min

Lab File: BN030453.D

Acq: 21 Mar 2024 19:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:240 Resp: 23233

Ion Ratio Lower Upper

240 100

120 18.2 15.9 23.9

236 29.7 23.8 35.6

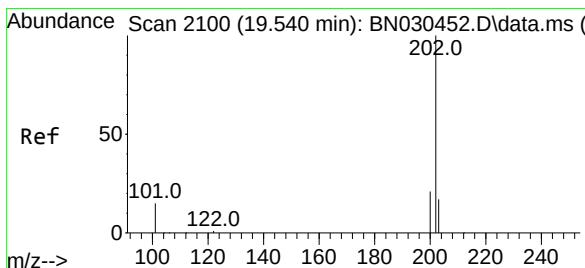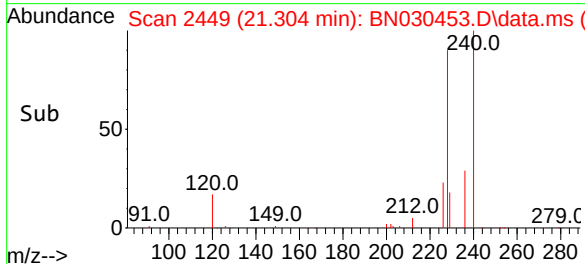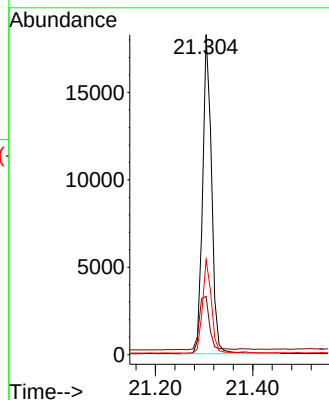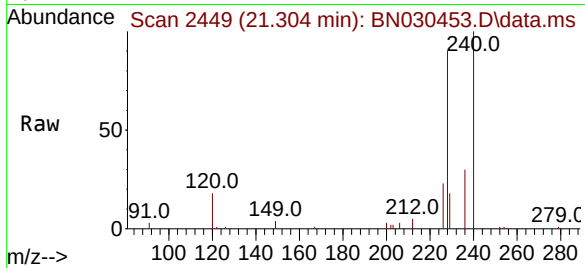

#30

Pyrene

Concen: 0.793 ng

RT: 19.540 min Scan# 2100

Delta R.T. -0.000 min

Lab File: BN030453.D

Acq: 21 Mar 2024 19:03




Tgt Ion:202 Resp: 92136


Ion Ratio Lower Upper

202 100

200 21.0 16.7 25.1

203 17.7 14.1 21.1


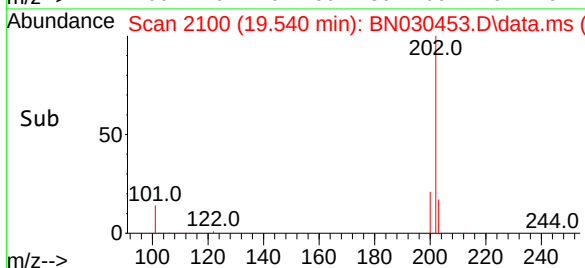
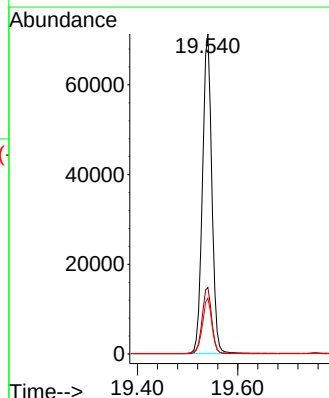
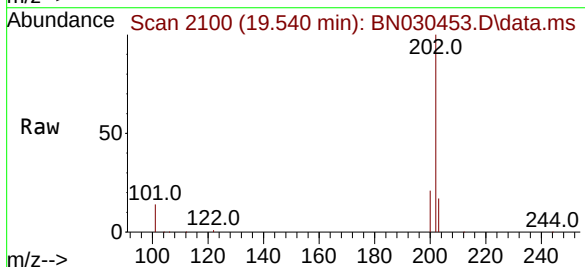




#31
 Terphenyl-d14
 Concen: 0.797 ng
 RT: 19.754 min Scan# 2146
 Delta R.T. -0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244 Resp: 41501
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.8 11.6
 122 22.1 17.1 25.7

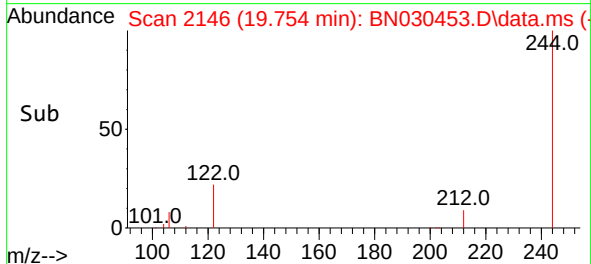

#32
 Benzo(a)anthracene
 Concen: 0.778 ng
 RT: 21.295 min Scan# 2448
 Delta R.T. 0.000 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03

Tgt Ion:228 Resp: 73175
 Ion Ratio Lower Upper
 228 100
 226 26.9 21.5 32.3
 229 19.7 15.8 23.6


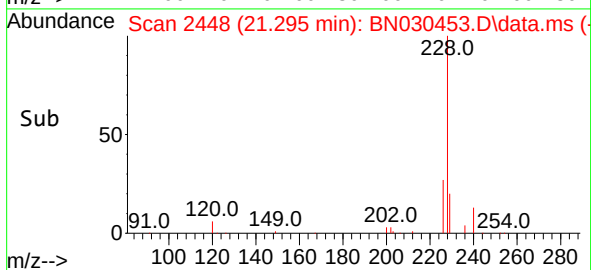

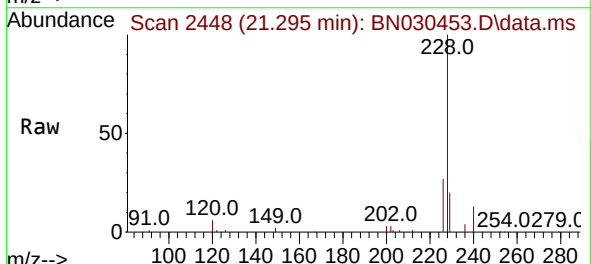


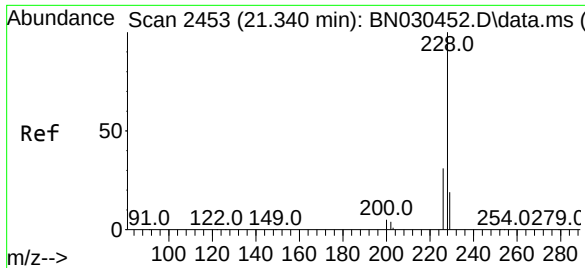

#33
Chrysene
Concen: 0.797 ng
RT: 21.340 min Scan# 2453
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:228	Resp:	79534
Ion Ratio	Lower	Upper
228	100	
226	31.2	24.6 37.0
229	19.5	15.2 22.8

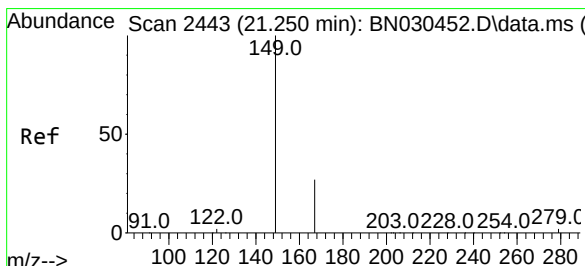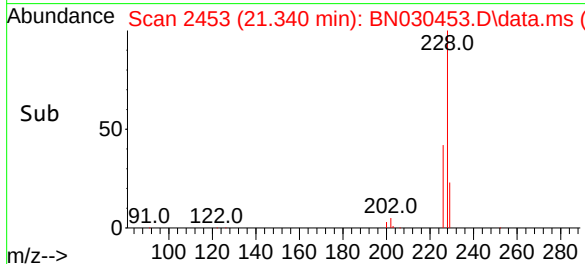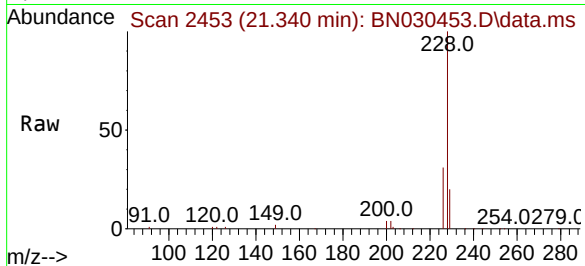

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.746 ng
RT: 21.250 min Scan# 2443
Delta R.T. 0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:149	Resp:	29758
Ion Ratio	Lower	Upper
149	100	
167	25.9	21.2 31.8
279	2.3	1.8 2.8

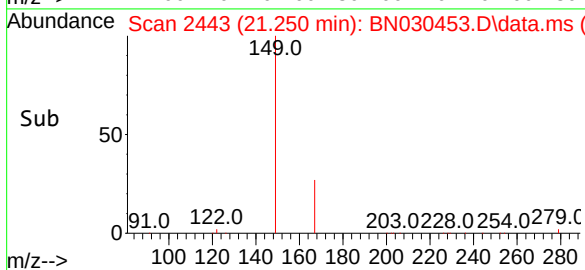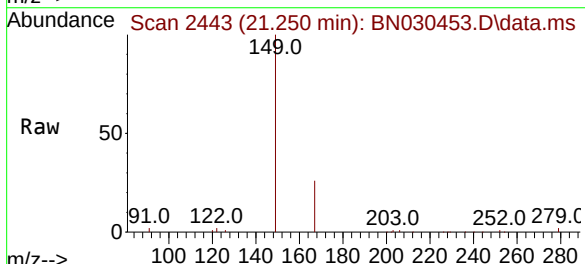



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.560 min Scan# 2967

Delta R.T. -0.000 min

Lab File: BN030453.D

Acq: 21 Mar 2024 19:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:264 Resp: 21271

Ion Ratio Lower Upper

264 100

260 27.0 21.9 32.9

265 41.6 32.6 48.8



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.758 ng

RT: 25.850 min Scan# 3750

Delta R.T. -0.003 min

Lab File: BN030453.D

Acq: 21 Mar 2024 19:03




Tgt Ion:276 Resp: 65260


Ion Ratio Lower Upper

276 100

138 32.1 24.8 37.2

277 25.2 19.1 28.7


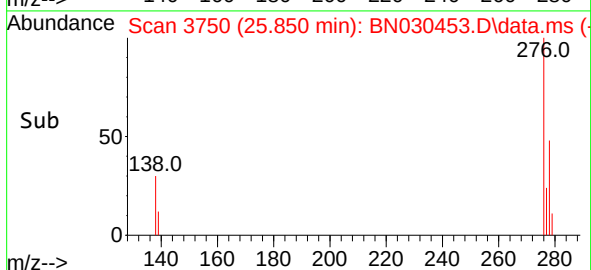






#37
Benzo(b)fluoranthene
Concen: 0.766 ng
RT: 22.885 min Scan# 2736
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 71527
Ion Ratio Lower Upper
252 100
253 21.9 18.2 27.2
125 13.5 12.0 18.0

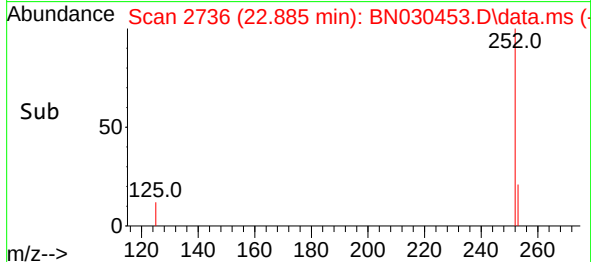

#38
Benzo(k)fluoranthene
Concen: 0.778 ng
RT: 22.929 min Scan# 2751
Delta R.T. -0.003 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:252 Resp: 72339
Ion Ratio Lower Upper
252 100
253 22.0 18.7 28.1
125 14.2 12.6 19.0




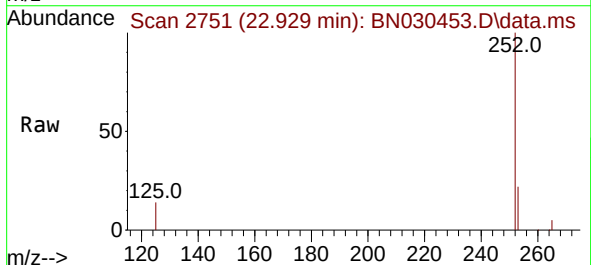




#39
Benzo(a)pyrene
Concen: 0.786 ng
RT: 23.464 min Scan# 2934
Delta R.T. -0.000 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 56697
Ion Ratio Lower Upper
252 100
253 22.5 19.4 29.0
125 15.7 14.6 22.0

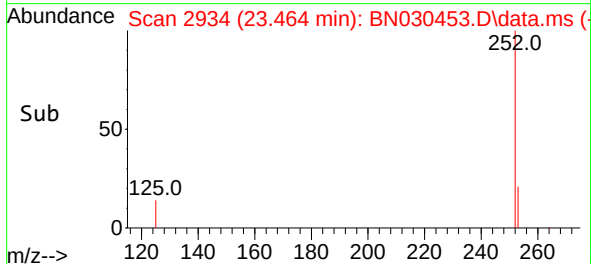

#40
Dibenzo(a,h)anthracene
Concen: 0.776 ng
RT: 25.870 min Scan# 3757
Delta R.T. -0.009 min
Lab File: BN030453.D
Acq: 21 Mar 2024 19:03

Tgt Ion:278 Resp: 53658
Ion Ratio Lower Upper
278 100
139 22.1 18.2 27.2
279 24.1 20.2 30.2

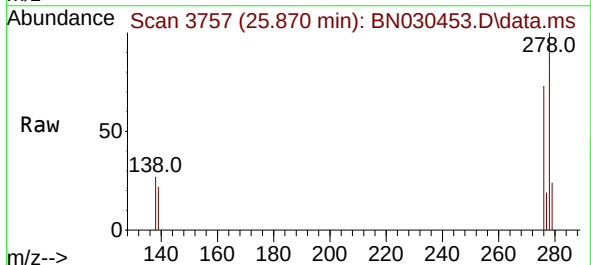

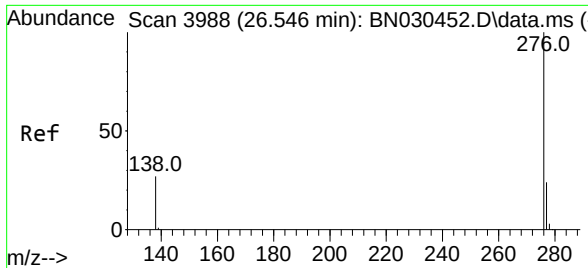

#41
 Benzo(g,h,i)perylene
 Concen: 0.768 ng
 RT: 26.543 min Scan# 3987
 Delta R.T. -0.003 min
 Lab File: BN030453.D
 Acq: 21 Mar 2024 19:03

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:	276	Resp:	58503
Ion	Ratio	Lower	Upper
276	100		
277	24.3	20.0	30.0
138	28.0	22.8	34.2

