
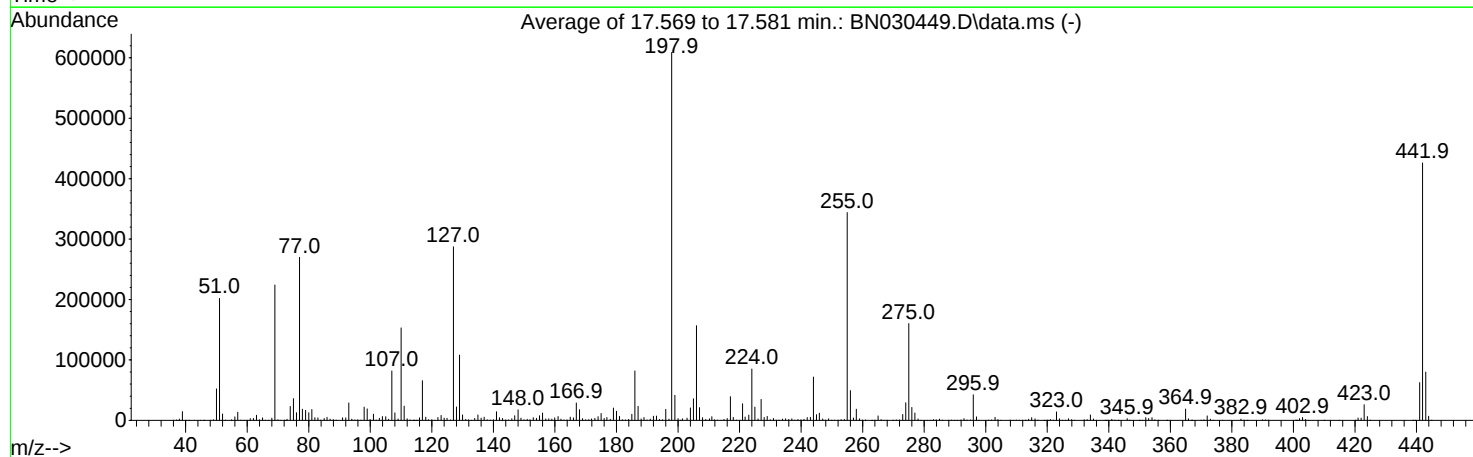


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032224\
Data File : BN030449.D
Acq On : 21 Mar 2024 16:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN032224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 22 00:01:57 2024

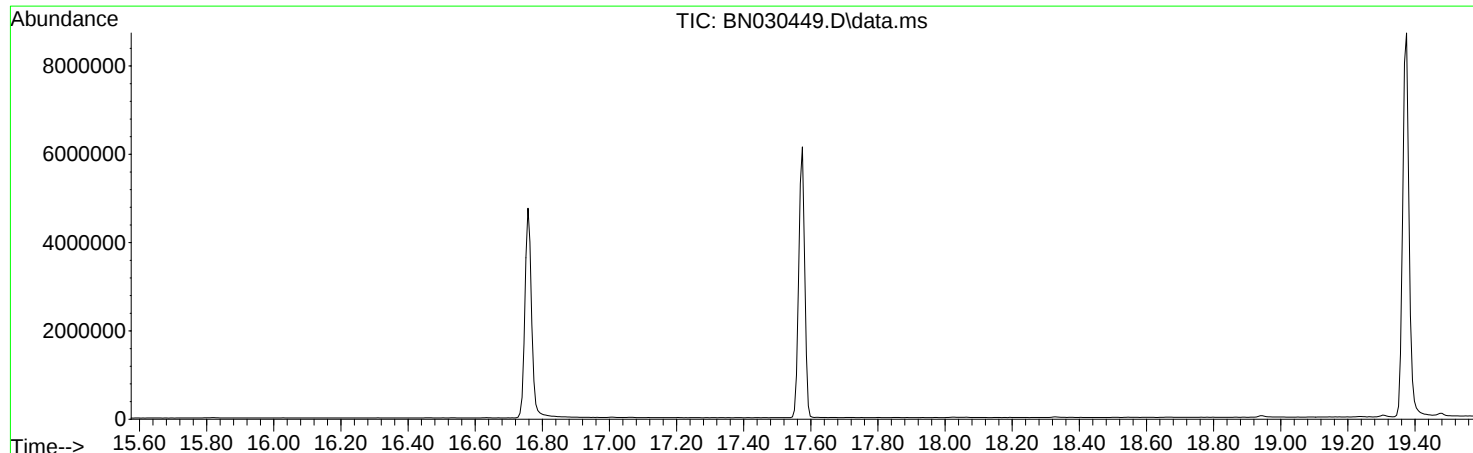




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	201941	PASS
68	69	0.00	2	1.6	3641	PASS
69	198	0.00	100	36.8	224050	PASS
70	69	0.00	2	0.5	1142	PASS
127	198	10	80	47.2	287403	PASS
197	198	0.00	2	0.4	2221	PASS
198	198	100	100	100.0	608853	PASS
199	198	5	9	6.8	41597	PASS
275	198	10	60	26.3	160235	PASS
365	198	1	100	3.1	18933	PASS
441	198	0.01	100	10.3	62589	PASS
442	442	50	100	100.0	426219	PASS
443	442	15	24	18.8	79944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032224\
Data File : BN030449.D
Acq On : 21 Mar 2024 16:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 22 02:28:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 22 02:28:35 2024
Response via : Initial Calibration

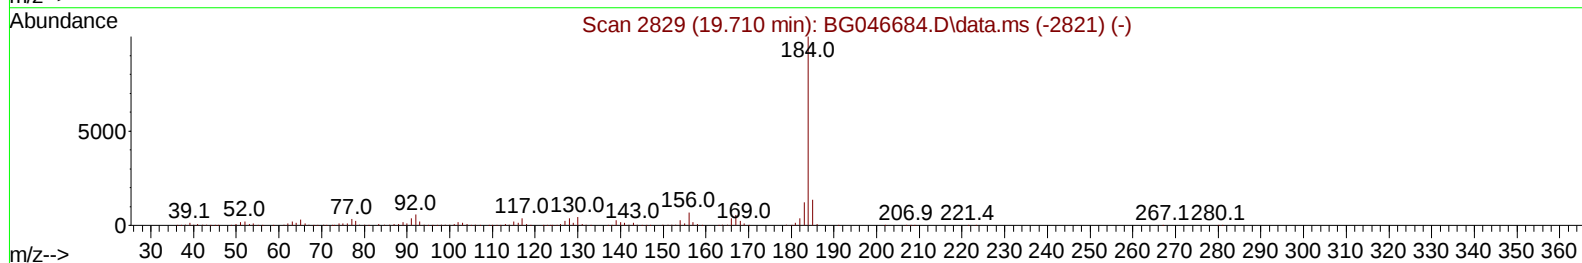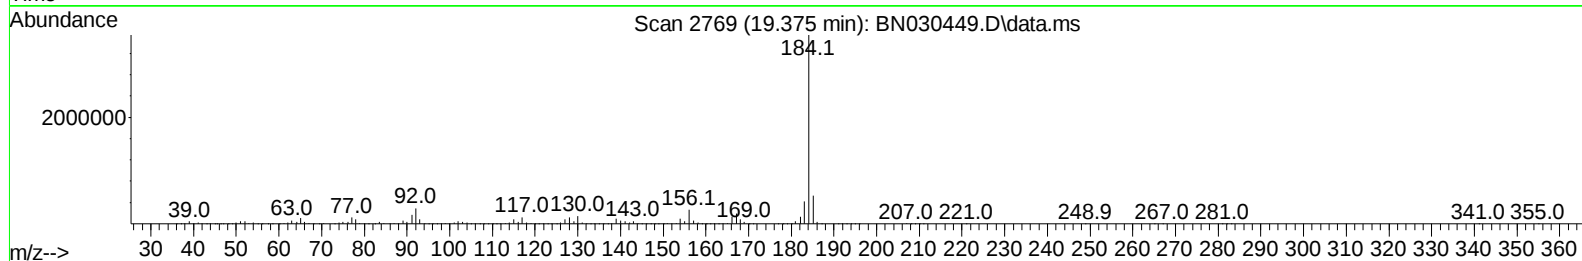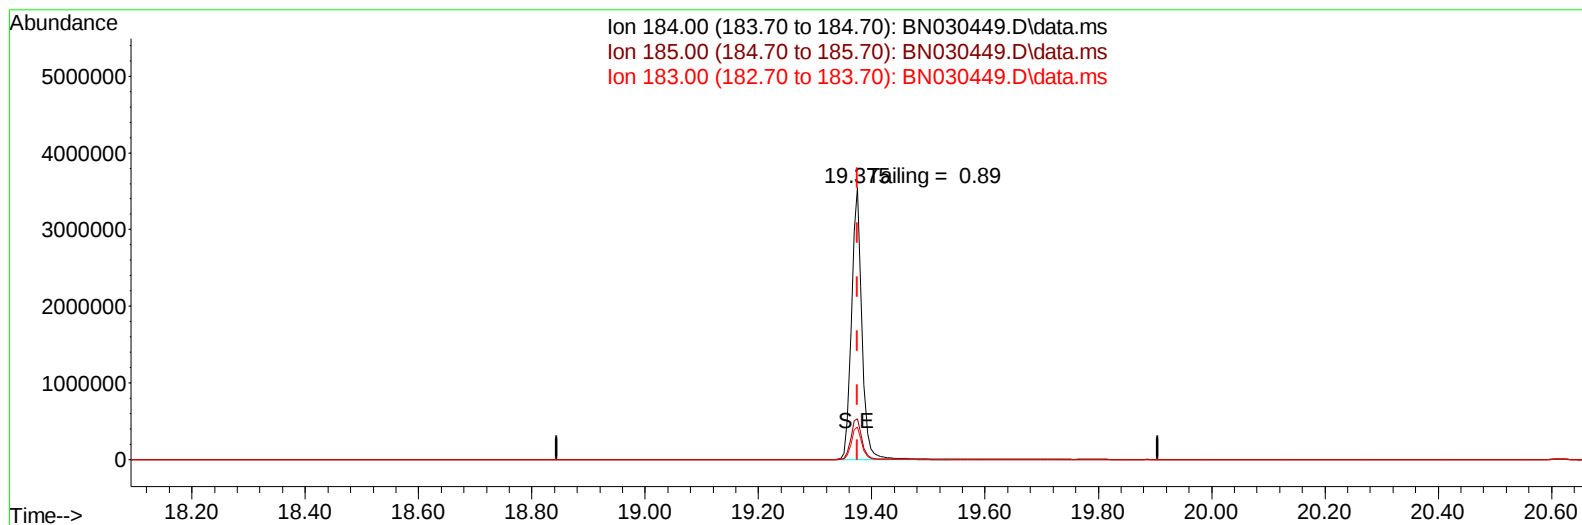

TIC: BN030449.D\data.ms

(77) Benzidine

19.375min (0.000) 0.00 ng

response 4549837

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.05
183.00	13.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2024	BNA_N	<u>BN030449.D</u>
Compound Name	Response	Retention Time
DDT	1850862	20.616
DDD	52484	20.169
DDE	1467	19.663
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53951	1904813	2.83

Instrument :
BNA_N
ClientSampleId :
DFTPP