

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032318\
 Data File : BN000577.D
 Acq On : 23 Mar 2018 14:46
 Operator : JU/SJ
 Sample : J1905-07DL3 500X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 23 17:46:08 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 23 17:43:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	172425	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	730585	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.03	164	413582	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.75	188	915023	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	818690	20.00	ng/ul	0.00
83) Perylene-d12	24.37	264	660761	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.41	99	710	0.04	ng/ul	-0.14
7) Bis-(2-Chloroethyl)ether-d	7.72	67	972	0.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.93	132	356	0.03	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	861	0.07	ng/ul	-0.07
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	10.35	143	444	0.07	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	11.35	131	1500	0.13	ng/ul	-0.04
43) Dimethylphthalate-d6	14.42	166	2365	0.07	ng/ul	0.00
46) Acenaphthylene-d8	14.72	160	2802	0.07	ng/ul	0.00
51) 4-Nitrophenol-d4	15.22	143	131	0.02	ng/ul	0.00
57) Fluorene-d10	16.01	176	4639	0.17	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.15	200	413	0.08	ng/ul	0.02
70) Anthracene-d10	17.85	188	5239	0.12	ng/ul	0.00
76) Pyrene-d10	20.11	212	3212	0.07	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.21	264	1275	0.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
55) 2,3,4,6-Tetrachlorophenol	15.65	232	67770	10.099	ng/ul#	90
68) Pentachlorophenol	17.41	266	628667	120.918	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032318\
Data File : BN000577.D
Acq On : 23 Mar 2018 14:46
Operator : JU/SJ
Sample : J1905-07DL3 500X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 23 17:46:08 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 23 17:43:46 2018
Response via : Initial Calibration

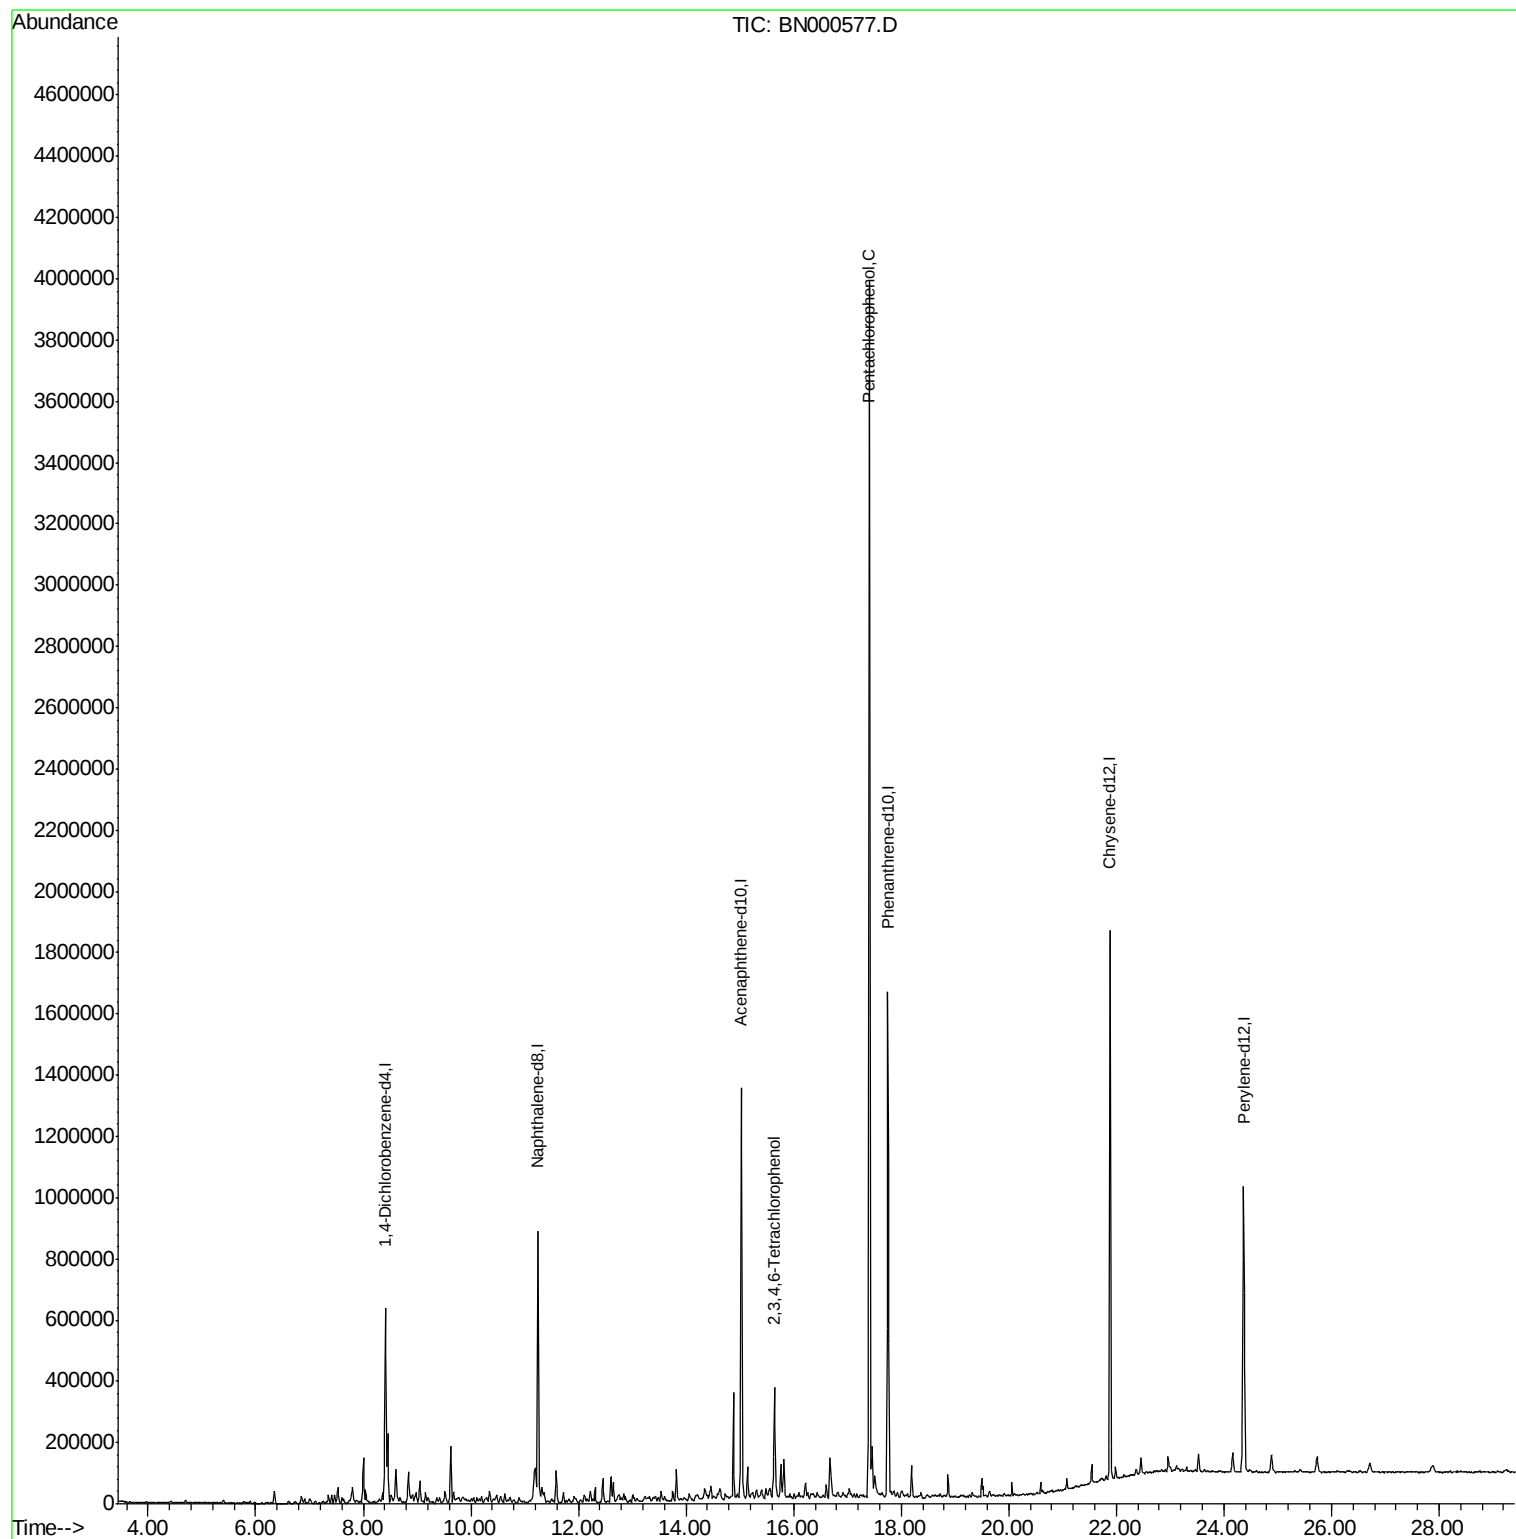


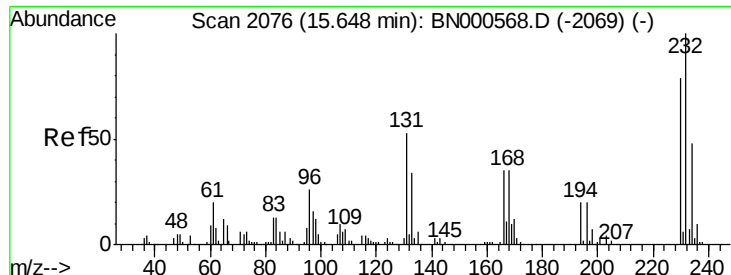




#55
 2,3,4,6-Tetrachlorophenol
 Concen: 10.099 ng/ul
 RT: 15.65 min Scan# 2076
 Delta R.T. 0.00 min
 Lab File: BN000577.D
 Acq: 23 Mar 2018 14:46

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:232 Resp: 67770
 Ion Ratio Lower Upper
 232 100
 131 51.1 48.0 72.0
 130 2.9 4.0 6.0#
 166 34.6 32.0 48.0

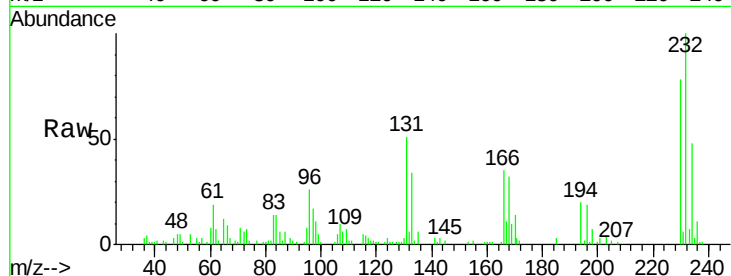


Abundance Ion 232.00 (231.70 to 232.70): E
 Ion 131.00 (130.70 to 131.70): E
 Ion 130.00 (129.70 to 130.70): E
 Ion 166.00 (165.70 to 166.70): E

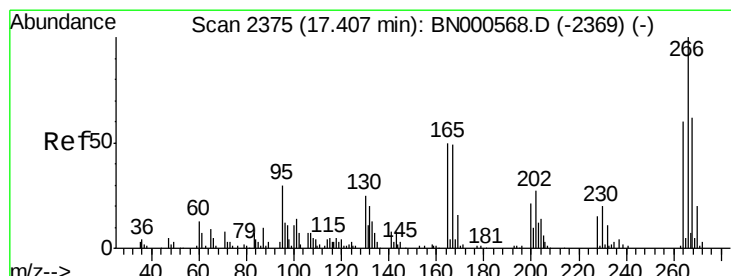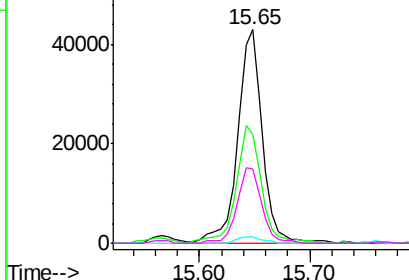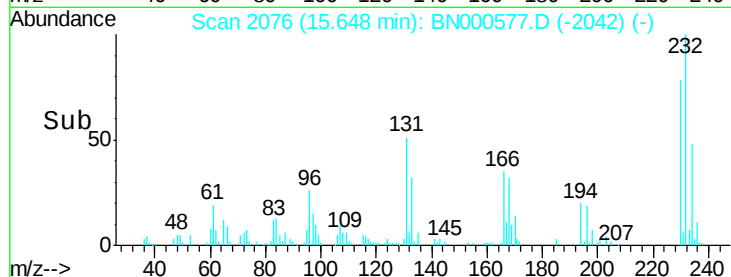

#68
 Pentachlorophenol
 Concen: 120.918 ng/ul
 RT: 17.41 min Scan# 2375
 Delta R.T. 0.00 min
 Lab File: BN000577.D
 Acq: 23 Mar 2018 14:46

Tgt Ion:266 Resp: 628667
 Ion Ratio Lower Upper
 266 100
 264 64.5 48.2 72.4
 268 63.5 52.3 78.5

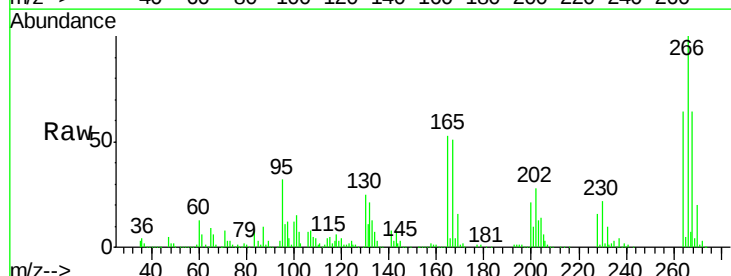

Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

