

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032318\
 Data File : BN000593.D
 Acq On : 23 Mar 2018 23:59
 Operator : JU/SJ
 Sample : J1955-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C1011

Quant Time: Mar 24 01:29:08 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 23 23:09:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	202159	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	868686	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.03	164	475849	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.75	188	1000122	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	817052	20.00	ng/ul	-0.01
83) Perylene-d12	24.35	264	645306	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.59	96	32058	5.66	ng/uL	0.00
5) Phenol-d5	7.55	99	568211	30.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.71	67	348205	32.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.93	132	424970	29.80	ng/ul	0.00
13) 4-Methylphenol-d8	9.12	113	456814	31.09	ng/ul	0.00
19) Nitrobenzene-d5	9.59	128	211129	29.92	ng/ul	0.00
22) 2-Nitrophenol-d4	10.32	143	222109	30.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.86	165	379758	28.99	ng/ul	0.00
29) 4-Chloroaniline-d4	11.38	131	548500	40.79	ng/ul	0.00
43) Dimethylphthalate-d6	14.42	166	1235550	32.87	ng/ul	0.00
46) Acenaphthylene-d8	14.73	160	1572296	31.70	ng/ul	0.00
51) 4-Nitrophenol-d4	15.21	143	168527	24.14	ng/ul	0.00
57) Fluorene-d10	16.01	176	1027017	32.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.12	200	117419	20.50	ng/ul	0.00
70) Anthracene-d10	17.85	188	1520570	31.63	ng/ul	0.00
76) Pyrene-d10	20.11	212	1525459	33.82	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.20	264	1001386	32.88	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.46	163	244940	6.587	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032318\
Data File : BN000593.D
Acq On : 23 Mar 2018 23:59
Operator : JU/SJ
Sample : J1955-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C1011

Quant Time: Mar 24 01:29:08 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 23 23:09:09 2018
Response via : Initial Calibration

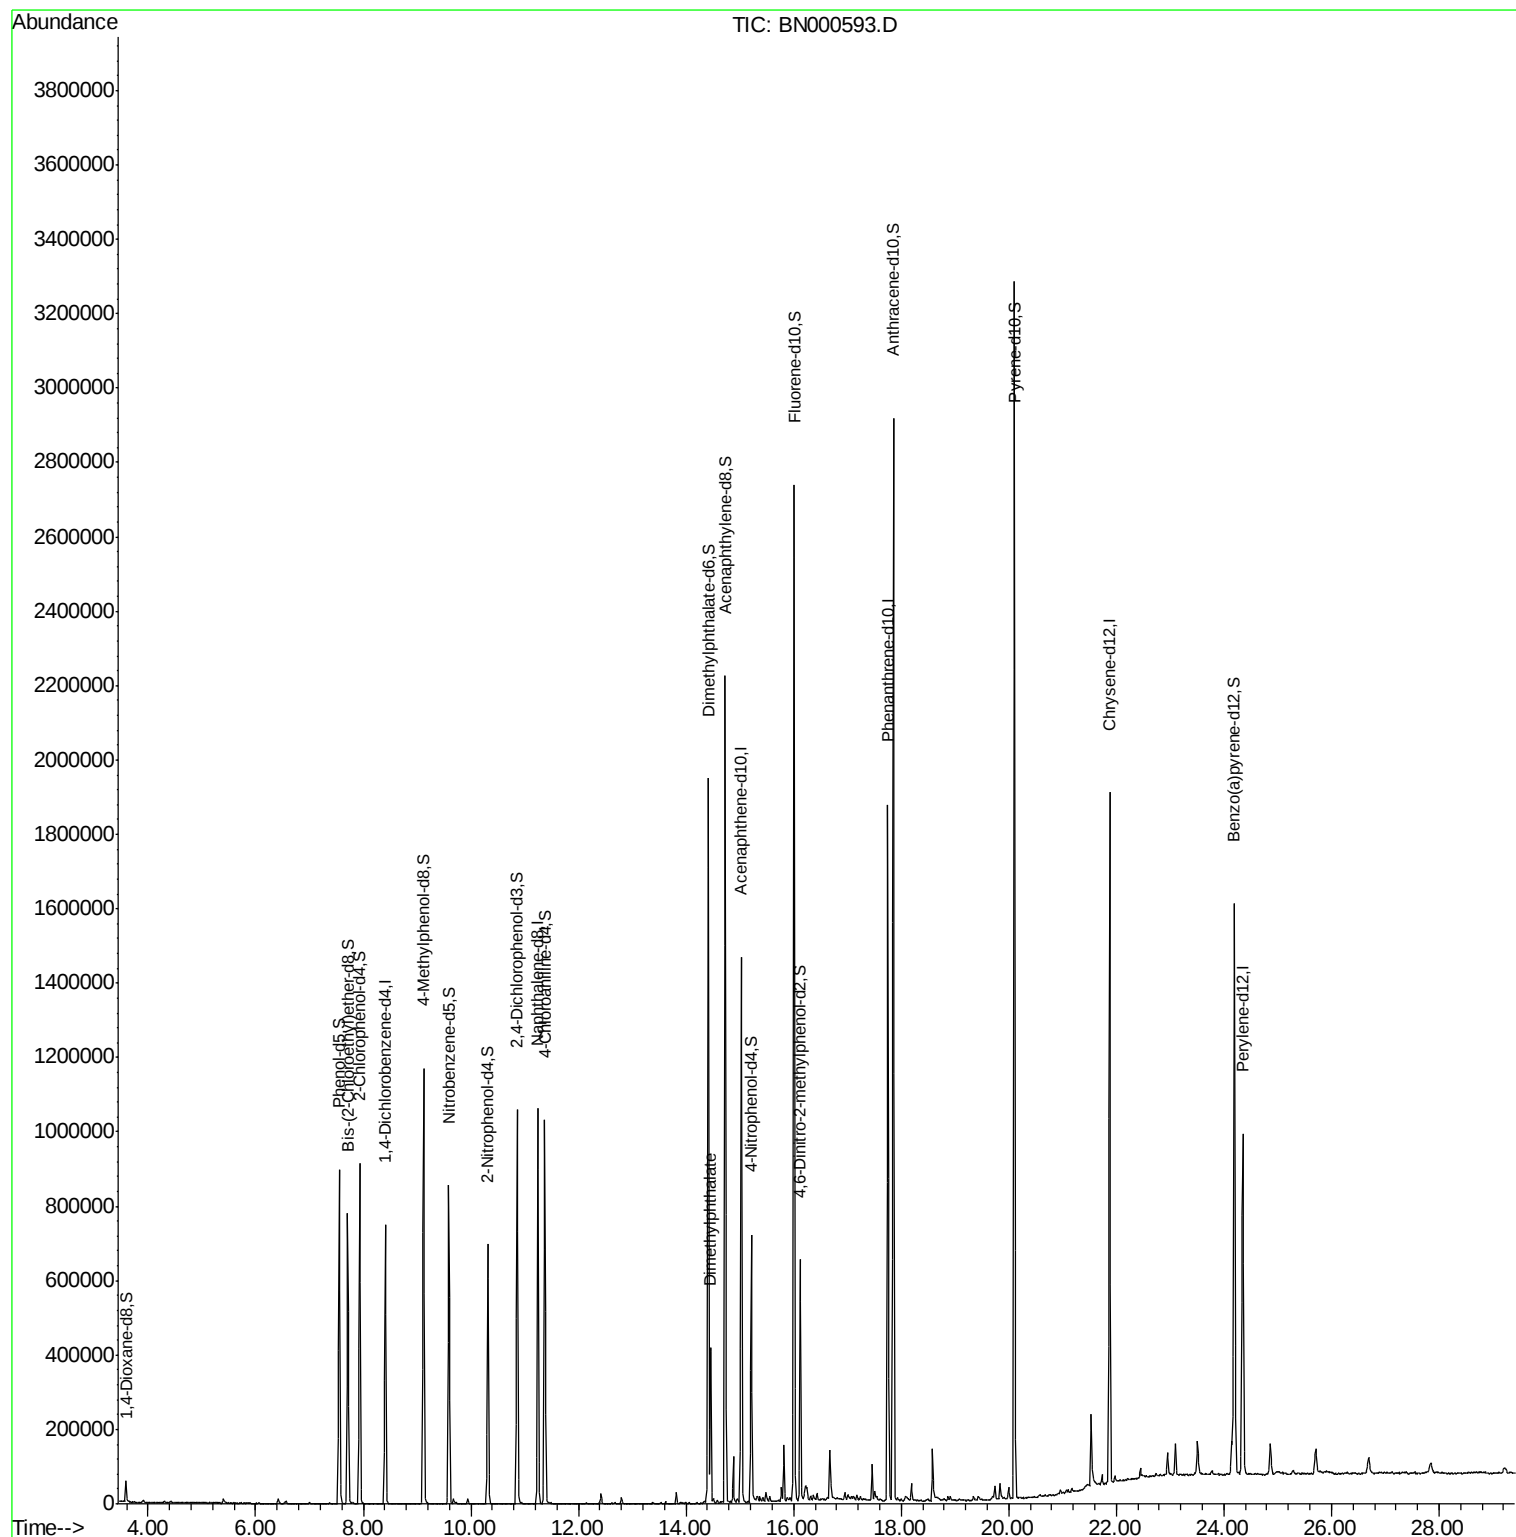

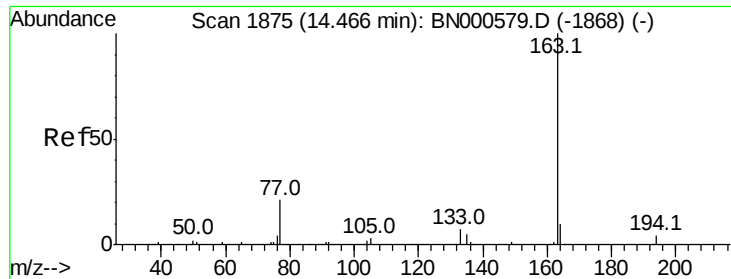

#44

Dimethylphthalate

Concen: 6.587 ng/ul

RT: 14.46 min Scan# 1874

Delta R.T. -0.01 min

Lab File: BN000593.D

Acq: 23 Mar 2018 23:59

Instrument :

BNA_N

ClientSampleId :

C1011


Tot Ion:163 Resp: 244940

Ion Ratio Lower Upper

163 100

194 3.8 4.0 6.0#

164 10.3 8.4 12.6

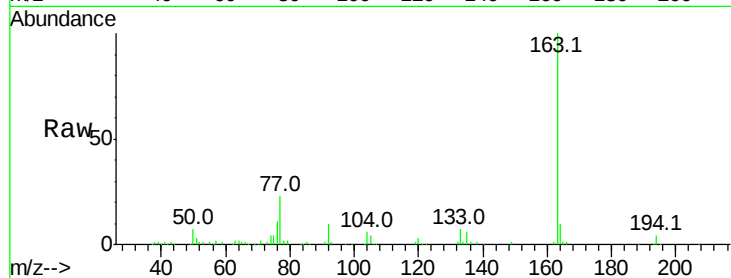

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

