

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
 Data File : BN000569.D
 Acq On : 23 Mar 2018 10:11
 Operator : JU/SJ
 Sample : J1905-13DL3 600X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM48DL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.408	163	165	172	rVB3	3369	4772	0.10%	0.029%
2	5.402	329	334	338	rBV3	3923	5699	0.12%	0.035%
3	6.855	576	581	584	rVB	5944	8100	0.18%	0.049%
4	7.102	617	623	628	rVB4	3644	5112	0.11%	0.031%
5	7.513	689	693	699	rVB2	3029	5674	0.12%	0.035%
6	7.631	711	713	720	rVB3	3688	5391	0.12%	0.033%
7	7.743	729	732	736	rVV	3267	4938	0.11%	0.030%
8	7.802	736	742	749	rVB2	13058	19699	0.43%	0.120%
9	8.407	838	845	851	rBV	587748	997845	21.84%	6.077%
10	8.449	851	852	861	rVB	48434	52289	1.14%	0.318%
11	8.601	871	878	882	rBV	44850	70613	1.55%	0.430%
12	8.837	913	918	930	rVB	40512	68535	1.50%	0.417%
13	9.525	1031	1035	1040	rBV3	6403	9573	0.21%	0.058%
14	9.678	1056	1061	1070	rBV	25809	44588	0.98%	0.272%
15	9.837	1084	1088	1095	rVB2	3701	7045	0.15%	0.043%
16	10.148	1136	1141	1146	rBV3	3745	6175	0.14%	0.038%
17	10.201	1146	1150	1155	rVB	6728	8322	0.18%	0.051%
18	10.266	1155	1161	1162	rBV	8745	13071	0.29%	0.080%
19	10.354	1172	1176	1183	rVB3	8095	13238	0.29%	0.081%
20	10.713	1232	1237	1240	rBV2	3776	5871	0.13%	0.036%
21	10.743	1240	1242	1246	rVB2	3092	4577	0.10%	0.028%
22	11.201	1313	1320	1322	rVV2	7260	12365	0.27%	0.075%
23	11.248	1322	1328	1337	rVV	816367	1412832	30.92%	8.604%
24	11.507	1367	1372	1376	rBV4	3369	7056	0.15%	0.043%
25	11.590	1381	1386	1390	rBV	15351	23677	0.52%	0.144%
26	12.101	1468	1473	1477	rBV3	3314	6406	0.14%	0.039%
27	12.160	1479	1483	1488	rVV2	3633	5494	0.12%	0.033%
28	12.454	1527	1533	1538	rBB3	11297	16570	0.36%	0.101%
29	12.648	1562	1566	1572	rVB2	8168	12134	0.27%	0.074%
30	12.748	1575	1583	1587	rBV3	7383	14545	0.32%	0.089%
31	13.437	1697	1700	1704	rBV2	3097	4966	0.11%	0.030%
32	13.601	1724	1728	1732	rBV	6857	8467	0.19%	0.052%
33	13.666	1736	1739	1742	rBV3	4162	4734	0.10%	0.029%
34	13.760	1749	1755	1760	rVB2	5485	7969	0.17%	0.049%

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
Data File : BN000569.D
Acq On : 23 Mar 2018 10:11
Operator : JU/SJ
Sample : J1905-13DL3 600X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM48DL3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Title : SVOA CALIBRATION

35	14.066	1803	1807	1813	rVB3	6467	11112	0.24%	0.068%
36	14.366	1854	1858	1862	rVB2	7349	8991	0.20%	0.055%
37	14.725	1914	1919	1924	rVB4	5195	7812	0.17%	0.048%
38	15.031	1964	1971	1980	rBV2	1278225	1902085	41.63%	11.584%
39	15.301	2011	2017	2023	rBV4	17894	35051	0.77%	0.213%
40	15.395	2031	2033	2038	rVB4	4366	5439	0.12%	0.033%
41	15.460	2038	2044	2050	rBV3	6382	11529	0.25%	0.070%
42	15.566	2057	2062	2066	rVB3	7056	10777	0.24%	0.066%
43	15.648	2066	2076	2084	rBV	243929	367040	8.03%	2.235%
44	15.760	2090	2095	2098	rBV2	5688	7868	0.17%	0.048%
45	16.013	2134	2138	2144	rVB2	8461	11906	0.26%	0.073%
46	16.813	2270	2274	2278	rBV2	11011	13576	0.30%	0.083%
47	17.407	2369	2375	2396	rBV	3062386	4568731	100.00%	27.824%
48	17.542	2396	2398	2402	rVB	9238	11783	0.26%	0.072%
49	17.760	2429	2435	2441	rBV2	1642535	2340550	51.23%	14.254%
50	17.854	2447	2451	2456	rBV2	6218	7448	0.16%	0.045%
51	19.983	2810	2813	2817	rBV2	8082	8602	0.19%	0.052%
52	20.113	2831	2835	2839	rBV5	4886	6210	0.14%	0.038%
53	21.883	3130	3136	3144	rBV	1814809	2392486	52.37%	14.571%
54	24.360	3550	3557	3567	rBV2	860728	1792580	39.24%	10.917%


Sum of corrected areas: 16419918

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
Data File : BN000569.D
Acq On : 23 Mar 2018 10:11
Operator : JU/SJ
Sample : J1905-13DL3 600X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM48DL3

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

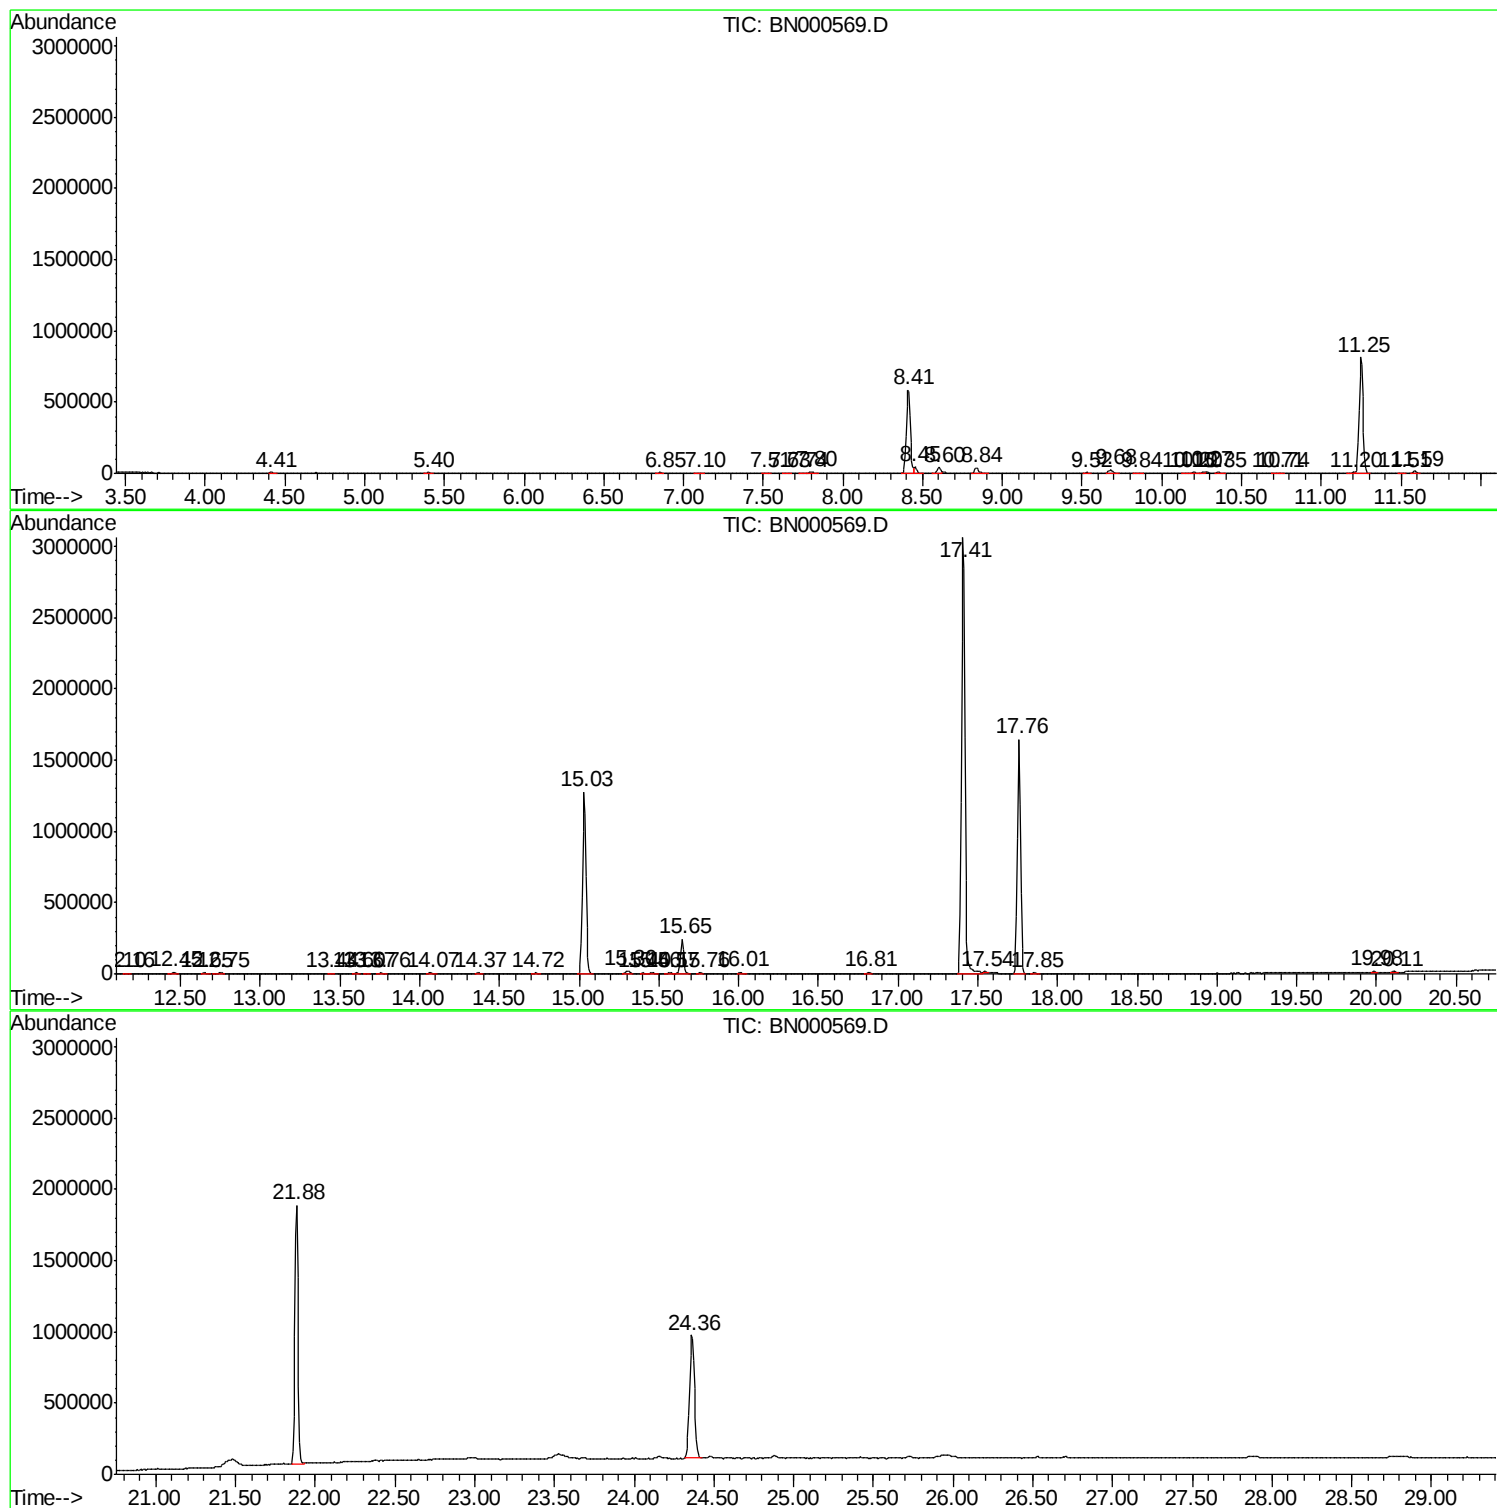

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
Data File : BN000569.D
Acq On : 23 Mar 2018 10:11
Operator : JU/SJ
Sample : J1905-13DL3 600X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM48DL3

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
Data File : BN000569.D
Acq On : 23 Mar 2018 10:11
Operator : JU/SJ
Sample : J1905-13DL3 600X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM48DL3

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc