

Data Path : Z:\HPCHEM1\BNA N\Data\BN032318\
 Data File : BN000576.D
 Acq On : 23 Mar 2018 14:12
 Operator : JU/SJ
 Sample : J1905-09DL2 400X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM44DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.696	210	214	220	rVB2	3401	5918	0.10%	0.032%
2	5.402	330	334	341	rBV3	6121	9556	0.17%	0.051%
3	6.349	490	495	501	rBV3	6346	9641	0.17%	0.051%
4	6.855	576	581	587	rVB2	9385	14876	0.26%	0.079%
5	7.108	621	624	628	rBV4	4784	6083	0.11%	0.032%
6	7.466	681	685	689	rBV	6287	8623	0.15%	0.046%
7	7.525	689	695	700	rVV2	10715	17212	0.30%	0.092%
8	7.637	711	714	719	rVV	6857	8916	0.16%	0.048%
9	7.743	722	732	736	rBV2	7484	13682	0.24%	0.073%
10	7.802	736	742	749	rVB2	16333	31118	0.55%	0.166%
11	8.002	770	776	780	rBV	18694	27957	0.49%	0.149%
12	8.043	780	783	786	rVV	10552	11814	0.21%	0.063%
13	8.078	786	789	793	rVB2	5302	7074	0.13%	0.038%
14	8.302	822	827	832	rBV3	3866	6987	0.12%	0.037%
15	8.360	832	837	839	rVV2	4625	6406	0.11%	0.034%
16	8.413	839	846	850	rVV	607358	1004948	17.78%	5.362%
17	8.455	850	853	860	rVV	96898	140443	2.48%	0.749%
18	8.519	860	864	870	rVB4	6485	11093	0.20%	0.059%
19	8.602	872	878	882	rVV	59458	92319	1.63%	0.493%
20	8.637	882	884	892	rVB2	11152	13980	0.25%	0.075%
21	8.837	913	918	927	rBV	49088	88081	1.56%	0.470%
22	8.996	936	945	949	rBV5	6428	18032	0.32%	0.096%
23	9.043	949	953	959	rVB5	10355	19290	0.34%	0.103%
24	9.160	965	973	977	rBV4	5276	10853	0.19%	0.058%
25	9.207	977	981	989	rVB2	5184	8602	0.15%	0.046%
26	9.519	1029	1034	1043	rVB4	14214	26807	0.47%	0.143%
27	9.625	1046	1052	1056	rBV	24277	37839	0.67%	0.202%
28	9.684	1056	1062	1069	rVV	44582	75146	1.33%	0.401%
29	9.843	1083	1089	1090	rBV	6001	8253	0.15%	0.044%
30	9.949	1104	1107	1113	rVB2	4247	7089	0.13%	0.038%
31	10.013	1113	1118	1122	rBV2	4052	6979	0.12%	0.037%
32	10.154	1138	1142	1145	rVV3	6855	10742	0.19%	0.057%
33	10.201	1145	1150	1155	rVB2	11802	19540	0.35%	0.104%
34	10.278	1155	1163	1171	rBV4	15534	44446	0.79%	0.237%

Data Path : Z:\HPCHEM1\BNA N\Data\BN032318\
 Data File : BN000576.D
 Acq On : 23 Mar 2018 14:12
 Operator : JU/SJ
 Sample : J1905-09DL2 400X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM44DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION

35	10.354	1171	1176	1182	rVB3	14235	25301	0.45%	0.135%
36	10.484	1187	1198	1200	rBV3	4128	9874	0.17%	0.053%
37	10.554	1206	1210	1217	rVB7	3582	8721	0.15%	0.047%
38	10.631	1217	1223	1227	rBV3	4648	7872	0.14%	0.042%
39	10.719	1231	1238	1240	rBV3	9910	16723	0.30%	0.089%
40	10.896	1264	1268	1273	rBV	7196	11285	0.20%	0.060%
41	10.984	1278	1283	1288	rVB2	4352	6439	0.11%	0.034%
42	11.196	1305	1319	1322	rBV4	23234	60986	1.08%	0.325%
43	11.249	1322	1328	1335	rVB	837430	1448933	25.64%	7.731%
44	11.325	1335	1341	1344	rBV3	9420	14899	0.26%	0.079%
45	11.513	1368	1373	1379	rBV5	4188	10968	0.19%	0.059%
46	11.590	1379	1386	1395	rVB	41910	71106	1.26%	0.379%
47	11.719	1399	1408	1411	rBV3	6919	13334	0.24%	0.071%
48	11.813	1420	1424	1434	rVB4	5595	14096	0.25%	0.075%
49	11.925	1434	1443	1444	rBV3	4486	8171	0.14%	0.044%
50	12.107	1466	1474	1478	rBV3	9110	18736	0.33%	0.100%
51	12.166	1479	1484	1489	rVV	8662	14748	0.26%	0.079%
52	12.219	1489	1493	1498	rVV4	5230	9494	0.17%	0.051%
53	12.307	1502	1508	1511	rVB3	6470	8810	0.16%	0.047%
54	12.454	1527	1533	1543	rBV2	30333	49564	0.88%	0.264%
55	12.601	1553	1558	1562	rBV4	11833	21333	0.38%	0.114%
56	12.648	1562	1566	1573	rVB2	23972	35794	0.63%	0.191%
57	12.748	1576	1583	1588	rVV4	12878	28355	0.50%	0.151%
58	12.790	1588	1590	1598	rVV4	8746	14009	0.25%	0.075%
59	13.013	1623	1628	1636	rBV4	5722	15854	0.28%	0.085%
60	13.201	1656	1660	1664	rBV4	4461	7008	0.12%	0.037%
61	13.331	1678	1682	1685	rVB2	5868	7612	0.13%	0.041%
62	13.543	1713	1718	1723	rBV2	6123	8675	0.15%	0.046%
63	13.601	1723	1728	1735	rVB2	10745	14377	0.25%	0.077%
64	13.666	1735	1739	1741	rBV2	6326	7349	0.13%	0.039%
65	13.754	1748	1754	1760	rVB4	4988	9506	0.17%	0.051%
66	13.819	1760	1765	1775	rBV5	12973	26085	0.46%	0.139%
67	14.066	1799	1807	1814	rBV2	12007	20488	0.36%	0.109%
68	14.201	1826	1830	1834	rVB3	4337	6684	0.12%	0.036%
69	14.366	1849	1858	1863	rBV7	13377	27493	0.49%	0.147%
70	14.472	1870	1876	1881	rVB4	5299	10447	0.18%	0.056%
71	14.731	1913	1920	1924	rVB	12888	17735	0.31%	0.095%

Data Path : Z:\HPCHEM1\BNA N\Data\BN032318\
 Data File : BN000576.D
 Acq On : 23 Mar 2018 14:12
 Operator : JU/SJ
 Sample : J1905-09DL2 400X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAM44DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION

72	14.807	1931	1933	1937	rVV5	4866	6789	0.12%	0.036%
73	14.884	1941	1946	1951	rVB	45336	61513	1.09%	0.328%
74	15.031	1964	1971	1980	rBV2	1286936	1978649	35.01%	10.557%
75	15.142	1985	1990	1994	rVB	17868	20388	0.36%	0.109%
76	15.307	2010	2018	2025	rBV3	30623	65501	1.16%	0.349%
77	15.366	2025	2028	2031	rVV4	6204	8783	0.16%	0.047%
78	15.401	2031	2034	2037	rVV3	7050	7838	0.14%	0.042%
79	15.454	2039	2043	2047	rVV3	4876	8117	0.14%	0.043%
80	15.566	2056	2062	2066	rVB5	15711	27761	0.49%	0.148%
81	15.642	2066	2075	2085	rBV	319542	490638	8.68%	2.618%
82	15.760	2091	2095	2099	rBV	23835	30862	0.55%	0.165%
83	15.819	2099	2105	2114	rVB4	16467	31108	0.55%	0.166%
84	16.013	2133	2138	2142	rBV2	13091	18477	0.33%	0.099%
85	16.142	2156	2160	2164	rBV	6160	8371	0.15%	0.045%
86	16.219	2170	2173	2177	rVB3	5569	8110	0.14%	0.043%
87	16.319	2185	2190	2193	rBV5	3650	6663	0.12%	0.036%
88	16.607	2234	2239	2246	rBV2	4286	7044	0.12%	0.038%
89	16.678	2246	2251	2254	rBV2	16838	25517	0.45%	0.136%
90	16.813	2270	2274	2278	rBV2	20986	27784	0.49%	0.148%
91	17.407	2368	2375	2390	rBV	3834947	5651994	100.00%	30.157%
92	17.754	2428	2434	2441	rBV2	1618604	2376434	42.05%	12.680%
93	17.854	2445	2451	2456	rVB2	9502	14576	0.26%	0.078%
94	18.195	2505	2509	2513	rVB	11401	13743	0.24%	0.073%
95	18.872	2621	2624	2630	rVB3	8899	11963	0.21%	0.064%
96	19.489	2727	2729	2732	rBV3	6077	7639	0.14%	0.041%
97	20.113	2831	2835	2839	rBV3	7452	11356	0.20%	0.061%
98	20.589	2913	2916	2919	rBV4	4632	6256	0.11%	0.033%
99	21.883	3130	3136	3142	rBV	1709239	2215450	39.20%	11.821%
100	24.365	3550	3558	3567	rBV2	808532	1653552	29.26%	8.823%


Sum of corrected areas: 18742085

Data Path : Z:\HPCHEM1\BNA N\Data\BN032318\
Data File : BN000576.D
Acq On : 23 Mar 2018 14:12
Operator : JU/SJ
Sample : J1905-09DL2 400X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM44DL2

Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

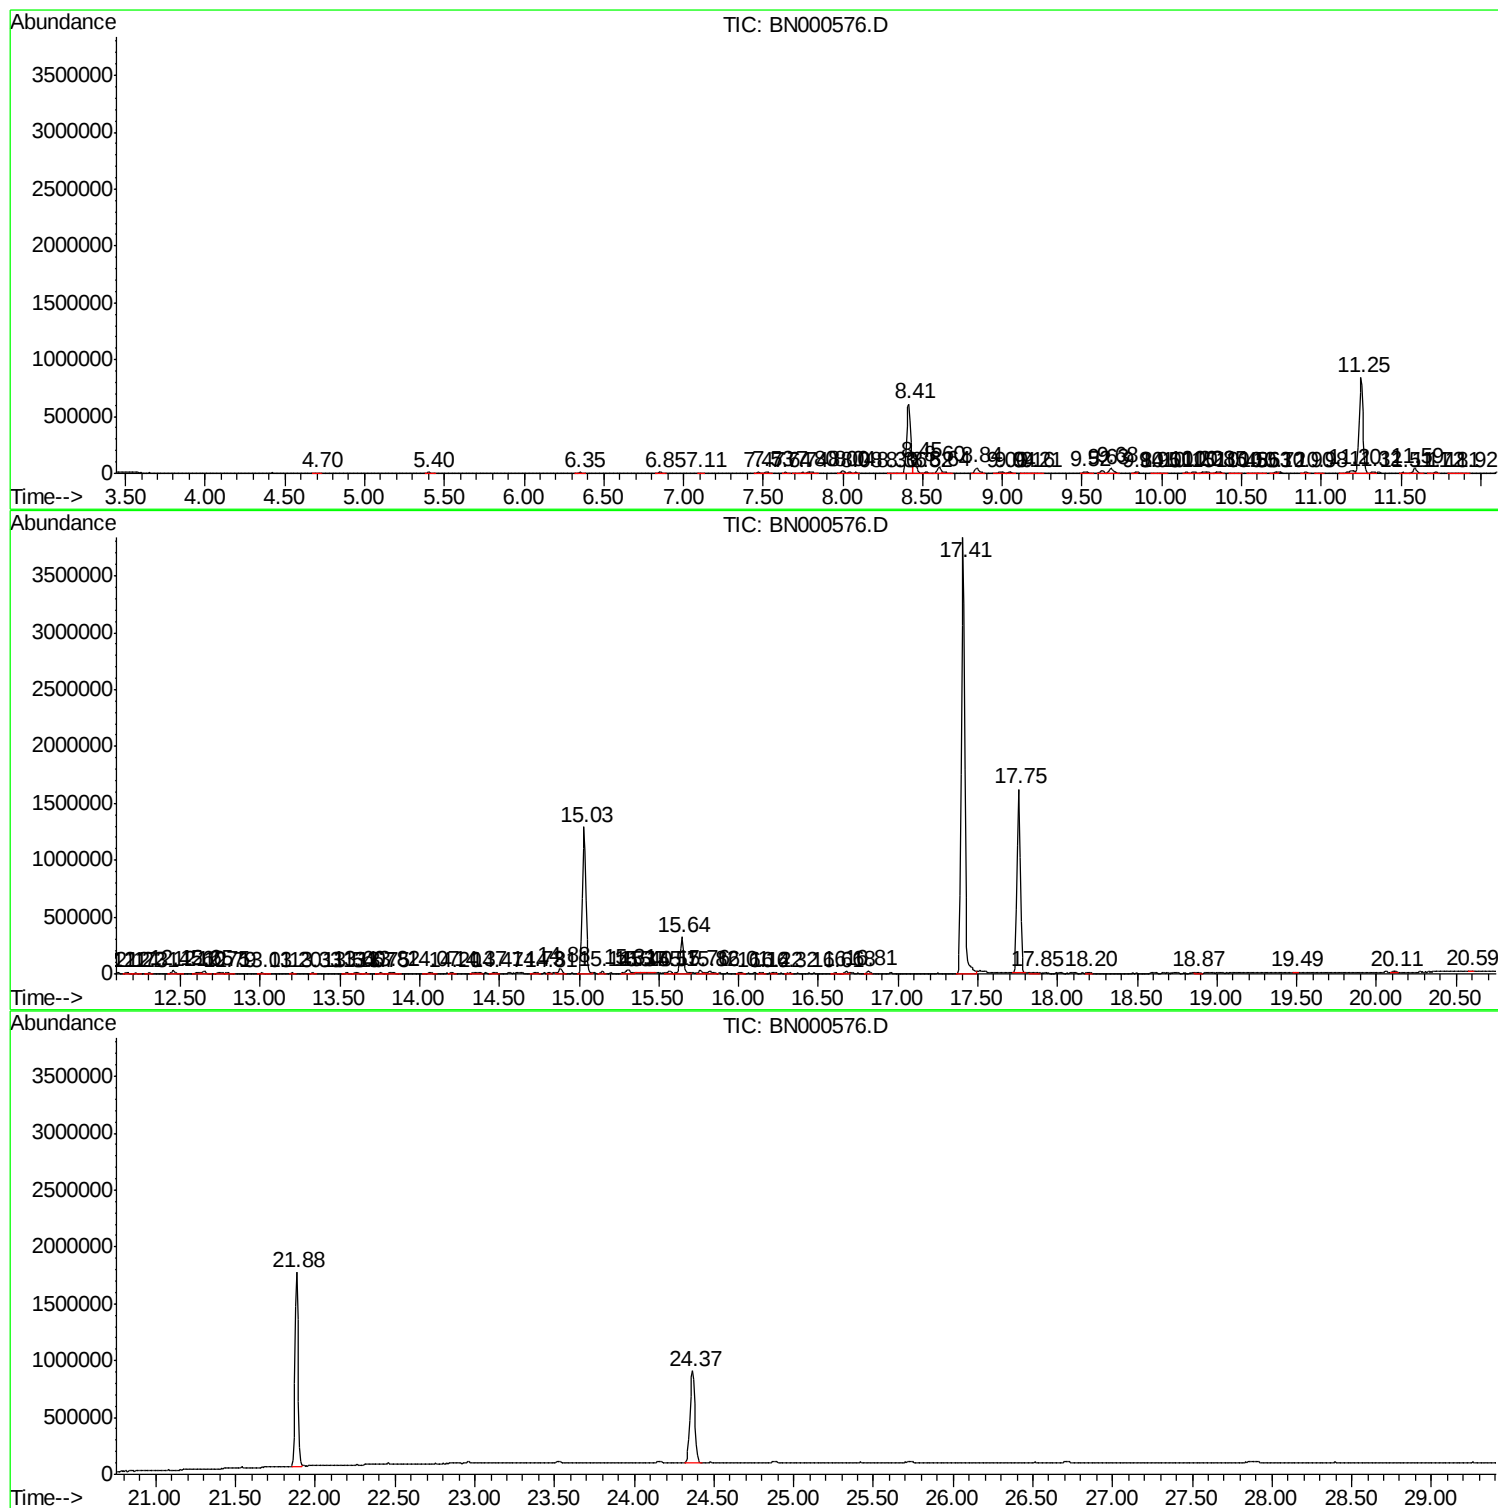

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
Data File : BN000576.D
Acq On : 23 Mar 2018 14:12
Operator : JU/SJ
Sample : J1905-09DL2 400X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM44DL2

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_N\Data\BN032318\
Data File : BN000576.D
Acq On : 23 Mar 2018 14:12
Operator : JU/SJ
Sample : J1905-09DL2 400X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAM44DL2

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc