

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
 Data File : BN014036.D
 Acq On : 23 Mar 2021 10:25
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Mar 23 11:05:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 19 14:40:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	5596	0.40	ng	0.00
7) Naphthalene-d8	10.479	136	20505	0.40	ng	# 0.00
13) Acenaphthene-d10	14.320	164	11661	0.40	ng	-0.01
19) Phenanthrene-d10	17.067	188	24714	0.40	ng	# 0.00
29) Chrysene-d12	21.239	240	24119	0.40	ng	#-0.01
36) Perylene-d12	23.448	264	23055	0.40	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.292	112	5943	0.46	ng	0.00
5) Phenol-d6	6.862	99	7584	0.46	ng	0.00
8) Nitrobenzene-d5	8.844	82	5589	0.41	ng	0.00
11) 2-Methylnaphthalene-d10	12.066	152	14123	0.44	ng	0.00
14) 2,4,6-Tribromophenol	15.817	330	1352	0.36	ng	0.00
15) 2-Fluorobiphenyl	12.950	172	18615	0.43	ng	0.00
27) Fluoranthene-d10	19.089	212	30133	0.44	ng	-0.01
31) Terphenyl-d14	19.689	244	24132	0.46	ng	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.246	88	3219	0.44	ng	97
3) n-Nitrosodimethylamine	3.593	42	1470	0.30	ng	# 99
6) bis(2-Chloroethyl)ether	7.128	93	6434	0.45	ng	95
9) Naphthalene	10.517	128	22760	0.45	ng	99
10) Hexachlorobutadiene	10.809	225	4267	0.45	ng	# 100
12) 2-Methylnaphthalene	12.137	142	15104	0.44	ng	98
16) Acenaphthylene	14.041	152	17889	0.40	ng	100
17) Acenaphthene	14.384	154	13688	0.42	ng	99
18) Fluorene	15.373	166	17152	0.41	ng	99
20) 4,6-Dinitro-2-methylph...	15.450	198	998	0.36	ng	# 76
21) 4-Bromophenyl-phenylether	16.264	248	5485	0.43	ng	# 84
22) Hexachlorobenzene	16.373	284	6363	0.43	ng	99
23) Atrazine	16.532	200	3346	0.39	ng	99
24) Pentachlorophenol	16.726	266	1198	0.35	ng	95
25) Phenanthrene	17.104	178	29037	0.43	ng	100
26) Anthracene	17.189	178	23567	0.42	ng	100
28) Fluoranthene	19.118	202	32614	0.43	ng	99
30) Pyrene	19.486	202	32848	0.44	ng	100
32) Benzo(a)anthracene	21.218	228	28722	0.42	ng	97
33) Chrysene	21.271	228	34624	0.47	ng	100
34) Bis(2-ethylhexyl)phtha...	21.154	149	8295	0.32	ng	99
35) Indeno(1,2,3-cd)pyrene	25.652	276	38116	0.47	ng	99
37) Benzo(b)fluoranthene	22.784	252	35244	0.42	ng	96
38) Benzo(k)fluoranthene	22.828	252	34579	0.42	ng	# 95
39) Benzo(a)pyrene	23.352	252	30770	0.43	ng	# 94
40) Dibenzo(a,h)anthracene	25.669	278	32350	0.42	ng	97
41) Benzo(g,h,i)perylene	26.330	276	34745	0.43	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
Data File : BN014036.D
Acq On : 23 Mar 2021 10:25
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Mar 23 11:05:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 19 14:40:09 2021
Response via : Initial Calibration

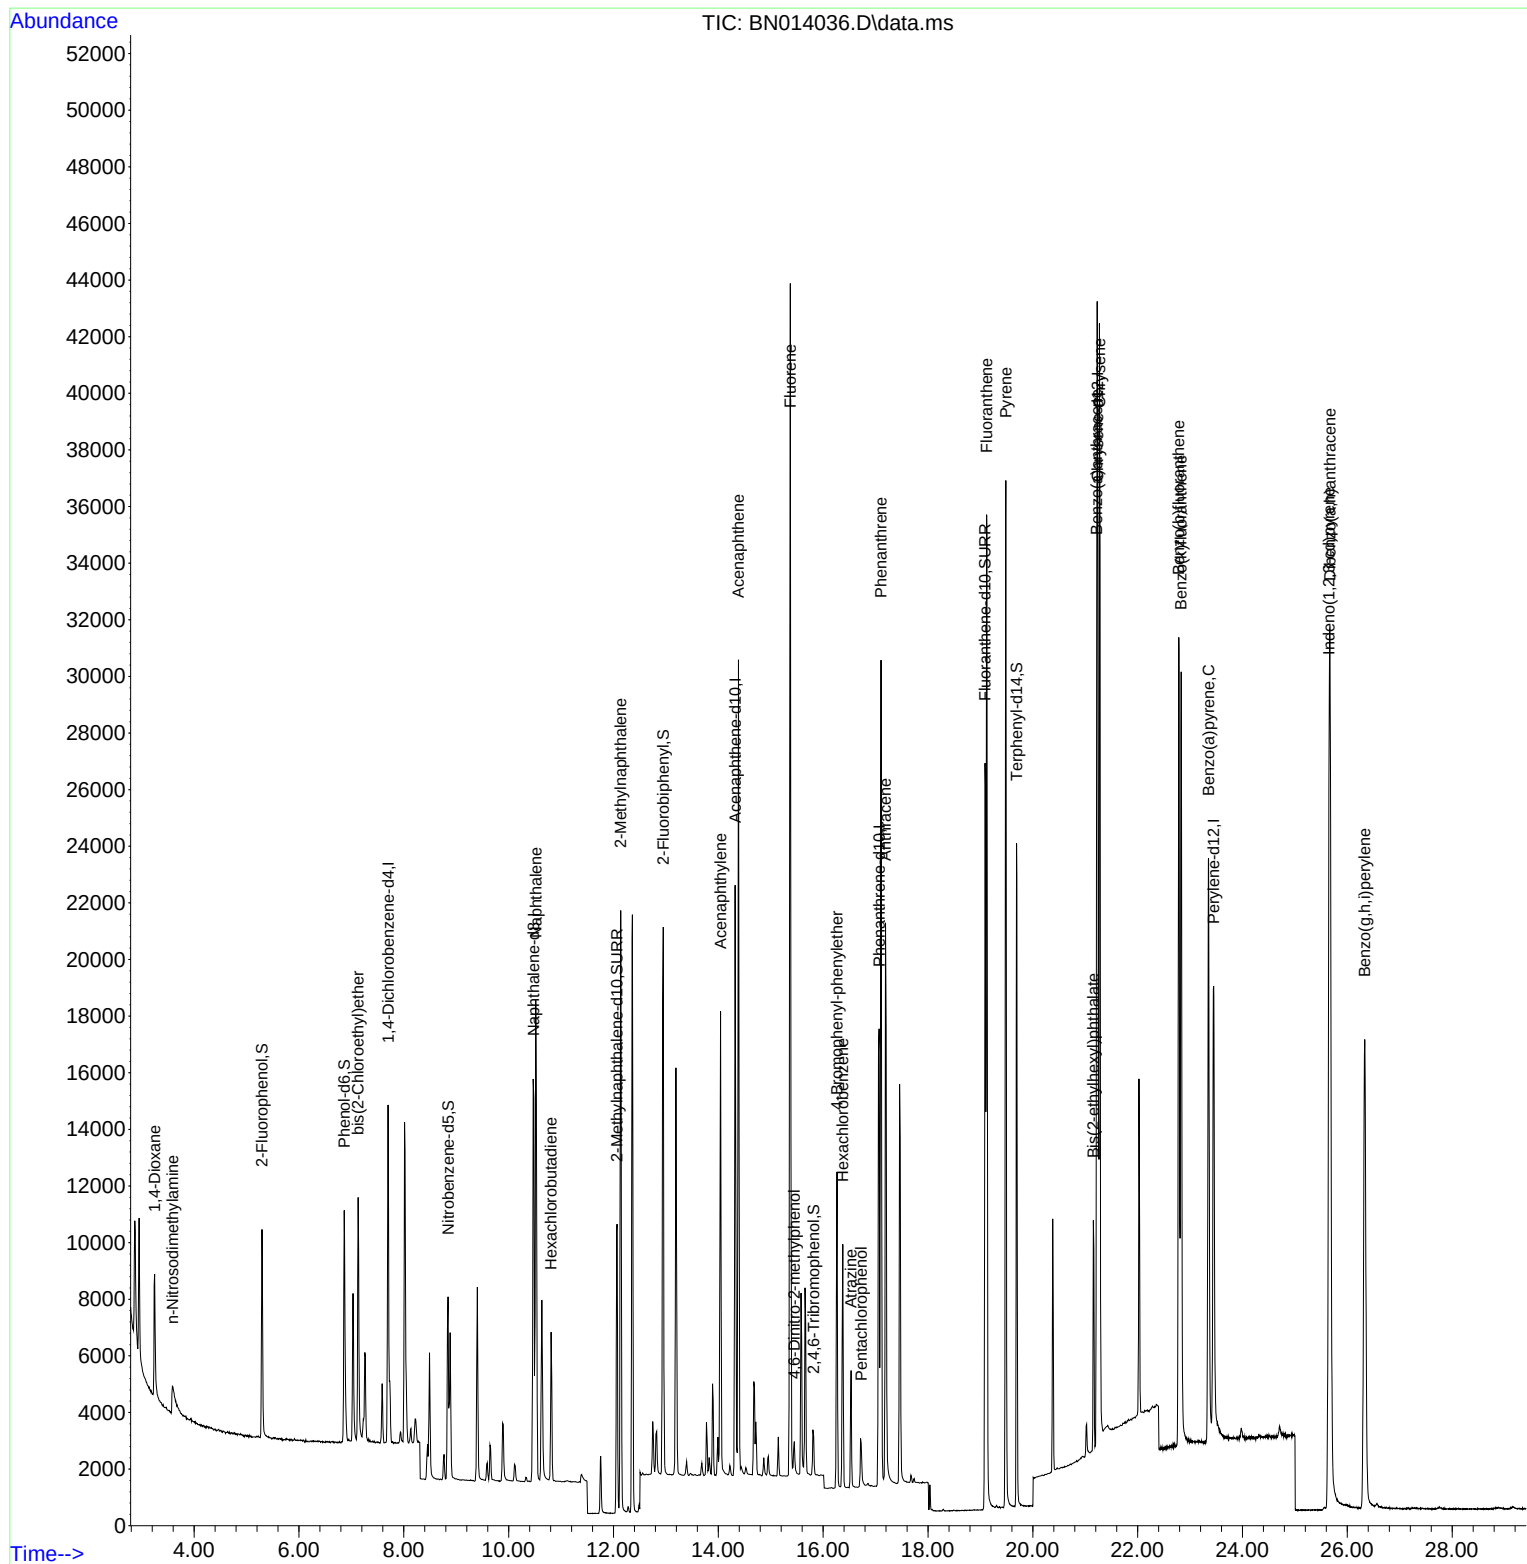







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.700 min Scan# 611
 Delta R.T. -0.000 min
 Lab File: BN014036.D
 Acq: 23 Mar 2021 10:25

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion: 152 Resp: 5596




Ion	Ratio	Lower	Upper
152	100		
150	155.0	121.8	182.8
115	59.1	46.6	69.8

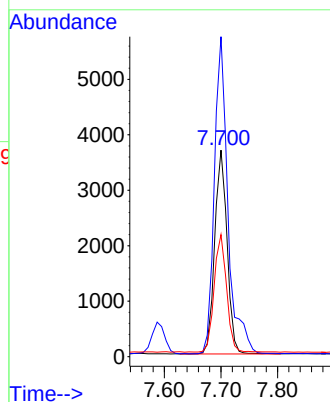


#2
 1,4-Dioxane
 Concen: 0.44 ng
 RT: 3.246 min Scan# 58
 Delta R.T. -0.000 min
 Lab File: BN014036.D
 Acq: 23 Mar 2021 10:25

Tgt Ion: 88 Resp: 3219

Ion	Ratio	Lower	Upper
88	100		
58	77.3	64.6	96.8
43	31.7	26.6	40.0









#3
n-Nitrosodimethylamine
Concen: 0.30 ng
RT: 3.593 min Scan# 101
Delta R.T. 0.016 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampled :
SSTDCCC0.4


Tgt Ion: 42 Resp: 1470
Ion Ratio Lower Upper
42 100
74 119.3 95.0 142.6
44 5.6 5.8 8.8#

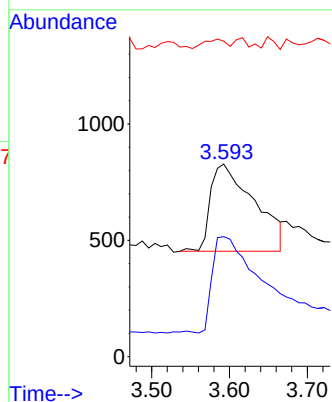

#4
2-Fluorophenol
Concen: 0.46 ng
RT: 5.292 min Scan# 312
Delta R.T. -0.009 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion: 112 Resp: 5943
Ion Ratio Lower Upper
112 100
64 60.3 44.3 66.5
63 31.9 23.0 34.6

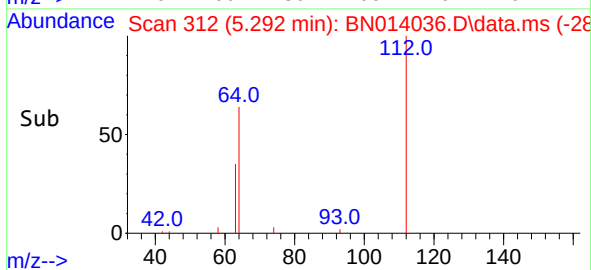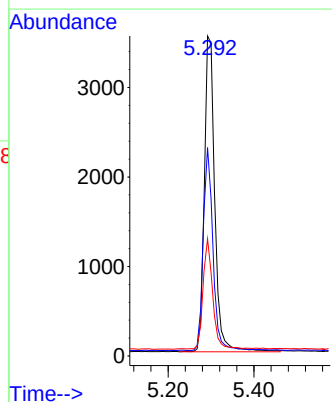







#5
Phenol-d6
Concen: 0.46 ng
RT: 6.862 min Scan# 507
Delta R.T. -0.009 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 7584




Ion	Ratio	Lower	Upper
99	100		
42	21.3	15.2	22.8
71	33.8	26.1	39.1




#6
bis(2-Chloroethyl)ether
Concen: 0.45 ng
RT: 7.128 min Scan# 540
Delta R.T. -0.009 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion: 93 Resp: 6434


Ion	Ratio	Lower	Upper
93	100		
63	81.8	60.8	91.2
95	33.0	26.0	39.0

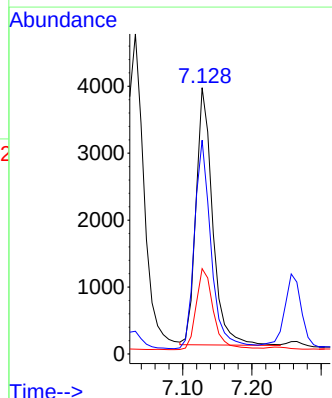






#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.479 min Scan# 858
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:	136	Resp:	20505
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.0	13.6
54	5.2	6.4	9.6#
68	4.2	4.5	6.7#



#8
Nitrobenzene-d5
Concen: 0.41 ng
RT: 8.844 min Scan# 729
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:	82	Resp:	5589
Ion	Ratio	Lower	Upper
82	100		
128	41.1	39.2	58.8
54	50.0	40.1	60.1


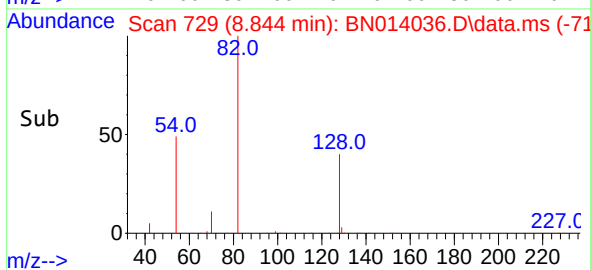




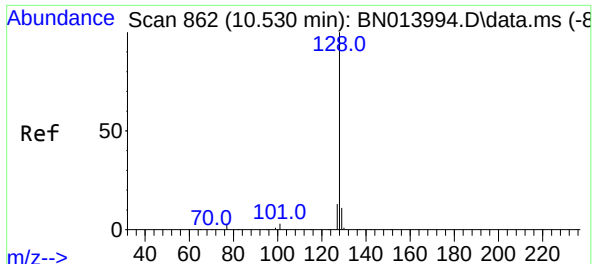

#9
Naphthalene
Concen: 0.45 ng
RT: 10.517 min Scan# 861
Delta R.T. -0.013 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	22760
Ion Ratio	Lower	Upper	
128	100		
129	11.2	9.0	13.4
127	13.5	10.4	15.6

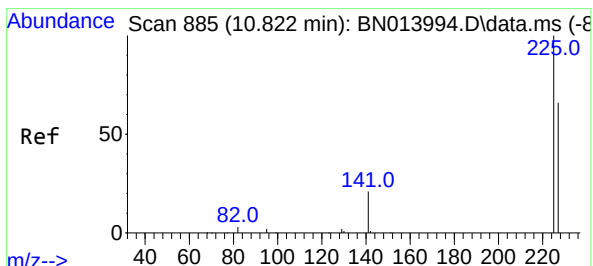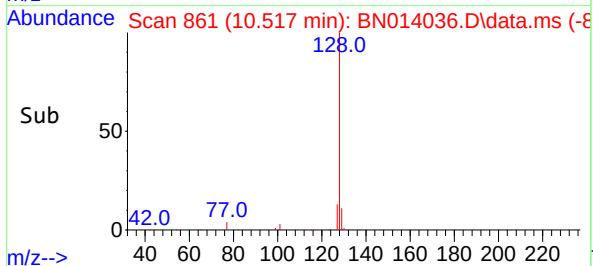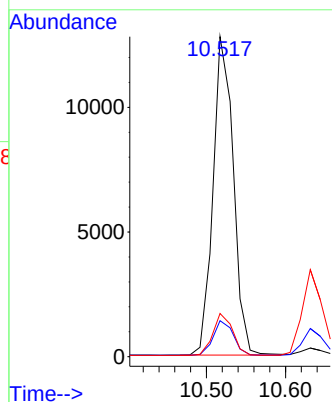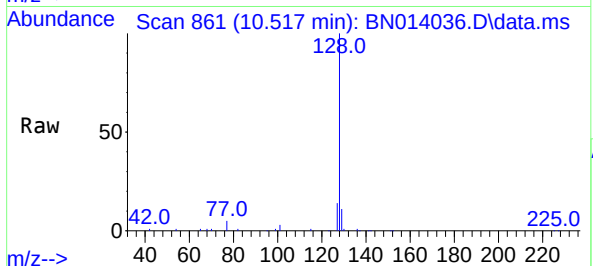

#10
Hexachlorobutadiene
Concen: 0.45 ng
RT: 10.809 min Scan# 884
Delta R.T. -0.013 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:	225	Resp:	4267
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.7	51.2	76.8


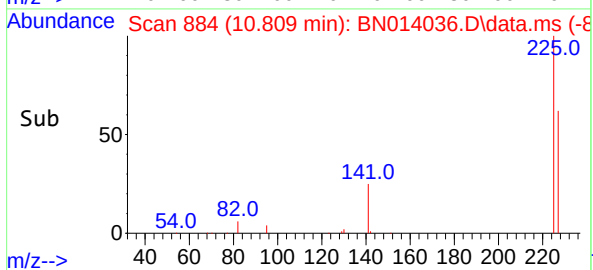
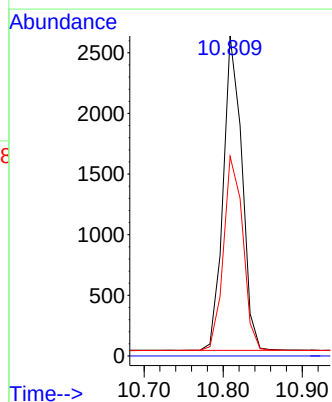
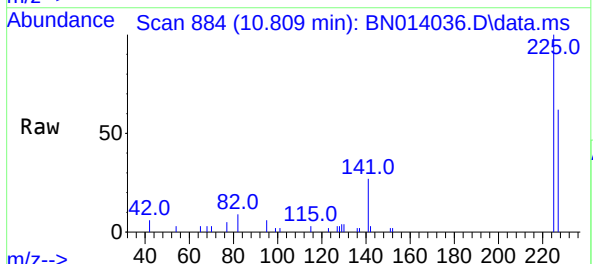




#11
2-Methylnaphthalene-d10
Concen: 0.44 ng
RT: 12.066 min Scan# 1065
Delta R.T. -0.005 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 14123
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2



#12
2-Methylnaphthalene
Concen: 0.44 ng
RT: 12.137 min Scan# 1081
Delta R.T. -0.005 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:142 Resp: 15104
Ion Ratio Lower Upper
142 100
141 89.3 70.5 105.7
115 35.5 27.4 41.0


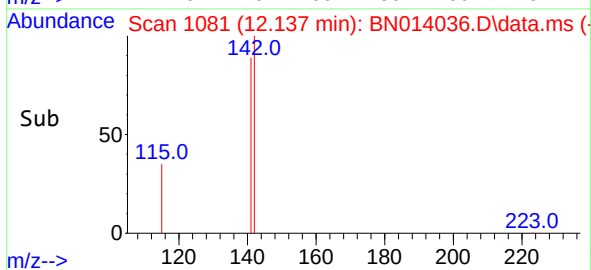






#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.320 min Scan# 1307
Delta R.T. -0.013 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 11661
Ion Ratio Lower Upper
164 100
162 101.8 79.6 119.4
160 46.5 36.0 54.0

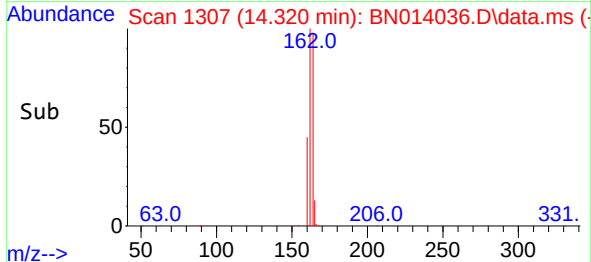

#14
2,4,6-Tribromophenol
Concen: 0.36 ng
RT: 15.817 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:330 Resp: 1352
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.4 26.8 40.2


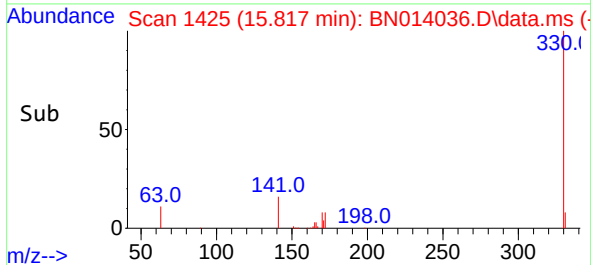

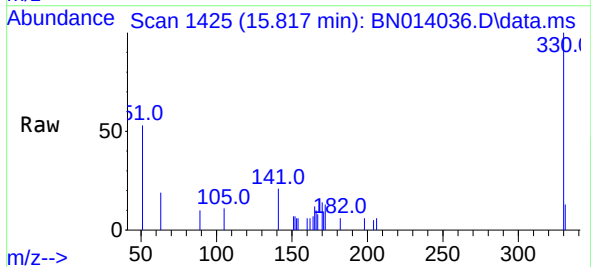




#15
2-Fluorobiphenyl
Concen: 0.43 ng
RT: 12.950 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	18615
Ion	Ratio	Lower	Upper
172	100		
171	32.8	28.6	42.8
170	21.8	18.9	28.3



#16
Acenaphthylene
Concen: 0.40 ng
RT: 14.041 min Scan# 1285
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:	152	Resp:	17889
Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.7	23.5
153	13.1	10.5	15.7


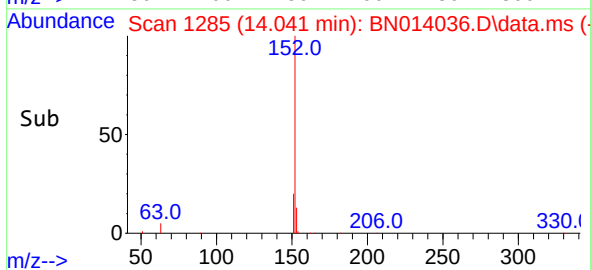






#17
Acenaphthene
Concen: 0.42 ng
RT: 14.384 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 13688
Ion Ratio Lower Upper
154 100
153 112.0 88.4 132.6
152 54.9 43.0 64.4

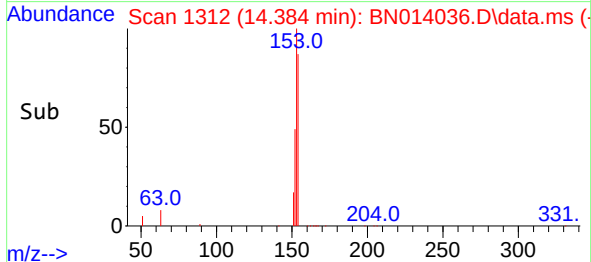

#18
Fluorene
Concen: 0.41 ng
RT: 15.373 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:166 Resp: 17152
Ion Ratio Lower Upper
166 100
165 98.1 77.8 116.8
167 13.7 10.6 16.0


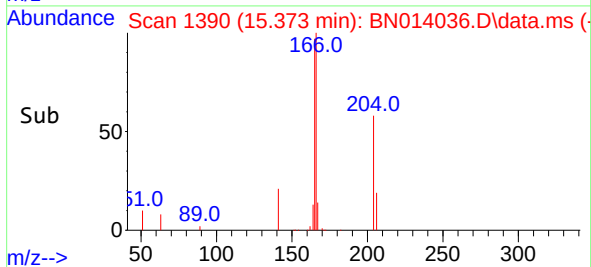

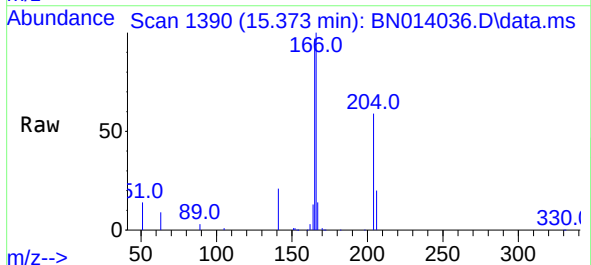


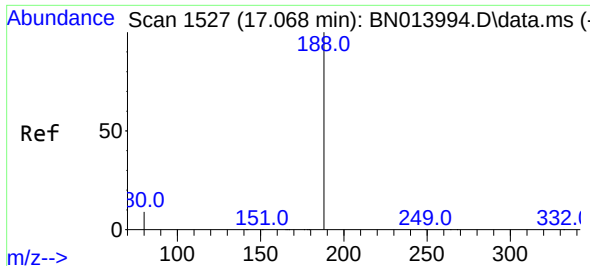

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.067 min Scan# 1527
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 24714
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.5 9.0 13.6#

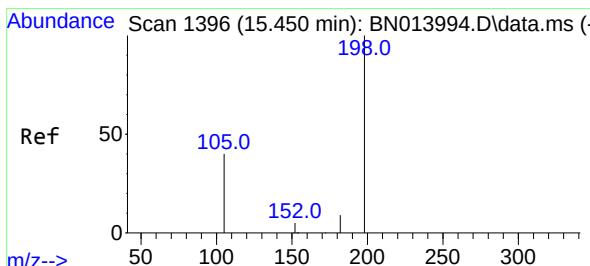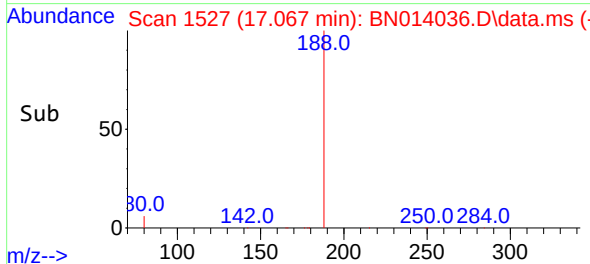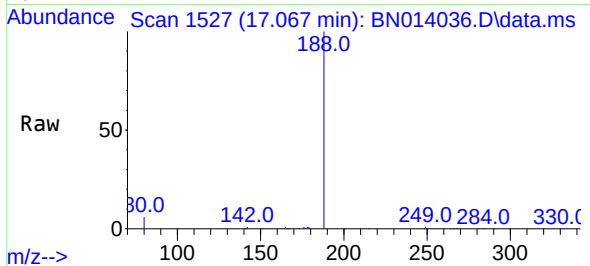

#20
4,6-Dinitro-2-methylphenol
Concen: 0.36 ng
RT: 15.450 min Scan# 1396
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:198 Resp: 998
Ion Ratio Lower Upper
198 100
51 106.4 61.7 92.5#
105 44.6 33.0 49.6


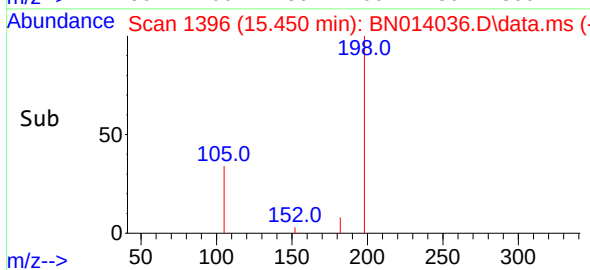

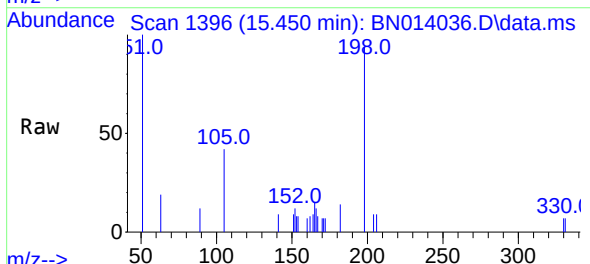




#21
4-Bromophenyl-phenylether
Concen: 0.43 ng
RT: 16.264 min Scan# 1461
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 5485
Ion Ratio Lower Upper
248 100
250 100.5 75.5 113.3
141 44.2 53.8 80.8#

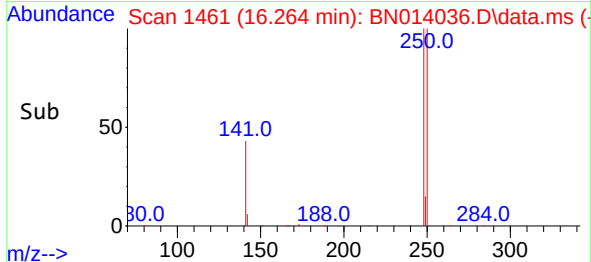

#22
Hexachlorobenzene
Concen: 0.43 ng
RT: 16.373 min Scan# 1470
Delta R.T. -0.013 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:284 Resp: 6363
Ion Ratio Lower Upper
284 100
142 35.5 27.9 41.9
249 30.8 24.2 36.2


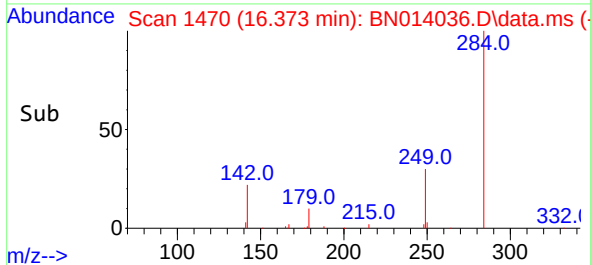

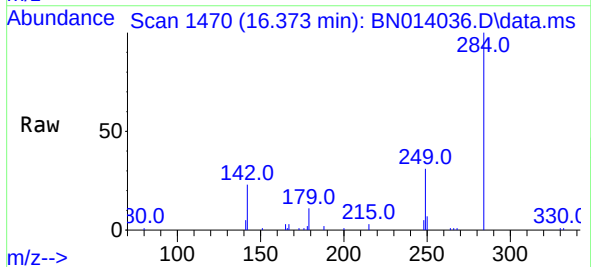


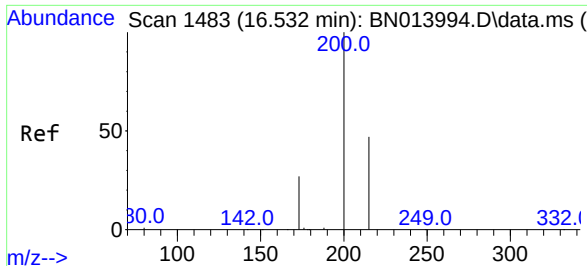

#23
Atrazine
Concen: 0.39 ng
RT: 16.532 min Scan# 1483
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	200	Resp:	3346
Ion Ratio	Lower	Upper	
200	100		
173	23.2	18.6	28.0
215	49.9	41.0	61.6

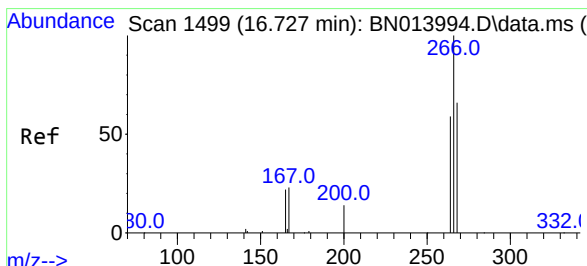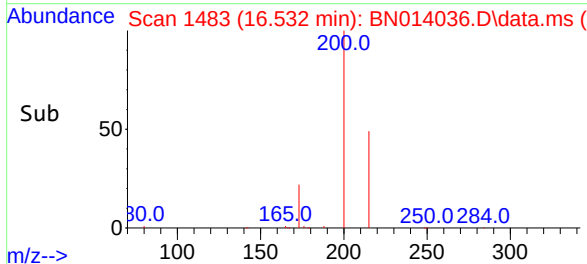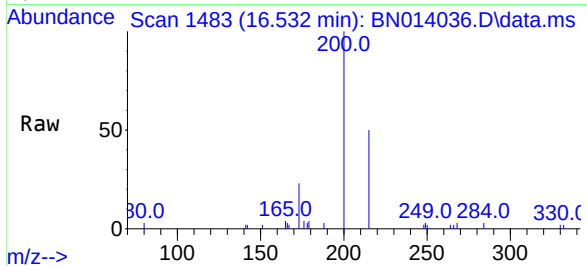

#24
Pentachlorophenol
Concen: 0.35 ng
RT: 16.726 min Scan# 1499
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:	266	Resp:	1198
Ion Ratio	Lower	Upper	
266	100		
264	64.7	51.6	77.4
268	59.9	54.6	82.0


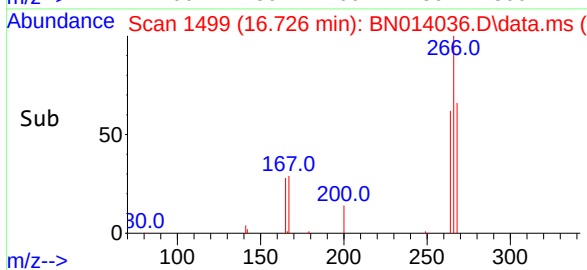

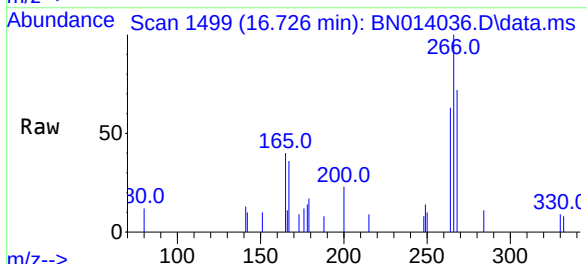


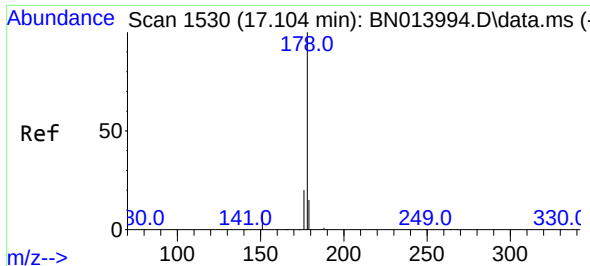

#25
Phenanthrene
Concen: 0.43 ng
RT: 17.104 min Scan# 1530
Delta R.T. -0.000 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	178	Resp:	29037
Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.0	22.4
179	15.3	12.3	18.5

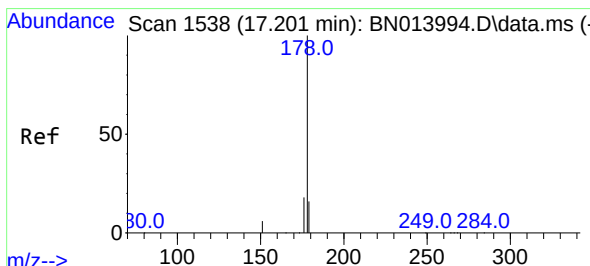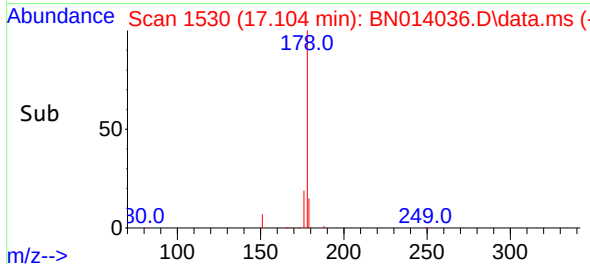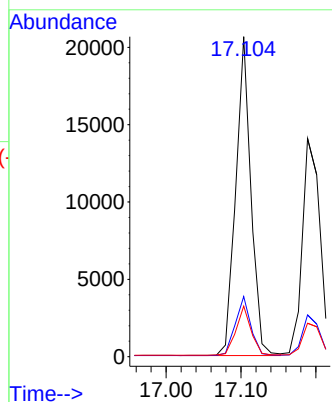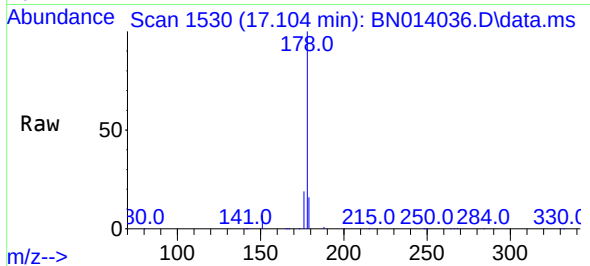

#26
Anthracene
Concen: 0.42 ng
RT: 17.189 min Scan# 1537
Delta R.T. -0.013 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:	178	Resp:	23567
Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.6	21.8
179	15.2	12.2	18.2


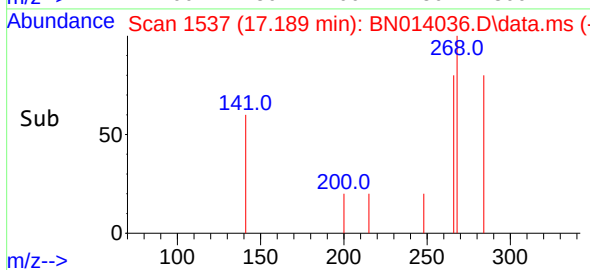

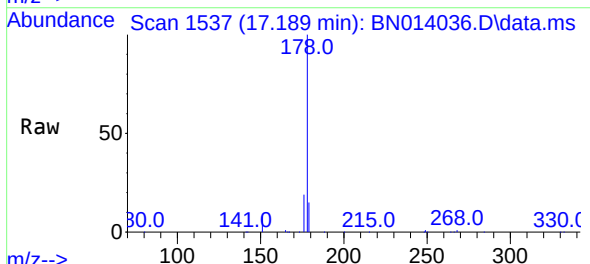




#27
Fluoranthene-d10
Concen: 0.44 ng
RT: 19.089 min Scan# 1821
Delta R.T. -0.010 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 30133
Ion Ratio Lower Upper
212 100
106 12.8 9.7 14.5
104 7.1 5.5 8.3

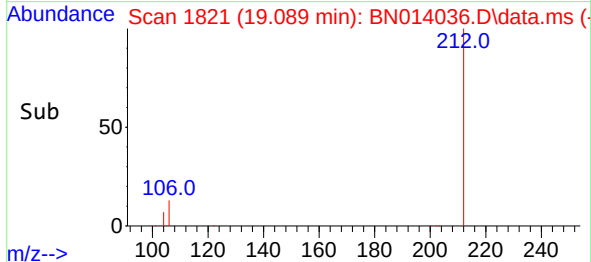

#28
Fluoranthene
Concen: 0.43 ng
RT: 19.118 min Scan# 1827
Delta R.T. -0.010 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:202 Resp: 32614
Ion Ratio Lower Upper
202 100
101 11.1 8.1 12.1
203 17.1 13.9 20.9


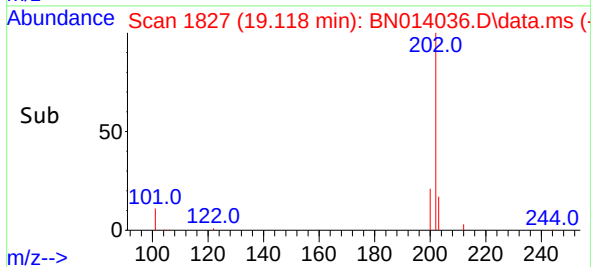

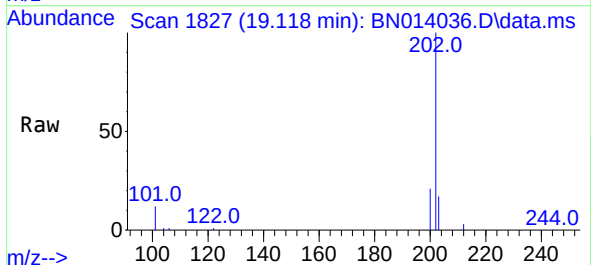




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.239 min Scan# 2122
Delta R.T. -0.011 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 24119
Ion Ratio Lower Upper
240 100
120 9.7 10.2 15.4#
236 25.8 21.3 31.9



#30
Pyrene
Concen: 0.44 ng
RT: 19.486 min Scan# 1901
Delta R.T. -0.005 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:202 Resp: 32848
Ion Ratio Lower Upper
202 100
200 20.4 16.3 24.5
203 17.4 14.0 21.0


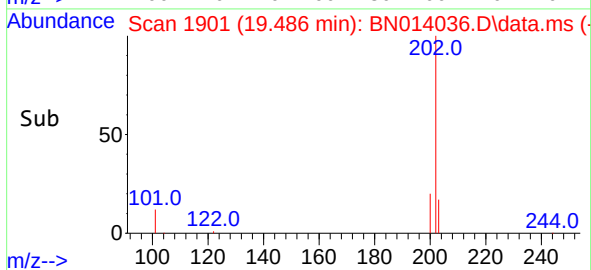




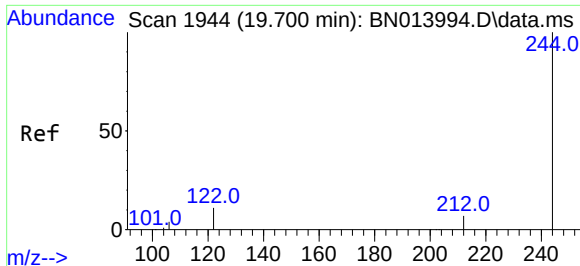

#31
Terphenyl-d14
Concen: 0.46 ng
RT: 19.689 min Scan# 1942
Delta R.T. -0.010 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 24132
Ion Ratio Lower Upper
244 100
212 7.9 6.1 9.1
122 12.8 9.8 14.8

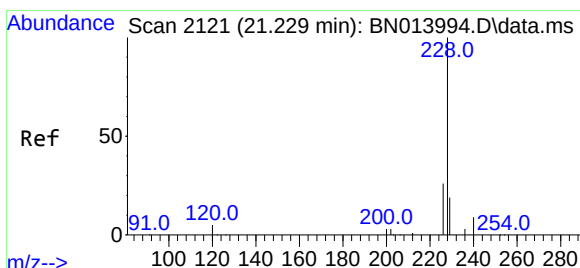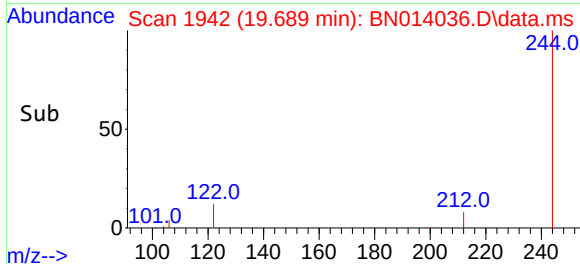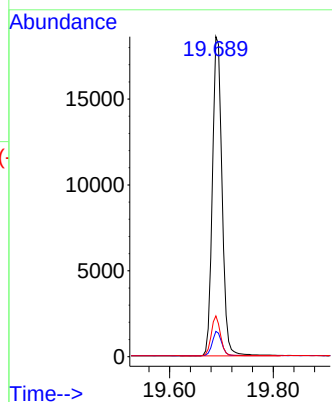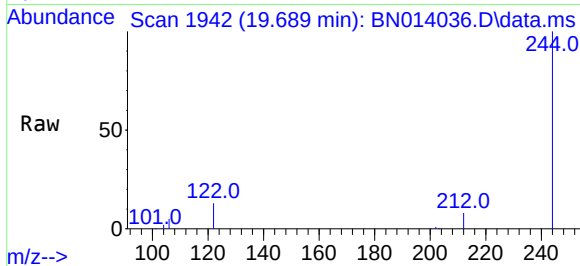

#32
Benzo(a)anthracene
Concen: 0.42 ng
RT: 21.218 min Scan# 2120
Delta R.T. -0.011 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:228 Resp: 28722
Ion Ratio Lower Upper
228 100
226 27.5 20.5 30.7
229 19.4 16.2 24.4


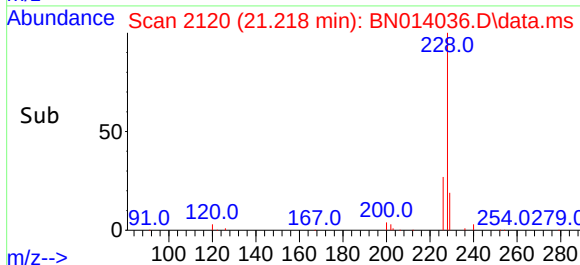

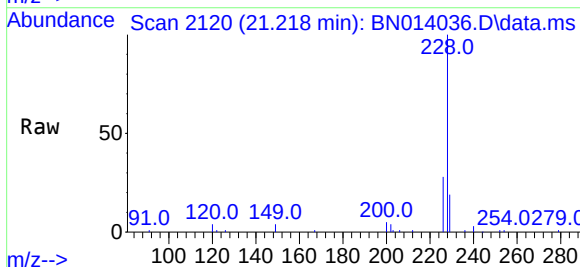


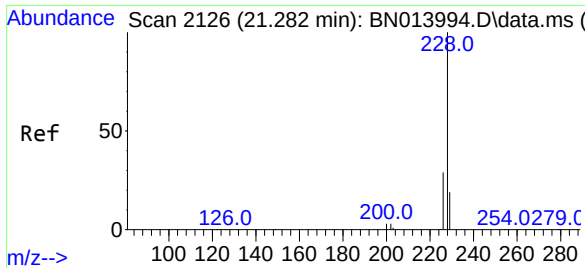

#33
Chrysene
Concen: 0.47 ng
RT: 21.271 min Scan# 2125
Delta R.T. -0.011 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	228	Resp:	34624
Ion Ratio	Lower	Upper	
228	100		
226	30.5	24.3	36.5
229	19.1	15.1	22.7

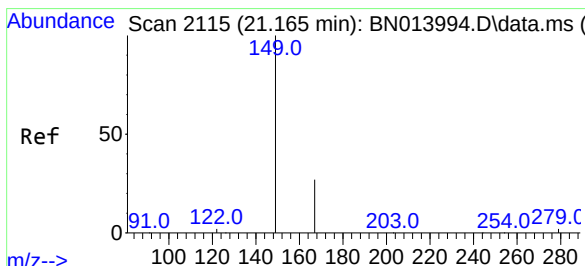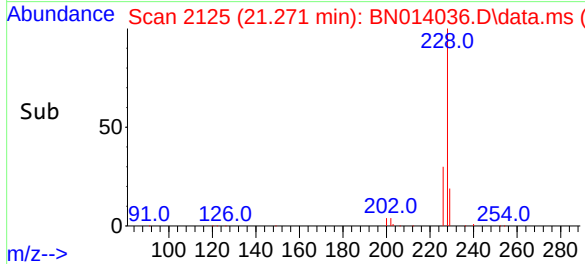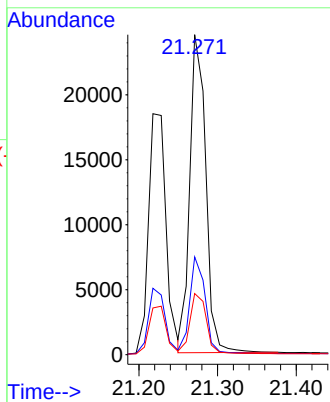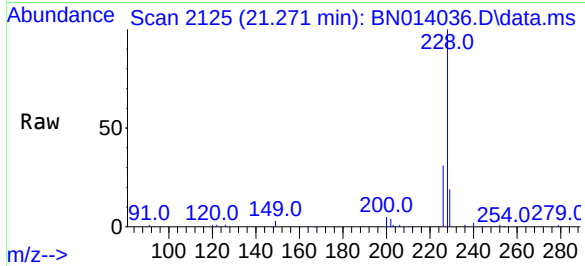

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.32 ng
RT: 21.154 min Scan# 2114
Delta R.T. -0.011 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:	149	Resp:	8295
Ion Ratio	Lower	Upper	
149	100		
167	27.0	22.1	33.1
279	4.5	3.5	5.3


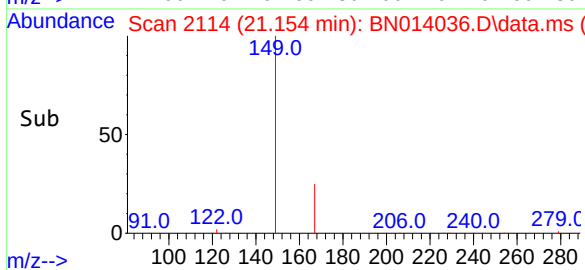

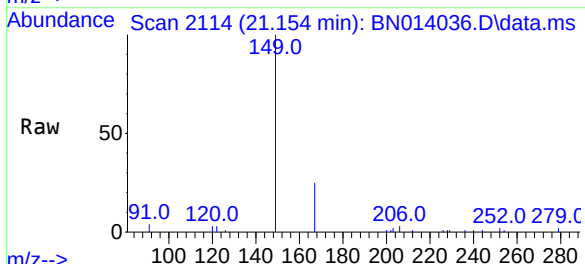




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.47 ng
RT: 25.652 min Scan# 3180
Delta R.T. -0.021 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:276 Resp: 38116
Ion Ratio Lower Upper
276 100
138 24.1 19.8 29.6
277 25.1 19.9 29.9



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.448 min Scan# 2536
Delta R.T. -0.011 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:264 Resp: 23055
Ion Ratio Lower Upper
264 100
260 24.5 19.3 28.9
265 35.5 66.2 99.4#

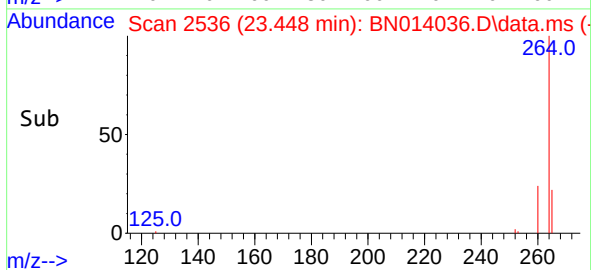



#37

Benzo(b)fluoranthene

Concen: 0.42 ng

RT: 22.784 min Scan# 2342





Delta R.T. -0.011 min

Lab File: BN014036.D

Acq: 23 Mar 2021 10:25

Tgt Ion:252	Resp:	35244
Ion Ratio	Lower	Upper
252	100	
253	24.4	20.4 30.6
125	11.8	11.6 17.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



#38

Benzo(k)fluoranthene

Concen: 0.42 ng




RT: 22.828 min Scan# 2355


Delta R.T. -0.011 min

Lab File: BN014036.D

Acq: 23 Mar 2021 10:25

Tgt Ion:252	Resp:	34579
Ion Ratio	Lower	Upper
252	100	
253	24.3	20.5 30.7
125	11.2	12.3 18.5#



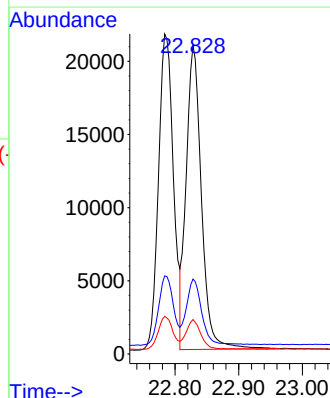
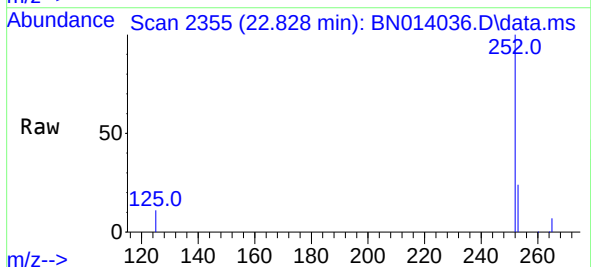




#39
Benzo(a)pyrene
Concen: 0.43 ng
RT: 23.352 min Scan# 2508
Delta R.T. -0.011 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 30770
Ion Ratio Lower Upper
252 100
253 25.7 21.8 32.6
125 13.3 14.6 21.8#

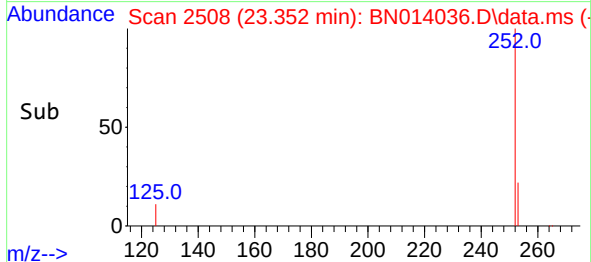

#40
Dibenzo(a,h)anthracene
Concen: 0.42 ng
RT: 25.669 min Scan# 3185
Delta R.T. -0.018 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Tgt Ion:278 Resp: 32350
Ion Ratio Lower Upper
278 100
139 16.8 13.1 19.7
279 24.9 21.4 32.0

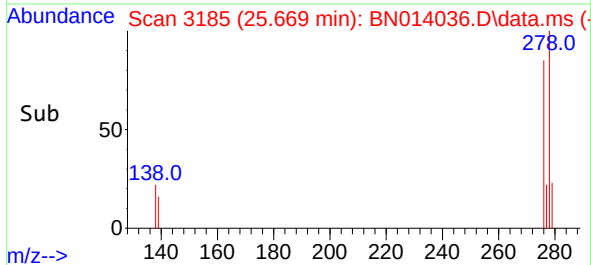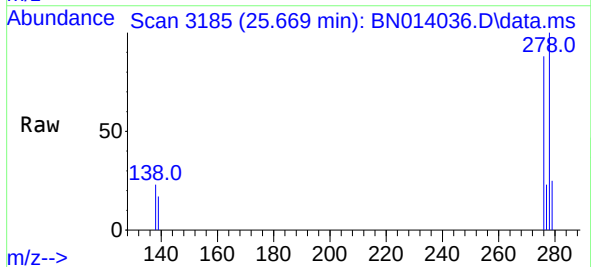

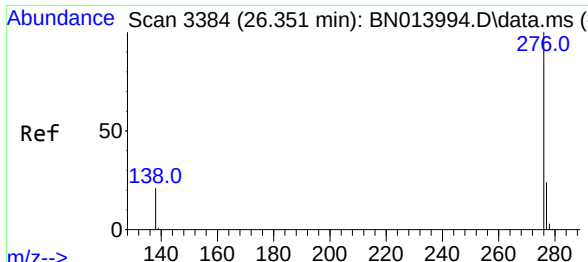

#41
Benzo(g,h,i)perylene
Concen: 0.43 ng
RT: 26.330 min Scan# 3378
Delta R.T. -0.021 min
Lab File: BN014036.D
Acq: 23 Mar 2021 10:25

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 34745
Ion Ratio Lower Upper
276 100
277 24.1 20.0 30.0
138 20.8 17.8 26.8

