
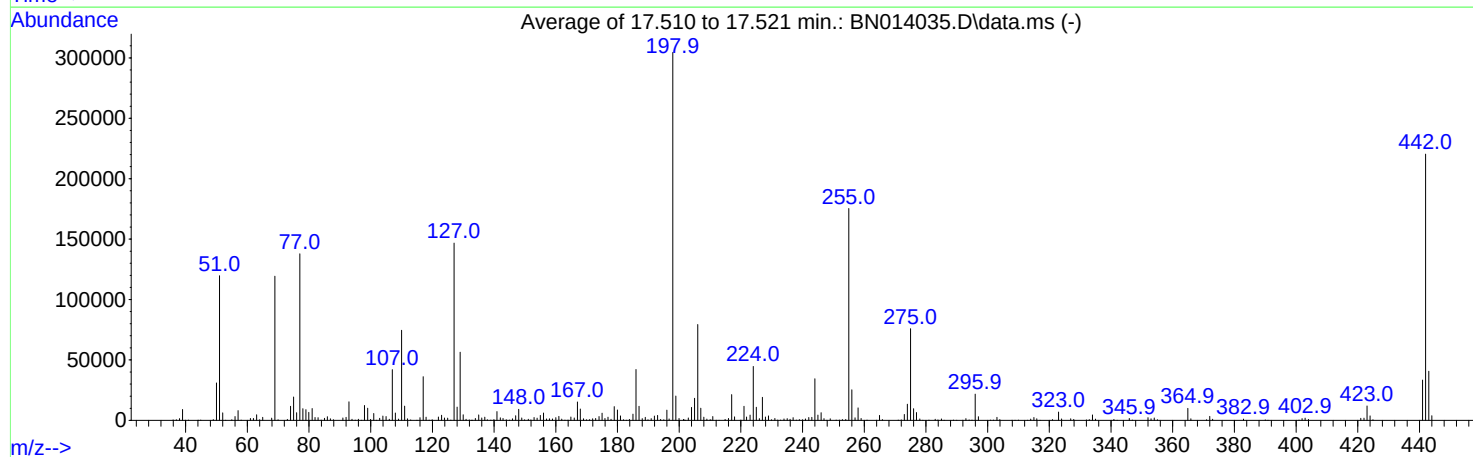


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
 Data File : BN014035.D
 Acq On : 23 Mar 2021 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

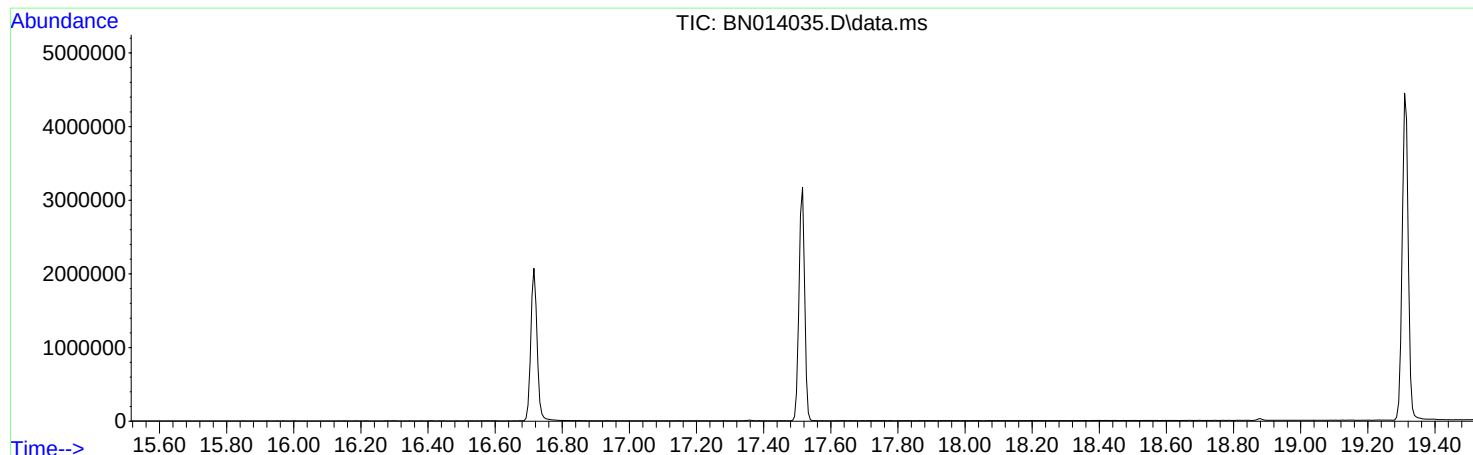




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	119763	PASS
68	69	0.00	2	1.5	1826	PASS
69	198	0.00	100	39.2	119336	PASS
70	69	0.00	2	0.5	571	PASS
127	198	10	80	48.2	146789	PASS
197	198	0.00	2	0.4	1230	PASS
198	198	100	100	100.0	304448	PASS
199	198	5	9	6.6	20092	PASS
275	198	10	60	24.9	75917	PASS
365	198	1	100	3.3	9943	PASS
441	198	0.01	100	11.0	33432	PASS
442	442	50	100	100.0	220352	PASS
443	442	15	24	18.5	40699	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
Data File : BN014035.D
Acq On : 23 Mar 2021 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 10:34:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

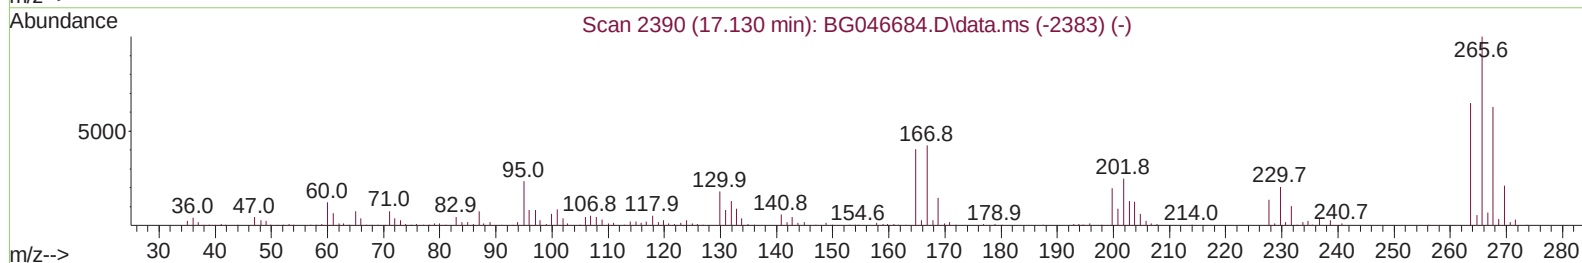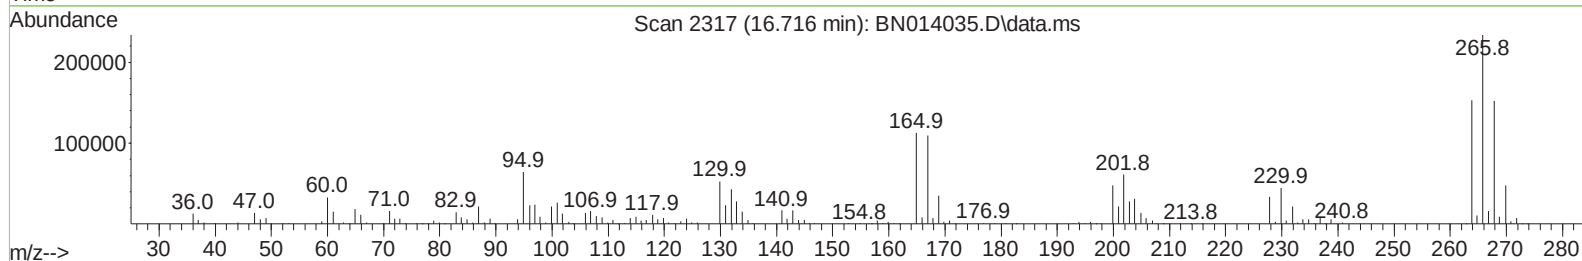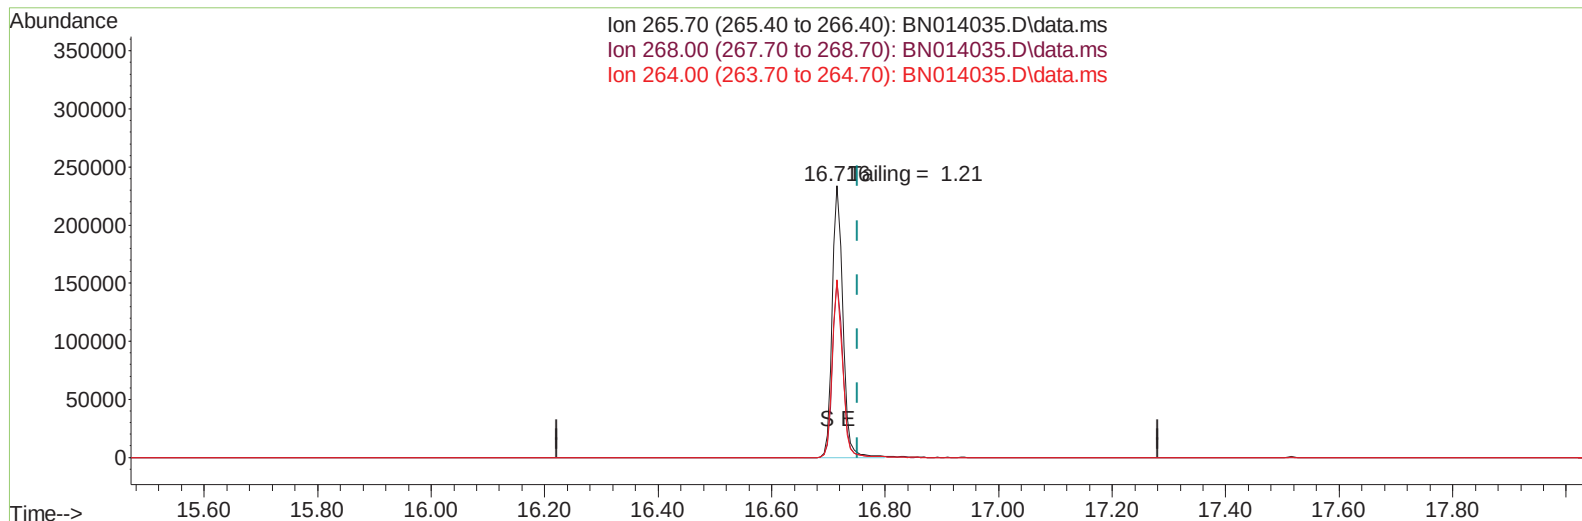

TIC: BN014035.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.035) 19139.53 ng




response 307464

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.01
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
Data File : BN014035.D
Acq On : 23 Mar 2021 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 23 10:34:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:12:06 2021
Response via : Initial Calibration

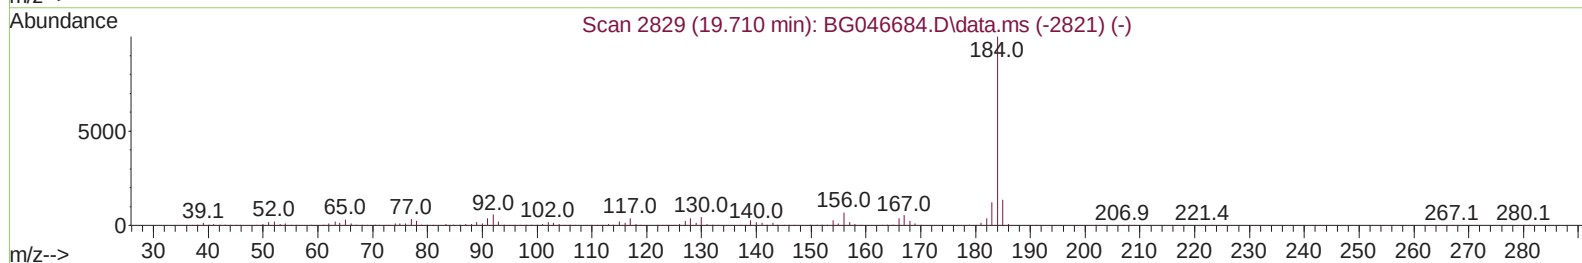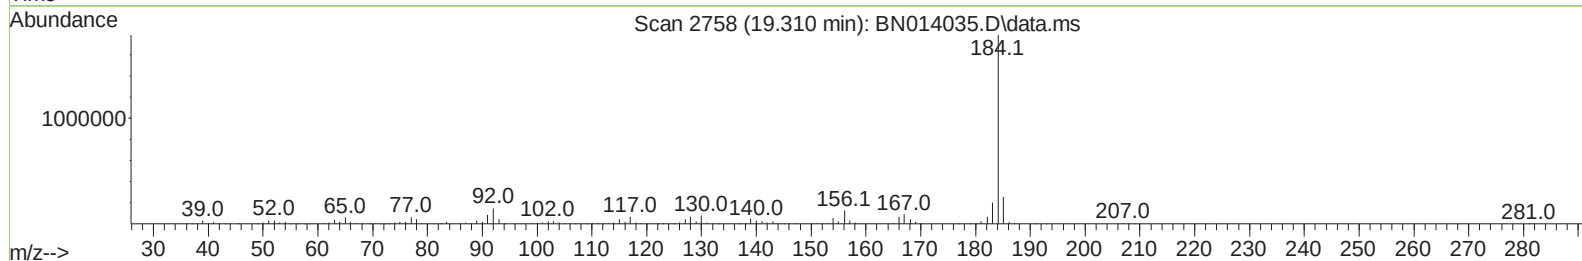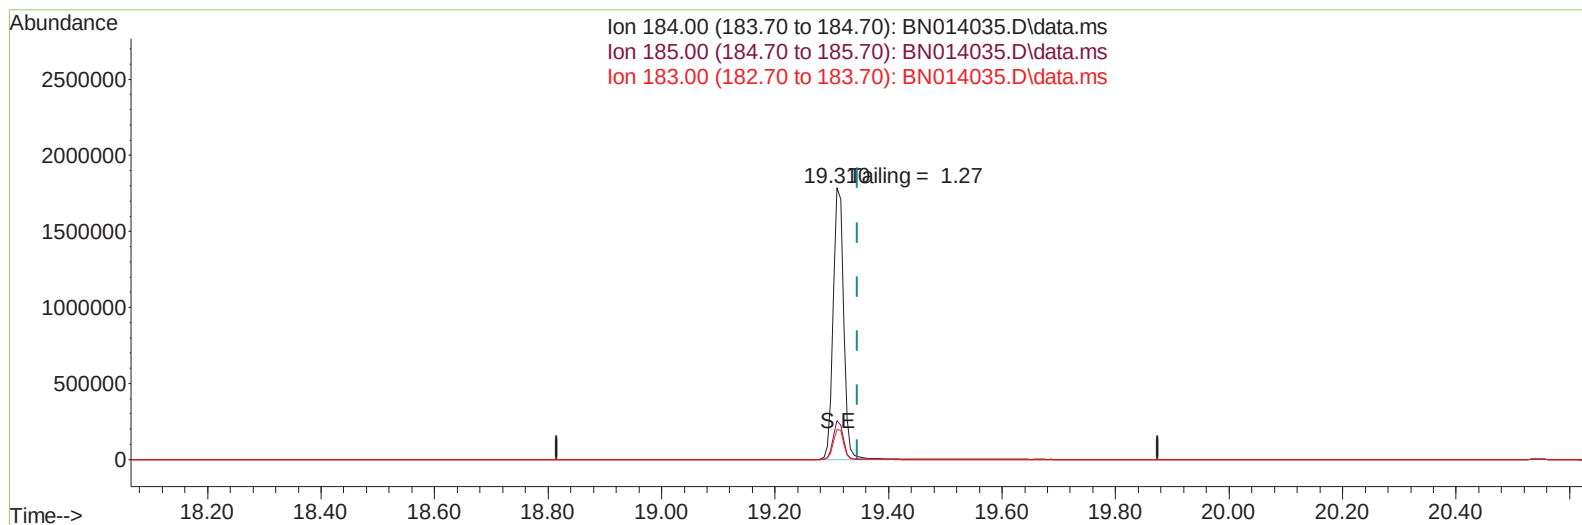

TIC: BN014035.D\data.ms

(77) Benzidine

19.310min (-0.035) 0.00 ng

response 2282471

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/23/2021	BNA_N	<u>BN014035.D</u>
Compound Name	Response	Retention Time
DDT	1068394	20.545
DDD	4592	20.104
DDE	1172	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5764	1074158	0.54