


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
 Data File : BN014052.D
 Acq On : 23 Mar 2021 21:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

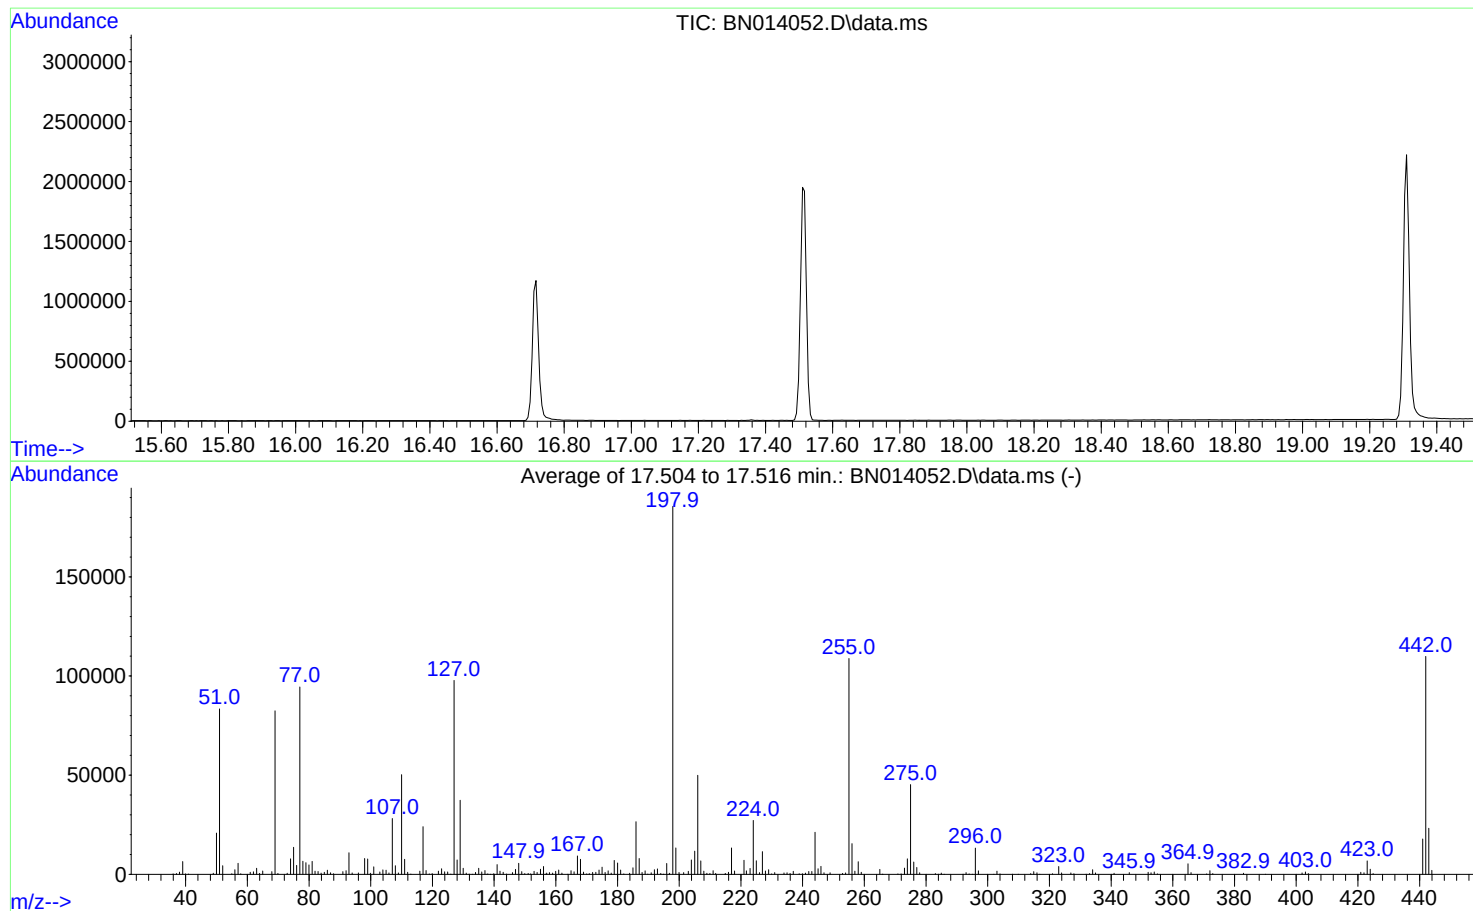




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	83461	PASS
68	69	0.00	2	1.6	1356	PASS
69	198	0.00	100	44.5	82477	PASS
70	69	0.00	2	0.6	481	PASS
127	198	10	80	52.7	97752	PASS
197	198	0.00	2	0.3	603	PASS
198	198	100	100	100.0	185475	PASS
199	198	5	9	7.2	13282	PASS
275	198	10	60	24.4	45264	PASS
365	198	1	100	2.9	5363	PASS
441	198	0.01	100	9.6	17846	PASS
442	442	50	100	100.0	109845	PASS
443	442	15	24	21.2	23267	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
Data File : BN014052.D
Acq On : 23 Mar 2021 21:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 24 04:12:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 07:31:37 2021
Response via : Initial Calibration

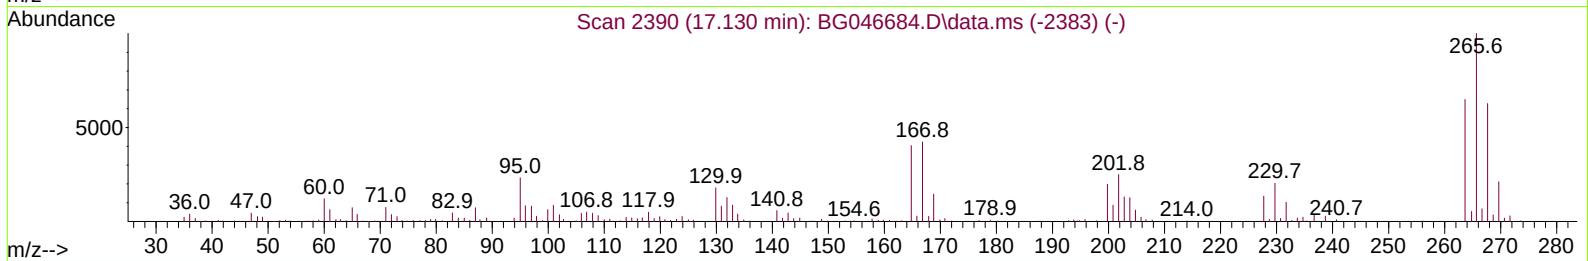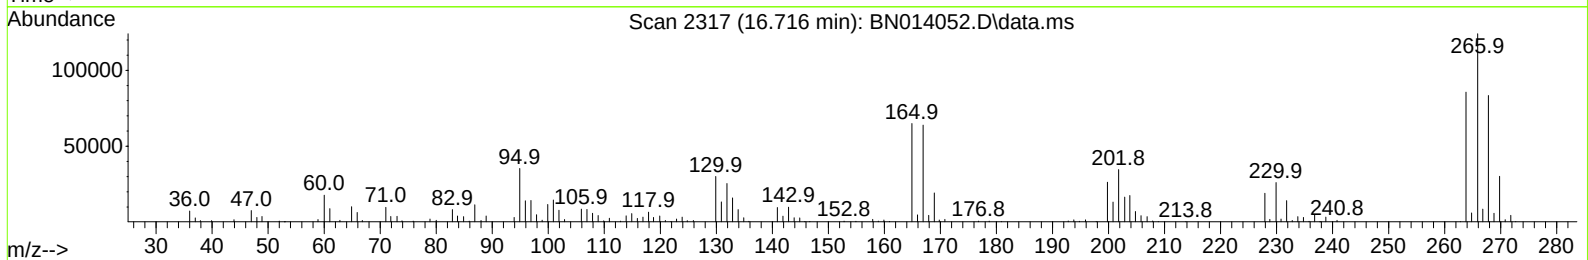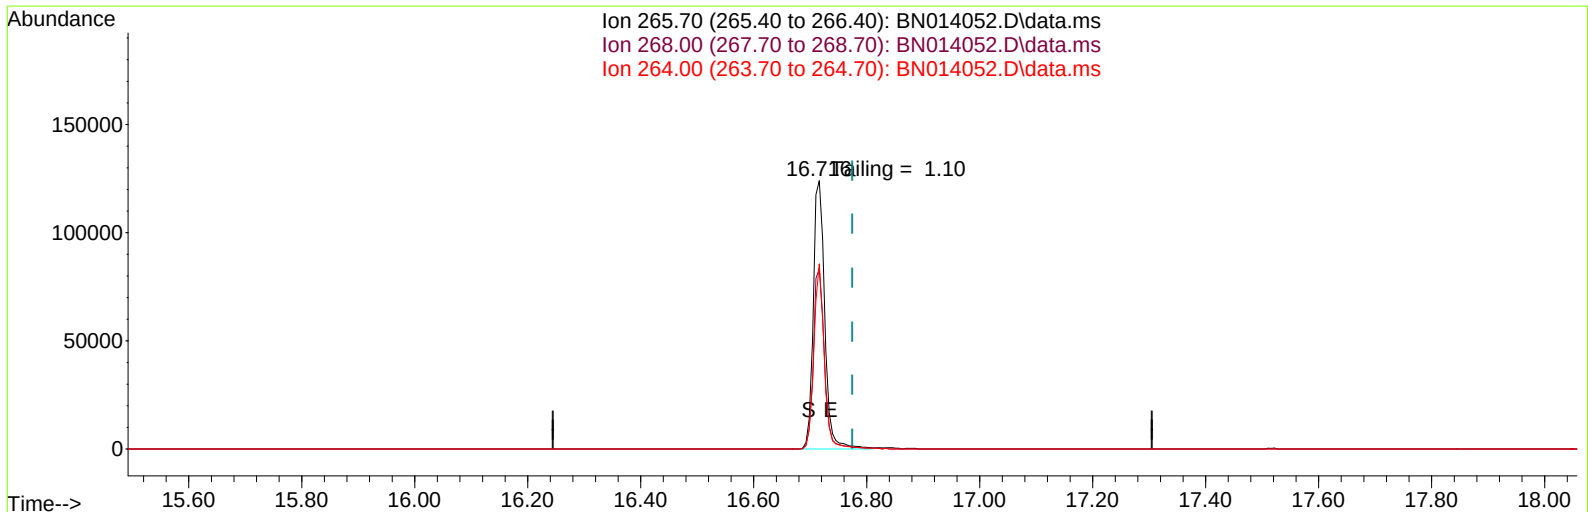

TIC: BN014052.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.059) 17928.70 ng




response 174890

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.28
264.00	61.60	68.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032321\
 Data File : BN014052.D
 Acq On : 23 Mar 2021 21:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 24 04:12:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 07:31:37 2021
 Response via : Initial Calibration

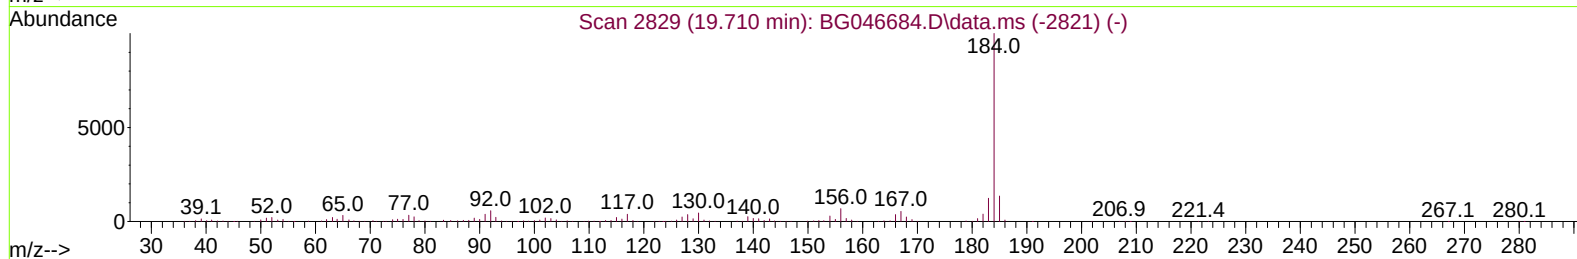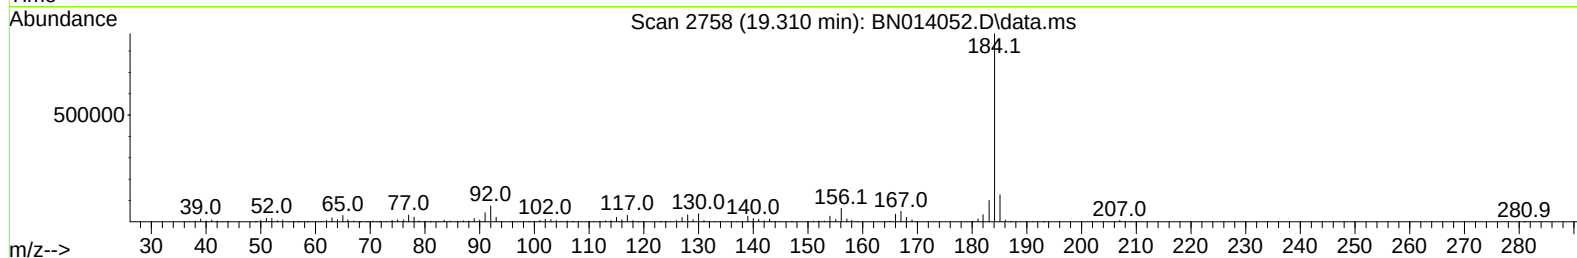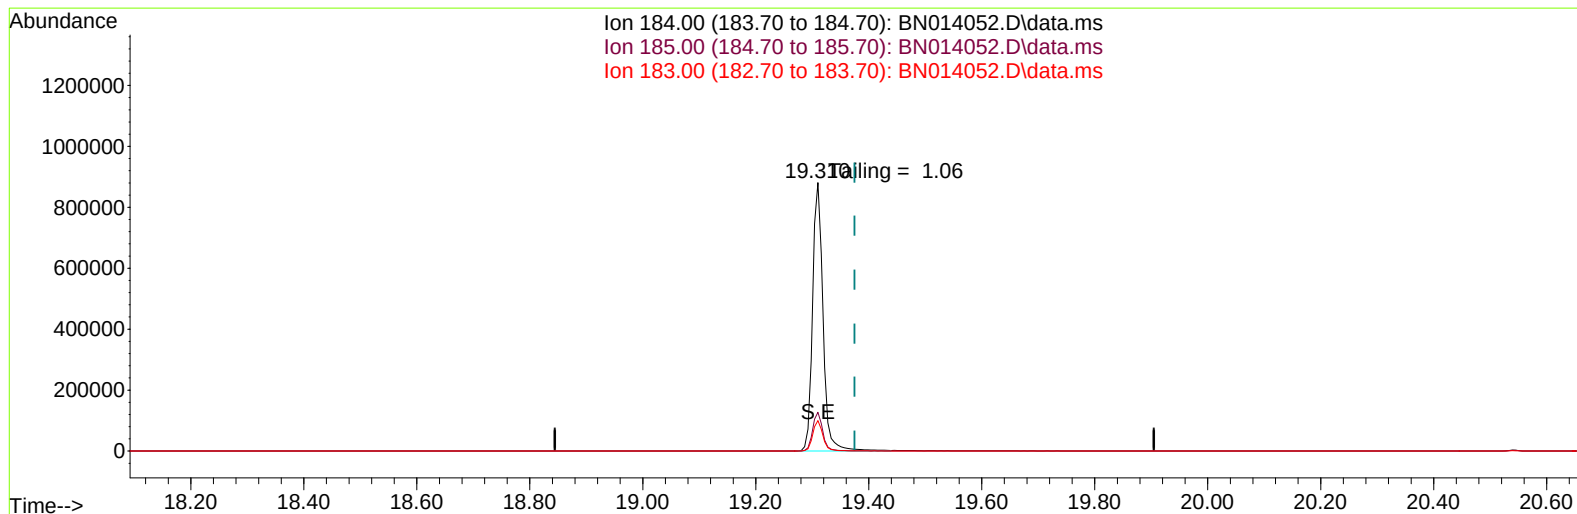

TIC: BN014052.D\data.ms

(77) Benzidine

19.310min (-0.065) 0.00 ng

response 1135423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/23/2021	BNA_N	<u>BN014052.D</u>
Compound Name	Response	Retention Time
DDT	671023	20.545
DDD	4959	20.104
DDE	1324	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6283	677306	0.93