
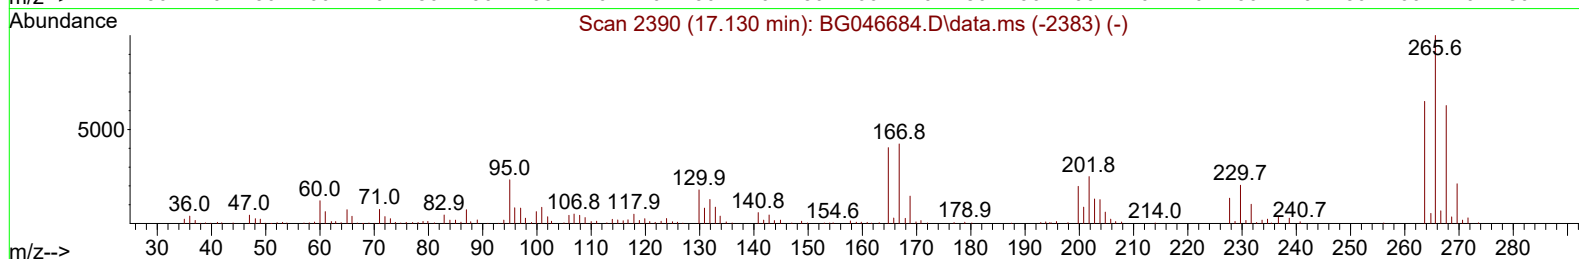
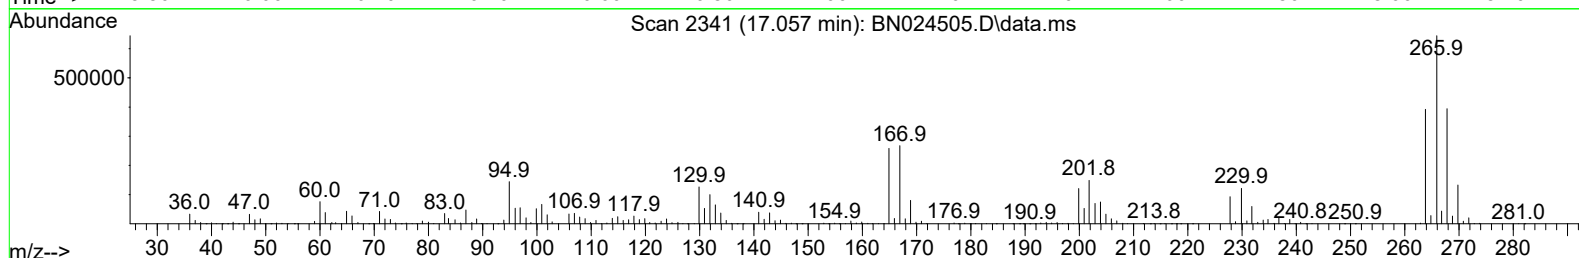


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032323\  
Data File : BN024505.D  
Acq On : 23 Mar 2023 09:41  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 07:47:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 24 07:47:00 2023  
Response via : Initial Calibration

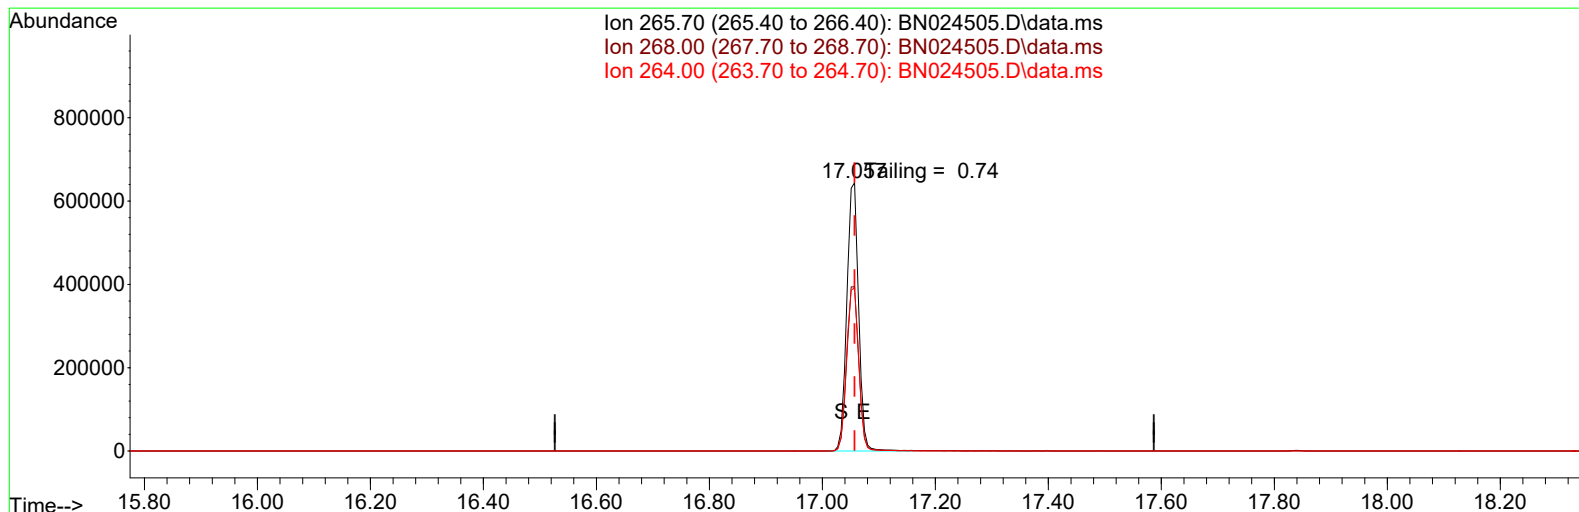

TIC: BN024505.D\data.ms

**(70) Pentachlorophenol (C)**




17.057min ( 0.000) 27298.50 ng

response 934479

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.21  |
| 264.00 | 61.60  | 60.83  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032323\  
Data File : BN024505.D  
Acq On : 23 Mar 2023 09:41  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 07:47:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 24 07:47:00 2023  
Response via : Initial Calibration

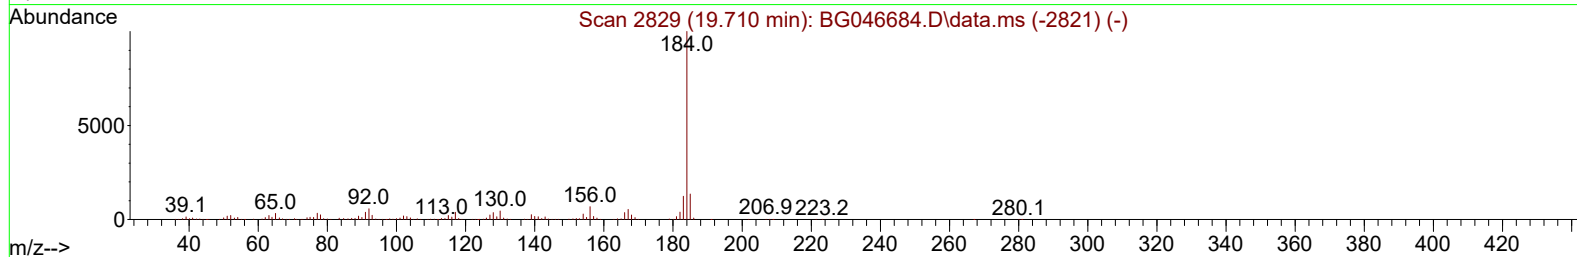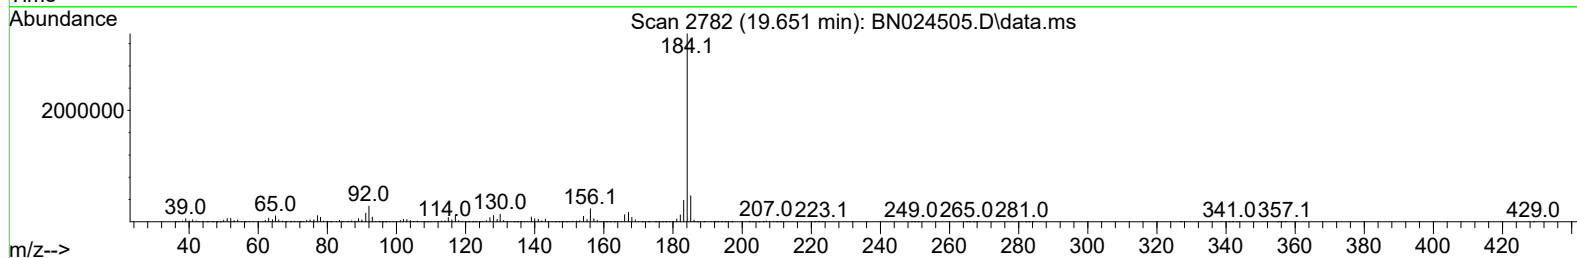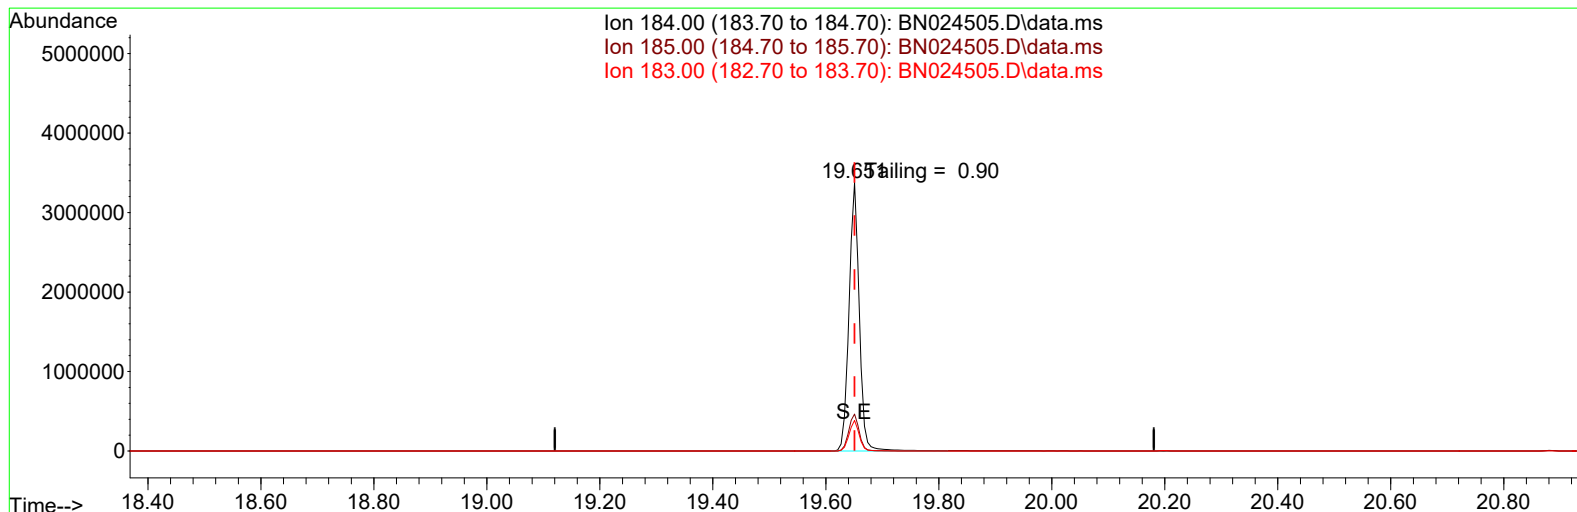

TIC: BN024505.D\data.ms

**(77) Benzidine**

19.651min ( 0.000) 1933907.47 ng

response 4292166

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.82  |
| 183.00 | 13.20  | 11.37  |
| 0.00   | 0.00   | 0.00   |