
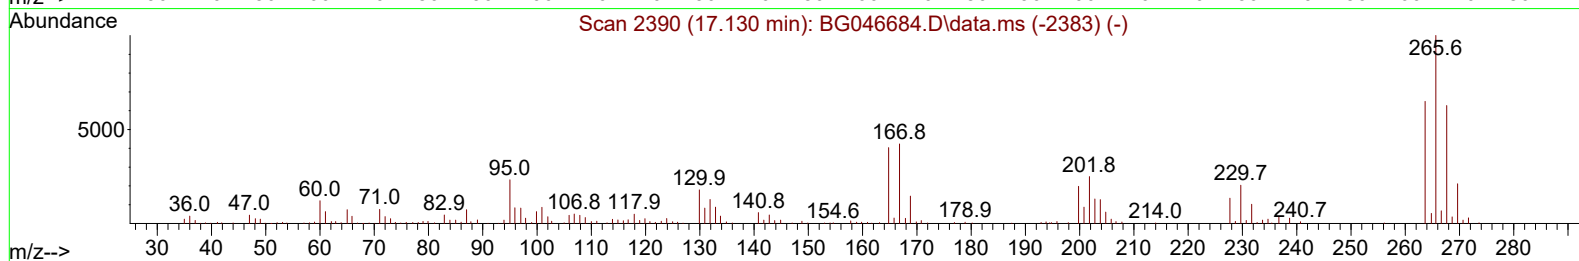
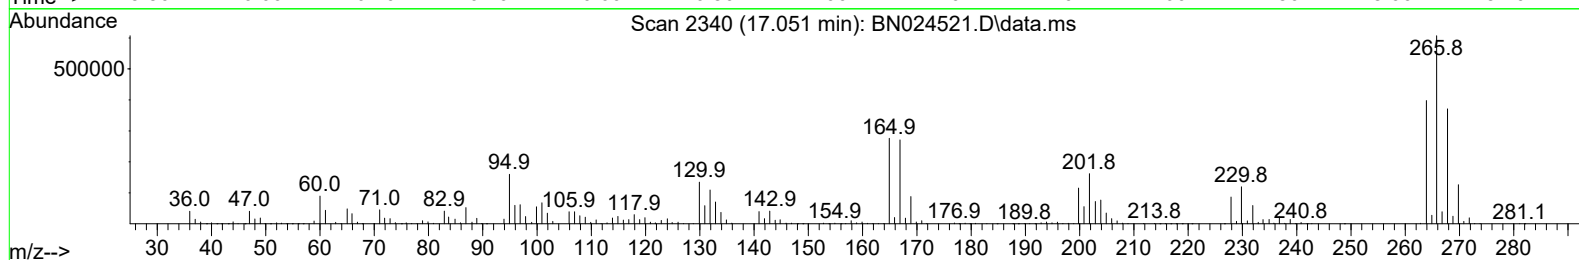


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\  
Data File : BN024521.D  
Acq On    : 23 Mar 2023   22:35  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Mar 24 07:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 24 07:47:00 2023
Response via : Initial Calibration

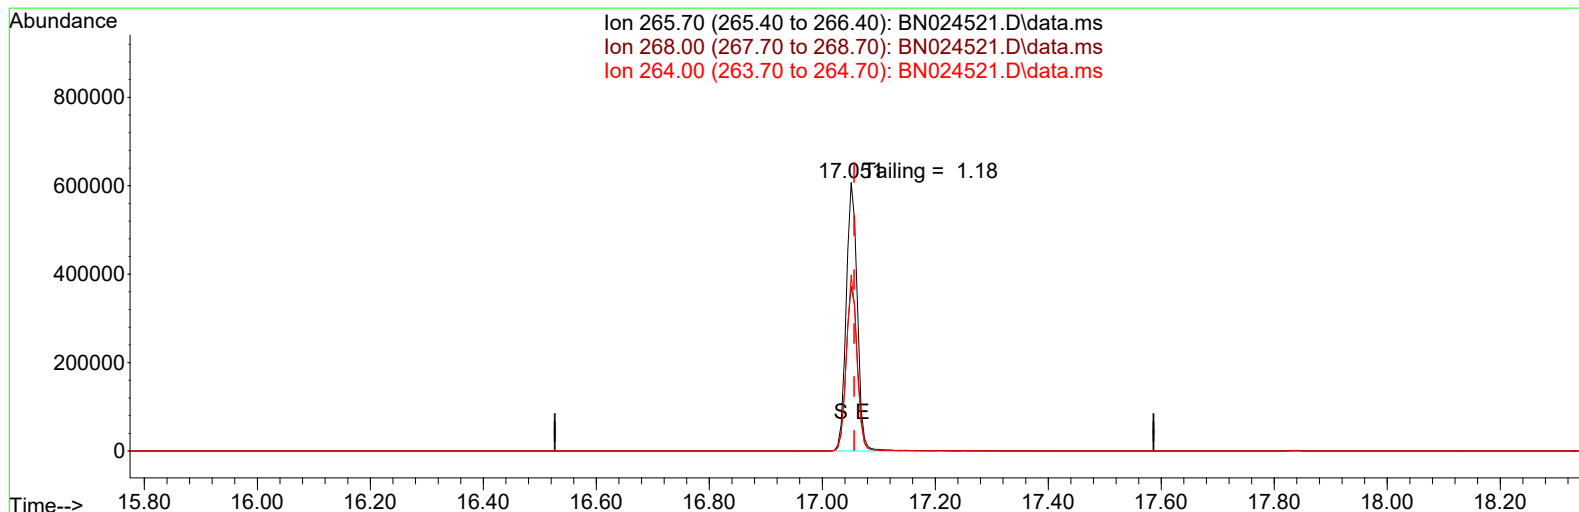

TIC: BN024521.D\data.ms

(70) Pentachlorophenol (C)




17.051min (-0.006) 26320.72 ng

response 832637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.15
264.00	61.60	65.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\
Data File : BN024521.D
Acq On : 23 Mar 2023 22:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 07:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 24 07:47:00 2023
Response via : Initial Calibration

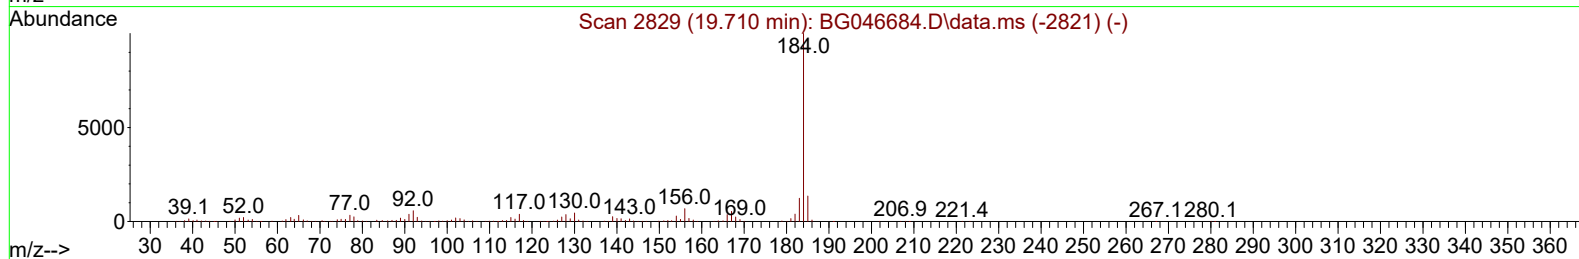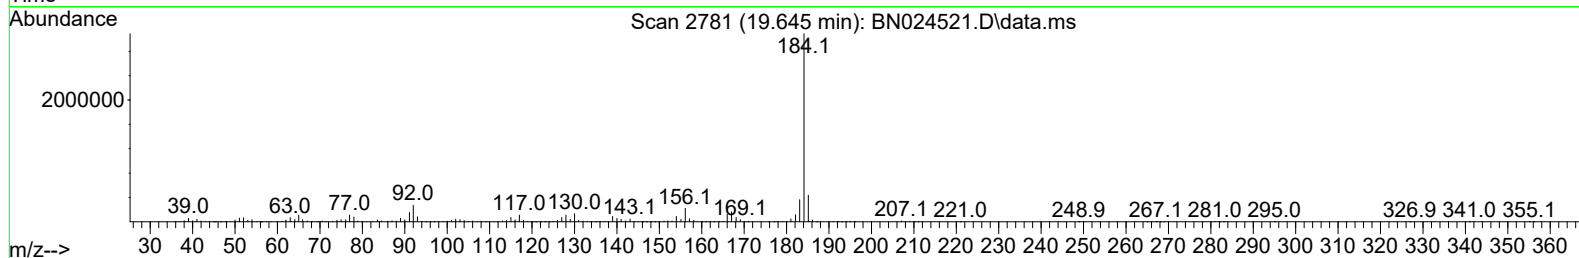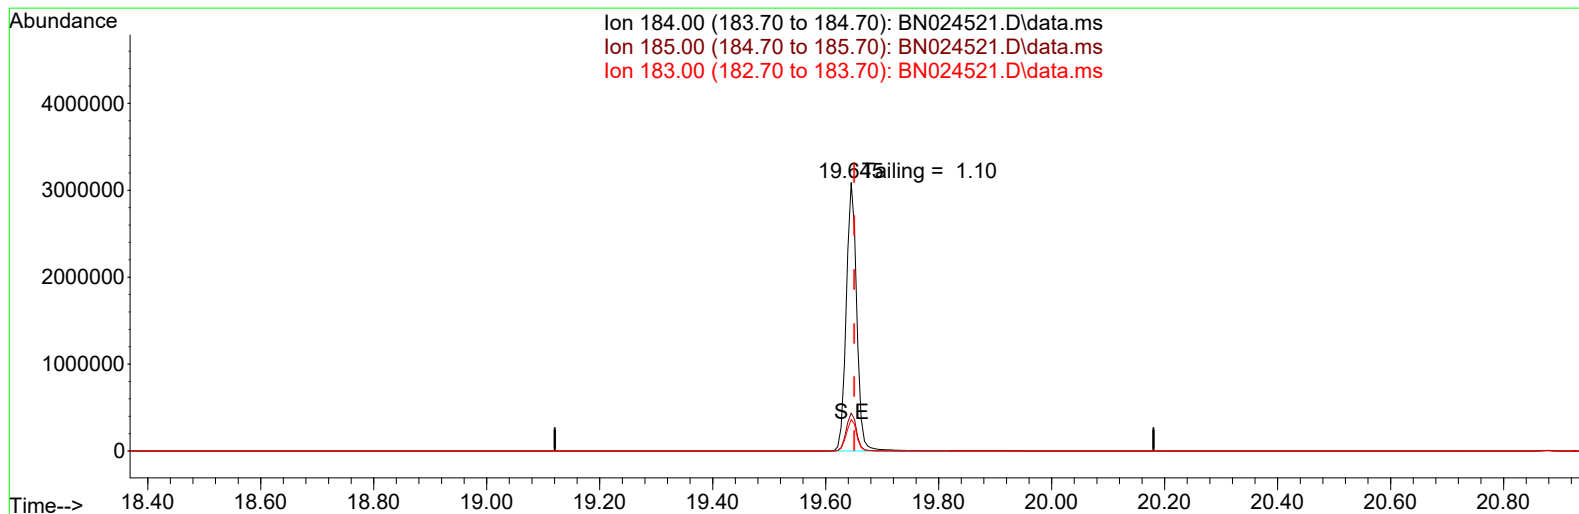

TIC: BN024521.D\data.ms

(77) Benzidine

19.645min (-0.006) 0.00 ng

response 3987787

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.79
0.00	0.00	0.00