

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\
 Data File : BN024535.D
 Acq On : 24 Mar 2023 07:43
 Operator : CG/JU
 Sample : 01941-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TT163S1-20230313

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

Quant Time: Mar 24 08:12:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 24 03:05:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.018	152	10531	0.400	ng	0.00
7) Naphthalene-d8	10.834	136	30296	0.400	ng	# 0.00
13) Acenaphthene-d10	14.654	164	15437	0.400	ng	0.00
19) Phenanthrene-d10	17.400	188	33535	0.400	ng	0.00
29) Chrysene-d12	21.583	240	19662	0.400	ng	# 0.00
35) Perylene-d12	24.085	264	15788	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.570	112	3946	0.169	ng	0.00
5) Phenol-d6	7.181	99	2692	0.090	ng	0.00
8) Nitrobenzene-d5	9.190	82	9559m	0.472	ng	0.00
11) 2-Methylnaphthalene-d10	12.418	152	16288	0.437	ng	0.00
14) 2,4,6-Tribromophenol	16.147	330	3033	0.384	ng	0.00
15) 2-Fluorobiphenyl	13.286	172	25487	0.437	ng	0.00
27) Fluoranthene-d10	19.429	212	34181	0.481	ng	0.00
31) Terphenyl-d14	20.016	244	19273	0.581	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.425	88	4230	0.369	ng	# 90
25) Phenanthrene	17.438	178	2062m	0.021	ng	
34) Bis(2-ethylhexyl)phtha...	21.484	149	3928	0.127	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\
Data File : BN024535.D
Acq On : 24 Mar 2023 07:43
Operator : CG/JU
Sample : 01941-07
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023


Quant Time: Mar 24 08:12:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 24 03:05:57 2023
Response via : Initial Calibration

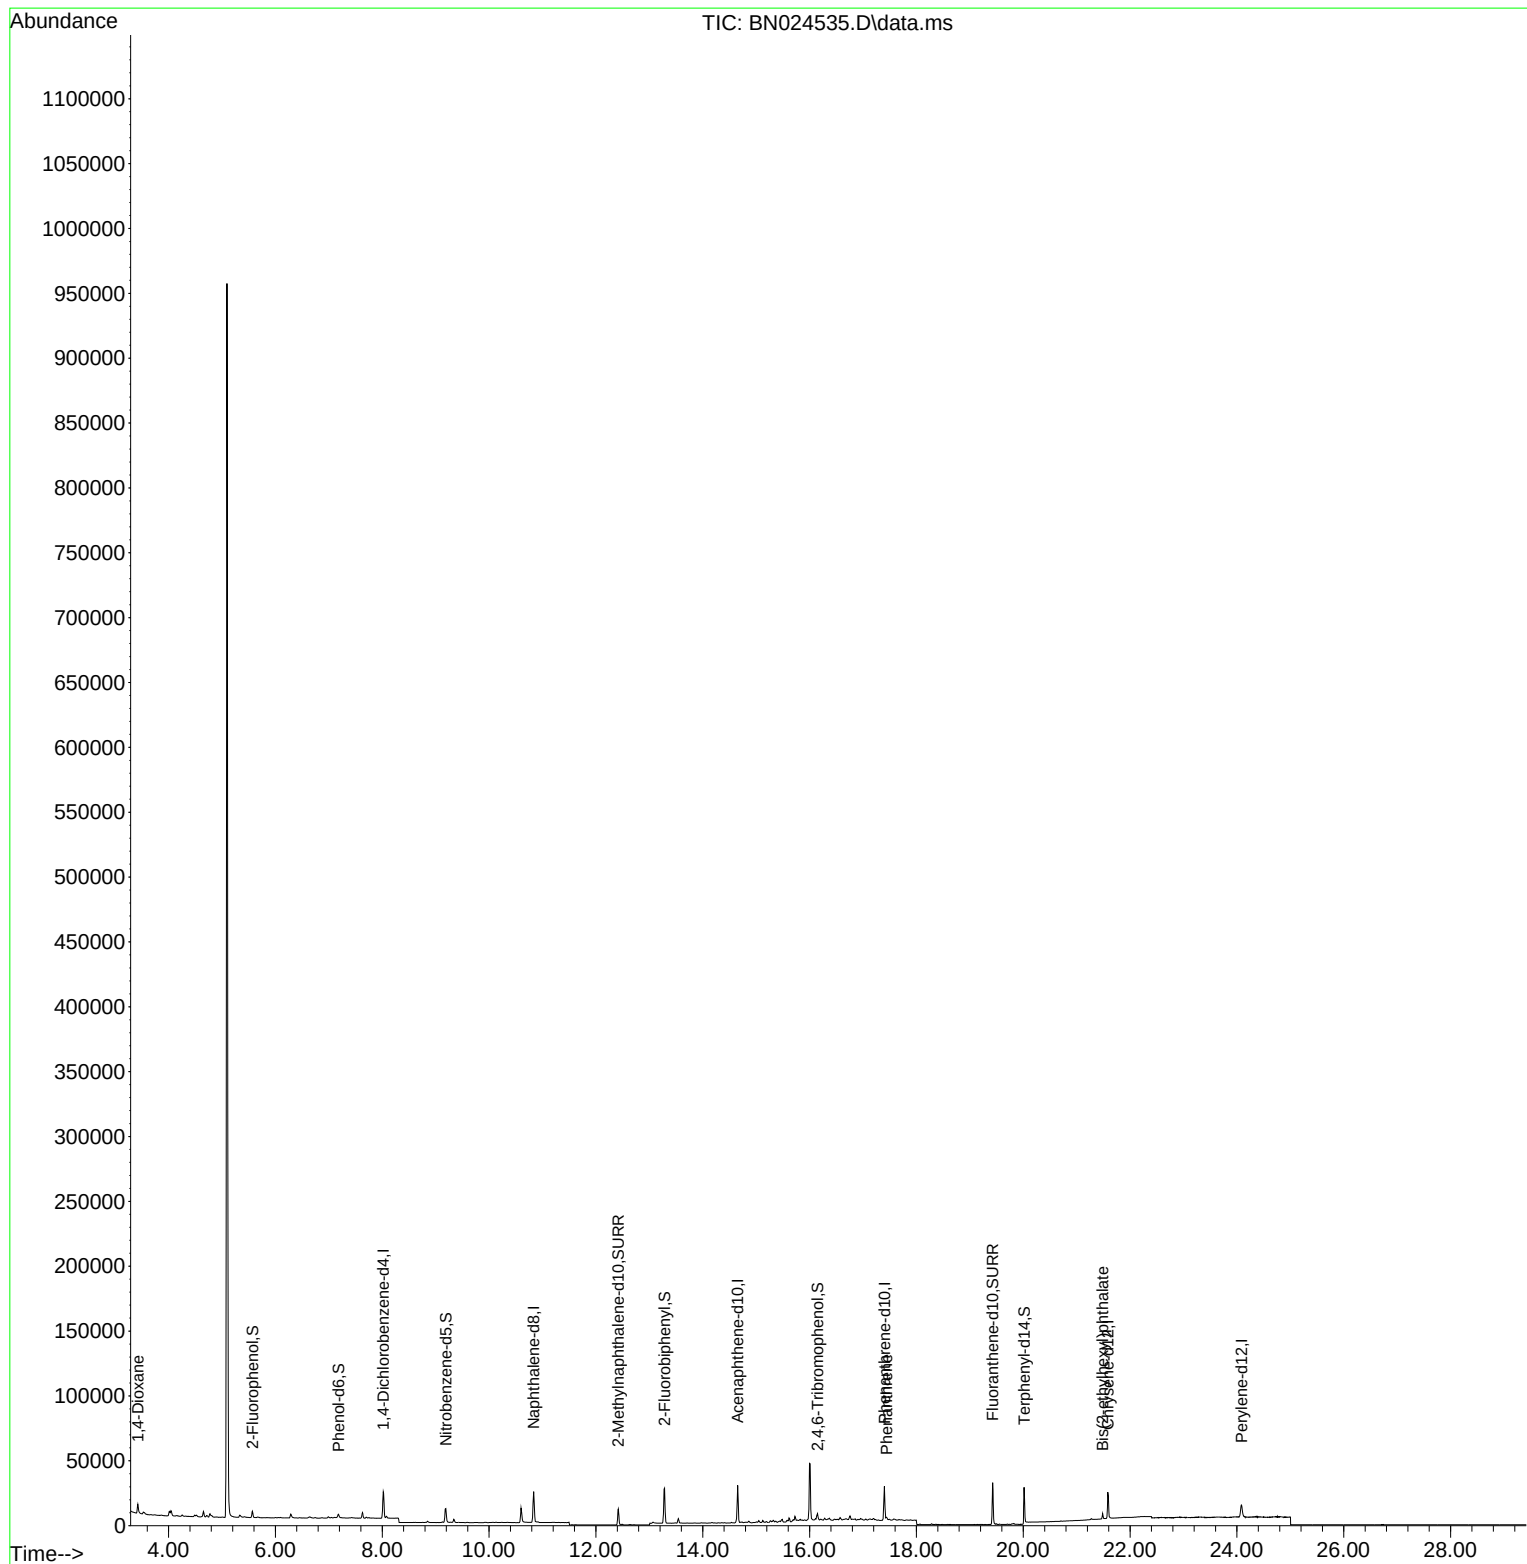

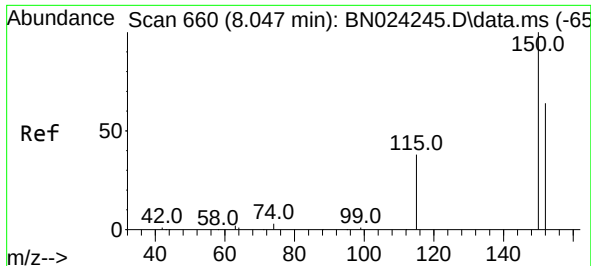

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.018 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43




Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

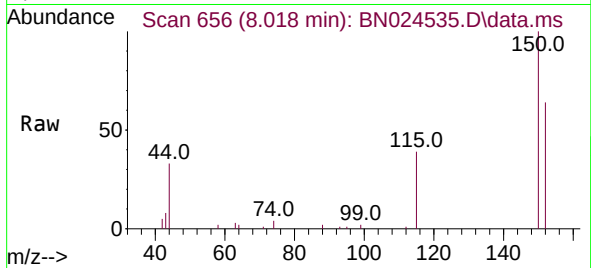

Tgt Ion: 152 Resp: 1053
Ion Ratio Lower Upper
152 100
150 157.0 124.7 187.1
115 61.6 49.1 73.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

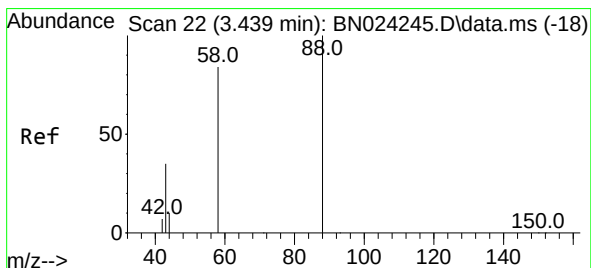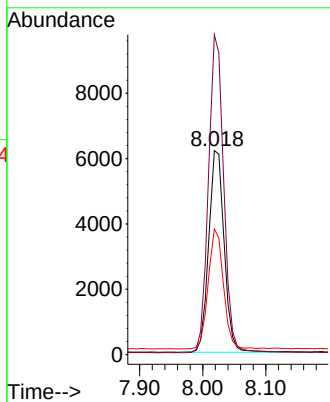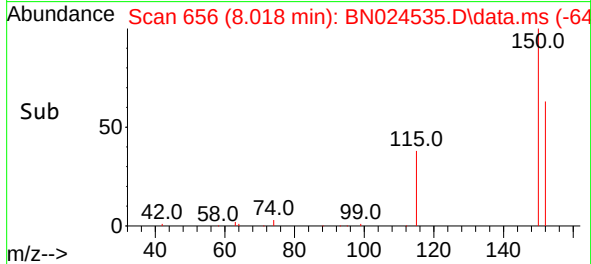

#2
1,4-Dioxane
Concen: 0.369 ng
RT: 3.425 min Scan# 20
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43


Tgt Ion: 88 Resp: 4230
Ion Ratio Lower Upper
88 100
43 55.3 29.0 43.4#
58 85.1 67.3 100.9

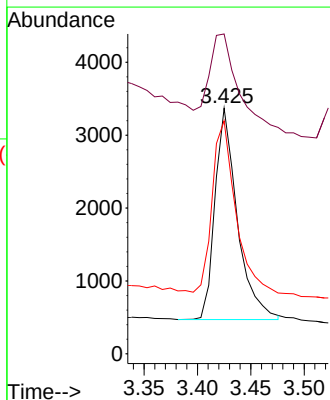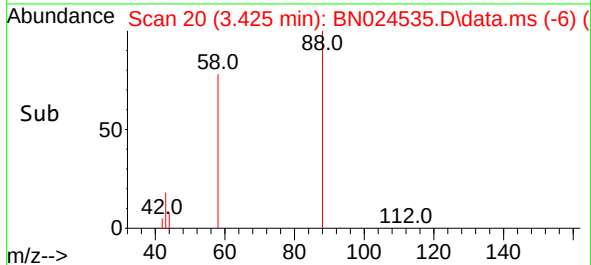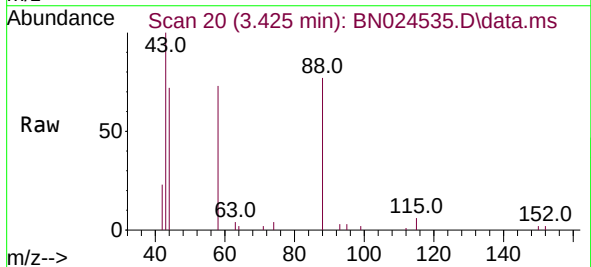

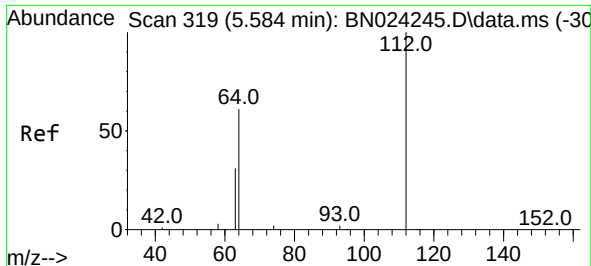

#4
2-Fluorophenol
Concen: 0.169 ng
RT: 5.570 min Scan# 319
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43




Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

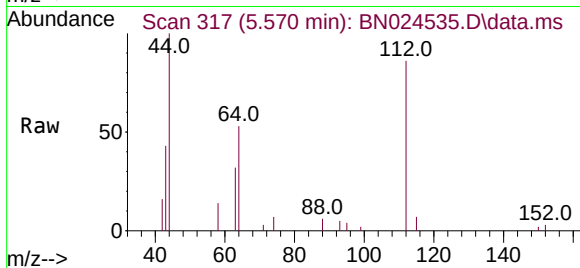

Tgt Ion: 112 Resp: 3946
Ion Ratio Lower Upper
112 100
64 62.4 49.0 73.6
63 33.9 25.7 38.5




Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 03/24/2023
Supervised By : Jagrut Upadhyay 03/24/2023

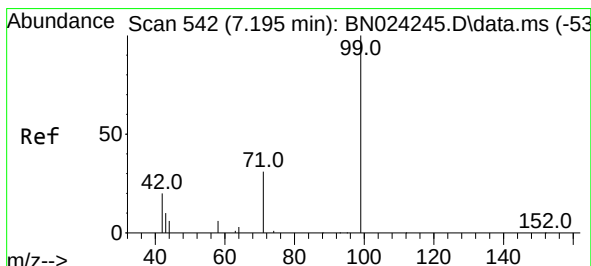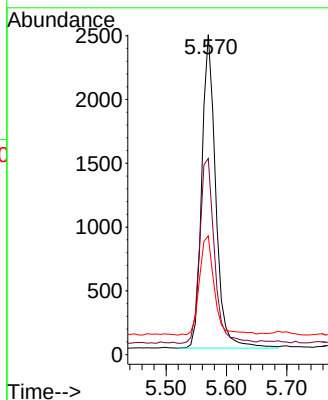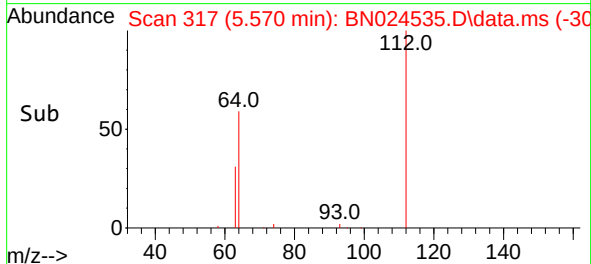

#5
Phenol-d6
Concen: 0.090 ng
RT: 7.181 min Scan# 540
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43


Tgt Ion: 99 Resp: 2692
Ion Ratio Lower Upper
99 100
42 27.2 20.1 30.1
71 39.2 25.8 38.8#

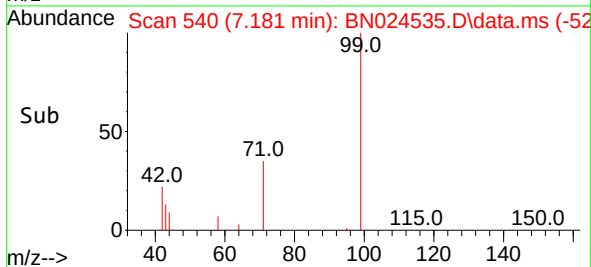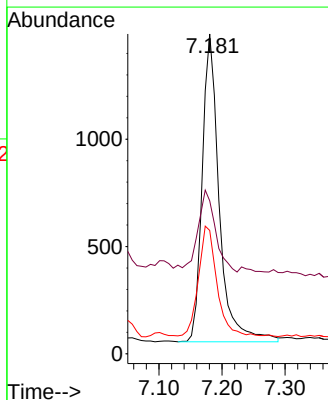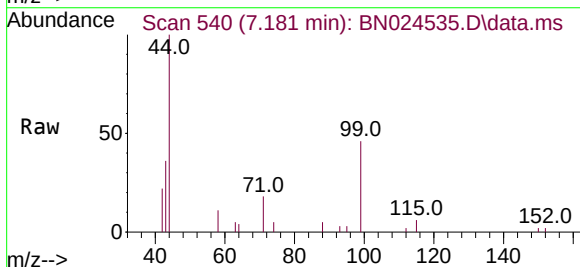

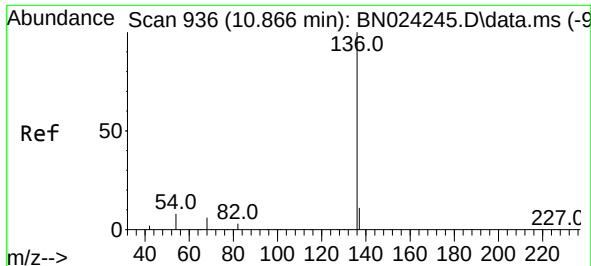

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.834 min Scan# 936
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43




Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

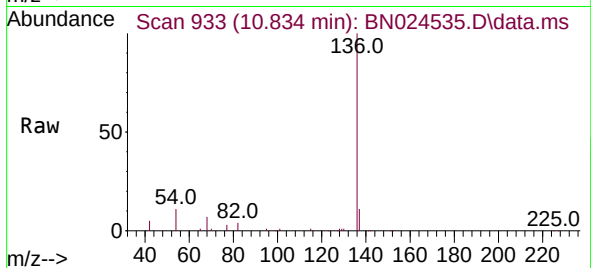

Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	10.9	7.1	10.7
68	7.5	5.3	7.9




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

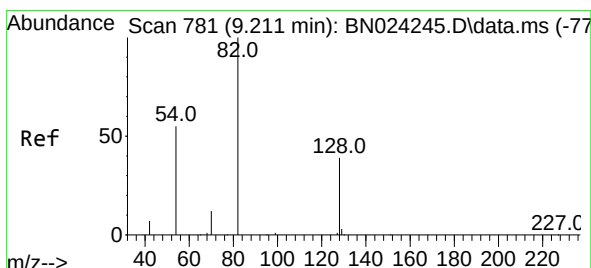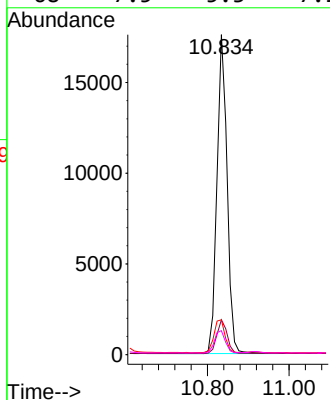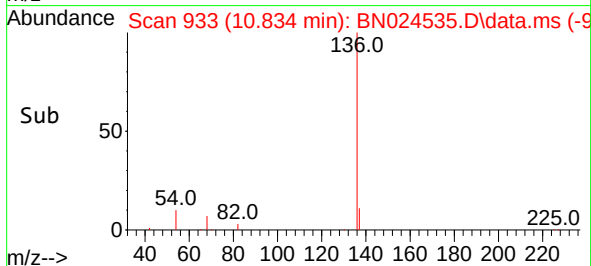

#8
Nitrobenzene-d5
Concen: 0.472 ng m
RT: 9.190 min Scan# 779
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43


Tgt Ion	Ratio	Lower	Upper
82	100		
128	44.0	32.4	48.6
54	56.5	45.2	67.8

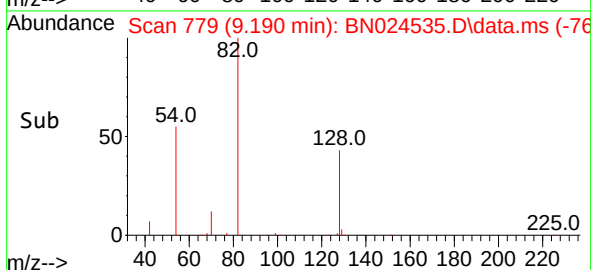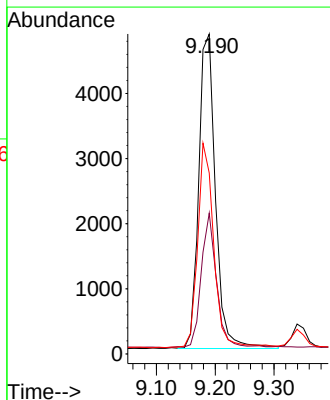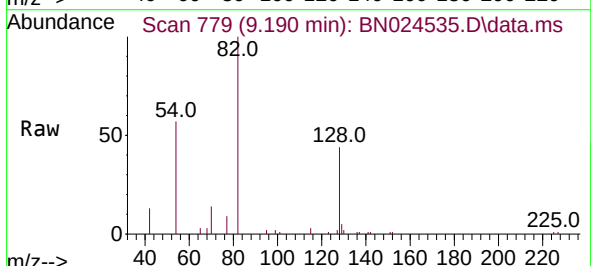

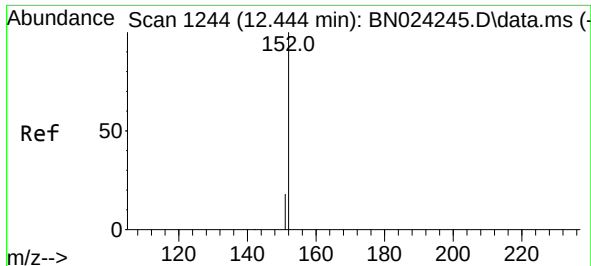

#11
2-Methylnaphthalene-d10
Concen: 0.437 ng
RT: 12.418 min Scan# 1237
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43




Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

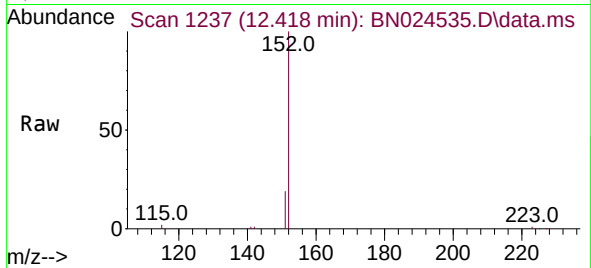


Tgt Ion:152 Resp: 16288
Ion Ratio Lower Upper
152 100
151 20.9 16.8 25.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

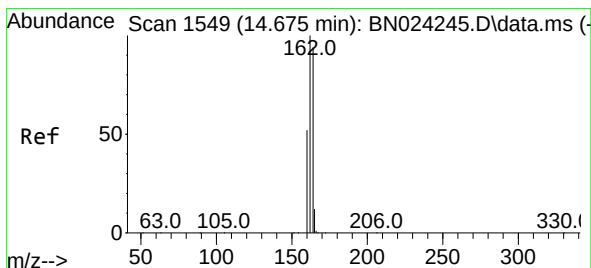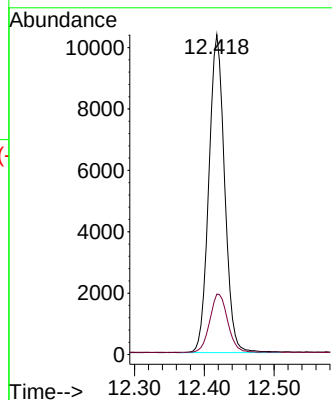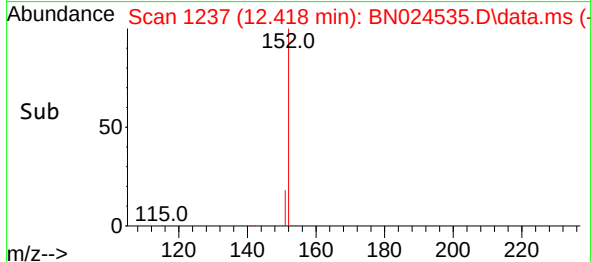


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.654 min Scan# 1547
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43

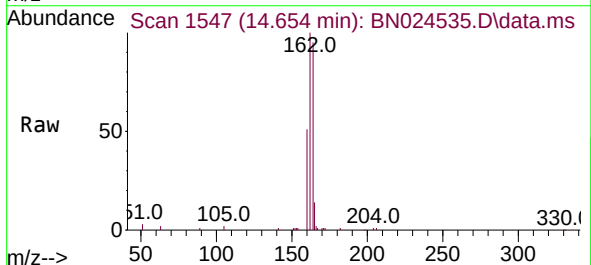


Tgt Ion:164 Resp: 15437
Ion Ratio Lower Upper
164 100
162 105.0 84.7 127.1
160 53.3 44.6 66.8

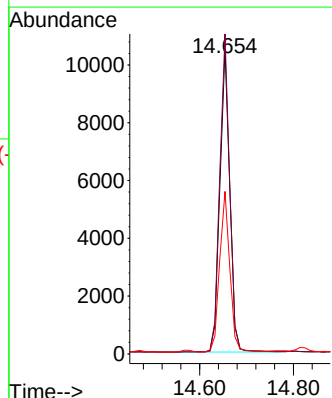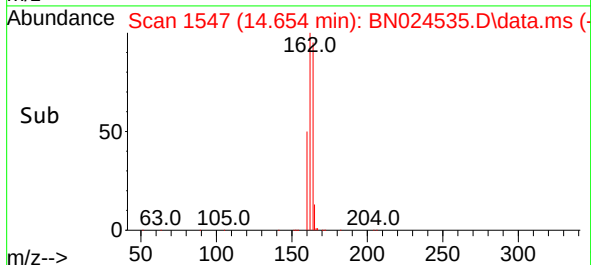

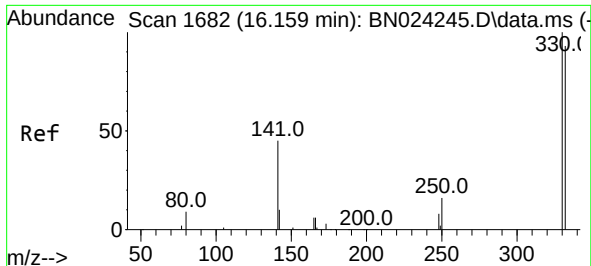

#14
2,4,6-Tribromophenol
Concen: 0.384 ng
RT: 16.147 min Scan# 1682
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43




Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

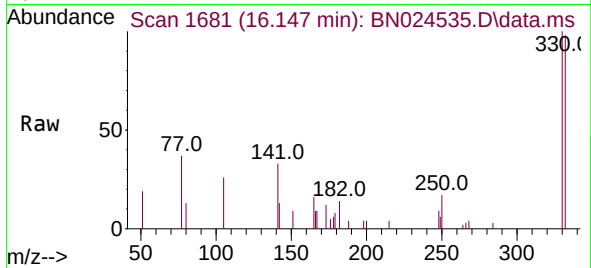

Tgt Ion: 330 Resp: 3033
Ion Ratio Lower Upper
330 100
332 96.3 78.0 117.0
141 38.9 30.8 46.2




Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 03/24/2023
Supervised By : Jagrut Upadhyay 03/24/2023

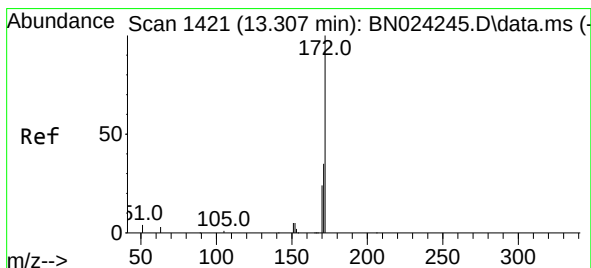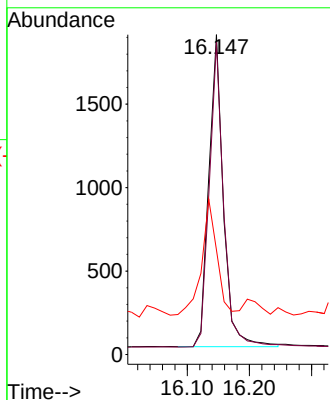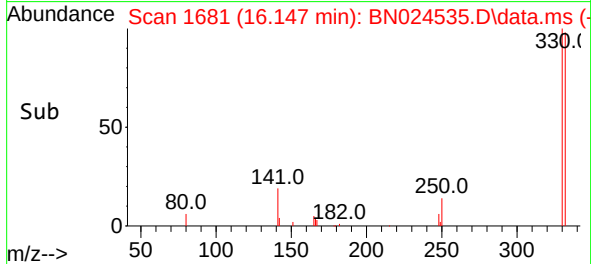

#15
2-Fluorobiphenyl
Concen: 0.437 ng
RT: 13.286 min Scan# 1419
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43

Tgt Ion: 172 Resp: 25487
Ion Ratio Lower Upper
172 100
171 34.1 27.8 41.8
170 22.7 19.0 28.6

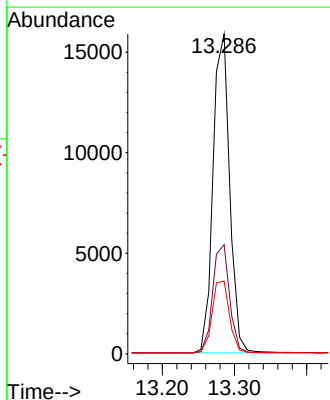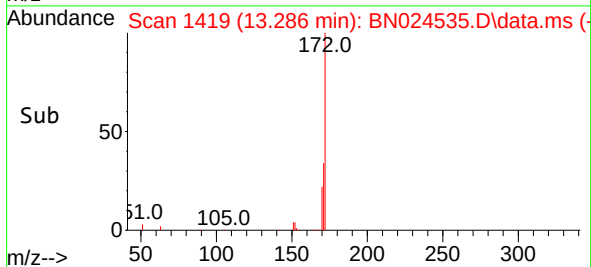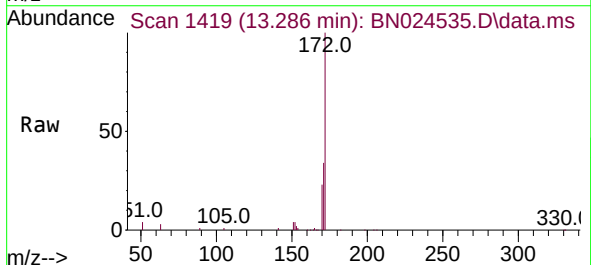

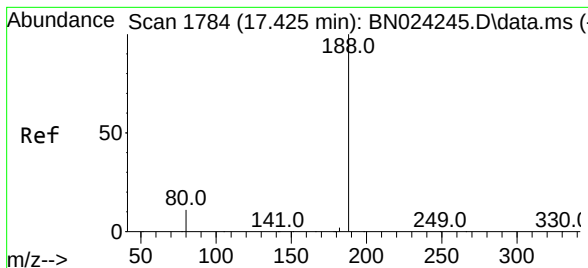

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.400 min Scan# 1784

Delta R.T. 0.000 min

Lab File: BN024535.D

Acq: 24 Mar 2023 07:43

Instrument :

BNA_N





ClientSampleId :

TT163S1-20230313

Tgt Ion:188 Resp: 33535
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 11.9 8.9 13.3

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

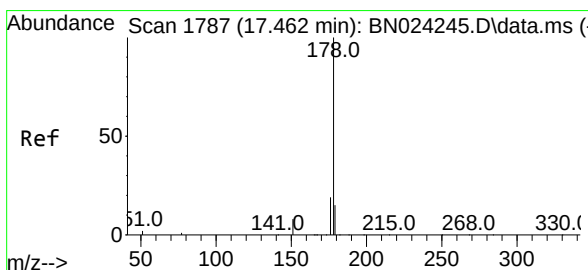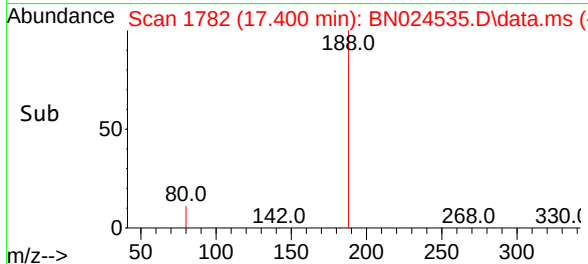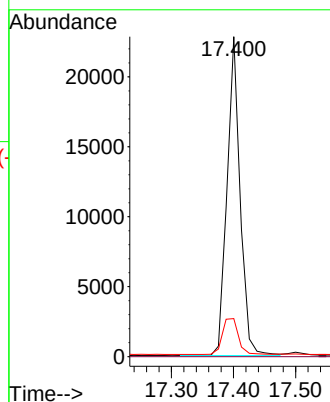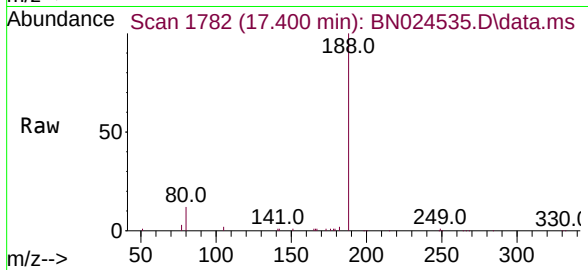

#25

Phenanthrene

Concen: 0.021 ng m




RT: 17.438 min Scan# 1785


Delta R.T. 0.000 min

Lab File: BN024535.D

Acq: 24 Mar 2023 07:43


Tgt Ion:178 Resp: 2062
 Ion Ratio Lower Upper
 178 100
 176 25.8 15.4 23.0#
 179 32.3 12.2 18.2#

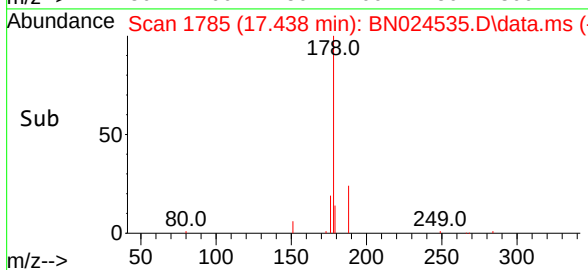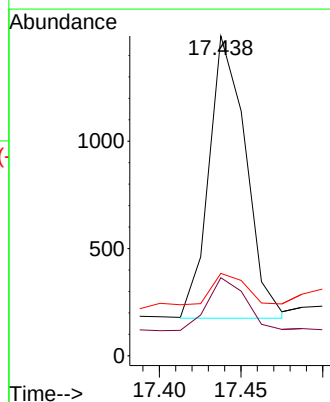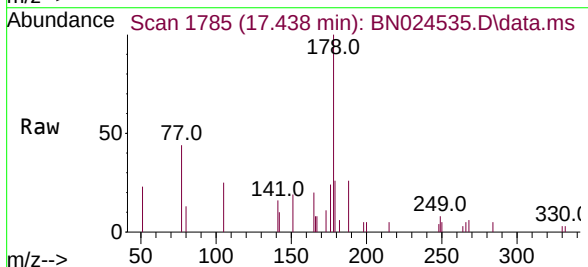

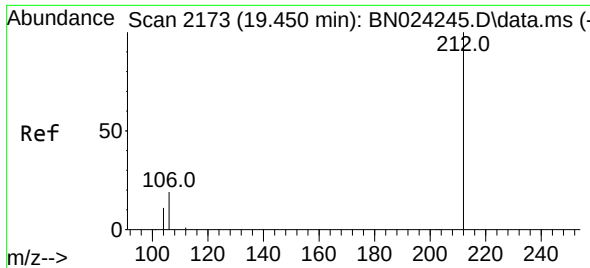

#27
Fluoranthene-d10
Concen: 0.481 ng
RT: 19.429 min Scan# 2173
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43




Instrument :
BNA_N
ClientSampleId :
TT163S1-20230313

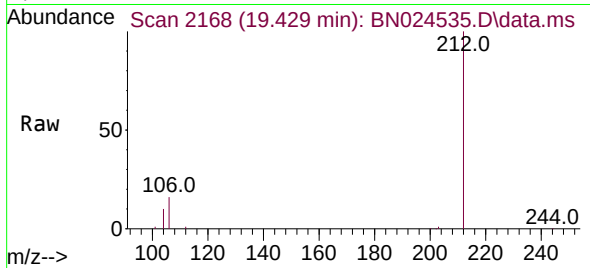

Tgt Ion:212 Resp: 3418
Ion Ratio Lower Upper
212 100
106 17.2 15.4 23.2
104 9.8 8.6 13.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

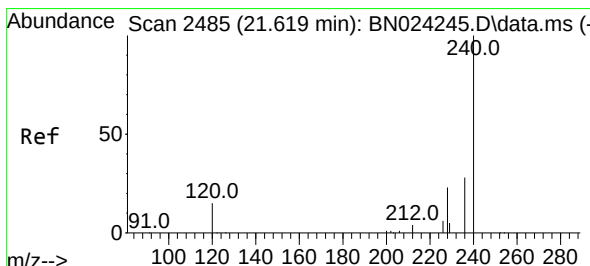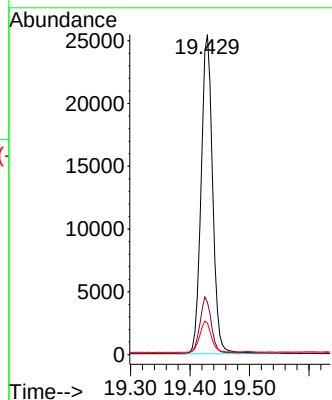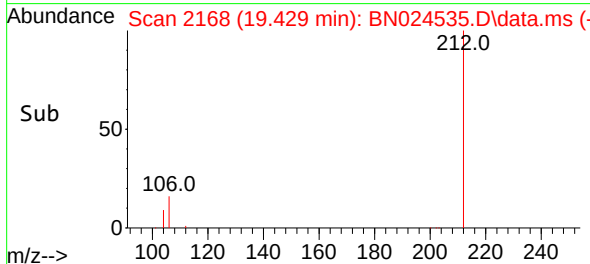

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.583 min Scan# 2481
Delta R.T. 0.000 min
Lab File: BN024535.D
Acq: 24 Mar 2023 07:43


Tgt Ion:240 Resp: 19662
Ion Ratio Lower Upper
240 100
120 21.2 12.8 19.2#
236 28.6 22.5 33.7

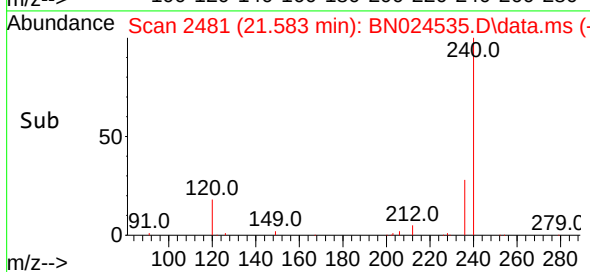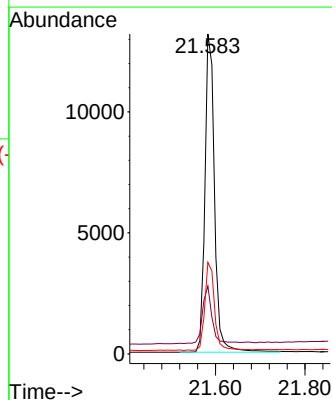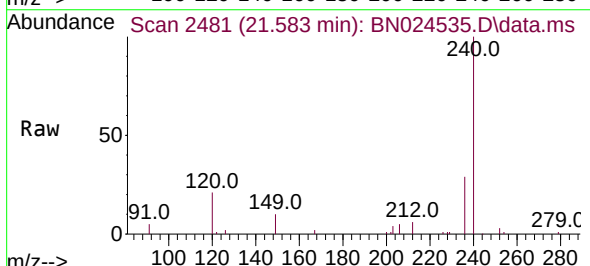

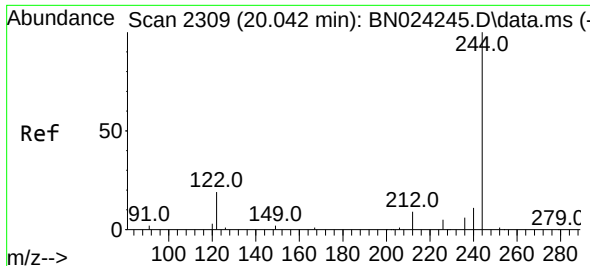

#31
 Terphenyl-d14
 Concen: 0.581 ng
 RT: 20.016 min Scan# 2309
 Delta R.T. 0.000 min
 Lab File: BN024535.D
 Acq: 24 Mar 2023 07:43




Instrument :
 BNA_N
 ClientSampleId :
 TT163S1-20230313

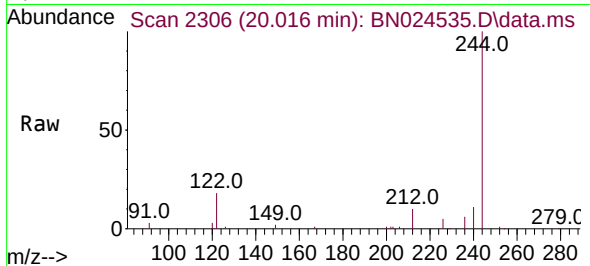


Tgt Ion:244 Resp: 19273
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.6 11.4
 122 17.8 15.1 22.7

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

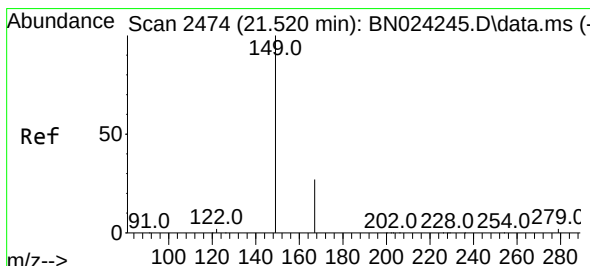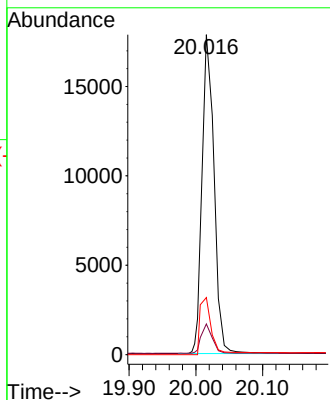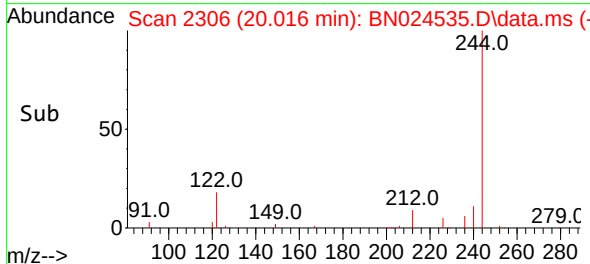


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.127 ng
 RT: 21.484 min Scan# 2470
 Delta R.T. 0.000 min
 Lab File: BN024535.D
 Acq: 24 Mar 2023 07:43

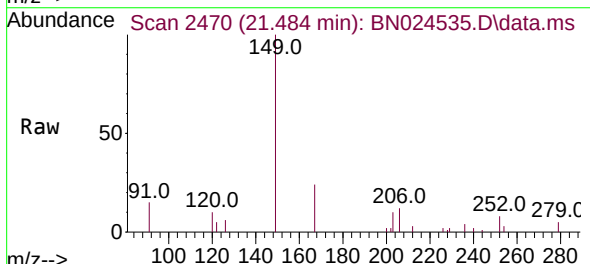


Tgt Ion:149 Resp: 3928
 Ion Ratio Lower Upper
 149 100
 167 26.4 21.2 31.8
 279 3.7 1.8 2.8

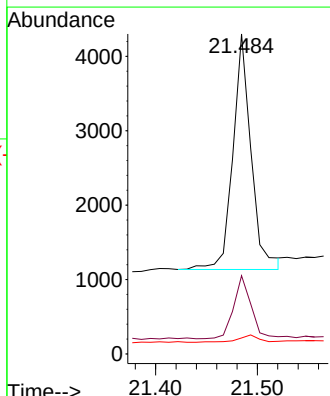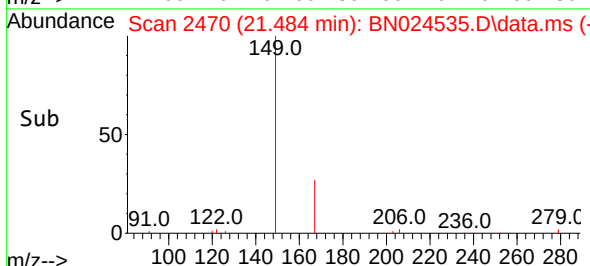

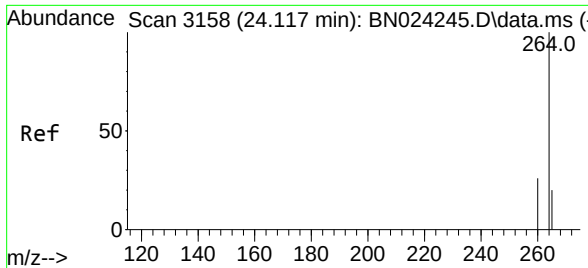

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.085 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BN024535.D
 Acq: 24 Mar 2023 07:43

Instrument :
 BNA_N
 ClientSampleId :
 TT163S1-20230313

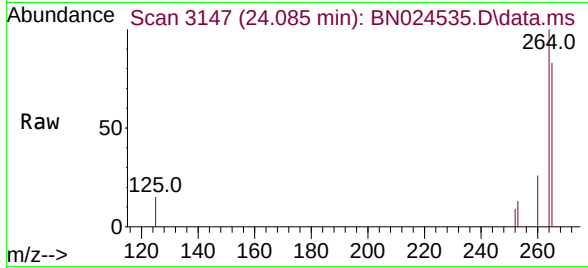

Tgt Ion:264 Resp: 15788
 Ion Ratio Lower Upper
 264 100
 260 26.5 21.4 32.2
 265 83.4 35.7 53.5

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

