
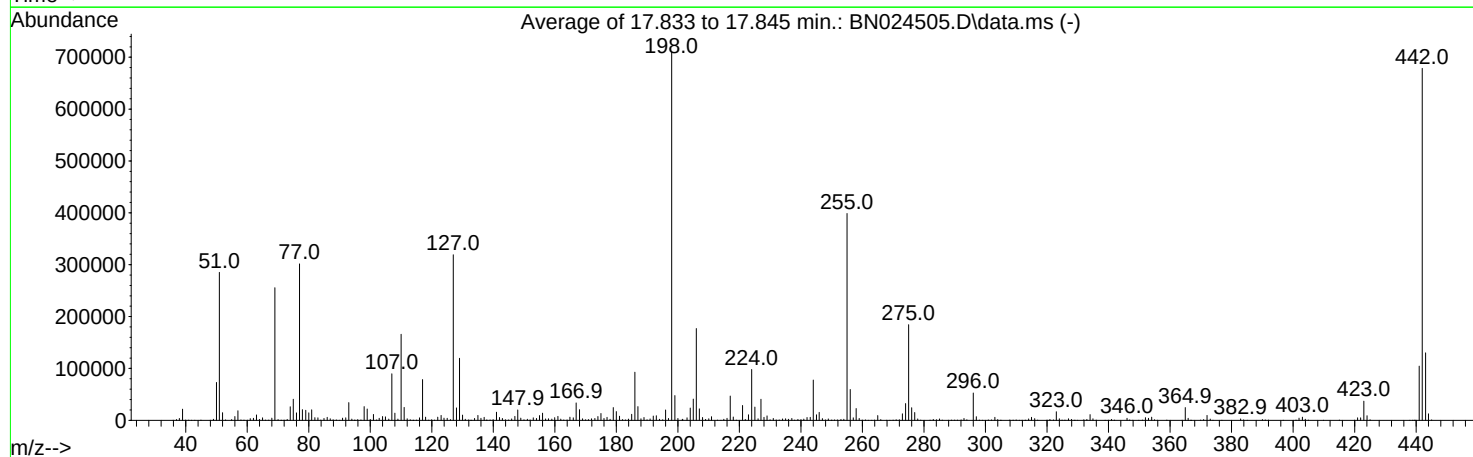


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032323\  
 Data File : BN024505.D  
 Acq On : 23 Mar 2023 09:41  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN031323.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 24 03:05:57 2023

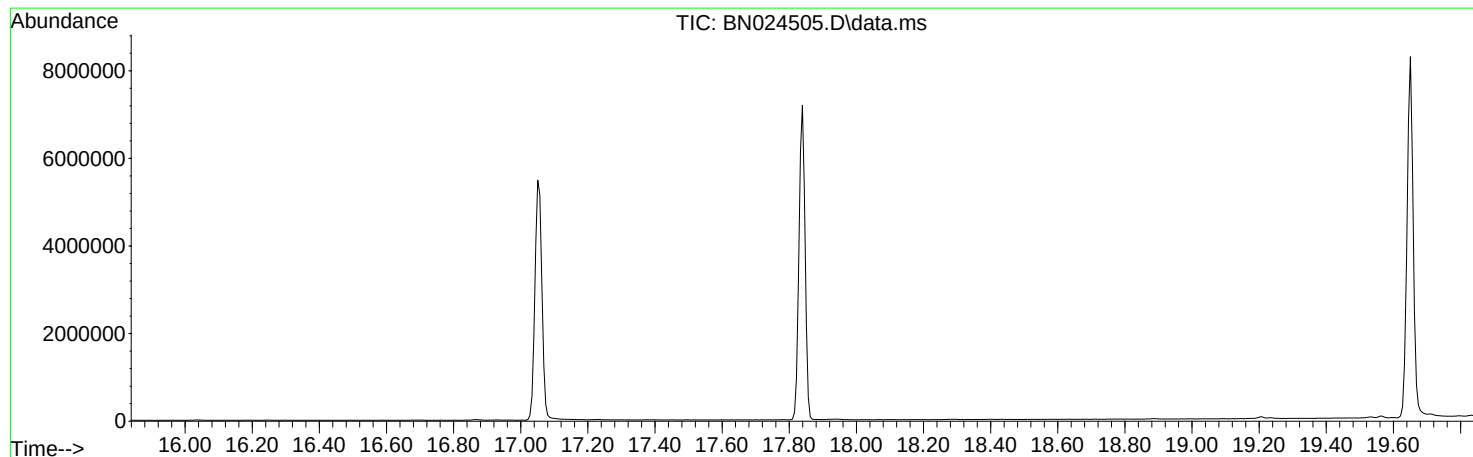




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.2         | 285366     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 4285       | PASS                |
| 69             | 198             | 0.00            | 100             | 36.0         | 255588     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 1352       | PASS                |
| 127            | 198             | 10              | 80              | 45.0         | 319296     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 3584       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 709269     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 47616      | PASS                |
| 275            | 198             | 10              | 60              | 26.0         | 184448     | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 24496      | PASS                |
| 441            | 198             | 0.01            | 100             | 14.7         | 104483     | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 678677     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 129891     | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032323\  
 Data File : BN024505.D  
 Acq On : 23 Mar 2023 09:41  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 24 07:47:04 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Mar 24 07:47:00 2023  
 Response via : Initial Calibration

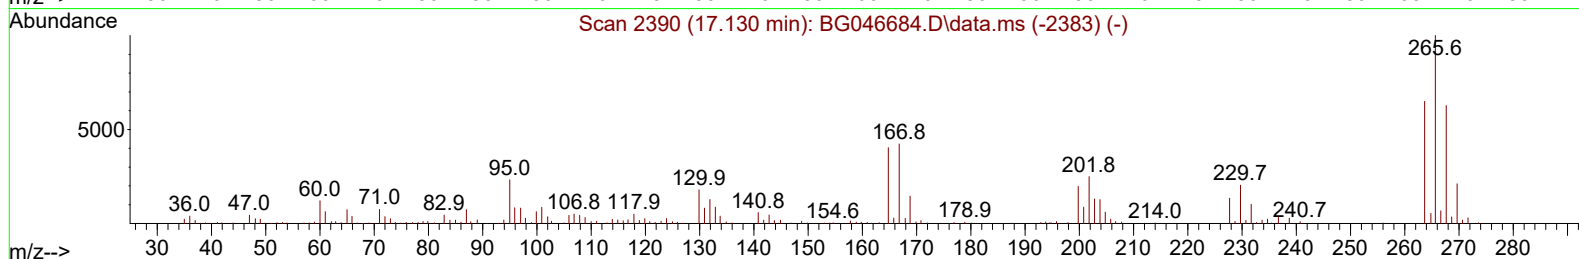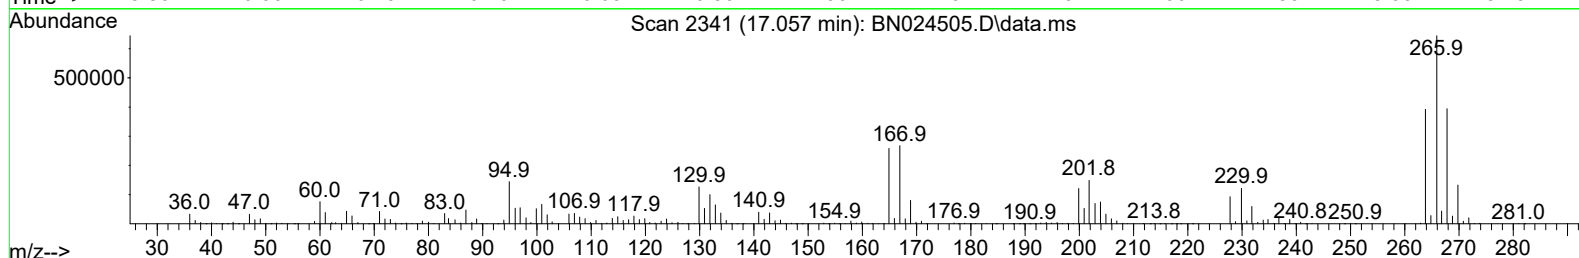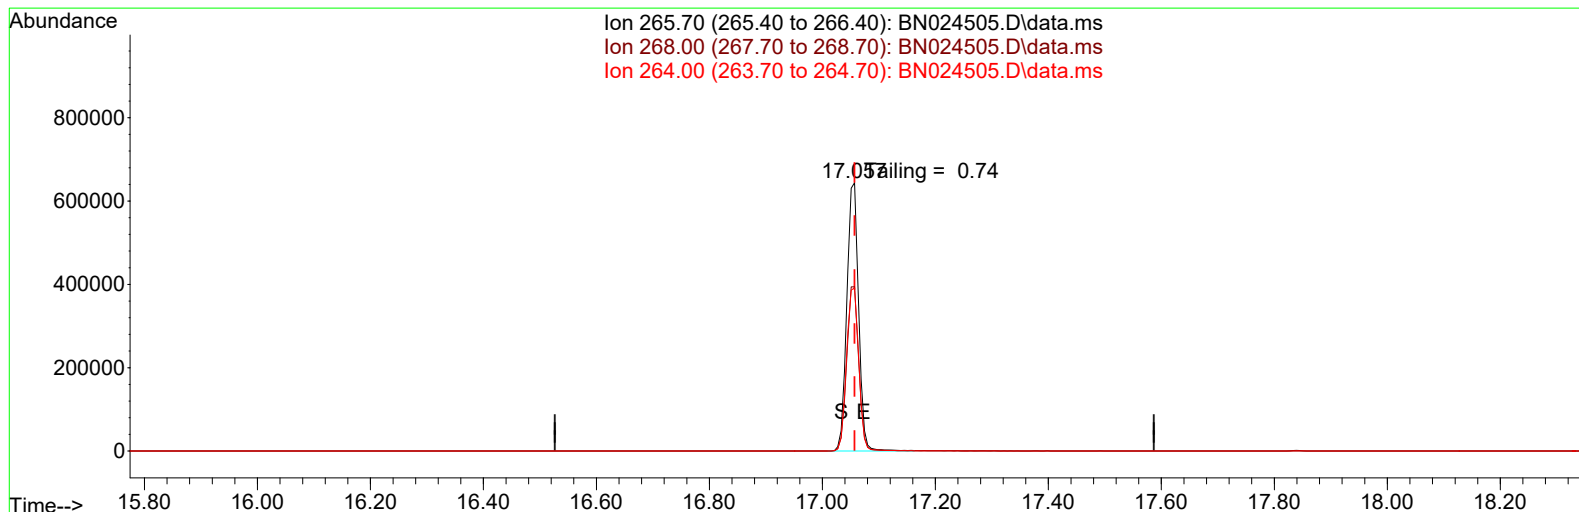

TIC: BN024505.D\data.ms

**(70) Pentachlorophenol (C)**

17.057min ( 0.000) 27298.50 ng




response 934479

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.21  |
| 264.00 | 61.60  | 60.83  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032323\  
Data File : BN024505.D  
Acq On : 23 Mar 2023 09:41  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 24 07:47:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 24 07:47:00 2023  
Response via : Initial Calibration

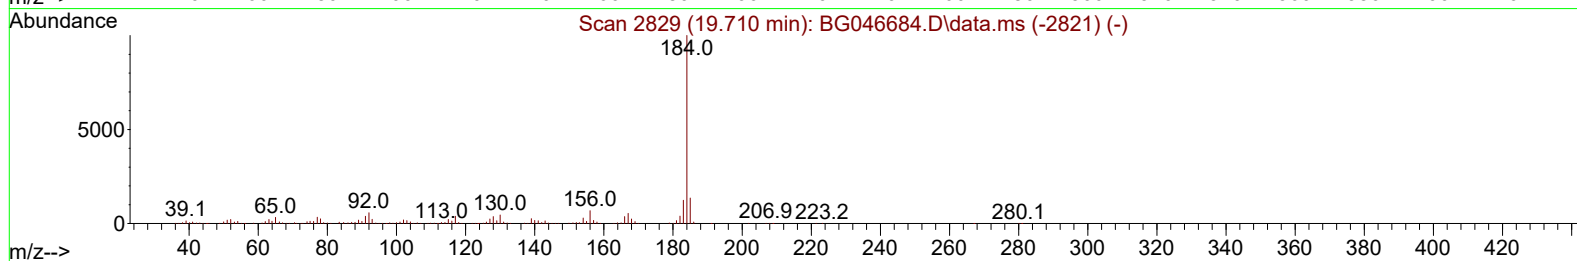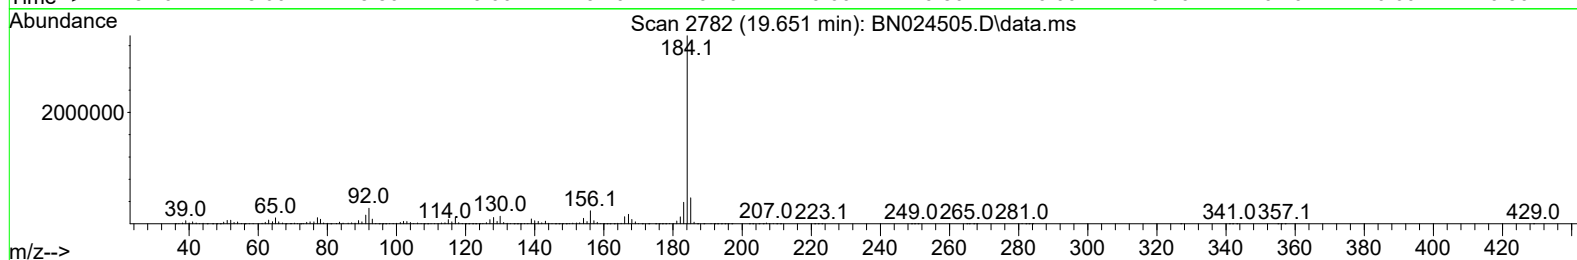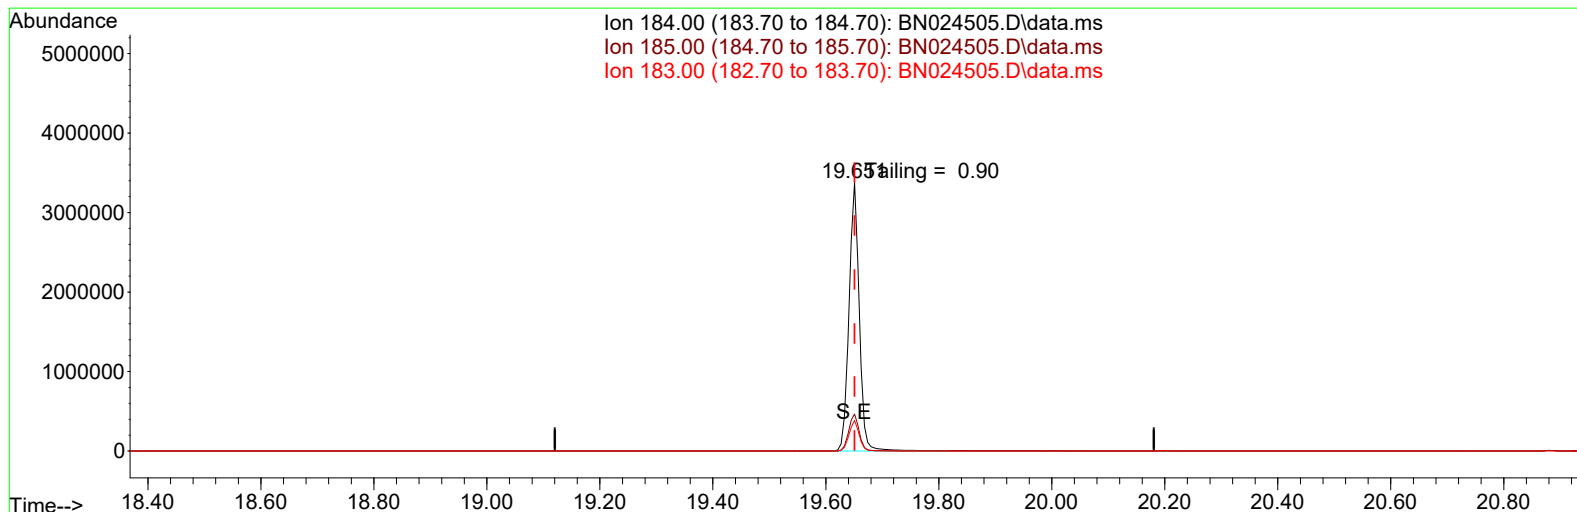

TIC: BN024505.D\data.ms

(77) Benzidine

19.651min ( 0.000) 1933907.47 ng

response 4292166

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.82  |
| 183.00 | 13.20  | 11.37  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/23/2023     | BNA_N            | <u>BN024505.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 2082491          | 20.88              |
| DDD           | 286689           | 20.439             |
| DDE           | 11829            | 19.933             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 298518        | 2381009          | 12.54              |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP