


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\
 Data File : BN024521.D
 Acq On : 23 Mar 2023 22:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 24 03:05:57 2023

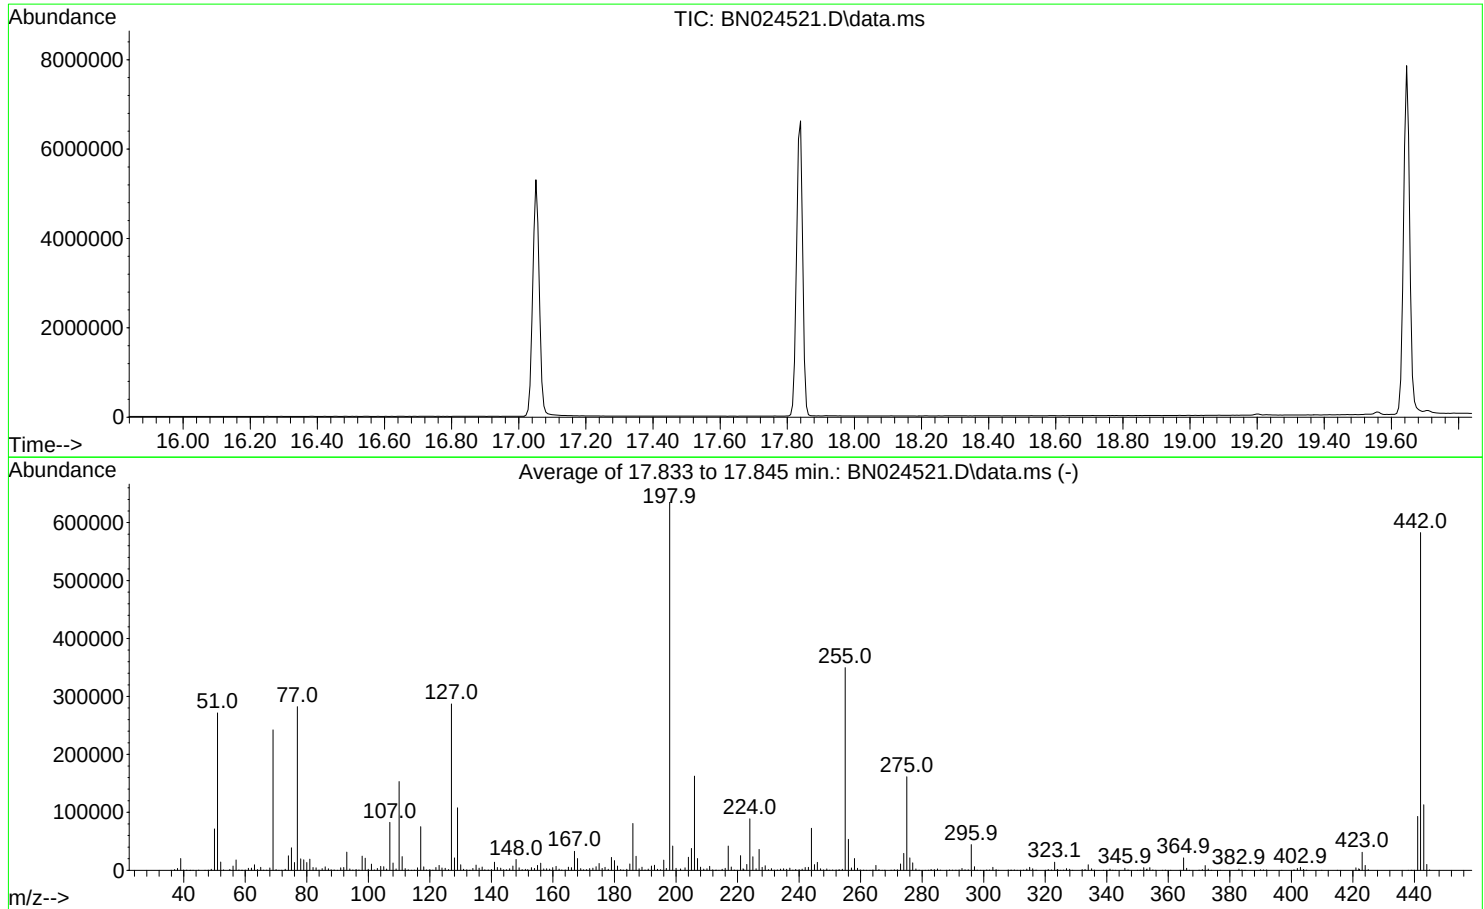




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	271467	PASS
68	69	0.00	2	1.6	3922	PASS
69	198	0.00	100	38.2	242453	PASS
70	69	0.00	2	0.5	1313	PASS
127	198	10	80	45.2	287125	PASS
197	198	0.00	2	0.5	3169	PASS
198	198	100	100	100.0	634816	PASS
199	198	5	9	6.6	41859	PASS
275	198	10	60	25.4	161392	PASS
365	198	1	100	3.4	21383	PASS
441	198	0.01	100	14.6	92944	PASS
442	442	50	100	100.0	582848	PASS
443	442	15	24	19.4	113016	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\
Data File : BN024521.D
Acq On : 23 Mar 2023 22:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 24 07:47:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 24 07:47:00 2023
Response via : Initial Calibration

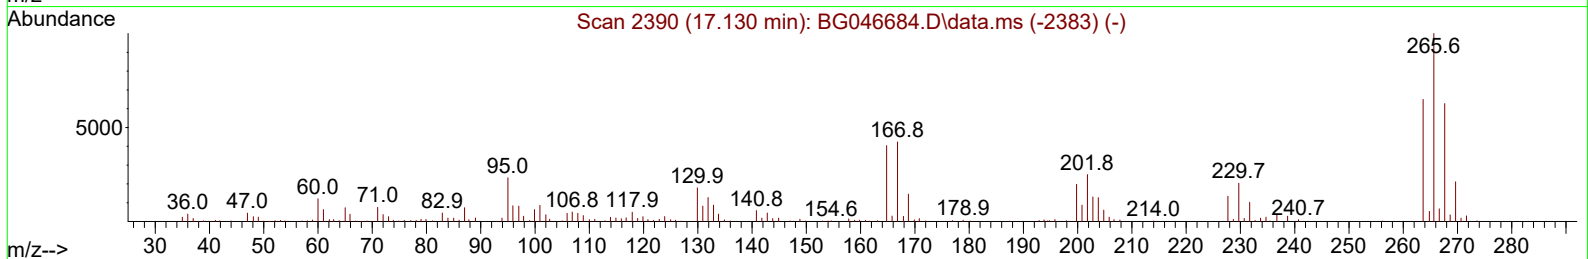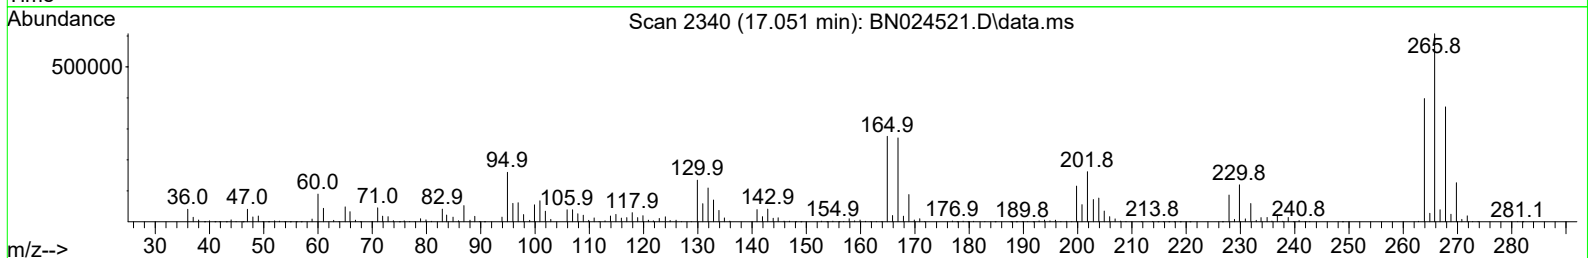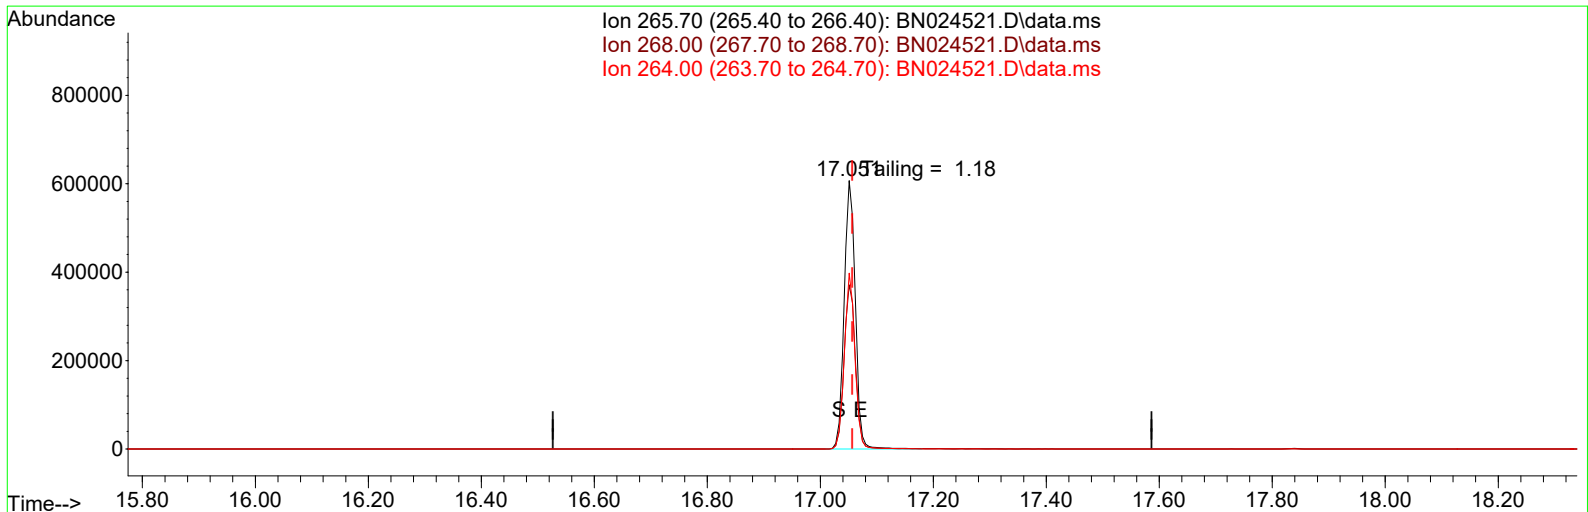

TIC: BN024521.D\data.ms

(70) Pentachlorophenol (C)

17.051min (-0.006) 26320.72 ng




response 832637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.15
264.00	61.60	65.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032323\
 Data File : BN024521.D
 Acq On : 23 Mar 2023 22:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 24 07:47:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 24 07:47:00 2023
 Response via : Initial Calibration

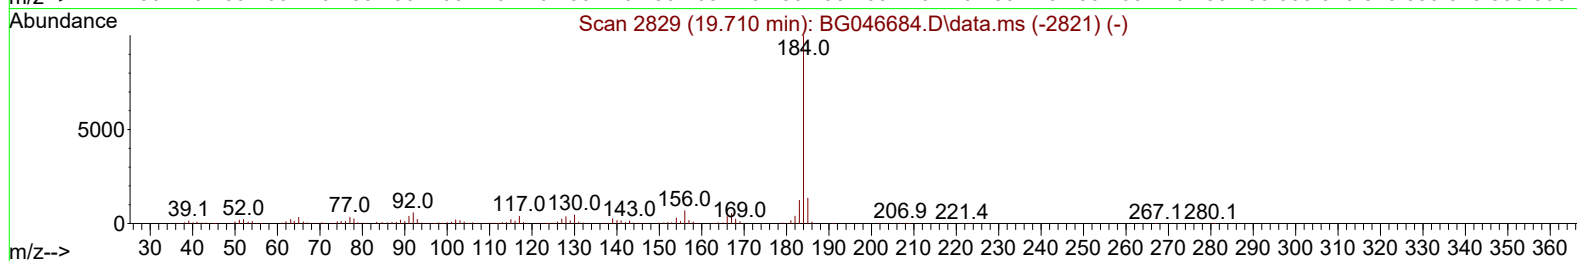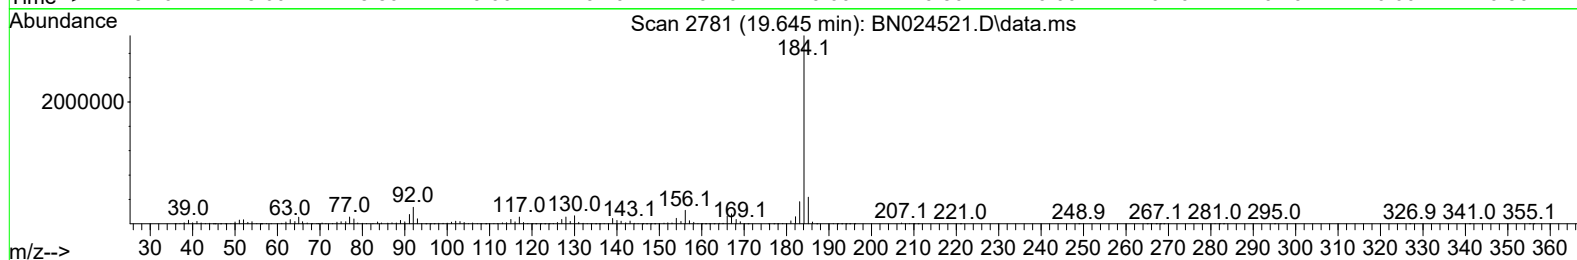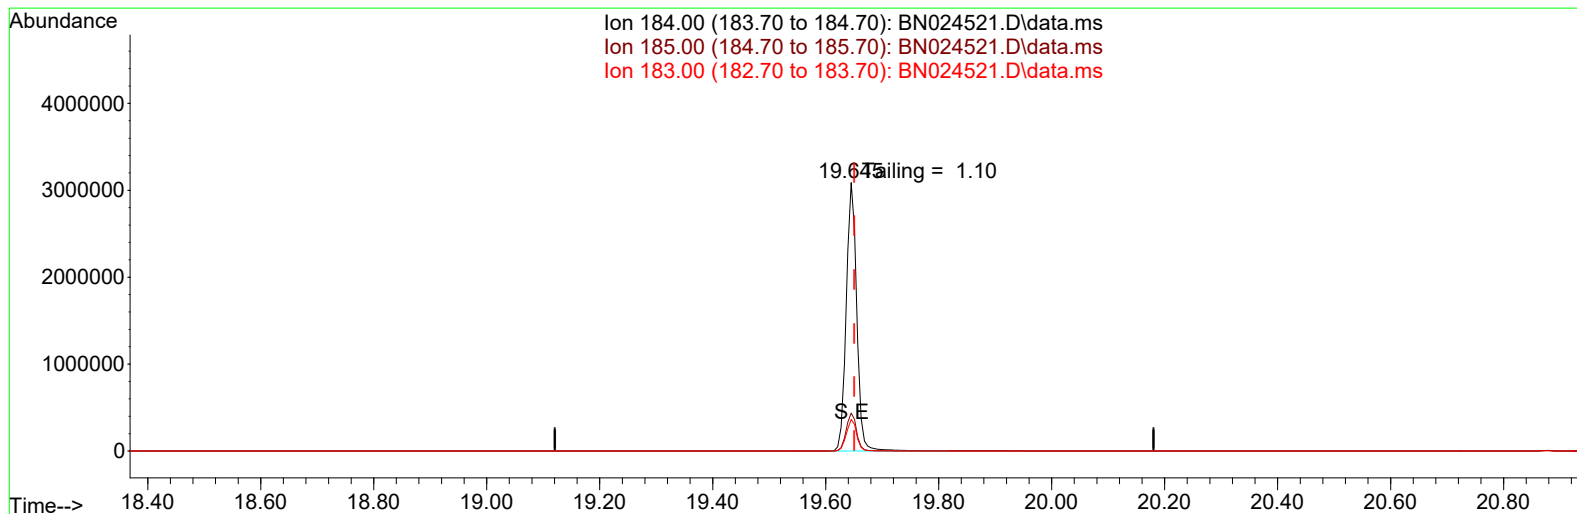

TIC: BN024521.D\data.ms

(77) Benzidine

19.645min (-0.006) 0.00 ng

response 3987787

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/23/2023	BNA_N	<u>BN024521.D</u>
Compound Name	Response	Retention Time
DDT	1962577	20.88
DDD	176862	20.433
DDE	8882	19.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
185744	2148321	8.65

Instrument :
BNA_N
ClientSampleId :
DFTPP