
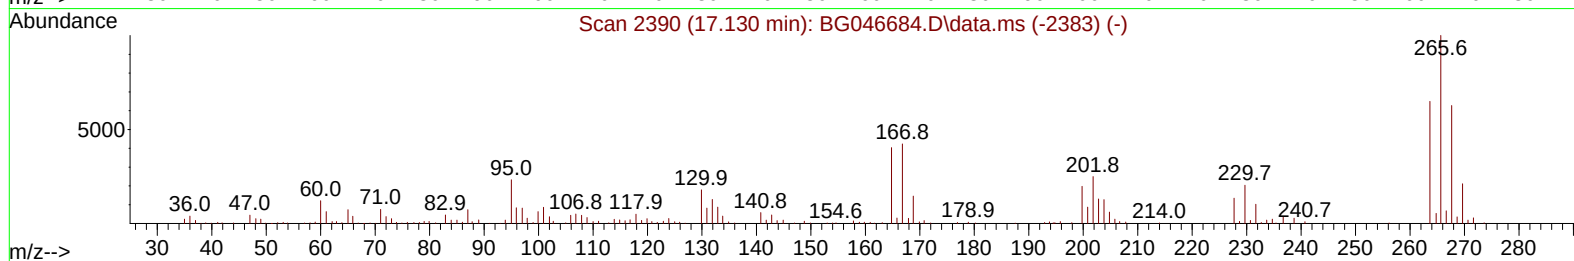
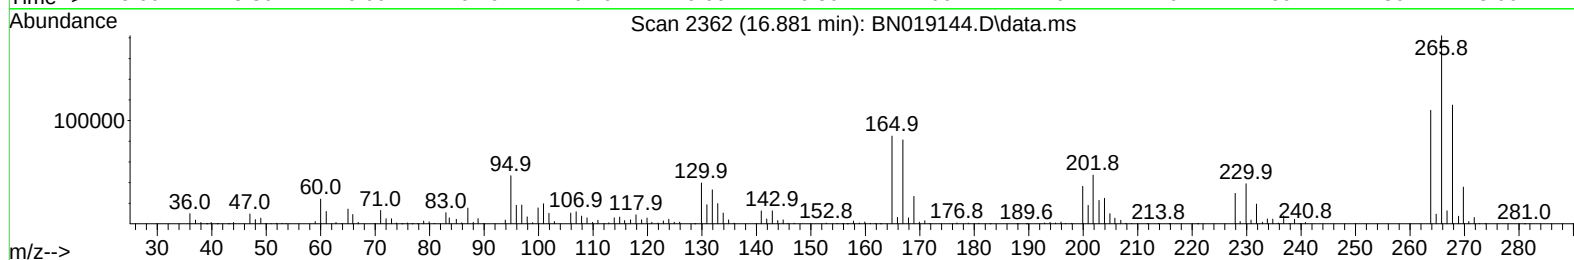


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032422\
 Data File : BN019144.D
 Acq On : 25 Mar 2022 03:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 05:13:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

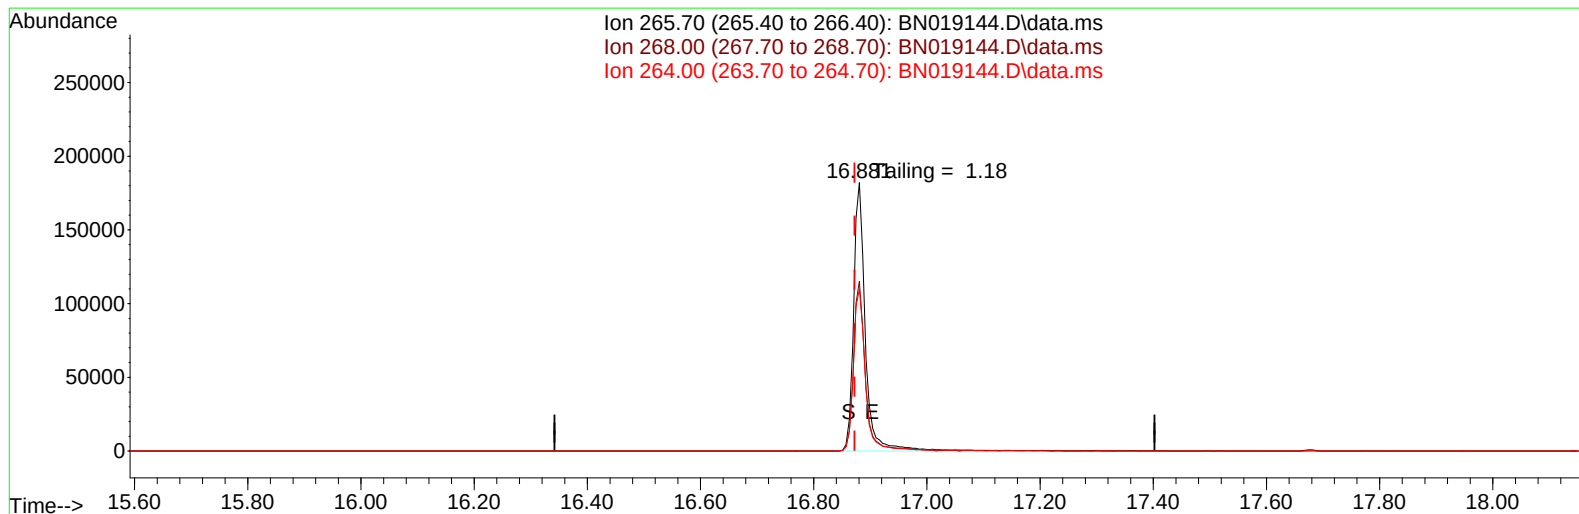

TIC: BN019144.D\data.ms

(70) Pentachlorophenol (C)




16.881min (+ 0.009) 16717.74 ng

response 261606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.22
264.00	61.60	60.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032422\
Data File : BN019144.D
Acq On : 25 Mar 2022 03:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 05:13:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

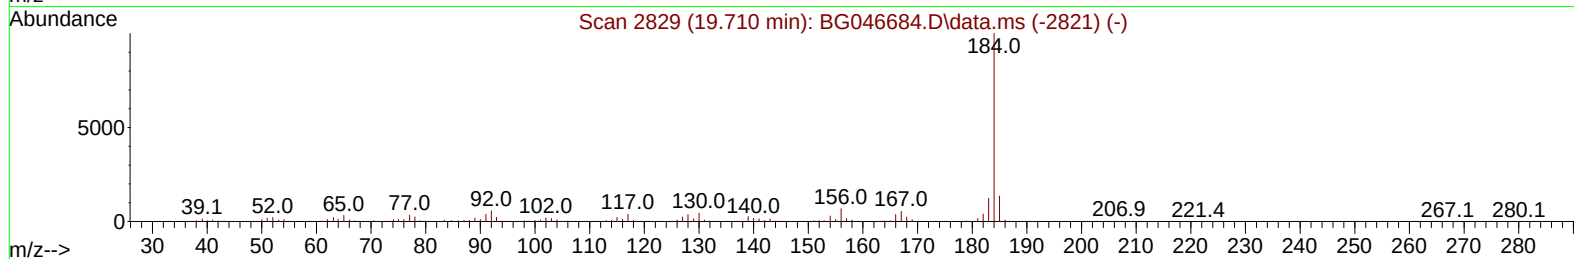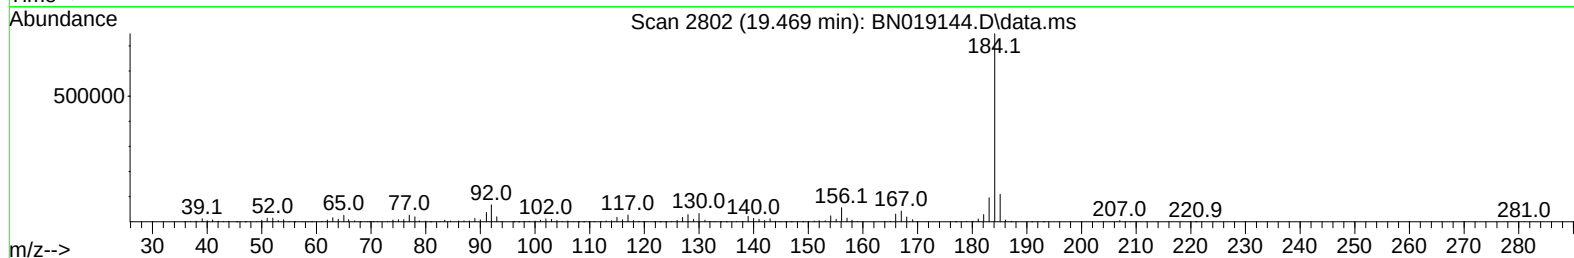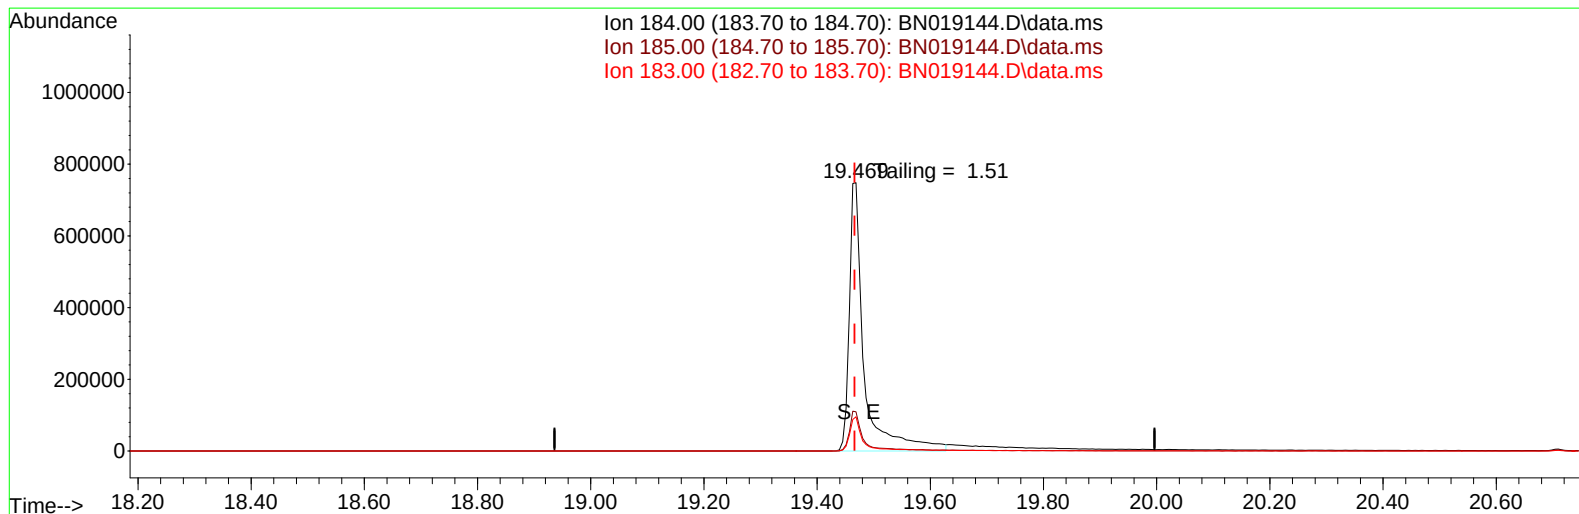

TIC: BN019144.D\data.ms

(77) Benzidine**19.469min (+ 0.003) 0.00 ng****response 1413522**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	12.75
0.00	0.00	0.00