


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032422\  
 Data File : BN019125.D  
 Acq On : 24 Mar 2022 14:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN031722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Mar 17 13:18:23 2022

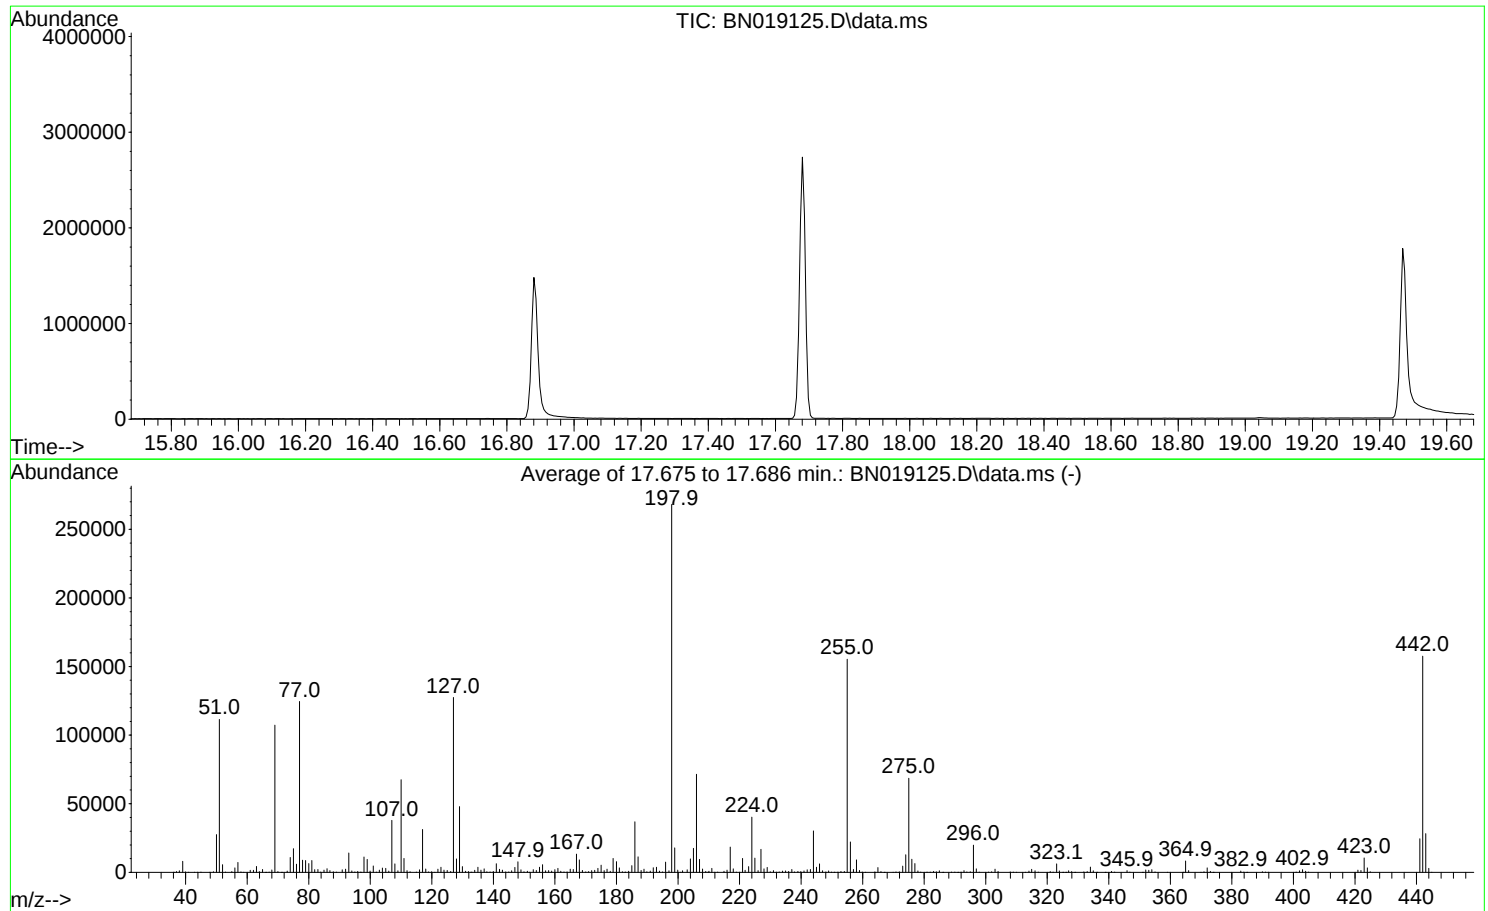




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.6         | 111473     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1778       | PASS                |
| 69             | 198             | 0.00            | 100             | 40.0         | 107296     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 623        | PASS                |
| 127            | 198             | 10              | 80              | 47.5         | 127427     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1192       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 268075     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 17830      | PASS                |
| 275            | 198             | 10              | 60              | 25.6         | 68552      | PASS                |
| 365            | 198             | 1               | 100             | 3.1          | 8233       | PASS                |
| 441            | 198             | 0.01            | 100             | 9.1          | 24485      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 157563     | PASS                |
| 443            | 442             | 15              | 24              | 17.9         | 28176      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032422\  
 Data File : BN019125.D  
 Acq On : 24 Mar 2022 14:26  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 25 05:02:16 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 23 16:56:32 2022  
 Response via : Initial Calibration

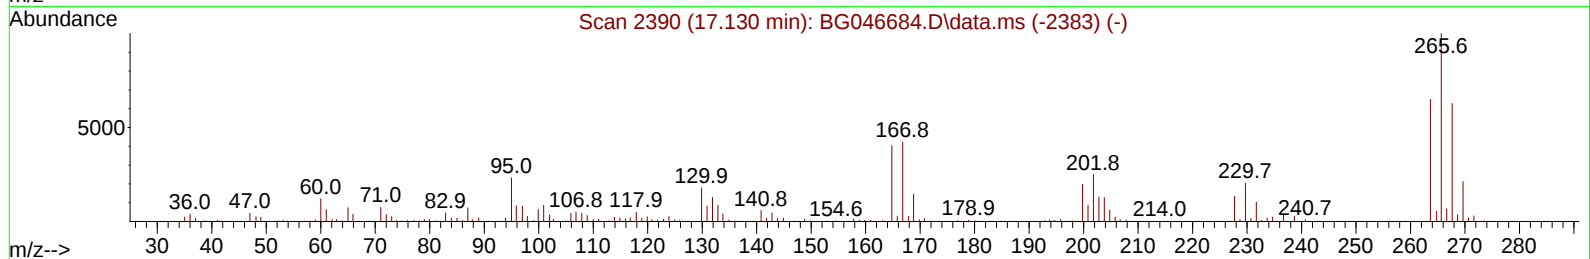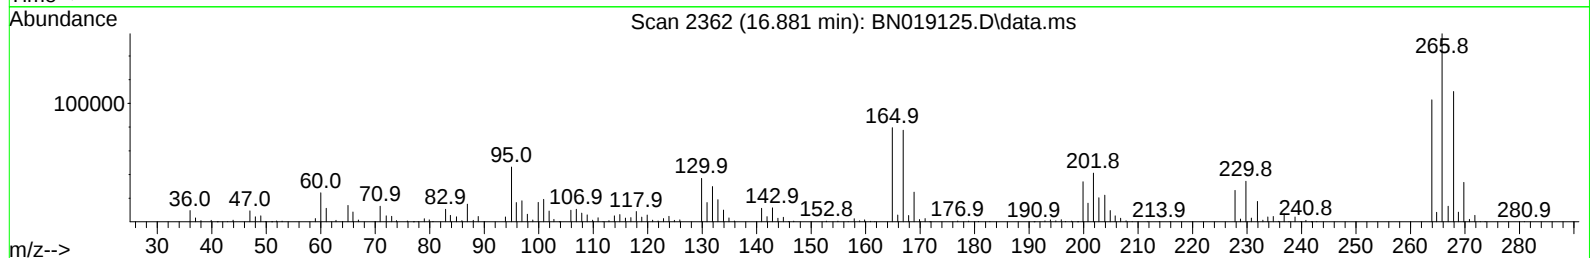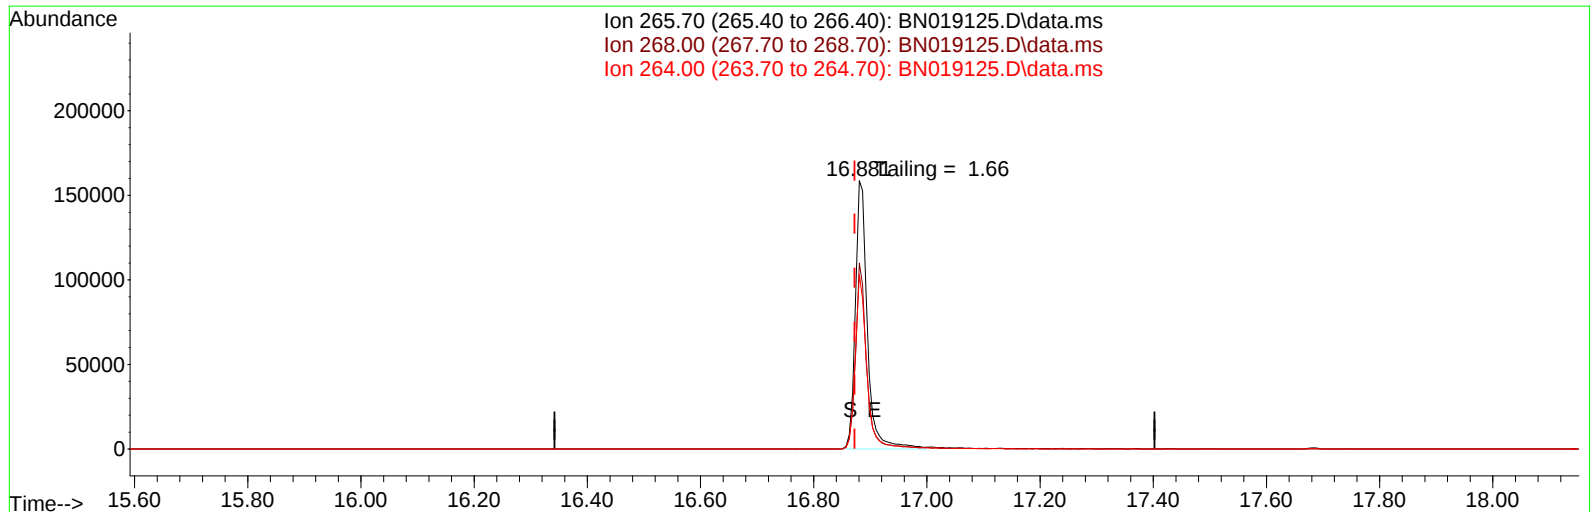

TIC: BN019125.D\data.ms

**(70) Pentachlorophenol (C)**

**16.881min (+ 0.009) 14899.83 ng**




**response 234211**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 69.27  |
| 264.00 | 61.60  | 64.91  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032422\  
Data File : BN019125.D  
Acq On : 24 Mar 2022 14:26  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 25 05:02:16 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 23 16:56:32 2022  
Response via : Initial Calibration

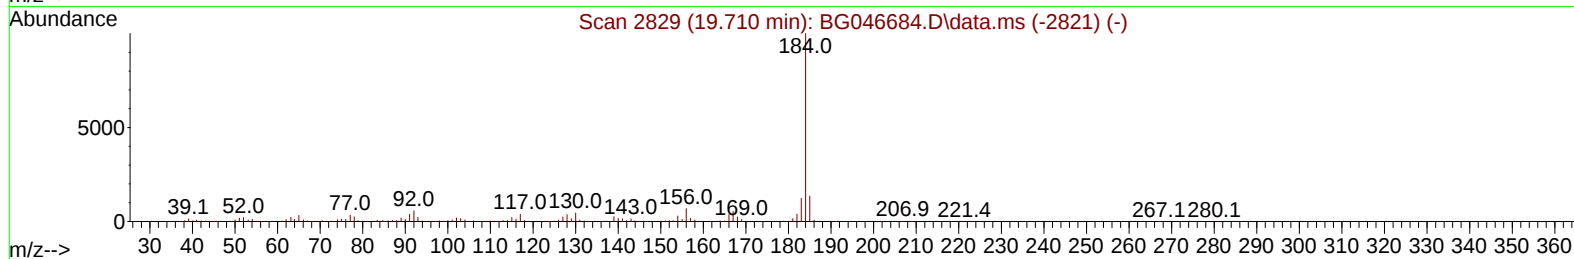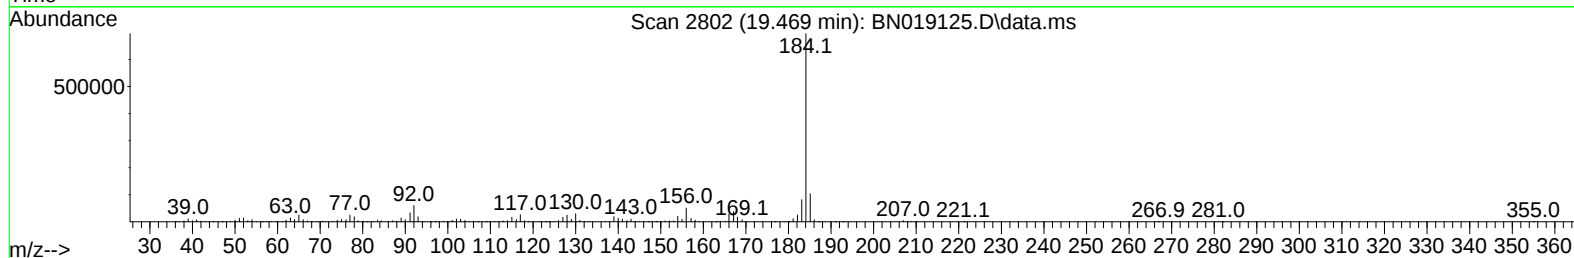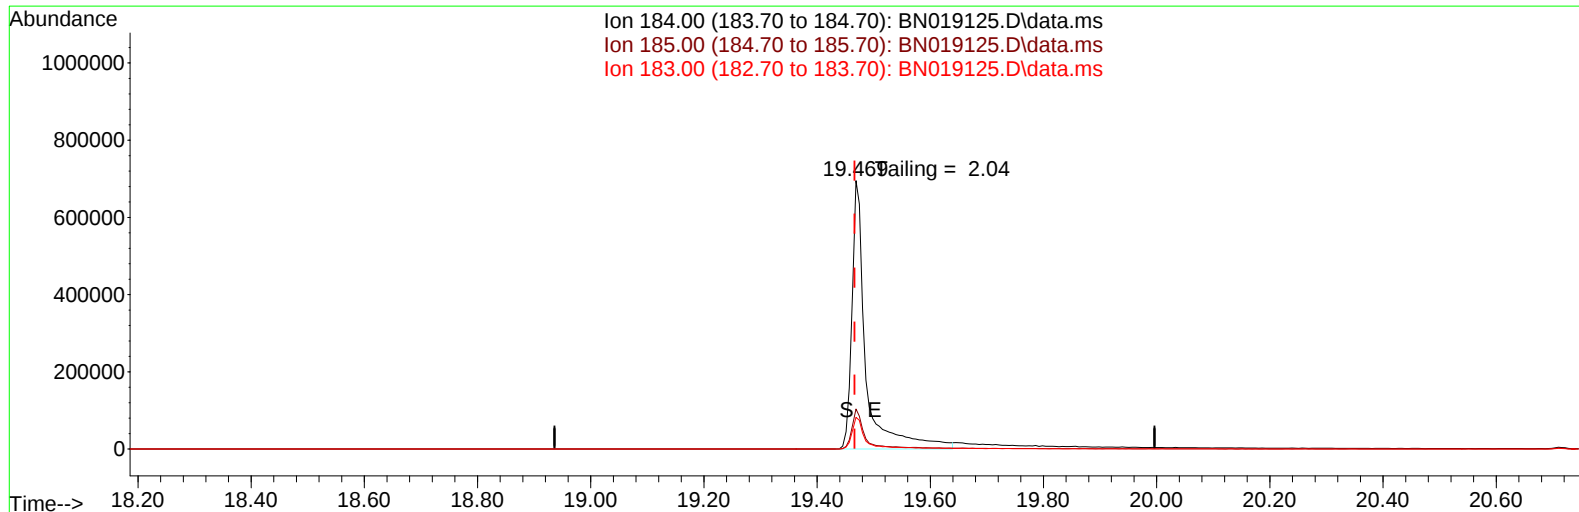

TIC: BN019125.D\data.ms

**(77) Benzidine**

**19.469min (+ 0.003) 0.00 ng**

**response 1209796**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.90  |
| 183.00 | 13.20  | 11.80  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/24/2022     | BNA_N            | <u>BN019125.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 909471           | 20.716             |
| DDD           | 10126            | 20.269             |
| DDE           | 618              | 19.763             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10744         | 920215           | 1.17               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP