
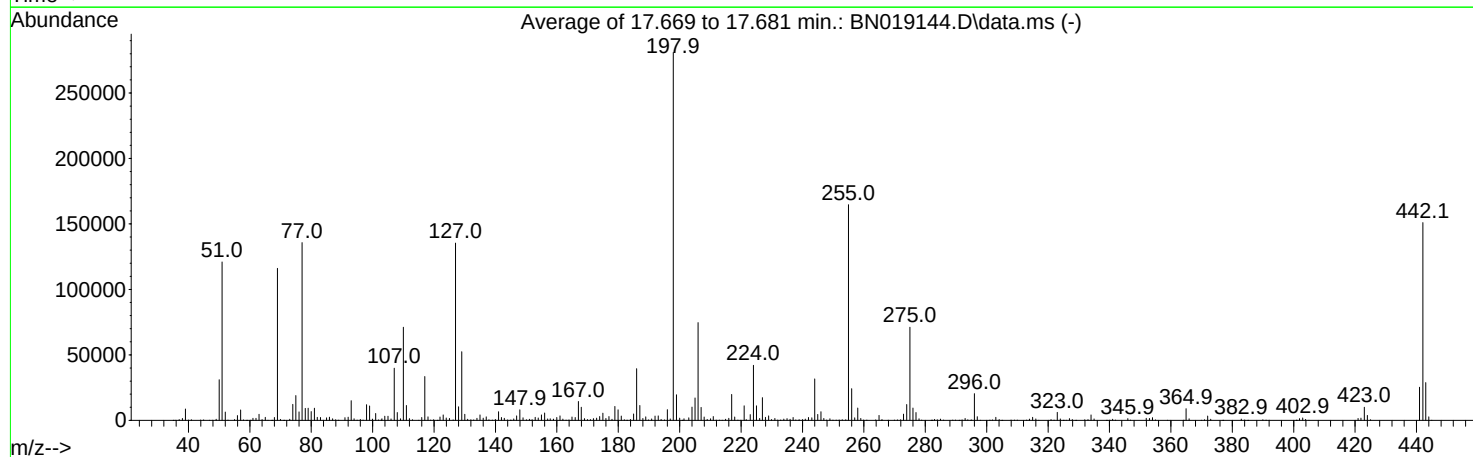


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032422\
 Data File : BN019144.D
 Acq On : 25 Mar 2022 03:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 13:18:23 2022

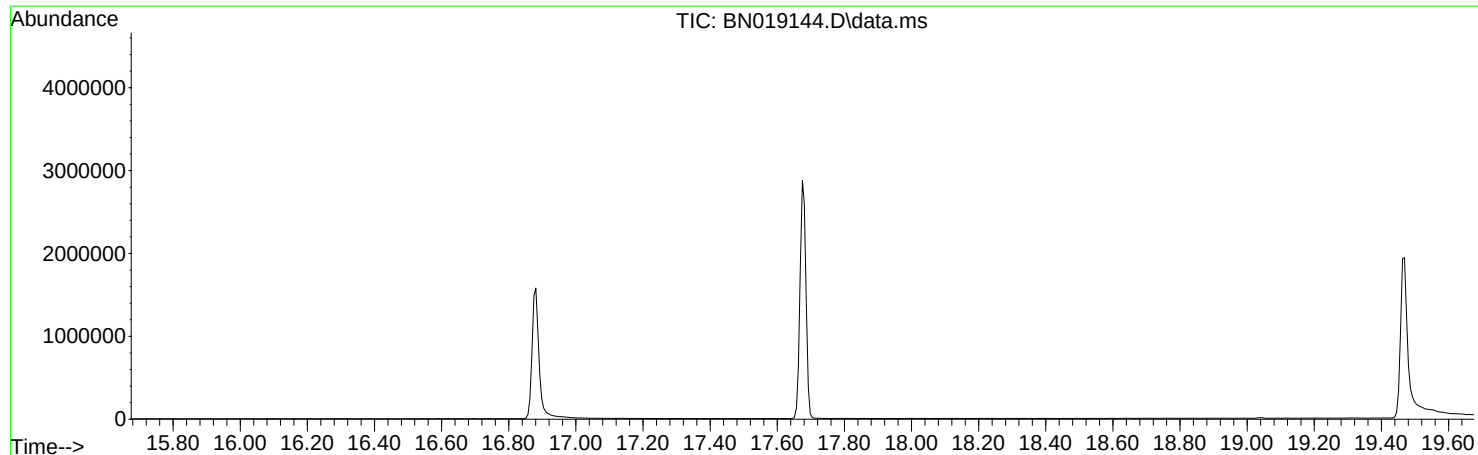




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	121028	PASS
68	69	0.00	2	1.9	2223	PASS
69	198	0.00	100	41.3	116099	PASS
70	69	0.00	2	0.6	692	PASS
127	198	10	80	48.2	135419	PASS
197	198	0.00	2	0.4	1072	PASS
198	198	100	100	100.0	280939	PASS
199	198	5	9	7.0	19535	PASS
275	198	10	60	25.3	71163	PASS
365	198	1	100	3.2	8921	PASS
441	198	0.01	100	9.0	25283	PASS
442	442	50	100	100.0	151003	PASS
443	442	15	24	19.1	28861	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032422\
Data File : BN019144.D
Acq On : 25 Mar 2022 03:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 25 05:13:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

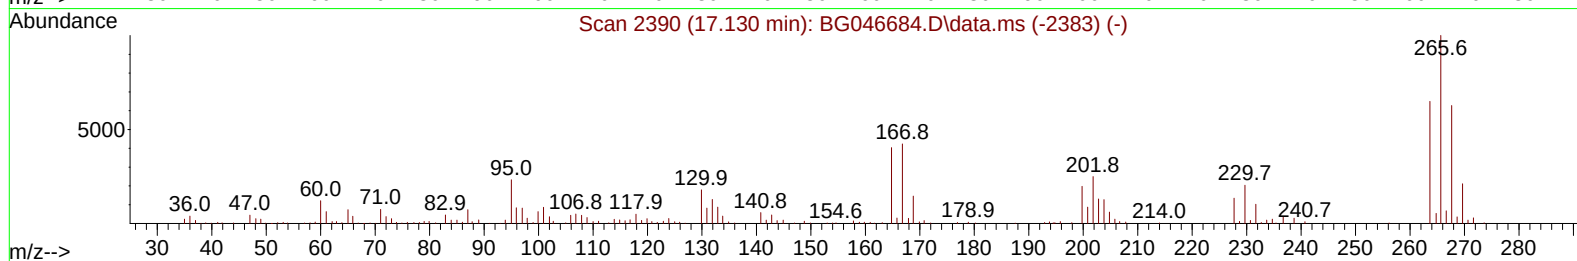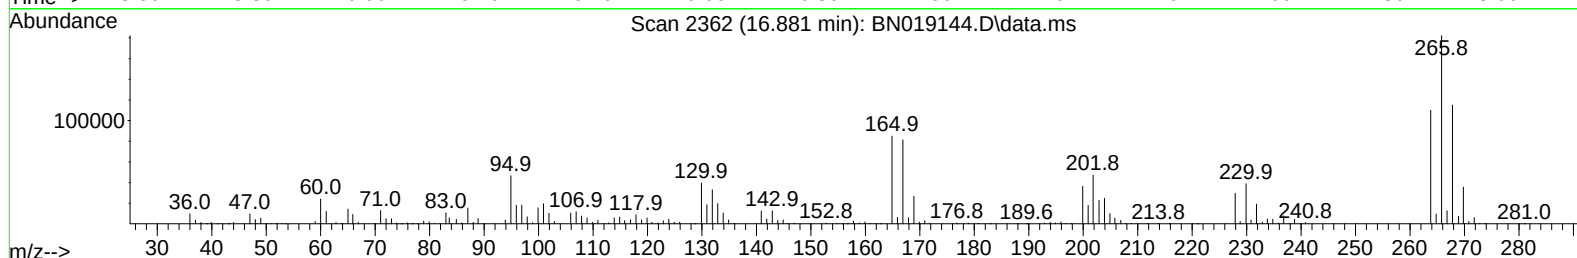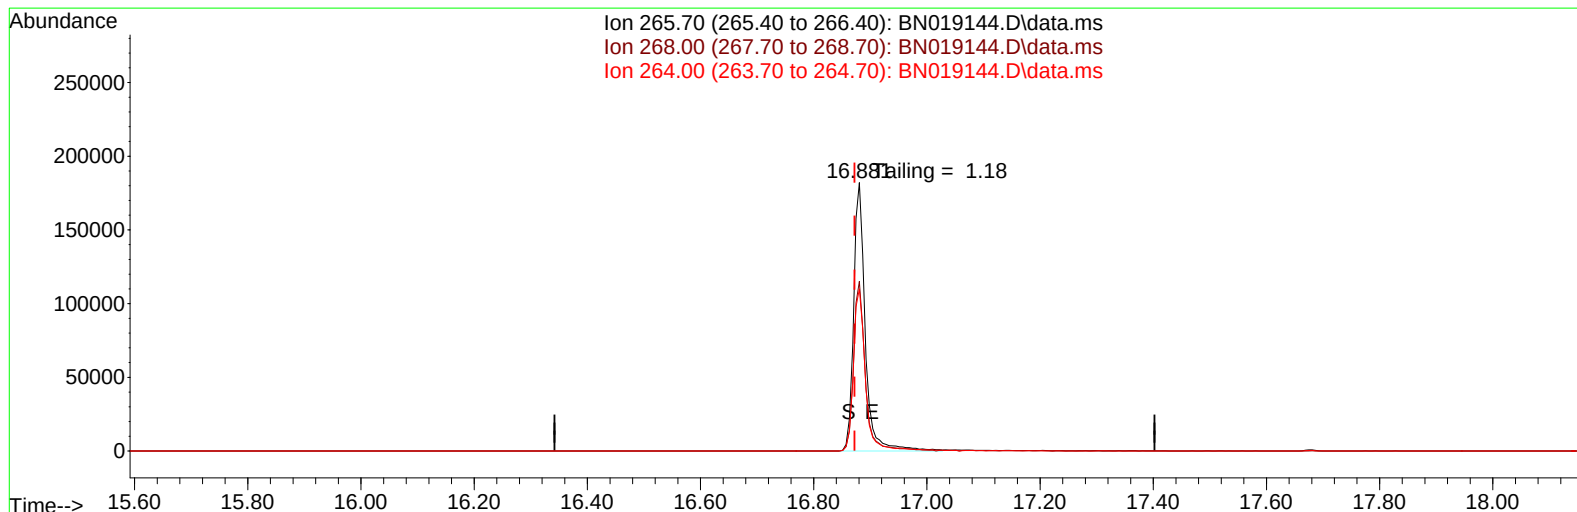

TIC: BN019144.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.009) 16717.74 ng




response 261606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.22
264.00	61.60	60.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032422\
 Data File : BN019144.D
 Acq On : 25 Mar 2022 03:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 05:13:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

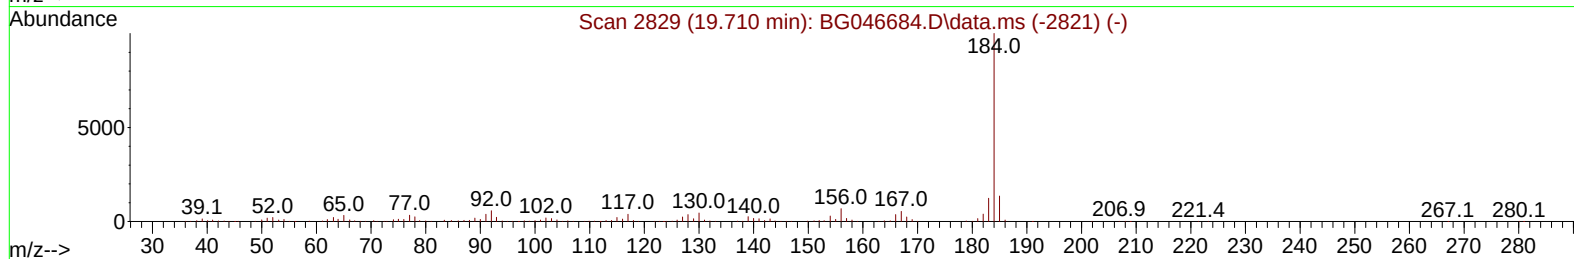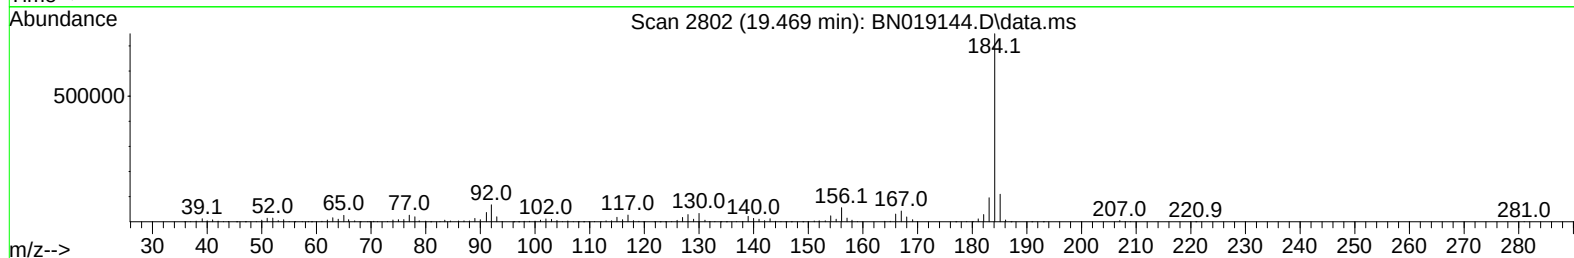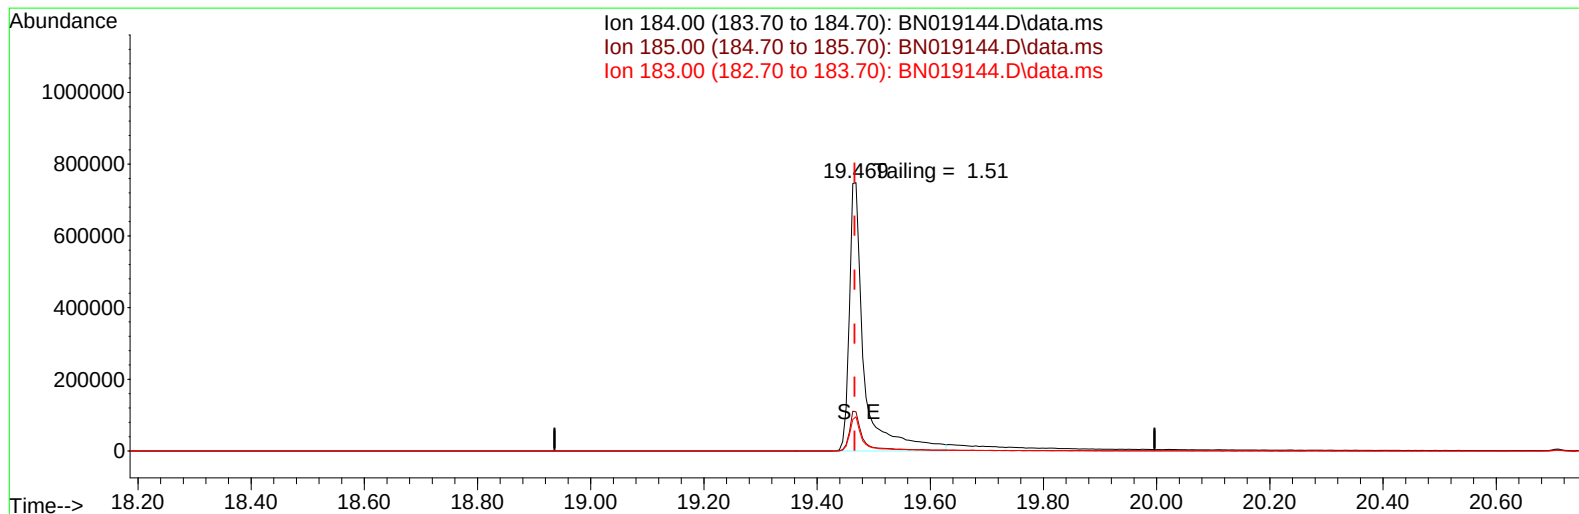

TIC: BN019144.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng

response 1413522

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	12.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/24/2022	BNA_N	<u>BN019144.D</u>
Compound Name	Response	Retention Time
DDT	998044	20.71
DDD	12599	20.269
DDE	500	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13099	1011143	1.30

Instrument :
BNA_N
ClientSampleId :
DFTPP