
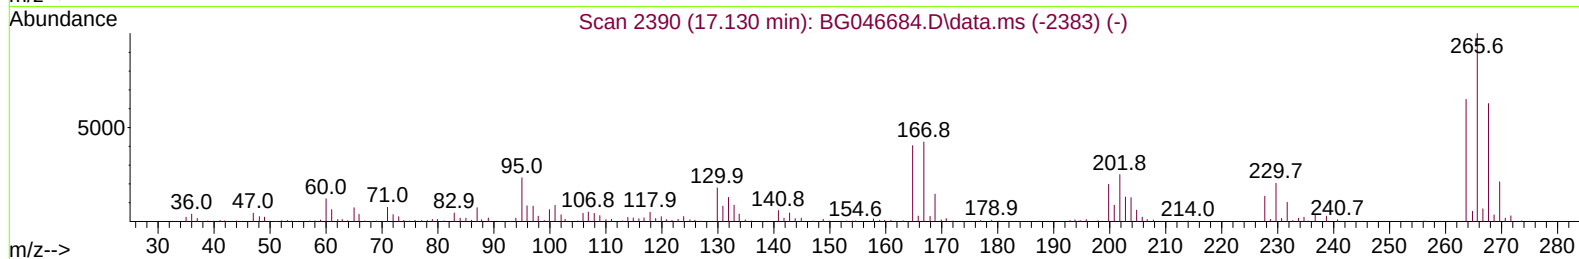
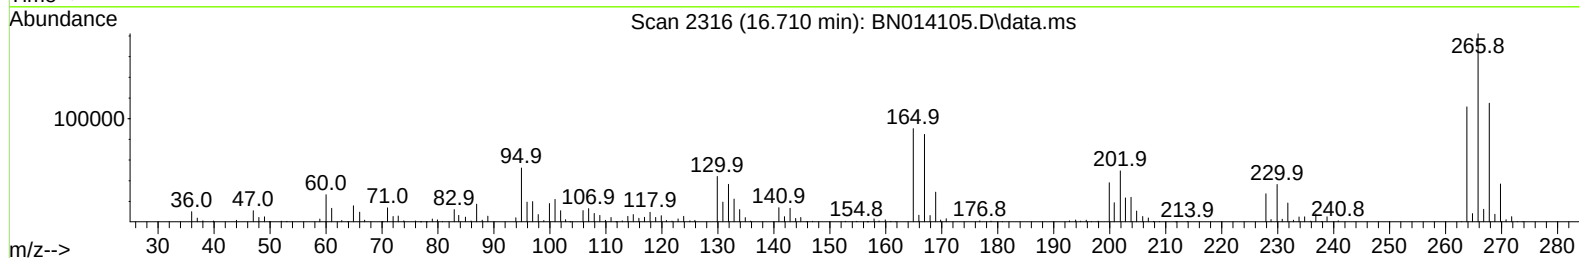


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032521\
Data File : BN014105.D
Acq On : 25 Mar 2021 14:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 02:17:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

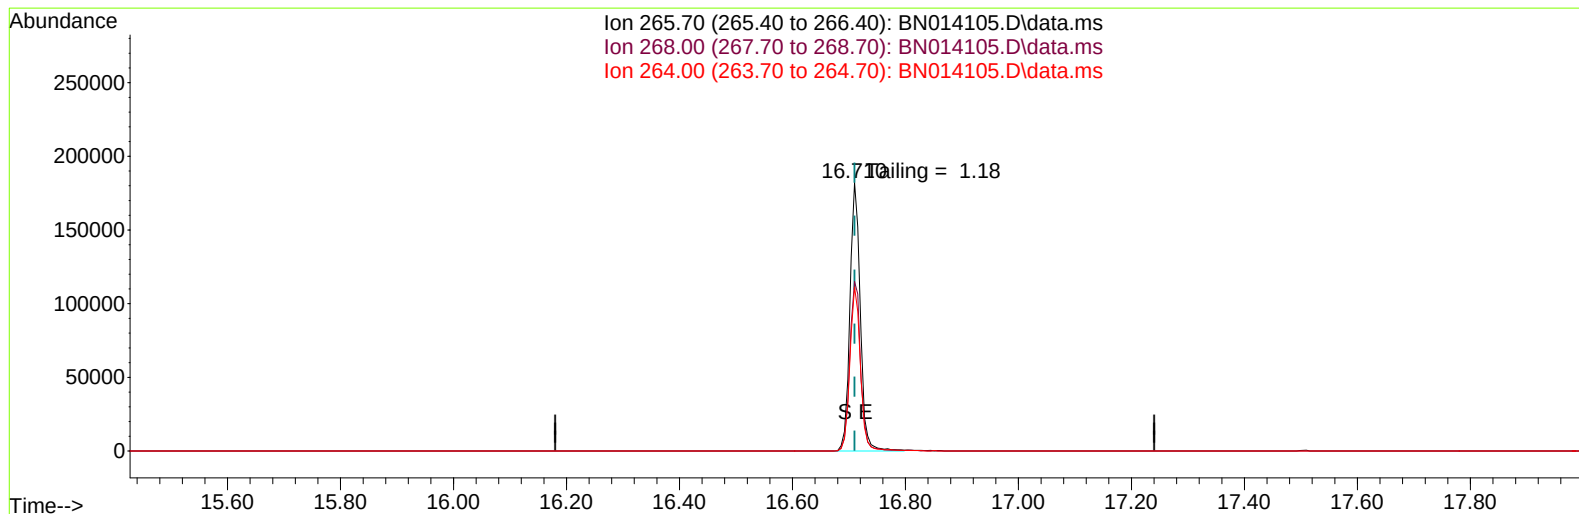

TIC: BN014105.D\data.ms

(70) Pentachlorophenol (C)




16.710min (-0.000) 25146.36 ng

response 234640

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.11
264.00	61.60	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032521\
Data File : BN014105.D
Acq On : 25 Mar 2021 14:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 02:17:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

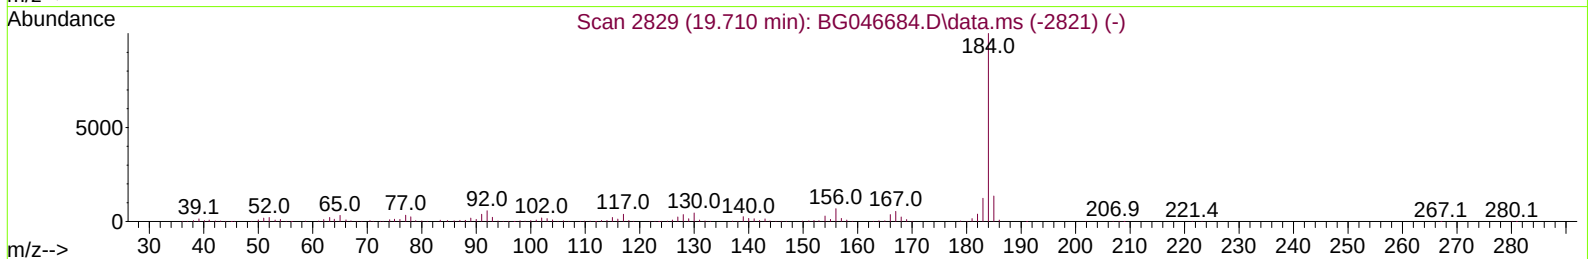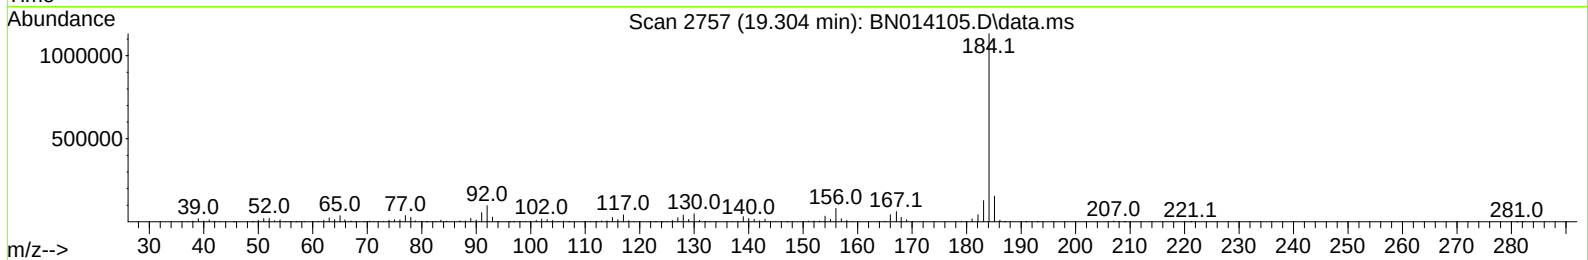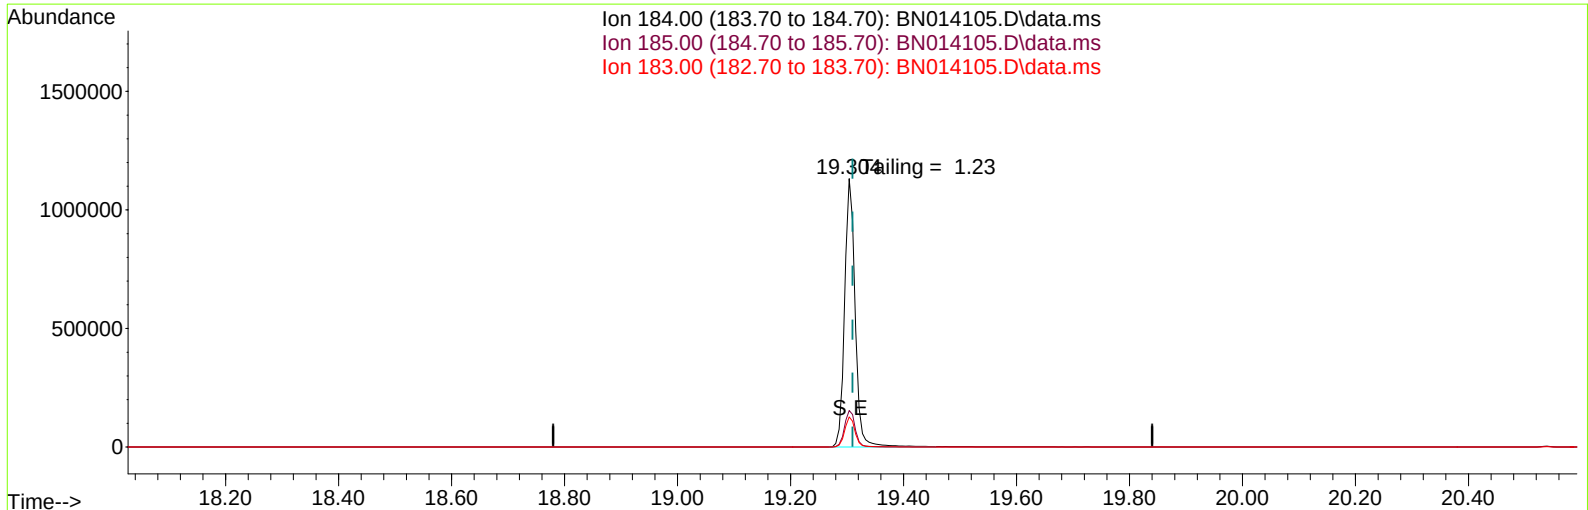

TIC: BN014105.D\data.ms

(77) Benzidine

19.304min (-0.006) 0.00 ng

response 1464060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.61
183.00	13.20	11.23
0.00	0.00	0.00