
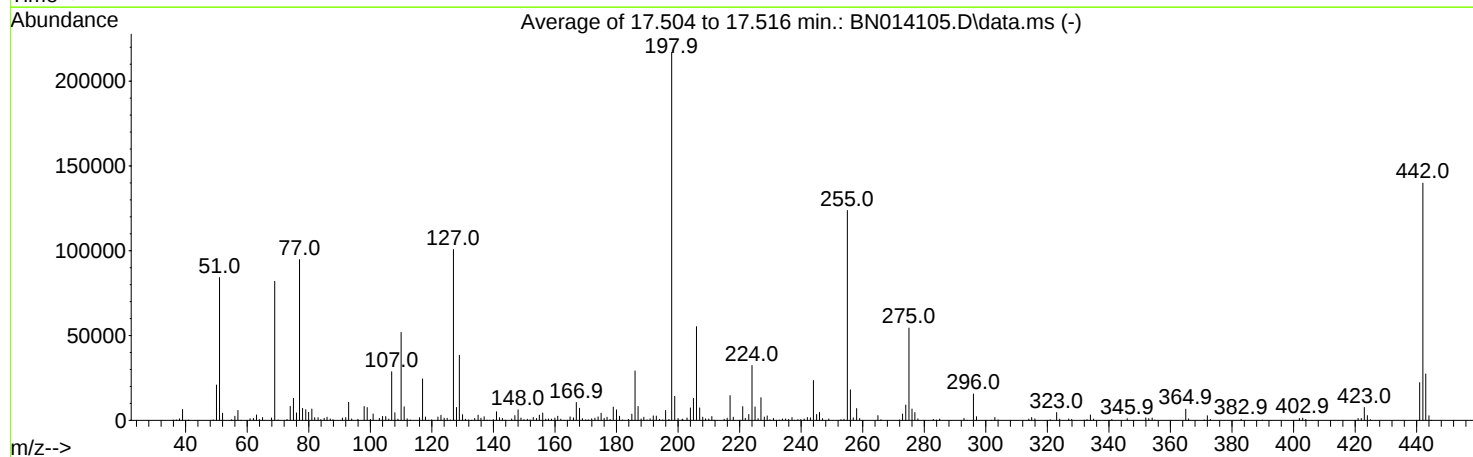


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032521\
 Data File : BN014105.D
 Acq On : 25 Mar 2021 14:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 23 11:06:27 2021

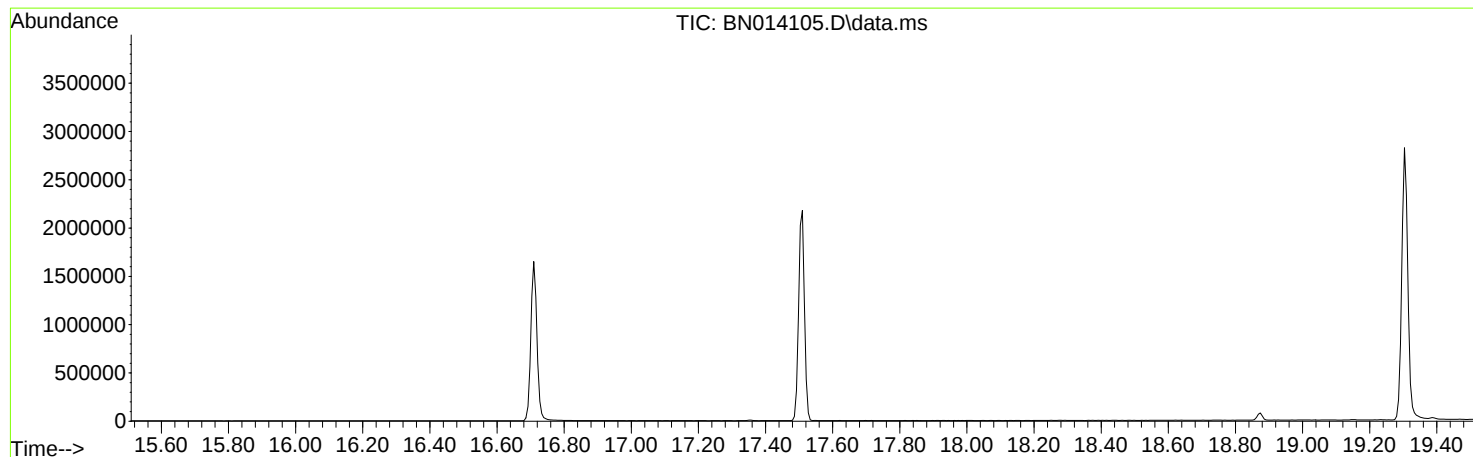

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	84237	PASS
68	69	0.00	2	1.7	1377	PASS
69	198	0.00	100	37.8	82011	PASS
70	69	0.00	2	0.3	265	PASS
127	198	10	80	46.5	100733	PASS
197	198	0.00	2	0.2	343	PASS
198	198	100	100	100.0	216853	PASS
199	198	5	9	6.5	14129	PASS
275	198	10	60	25.1	54408	PASS
365	198	1	100	3.0	6582	PASS
441	198	0.01	100	10.3	22253	PASS
442	442	50	100	100.0	139853	PASS
443	442	15	24	19.6	27349	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2021	BNA_N	<u>BN014105.D</u>
Compound Name	Response	Retention Time
DDT	802532	20.539
DDD	7828	20.098
DDE	1073	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8901	811433	1.10

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032521\
Data File : BN014105.D
Acq On : 25 Mar 2021 14:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 26 02:17:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

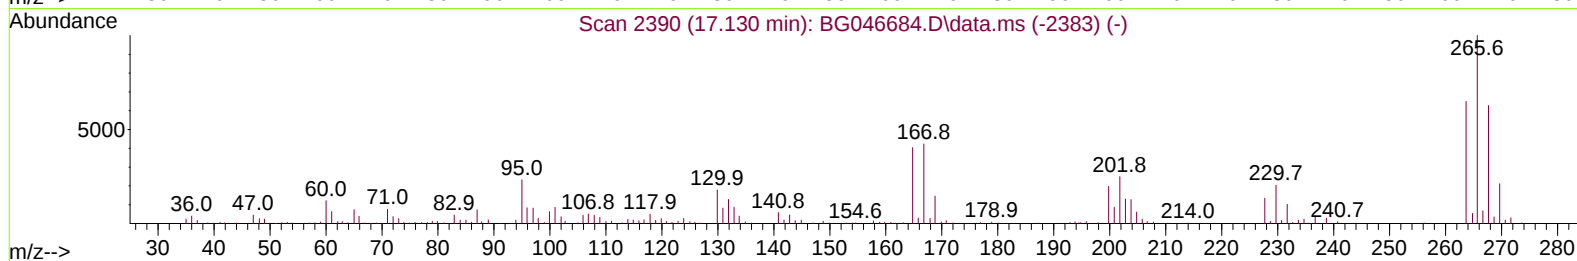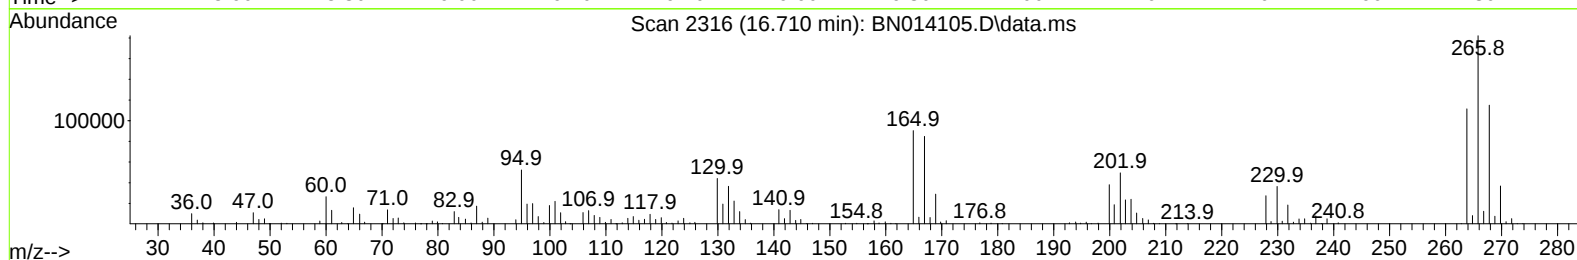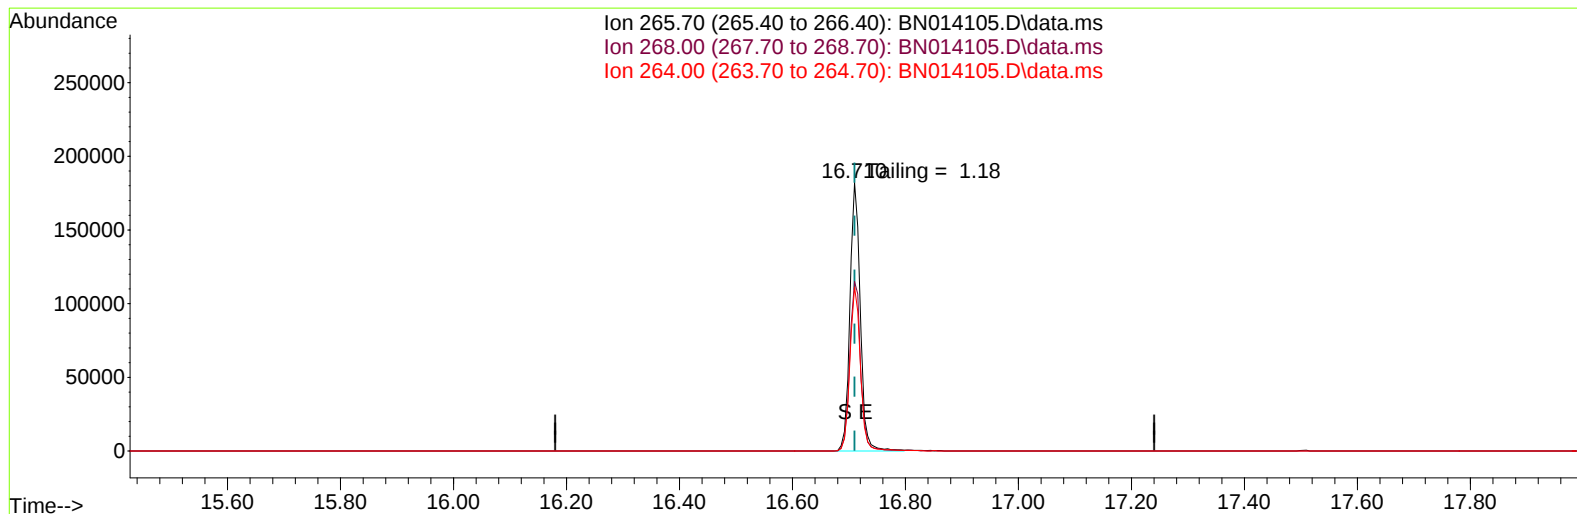

TIC: BN014105.D\data.ms

(70) Pentachlorophenol (C)

16.710min (-0.000) 25146.36 ng




response 234640

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.11
264.00	61.60	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032521\
Data File : BN014105.D
Acq On : 25 Mar 2021 14:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 26 02:17:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

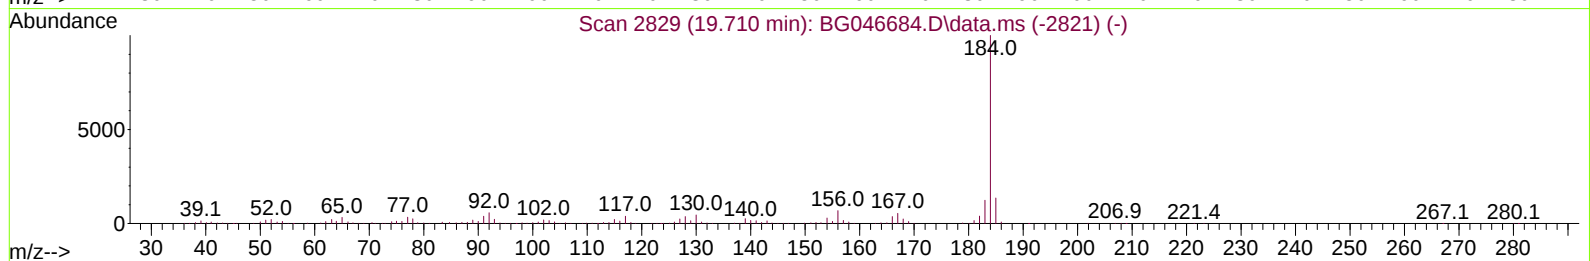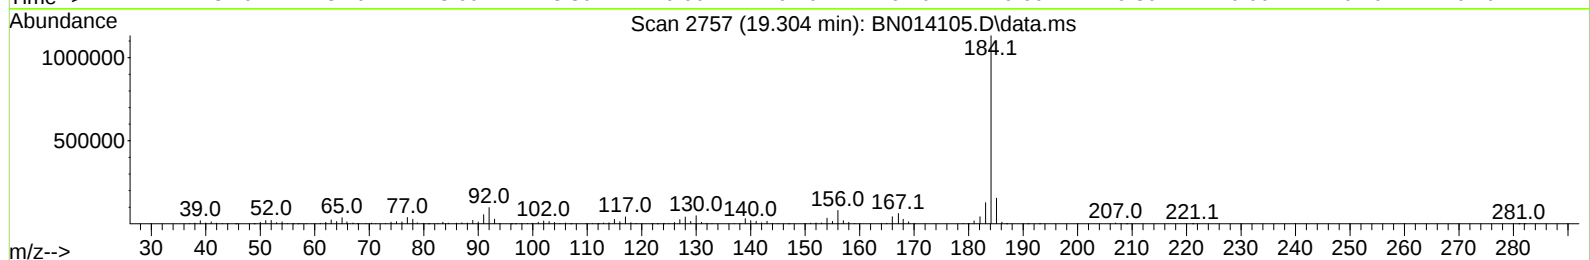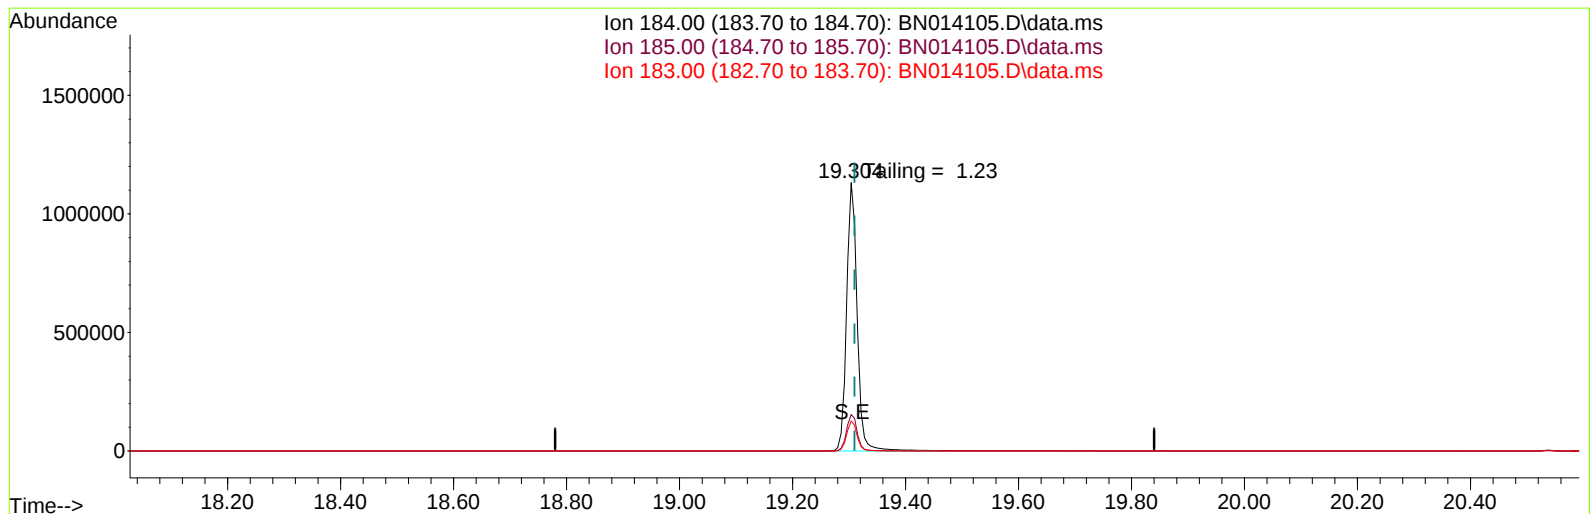

TIC: BN014105.D\data.ms

(77) Benzidine

19.304min (-0.006) 0.00 ng

response 1464060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.61
183.00	13.20	11.23
0.00	0.00	0.00