
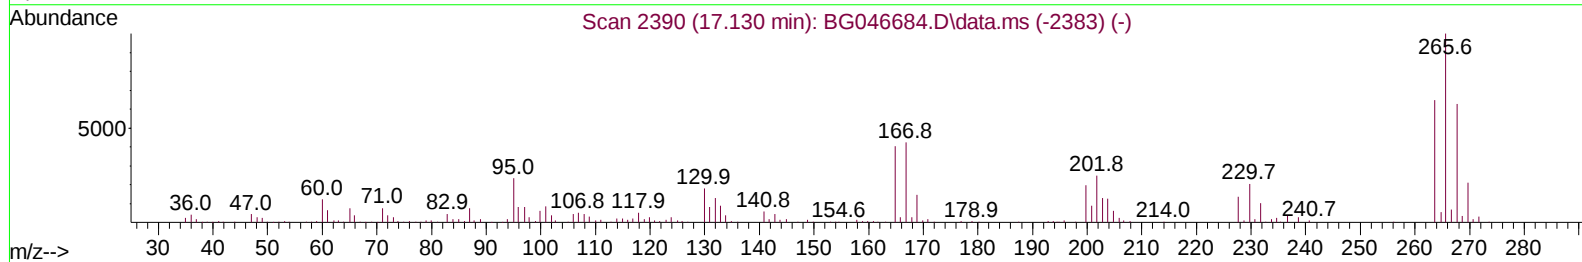
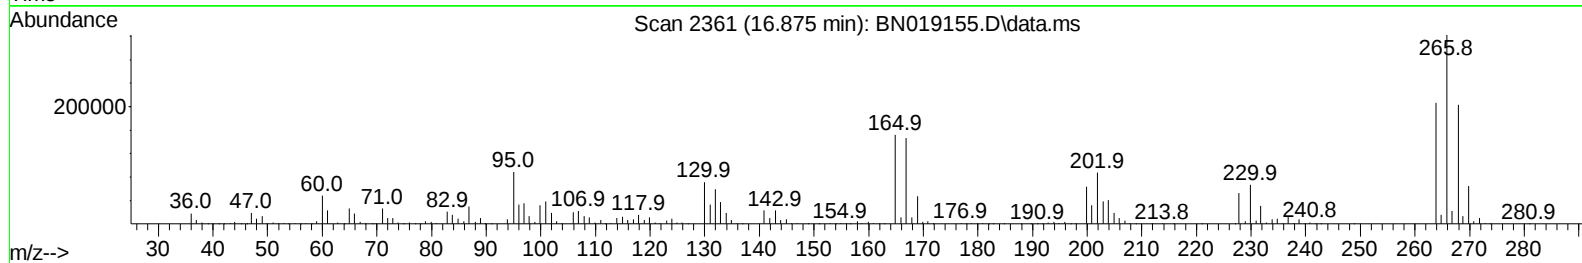


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
Data File : BN019155.D
Acq On : 25 Mar 2022 13:42
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 18:59:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:59:06 2022
Response via : Initial Calibration

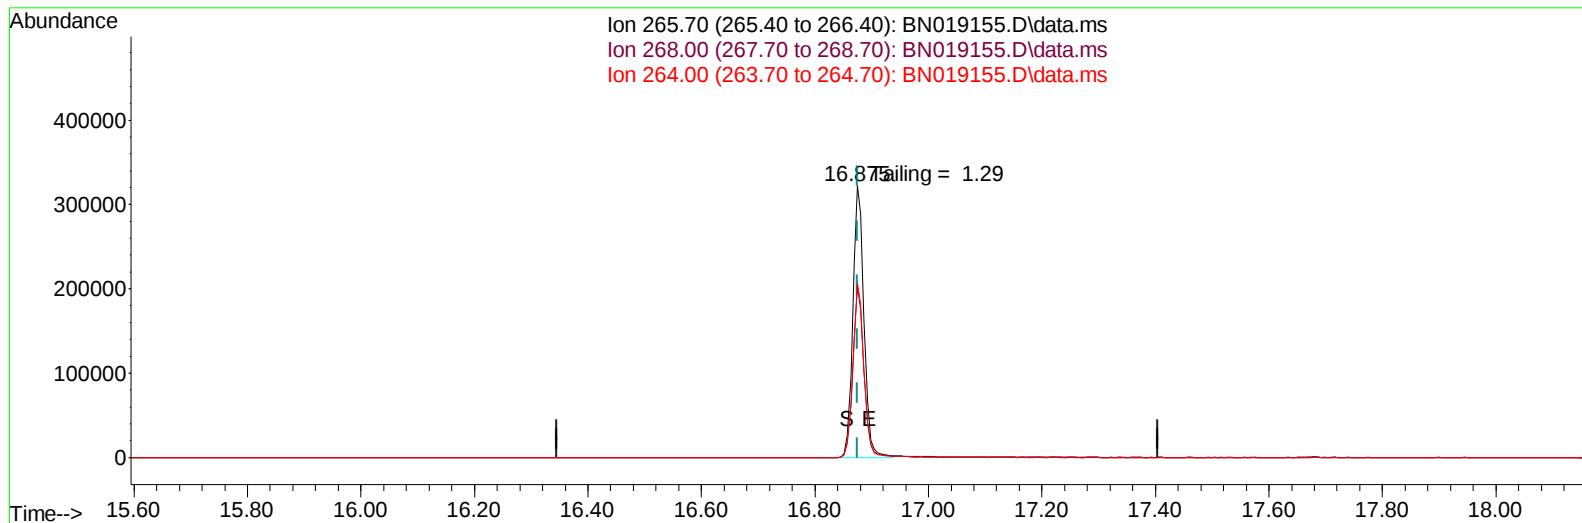




TIC: BN019155.D\data.ms

(70) Pentachlorophenol (C)**16.875min (0.000) 20586.23 ng****response 446701**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.18
264.00	61.60	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
Data File : BN019155.D
Acq On : 25 Mar 2022 13:42
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 18:59:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:59:06 2022
Response via : Initial Calibration

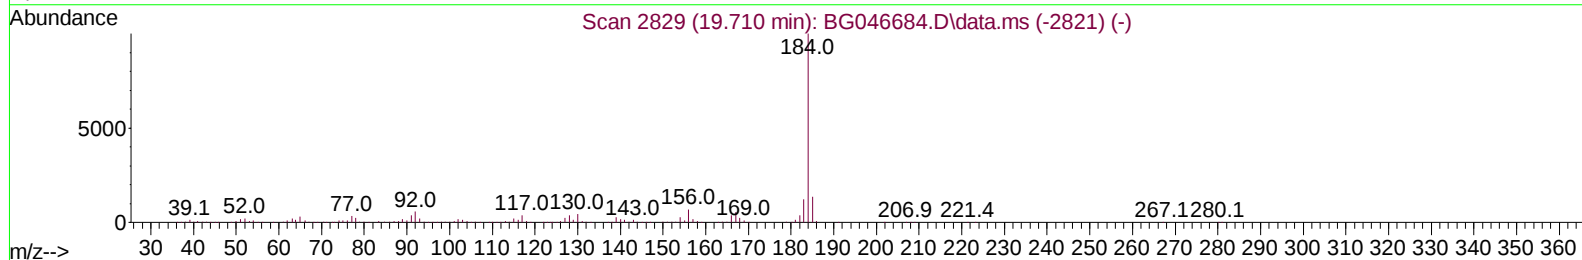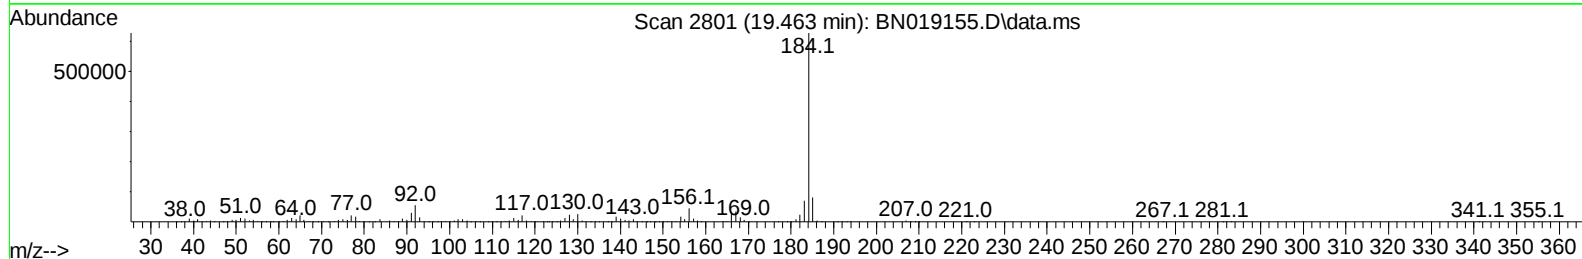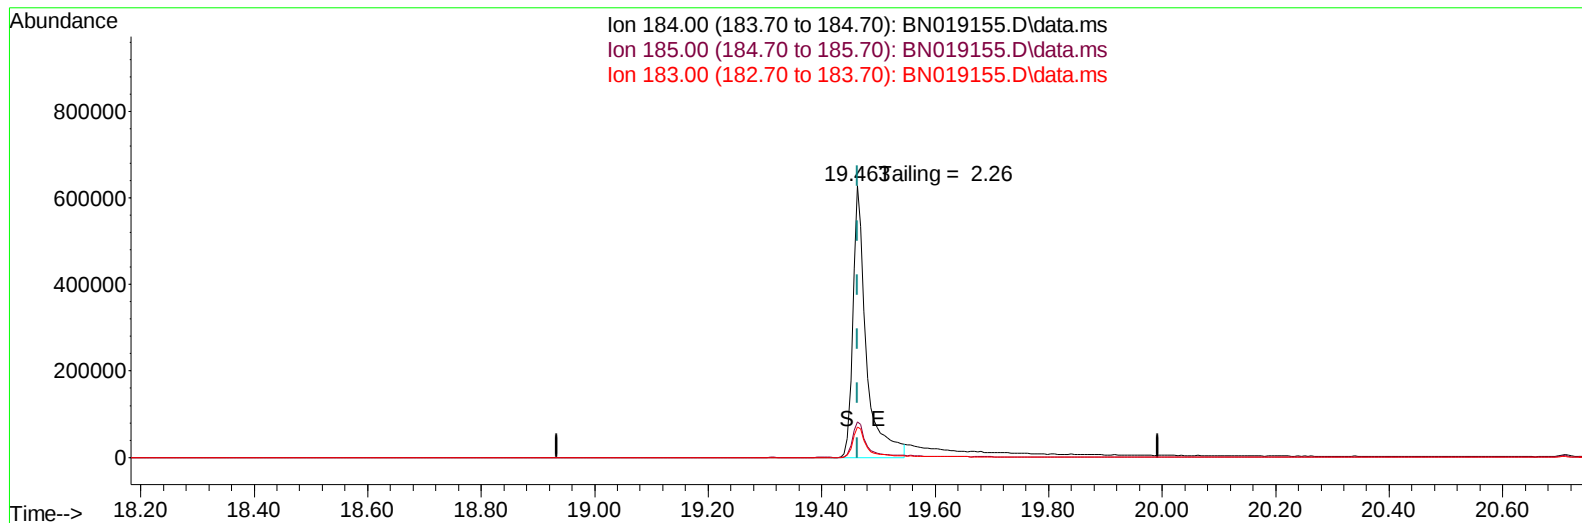

TIC: BN019155.D\data.ms

(77) Benzidine

19.463min (0.000) 0.00 ng m

response 1039596

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	11.27
0.00	0.00	0.00