
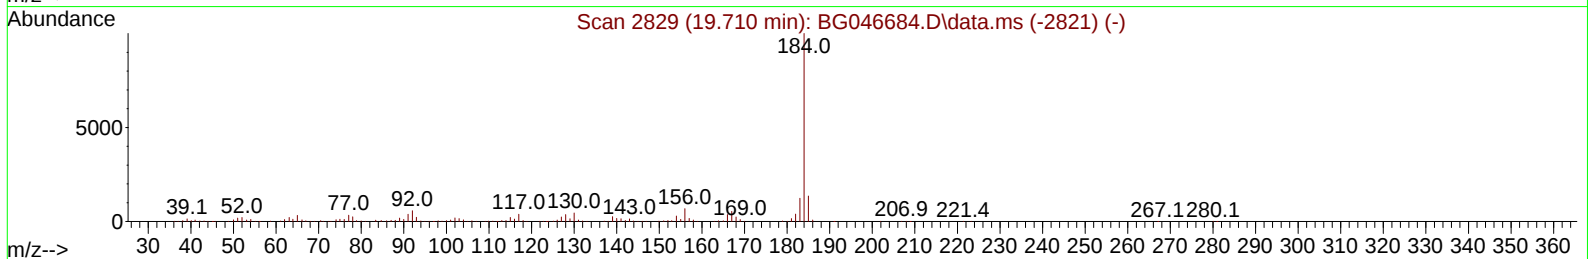
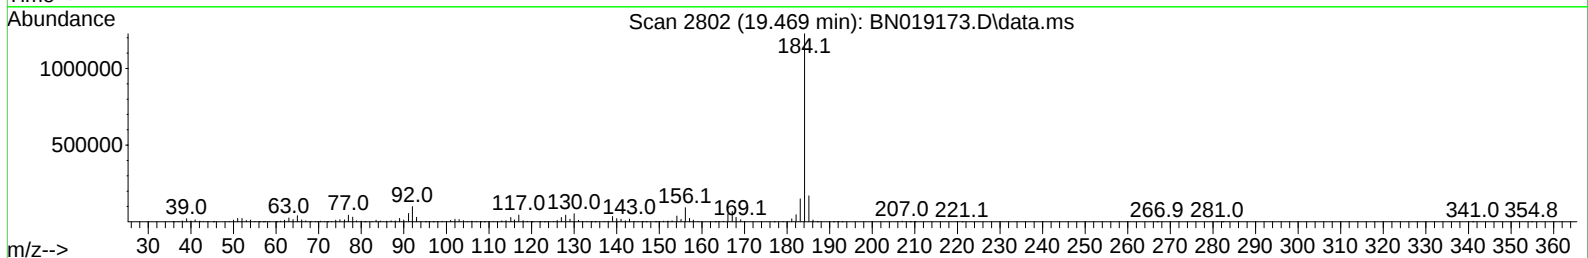


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
Data File : BN019173.D
Acq On : 26 Mar 2022 02:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:32:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

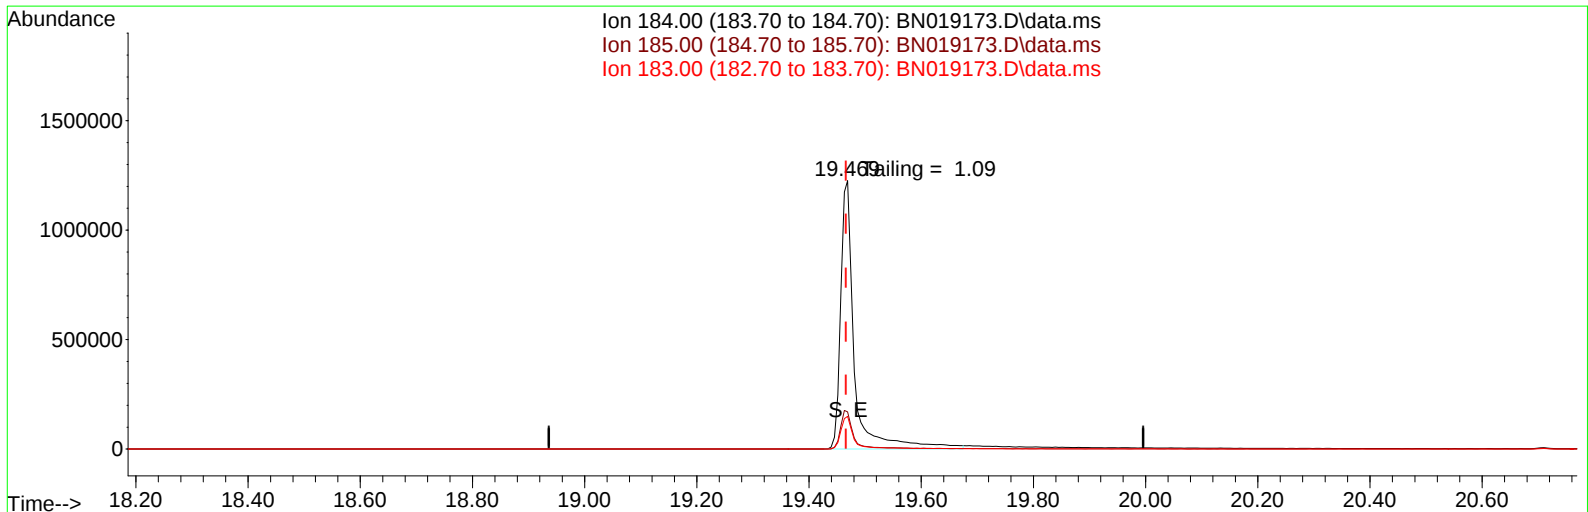




TIC: BN019173.D\data.ms

(77) Benzdine**19.469min (+ 0.003) 0.00 ng****response 2168160**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
Data File : BN019173.D
Acq On : 26 Mar 2022 02:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:32:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

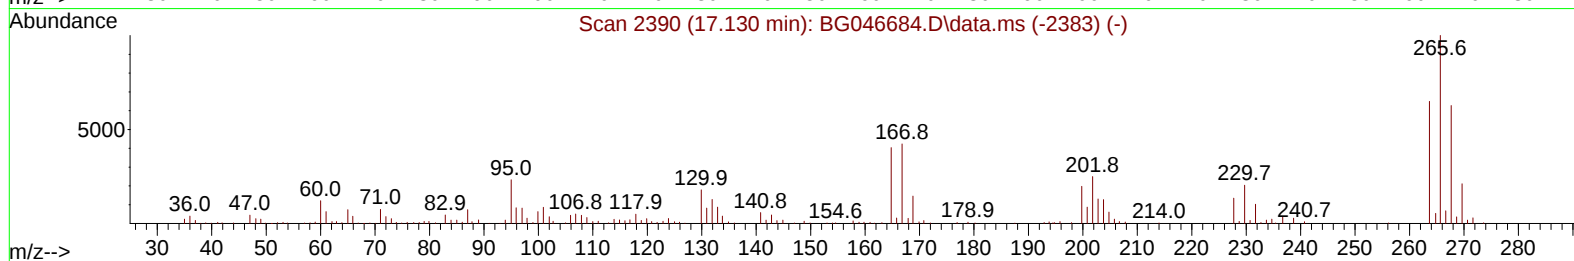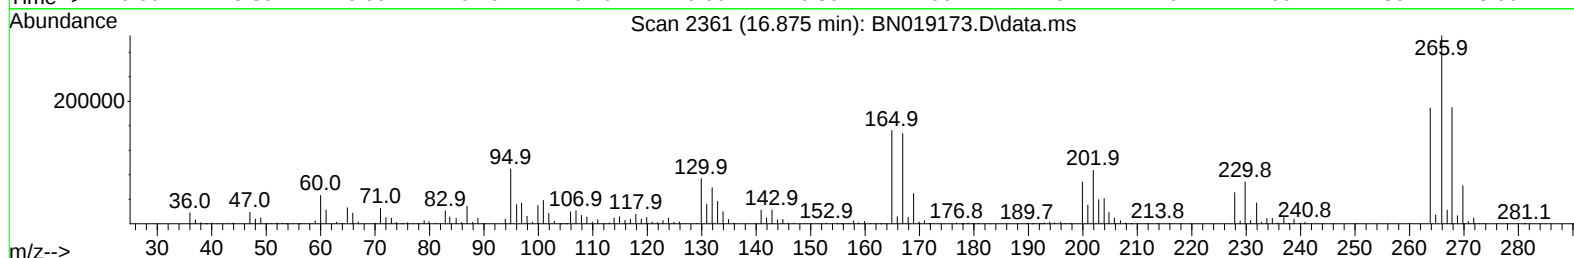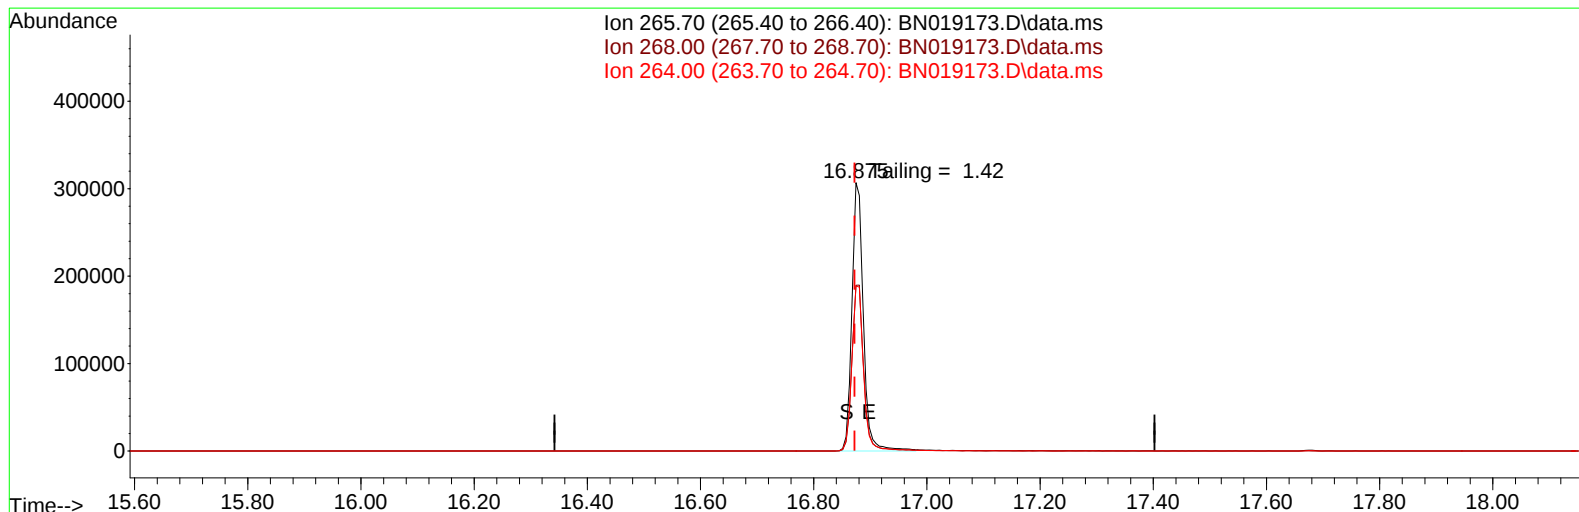

TIC: BN019173.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.003) 20800.50 ng

response 435190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.80
264.00	61.60	61.55
0.00	0.00	0.00