
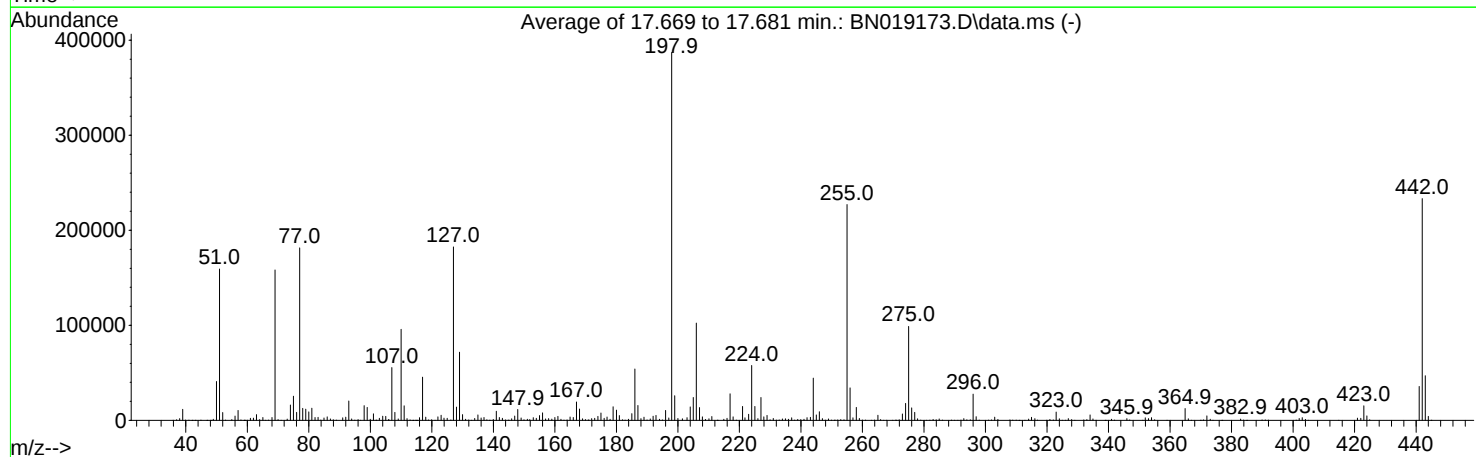


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
 Data File : BN019173.D
 Acq On : 26 Mar 2022 02:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 19:03:12 2022

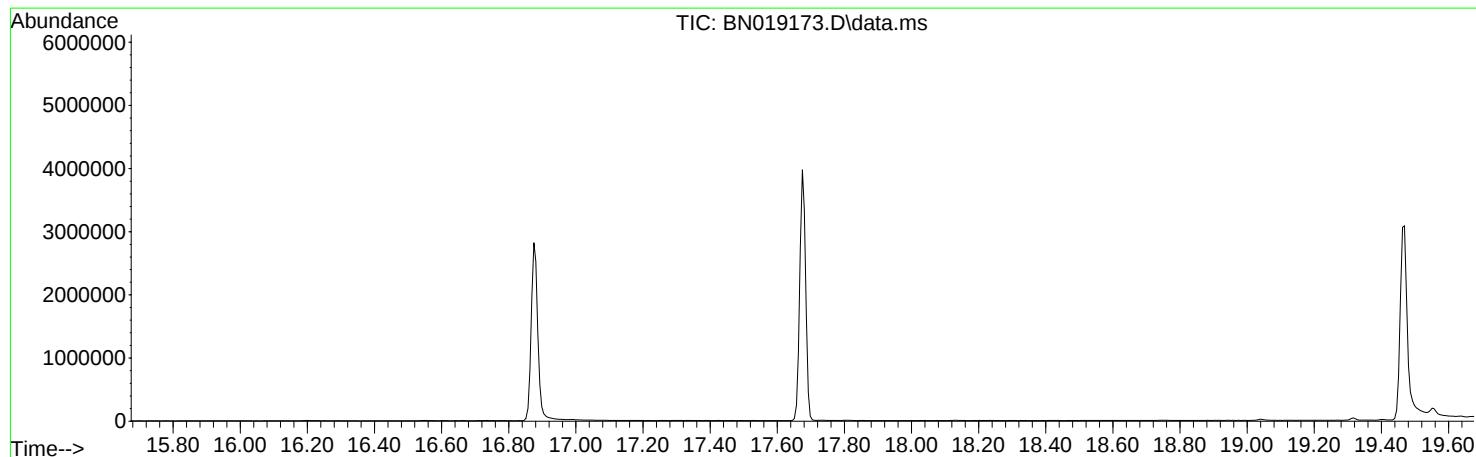




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	159277	PASS
68	69	0.00	2	1.9	2963	PASS
69	198	0.00	100	40.9	158187	PASS
70	69	0.00	2	0.5	820	PASS
127	198	10	80	47.1	182443	PASS
197	198	0.00	2	0.6	2515	PASS
198	198	100	100	100.0	387008	PASS
199	198	5	9	6.7	25955	PASS
275	198	10	60	25.5	98864	PASS
365	198	1	100	3.2	12480	PASS
441	198	0.01	100	9.2	35691	PASS
442	442	50	100	100.0	233333	PASS
443	442	15	24	20.1	47005	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
Data File : BN019173.D
Acq On : 26 Mar 2022 02:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 26 08:32:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

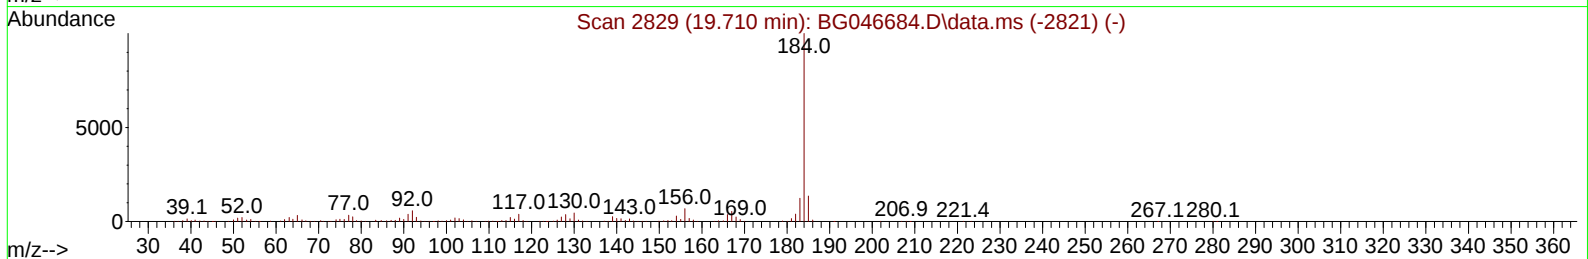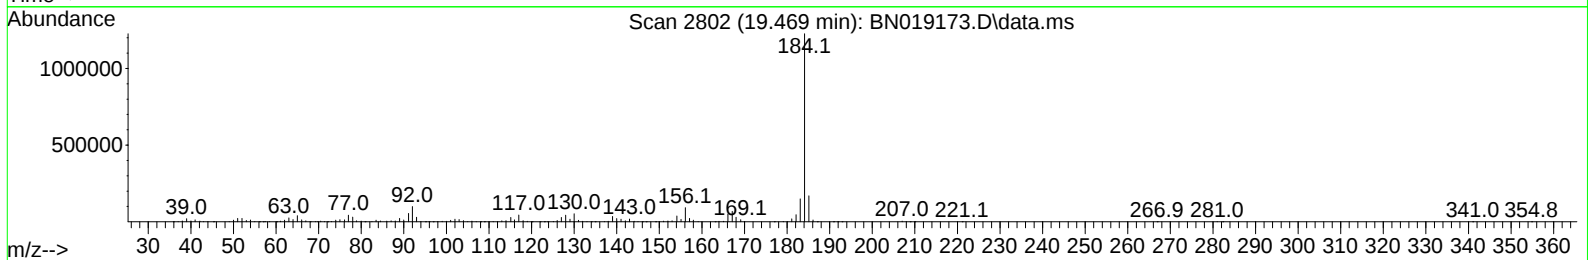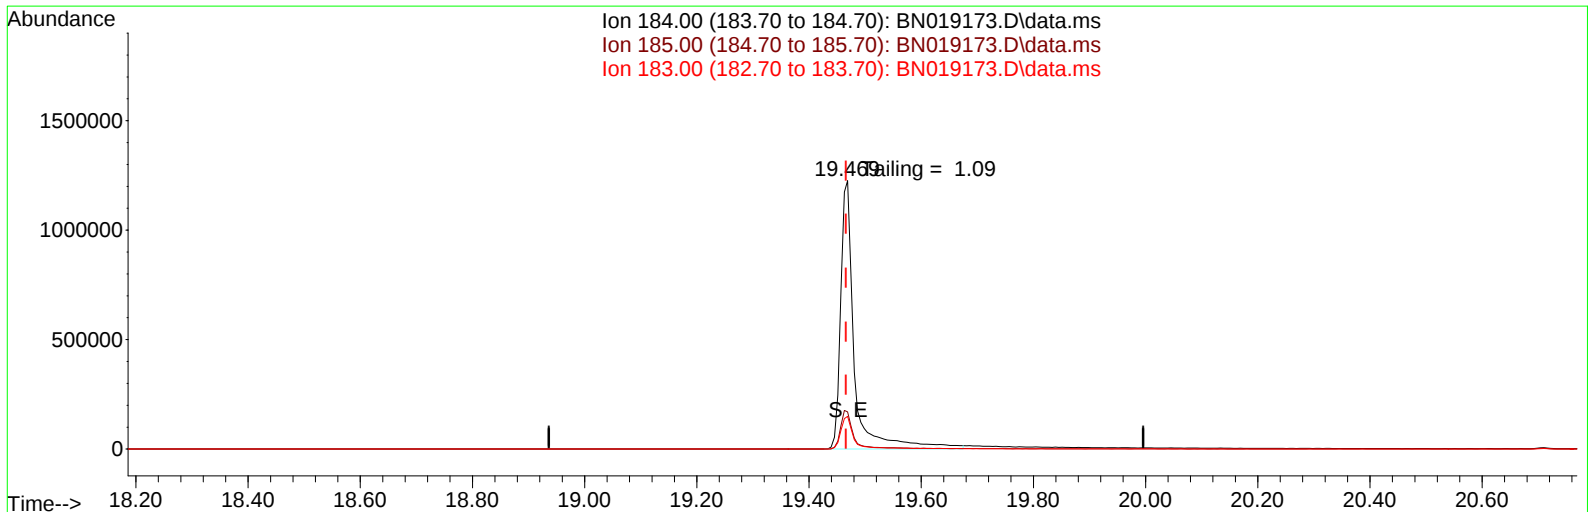

TIC: BN019173.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng




response 2168160

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032522\
 Data File : BN019173.D
 Acq On : 26 Mar 2022 02:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 26 08:32:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

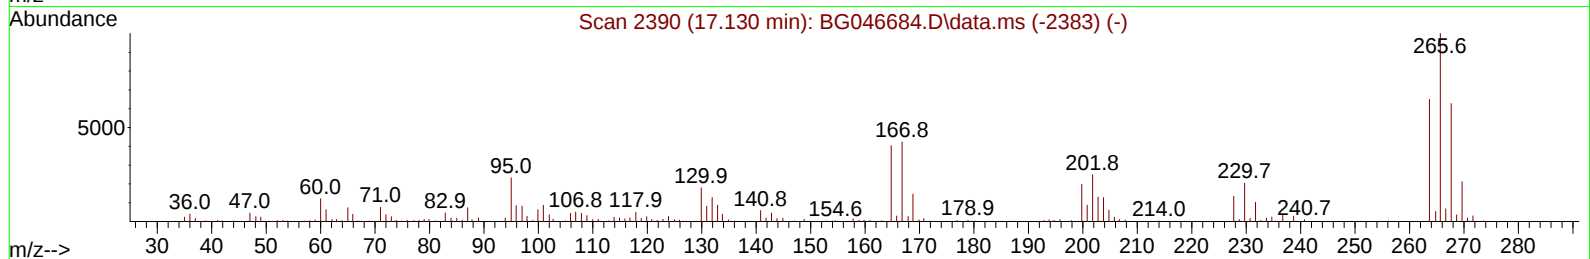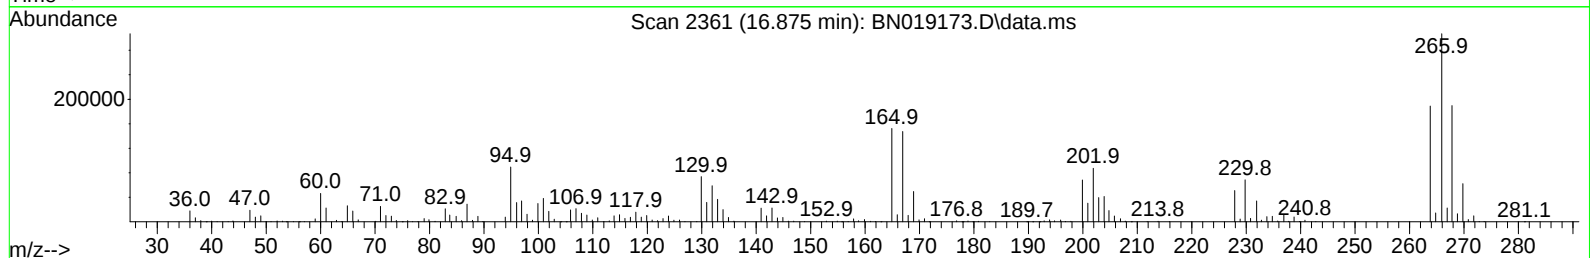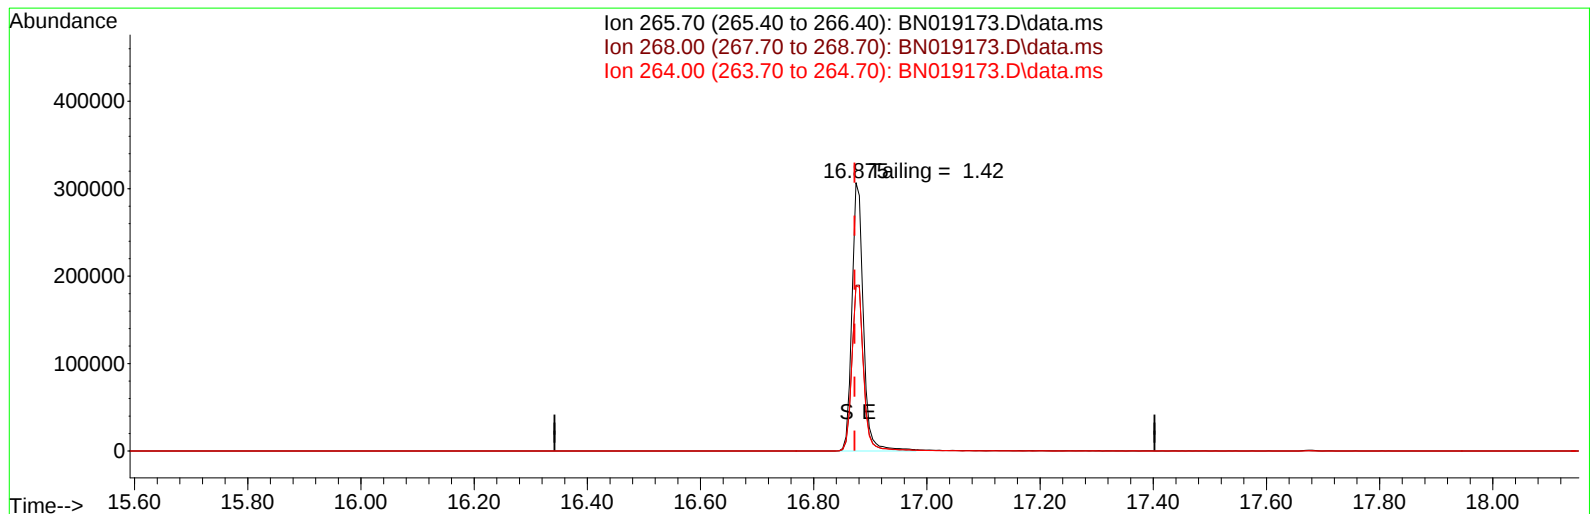

TIC: BN019173.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.003) 20800.50 ng

response 435190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.80
264.00	61.60	61.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2022	BNA_N	<u>BN019173.D</u>
Compound Name	Response	Retention Time
DDT	1313077	20.71
DDD	30505	20.269
DDE	823	19.759
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31328	1344405	2.33

Instrument :
BNA_N
ClientSampleId :
DFTPP