




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030481.D
Acq On : 25 Mar 2024 15:03
Operator : MA/JU
Sample : P1813-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOLY0

Manual IntegrationsAPPROVED

Quant Time: Mar 25 15:31:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

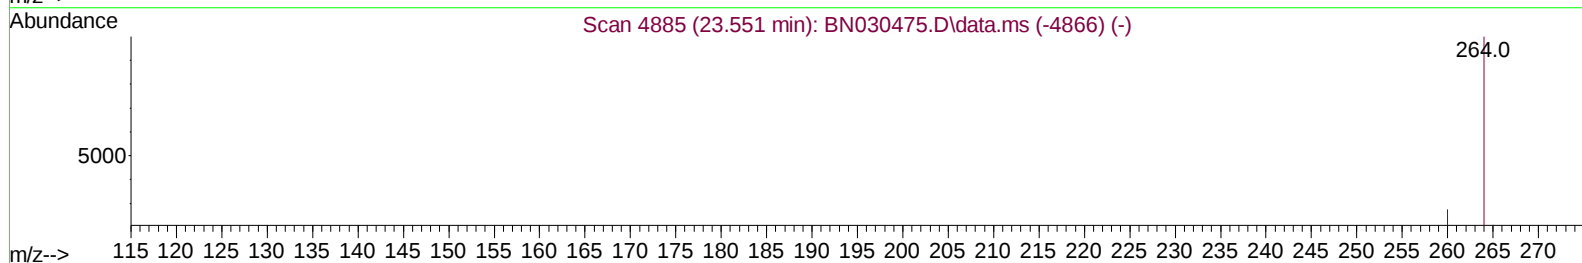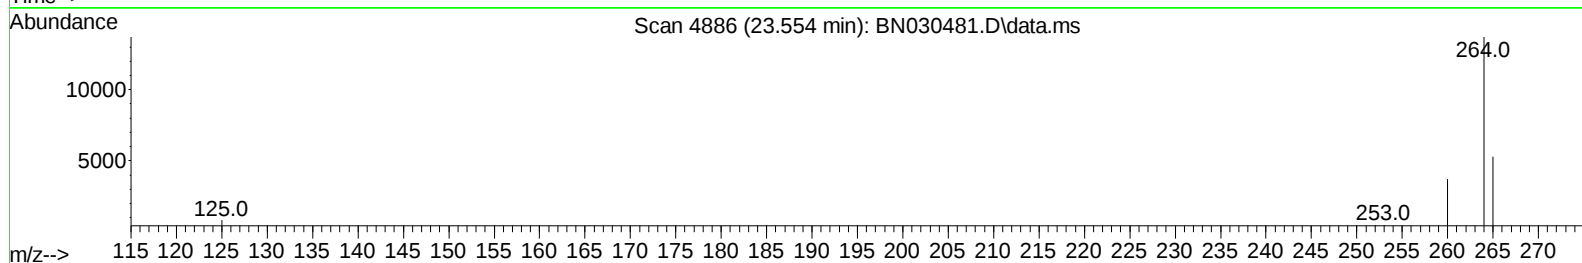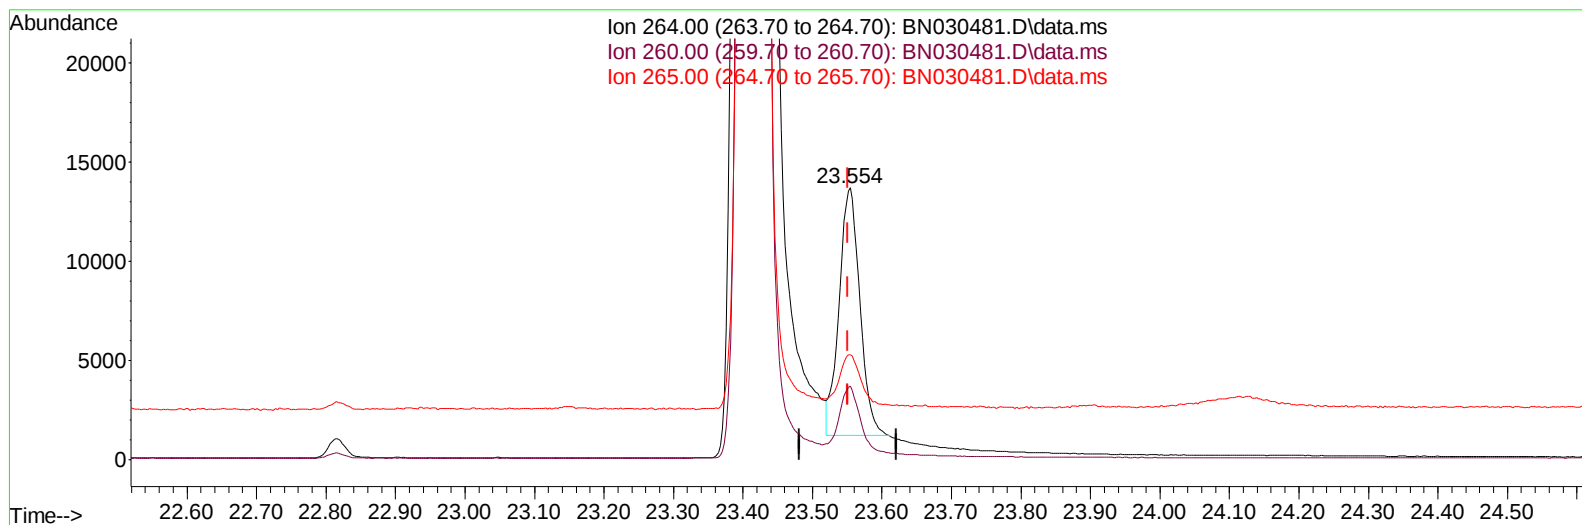

TIC: BN030481.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul

response 26012

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	27.00
265.00	41.20	38.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030481.D
Acq On : 25 Mar 2024 15:03
Operator : MA/JU
Sample : P1813-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOLY0

Manual IntegrationsAPPROVED

Quant Time: Mar 25 15:31:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

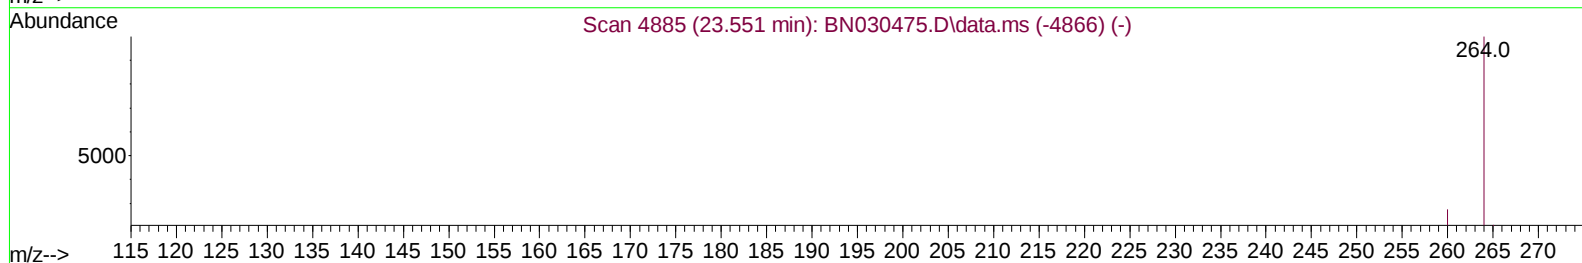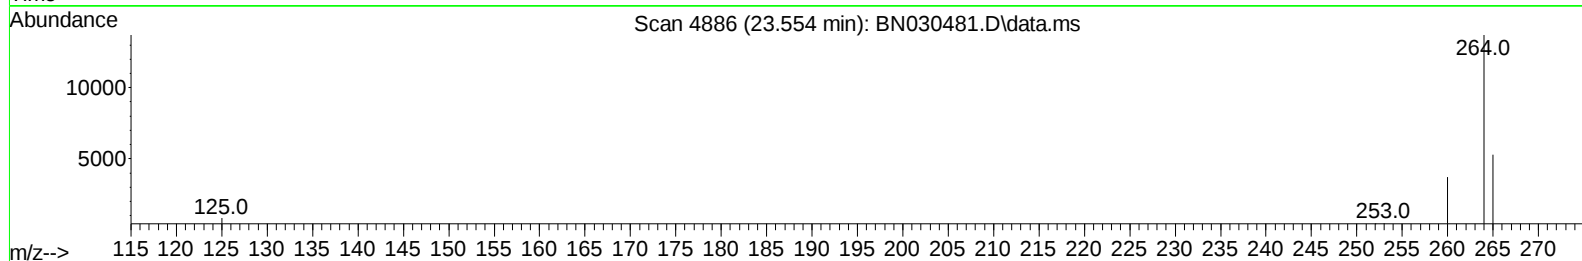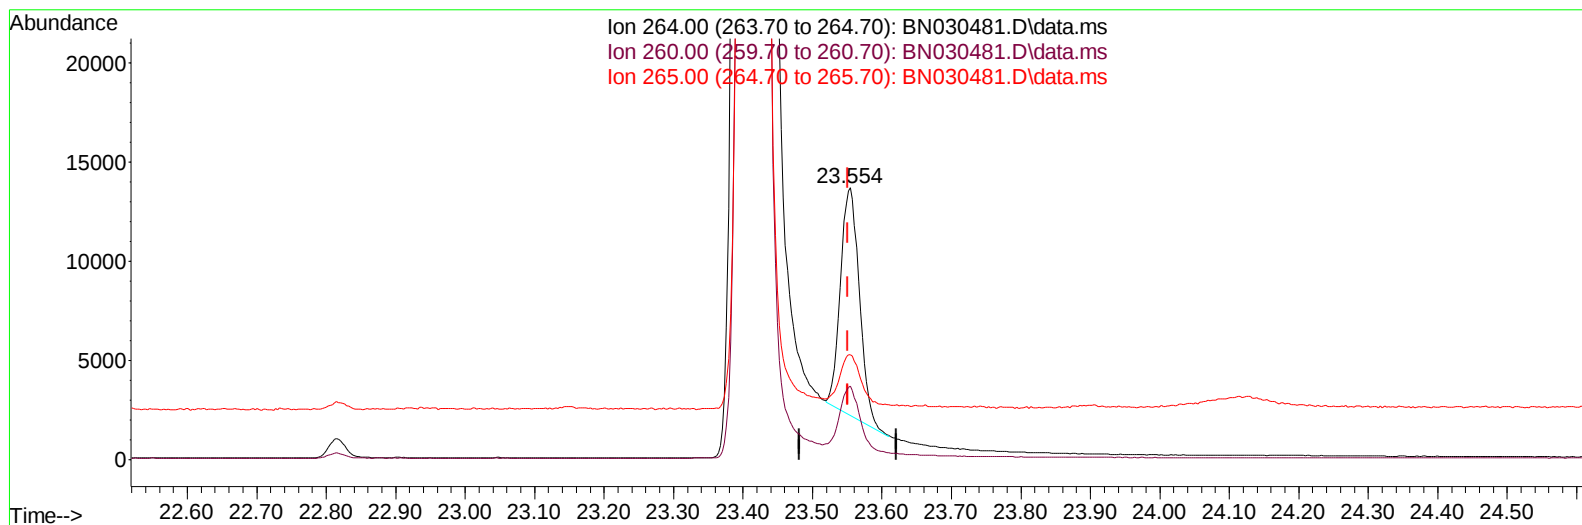

TIC: BN030481.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul m

response 21533

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	27.00
265.00	41.20	38.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030481.D
 Acq On : 25 Mar 2024 15:03
 Operator : MA/JU
 Sample : P1813-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LY0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 15:31:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.729	152	9104	0.400	ng/ul	0.00
4) Naphthalene-d8	10.513	136	26818	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.363	164	15094	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.108	188	35035	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	25753	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264	21533m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	40871	3.821	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152	8997	0.238	ng/ul	0.00
18) Fluoranthene-d10	19.142	212	25094	0.312	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030481.D
Acq On : 25 Mar 2024 15:03
Operator : MA/JU
Sample : P1813-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY0

Manual IntegrationsAPPROVED

Quant Time: Mar 25 15:31:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

