
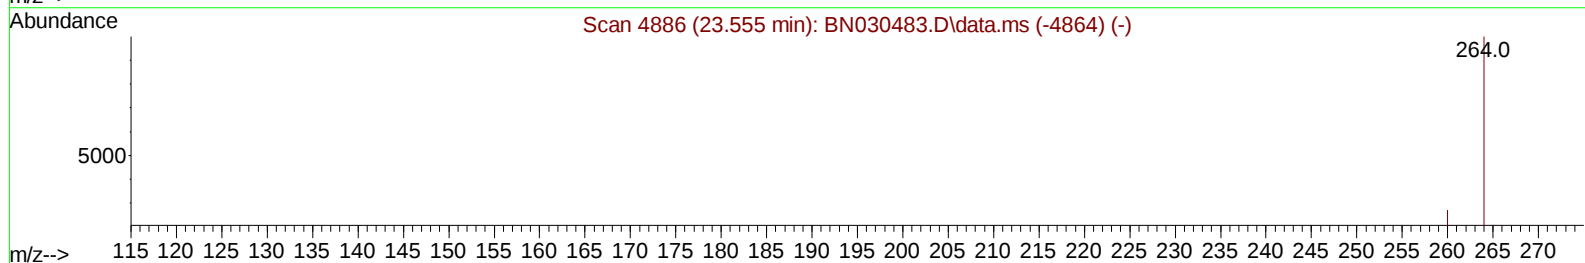
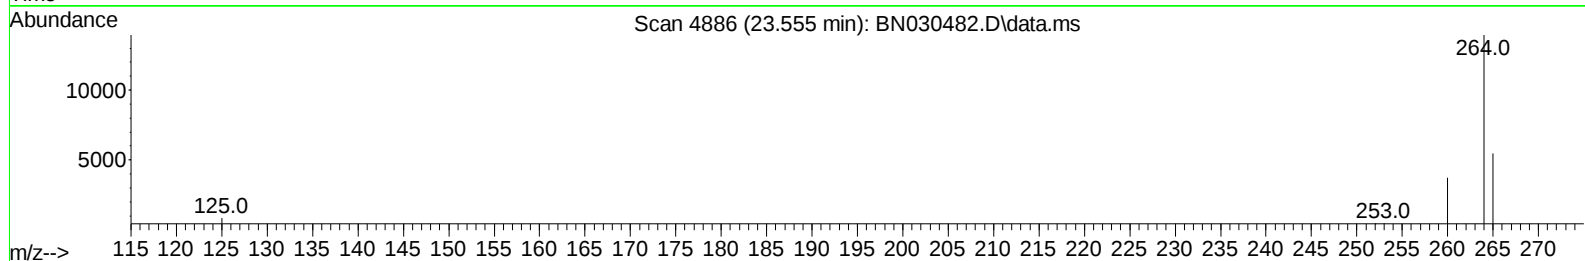


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030482.D
Acq On : 25 Mar 2024 15:40
Operator : MA/JU
Sample : P1813-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 28 01:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

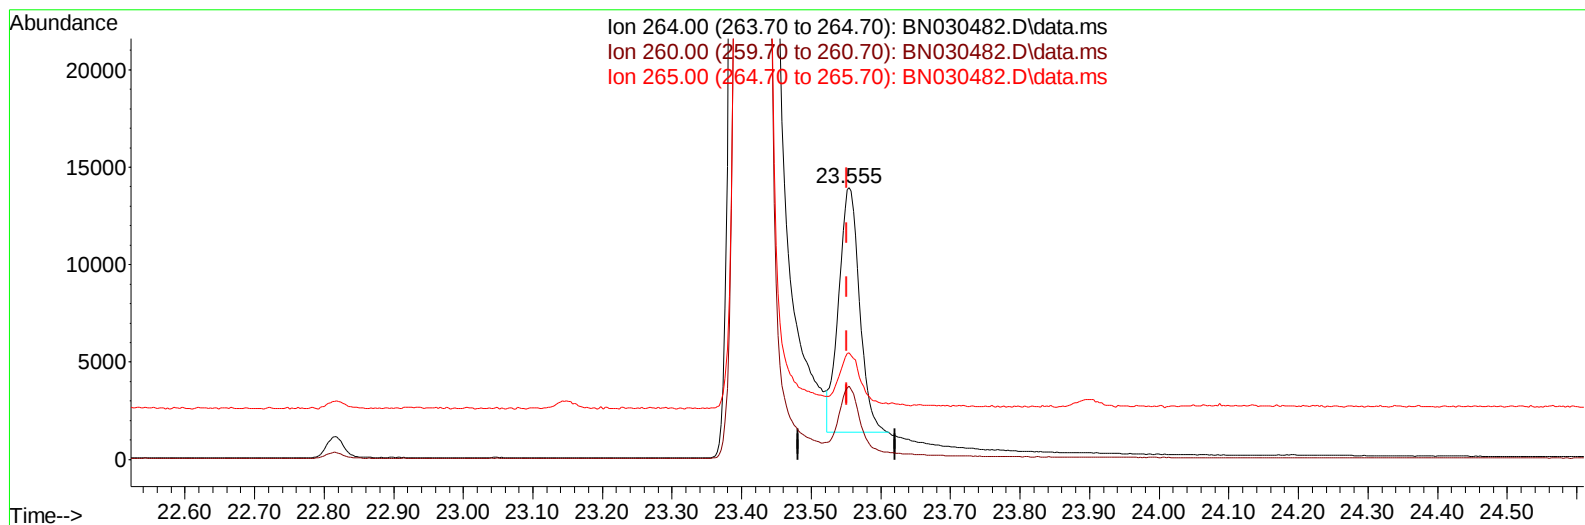

TIC: BN030482.D\data.ms

(23) Perylene-d12 (I)




23.555min (+ 0.004) 0.40 ng/ul

response 26229

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.90
265.00	41.20	39.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030482.D
Acq On : 25 Mar 2024 15:40
Operator : MA/JU
Sample : P1813-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 28 01:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

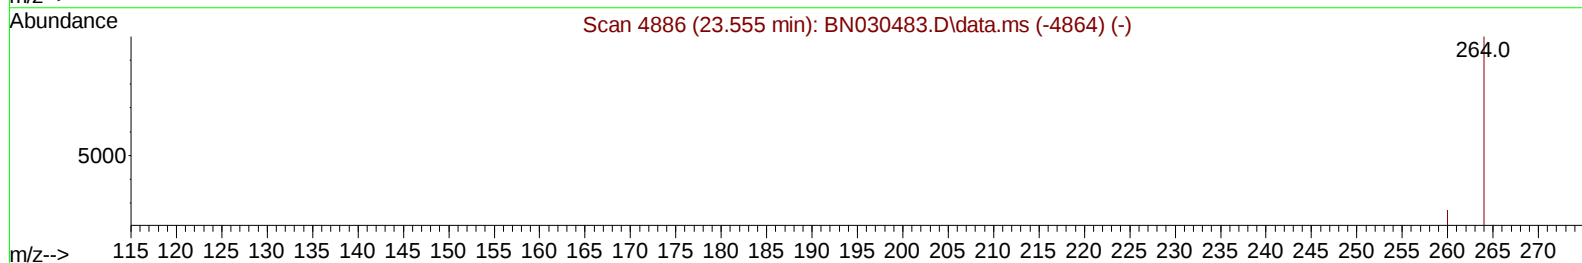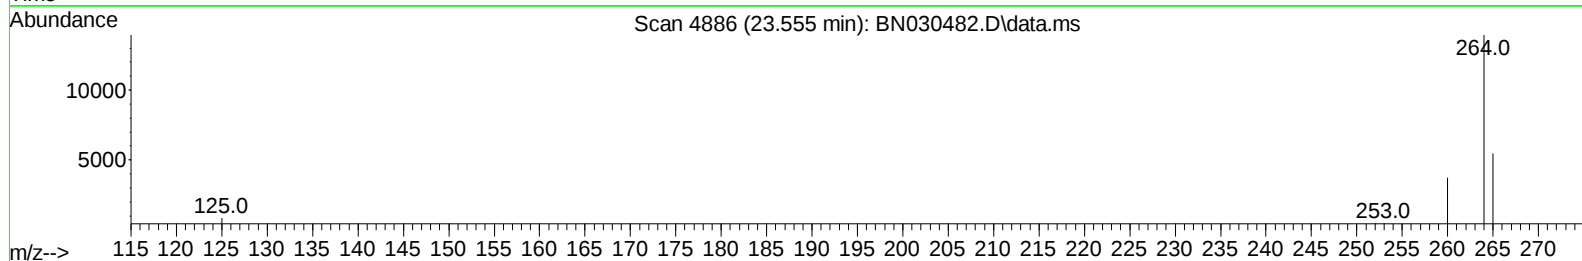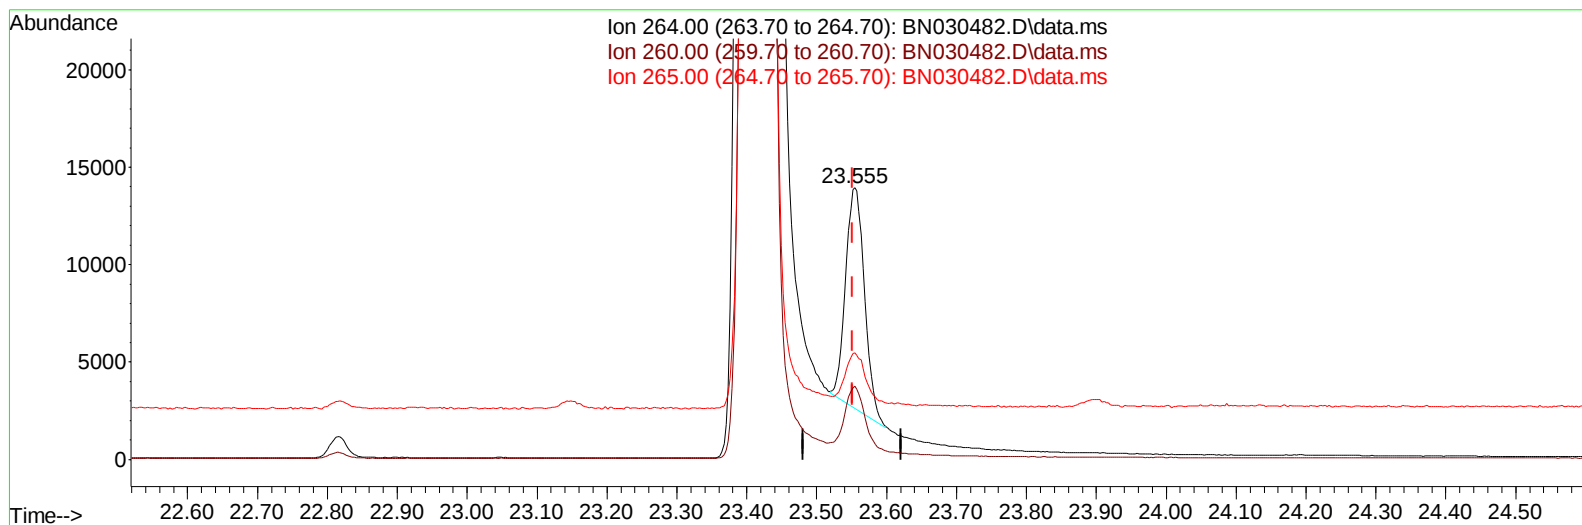

TIC: BN030482.D\data.ms

(23) Perylene-d12 (I)

23.555min (+ 0.004) 0.40 ng/ul m

response 21133

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.90
265.00	41.20	39.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030482.D
 Acq On : 25 Mar 2024 15:40
 Operator : MA/JU
 Sample : P1813-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 28 01:39:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	9639	0.400	ng/ul	0.00
4) Naphthalene-d8	10.511	136	28354	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.366	164	16041	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.111	188	36832	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	26273	0.400	ng/ul	0.00
23) Perylene-d12	23.555	264	21133m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	46486	4.104	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.106	152	10978	0.275	ng/ul	0.00
18) Fluoranthene-d10	19.140	212	29489	0.360	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.256	88	2649	0.226	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030482.D
Acq On : 25 Mar 2024 15:40
Operator : MA/JU
Sample : P1813-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 28 01:39:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

