




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030485.D
Acq On : 25 Mar 2024 17:33
Operator : MA/JU
Sample : PB159747BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK747

Manual IntegrationsAPPROVED

Quant Time: Mar 25 18:57:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

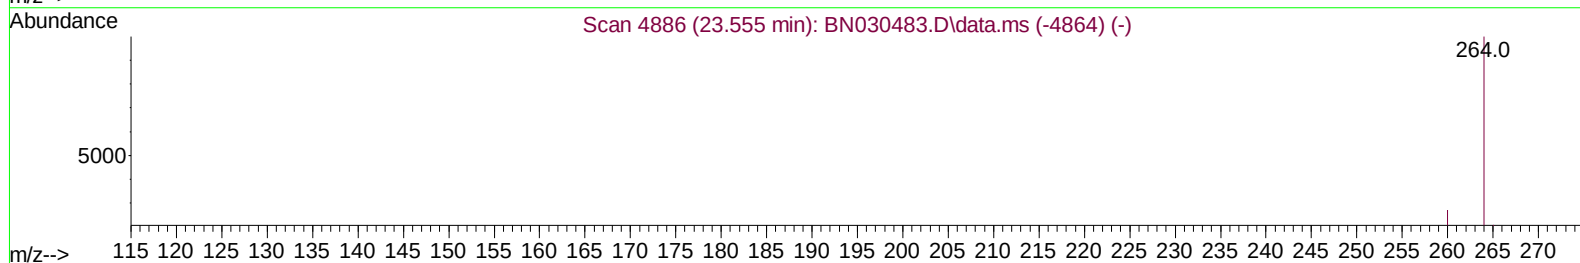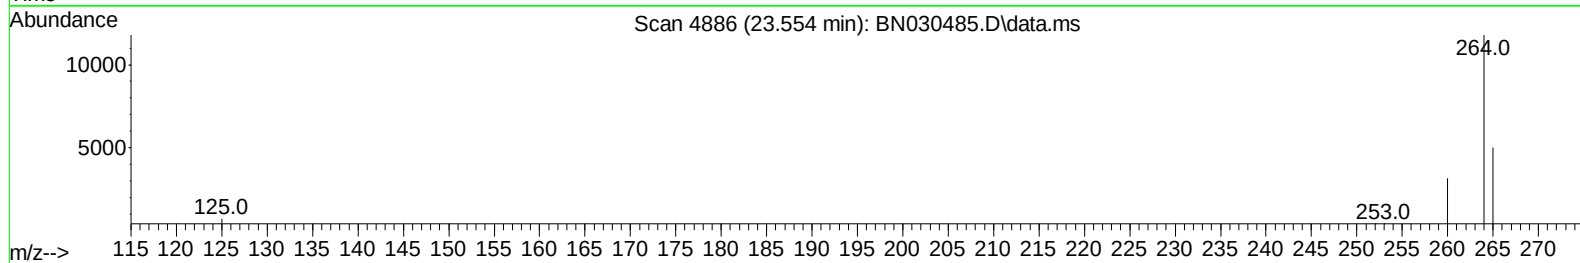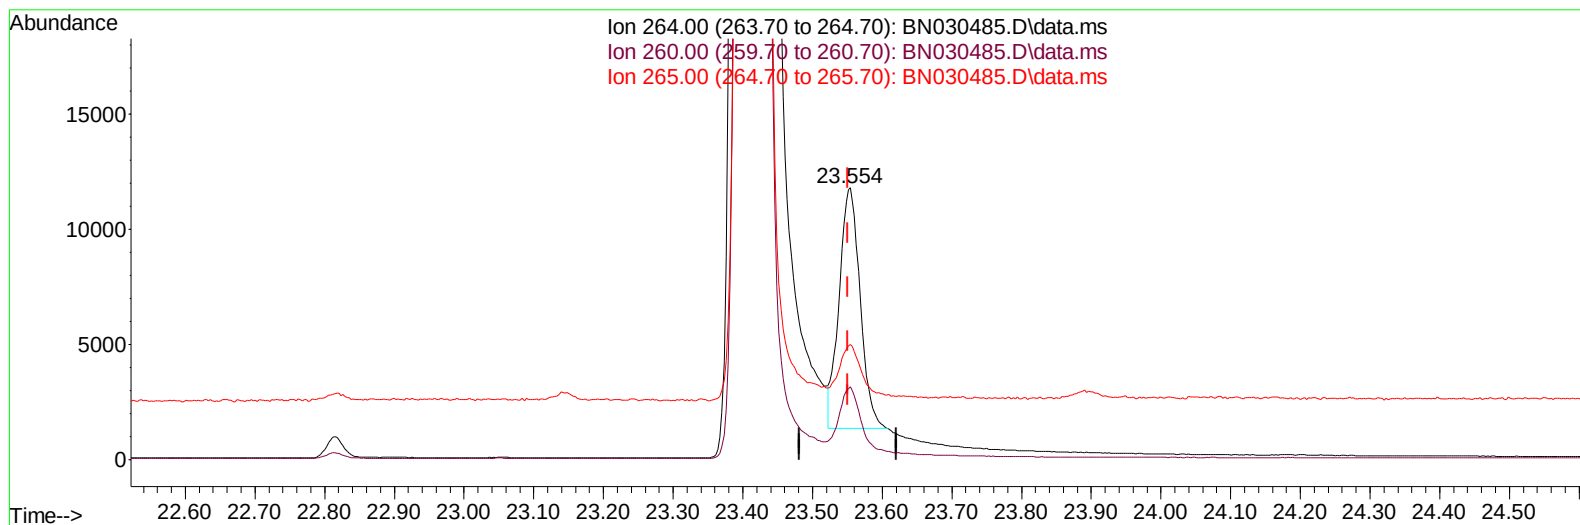

TIC: BN030485.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul

response 21825

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.67
265.00	41.20	42.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030485.D
Acq On : 25 Mar 2024 17:33
Operator : MA/JU
Sample : PB159747BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK747

Manual IntegrationsAPPROVED

Quant Time: Mar 25 18:57:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

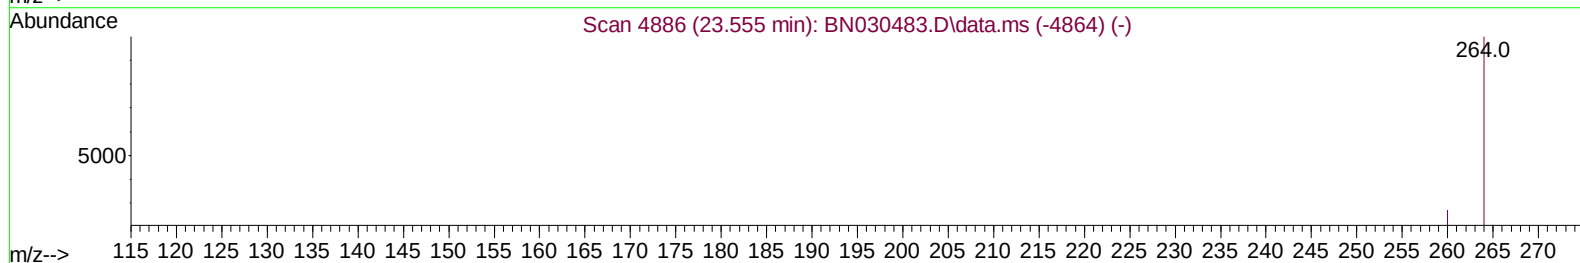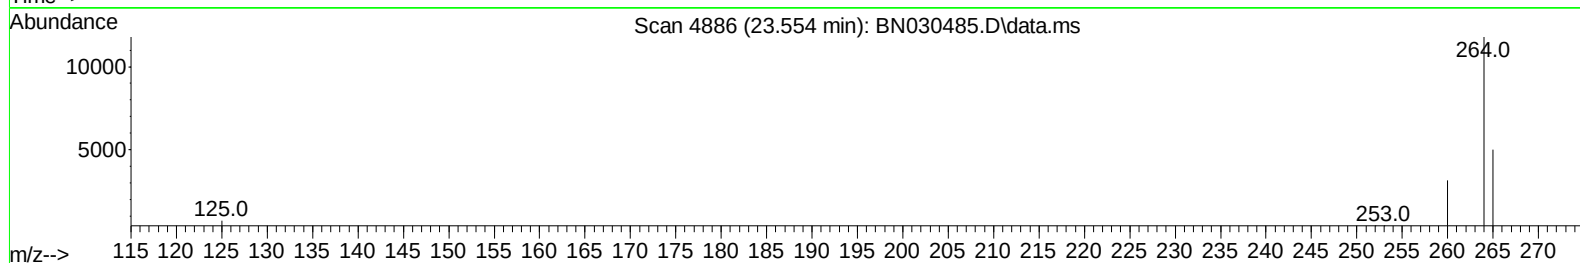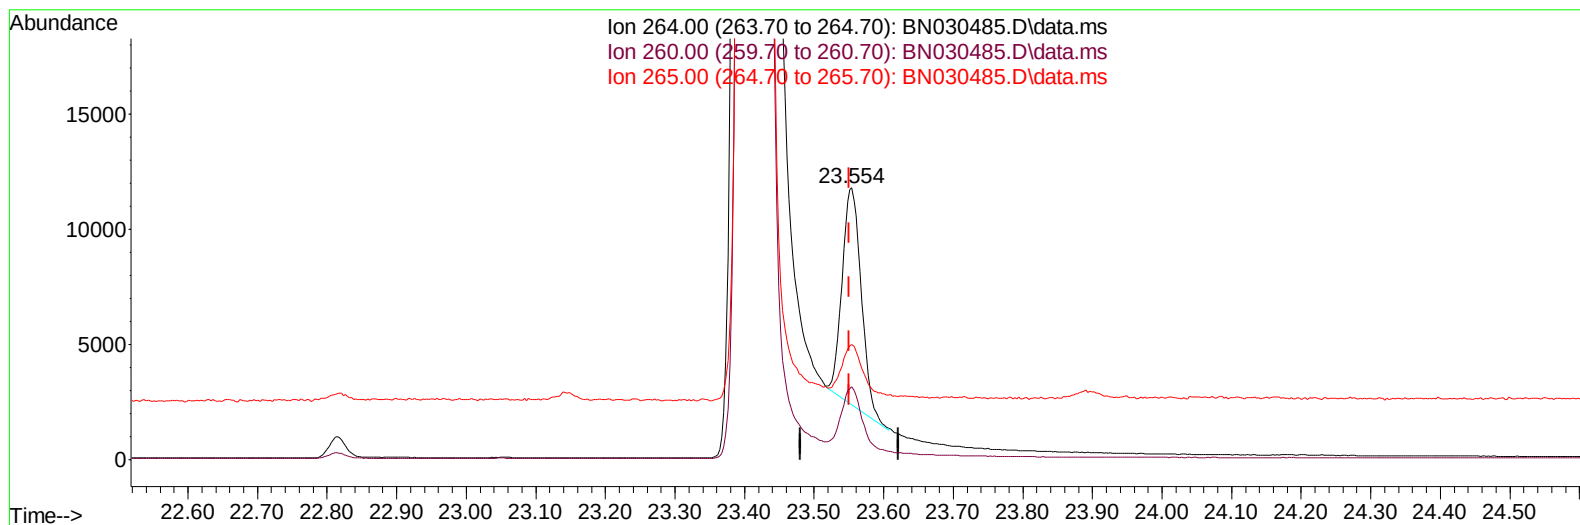

TIC: BN030485.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul m

response 17835

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.67
265.00	41.20	42.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030485.D
 Acq On : 25 Mar 2024 17:33
 Operator : MA/JU
 Sample : PB159747BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK747

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 18:57:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	8971	0.400	ng/ul	0.00
4) Naphthalene-d8	10.513	136	26714	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.363	164	14935	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.112	188	33811	0.400	ng/ul	0.00
17) Chrysene-d12	21.301	240	20910	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264	17835m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	64745	6.142	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152	12013	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.142	212	25816	0.396	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030485.D
Acq On : 25 Mar 2024 17:33
Operator : MA/JU
Sample : PB159747BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK747

Manual IntegrationsAPPROVED

Quant Time: Mar 25 18:57:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

