
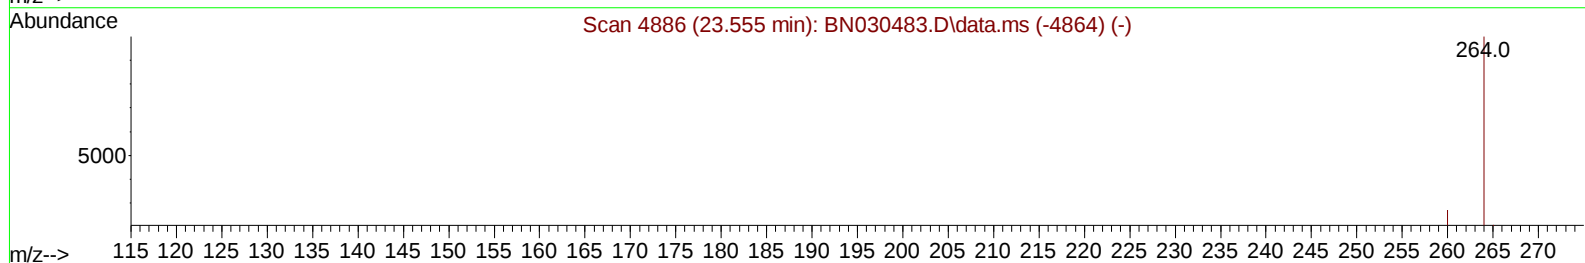
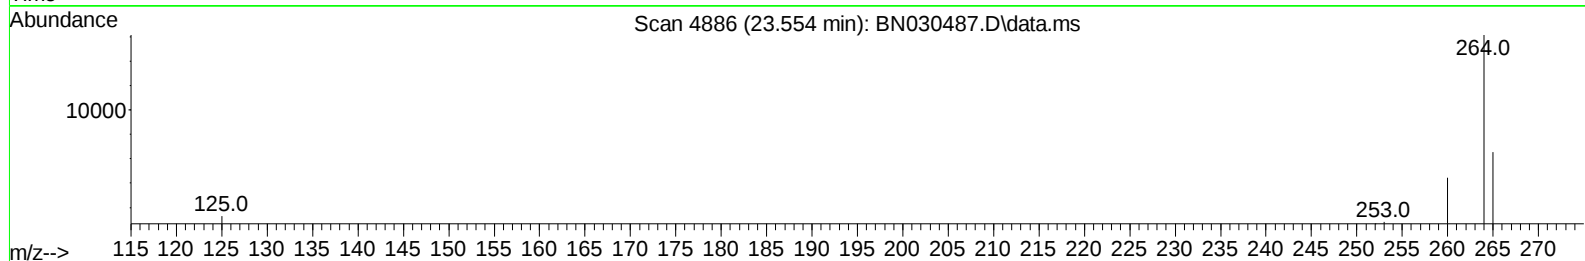


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030487.D
Acq On : 25 Mar 2024 18:46
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 28 01:41:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

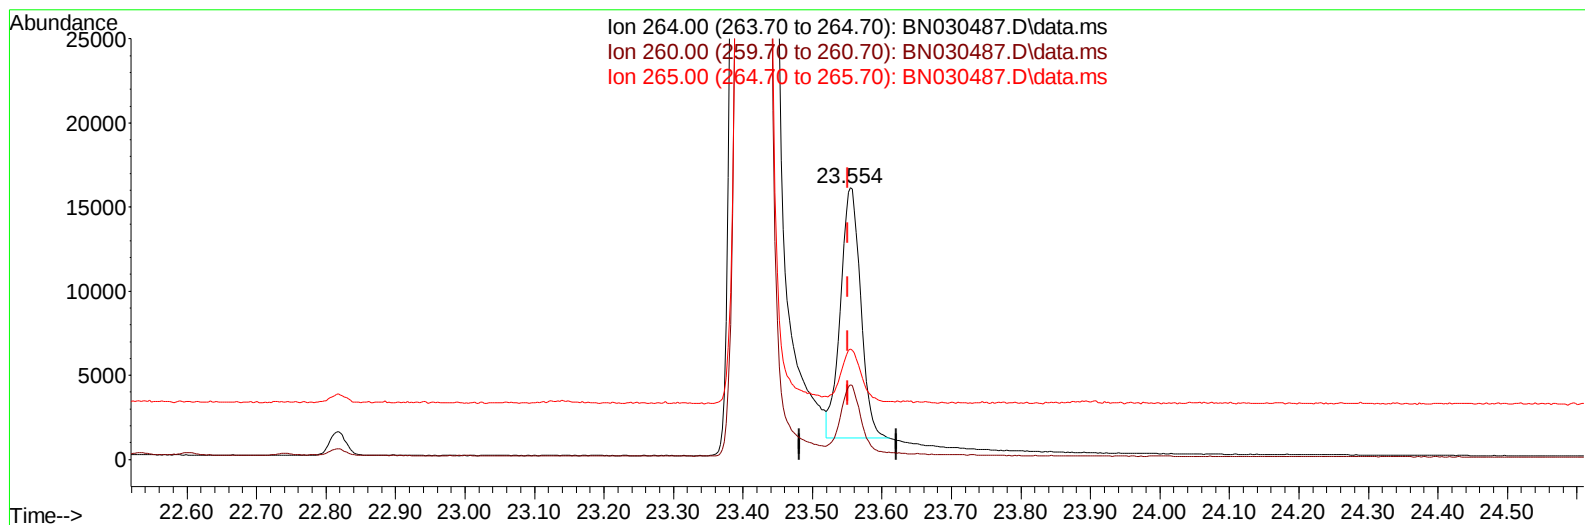

TIC: BN030487.D\data.ms

(23) Perylene-d12 (I)




23.554min (+ 0.003) 0.40 ng/ul

response 30215

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	27.53
265.00	41.20	40.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030487.D
Acq On : 25 Mar 2024 18:46
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 28 01:41:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

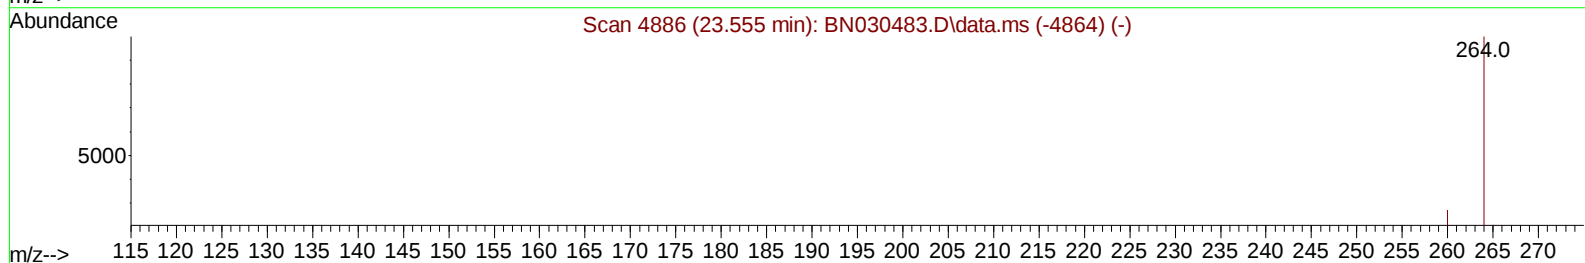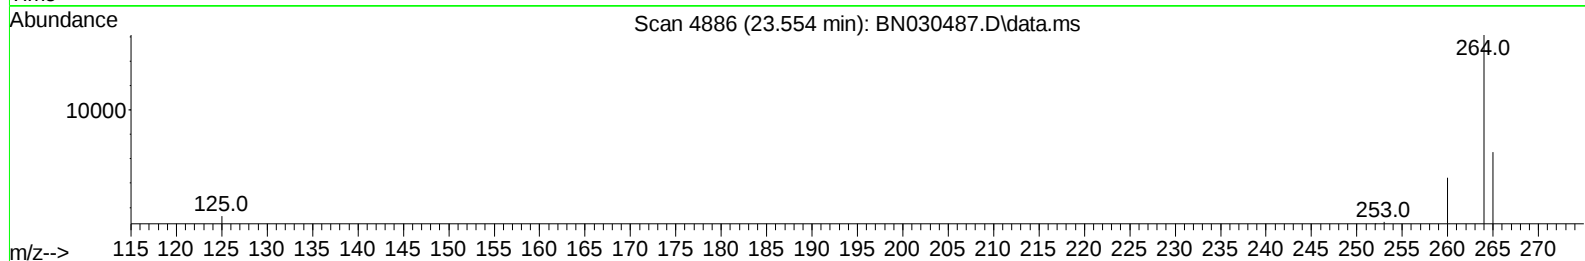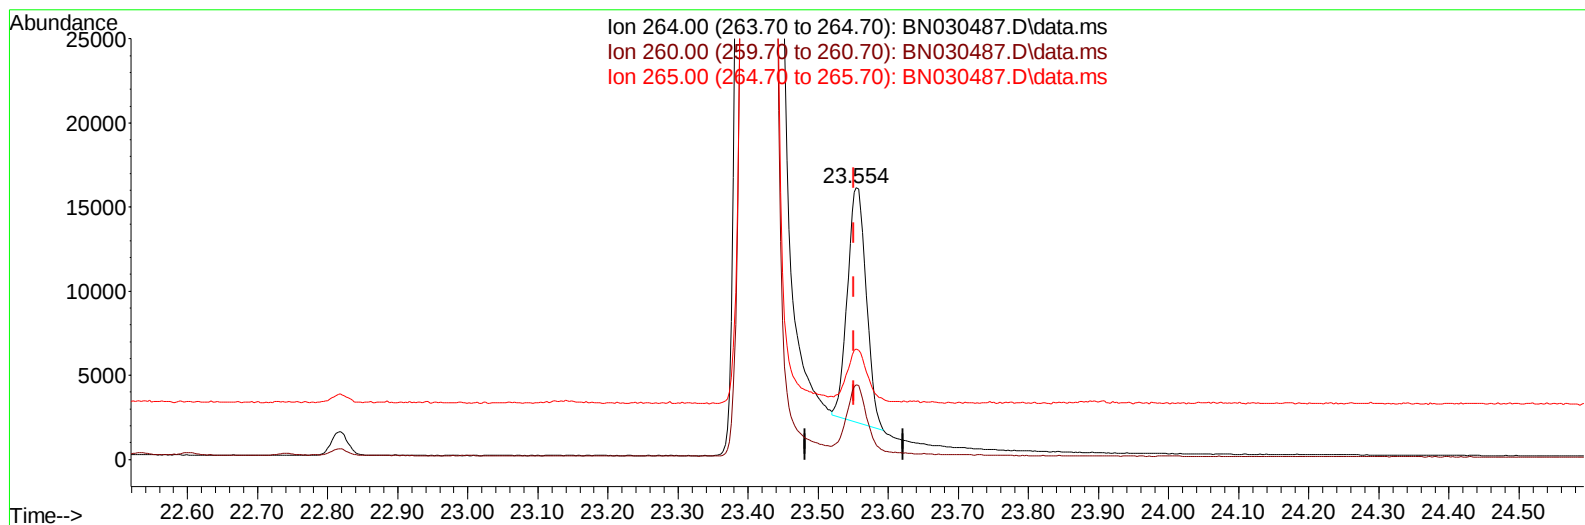

TIC: BN030487.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul m

response 25973

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	27.53
265.00	41.20	40.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030487.D
 Acq On : 25 Mar 2024 18:46
 Operator : MA/JU
 Sample : P1813-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 28 01:41:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.729	152	11285	0.400	ng/ul	0.00
4) Naphthalene-d8	10.513	136	36030	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.363	164	23431	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.112	188	49539	0.400	ng/ul #	0.00
17) Chrysene-d12	21.304	240	34100	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264	25973m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	52920	3.991	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152	17074	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.142	212	40259	0.378	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.256	88	2994	0.218	ng/ul#	13

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030487.D
Acq On : 25 Mar 2024 18:46
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 28 01:41:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

