




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030488.D
Acq On : 25 Mar 2024 19:22
Operator : MA/JU
Sample : P1813-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY2

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

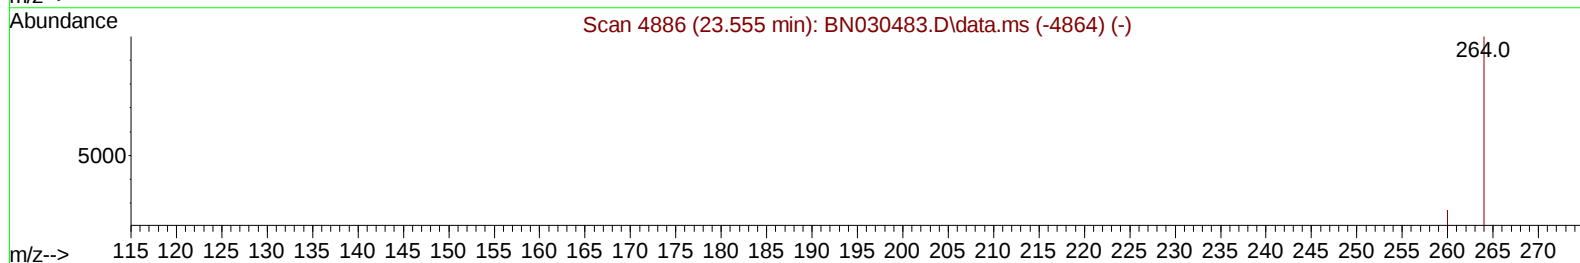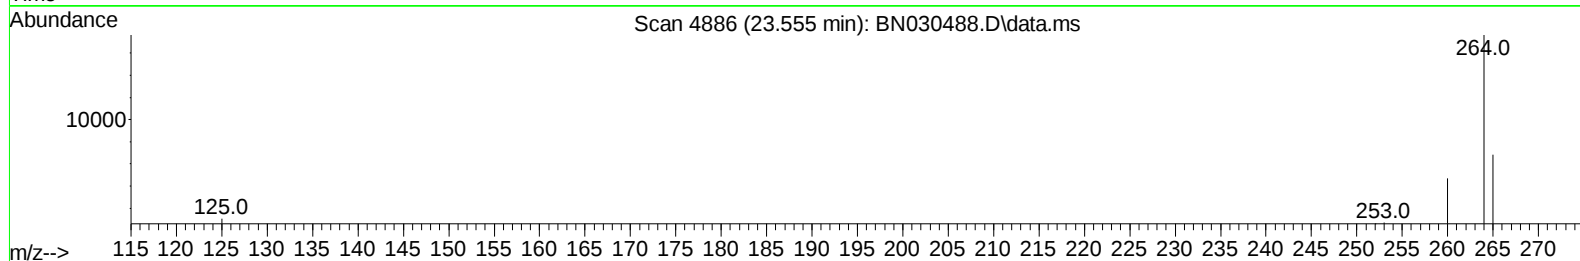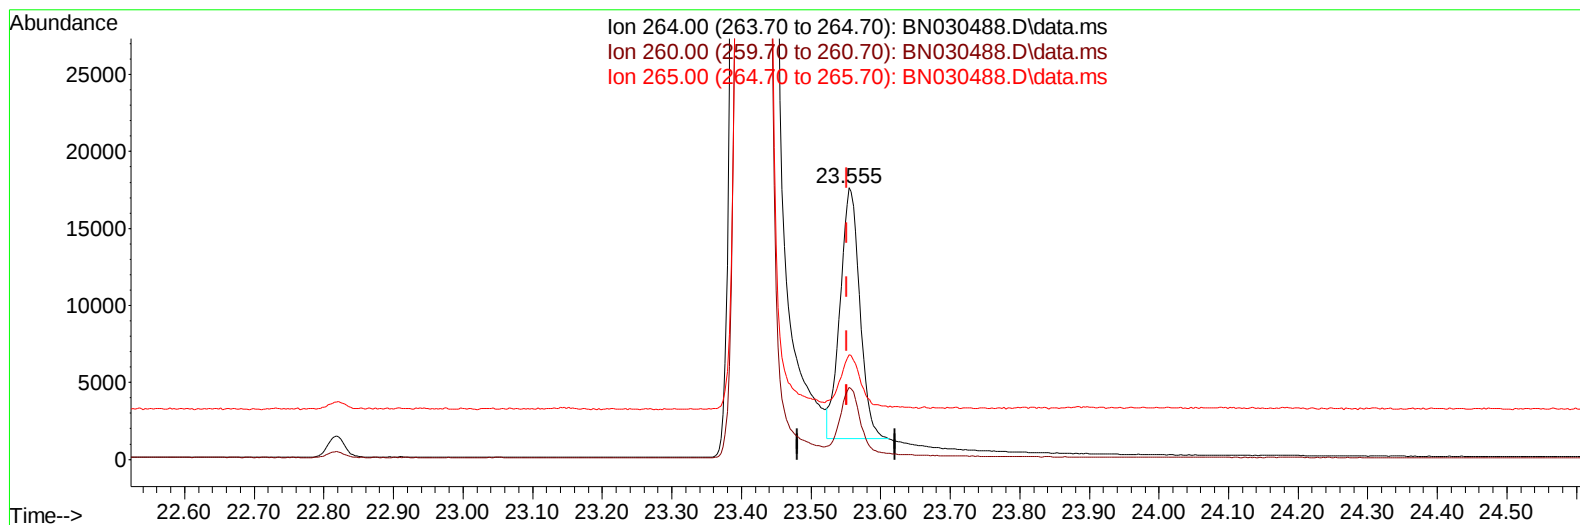

TIC: BN030488.D\data.ms

(23) Perylene-d12 (I)

23.555min (+ 0.004) 0.40 ng/u1

response 32096

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.50
265.00	41.20	38.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030488.D
Acq On : 25 Mar 2024 19:22
Operator : MA/JU
Sample : P1813-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY2

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

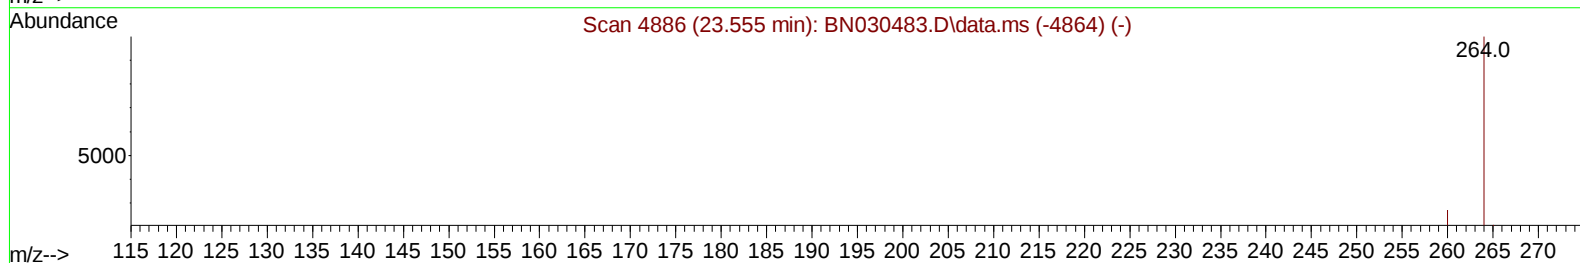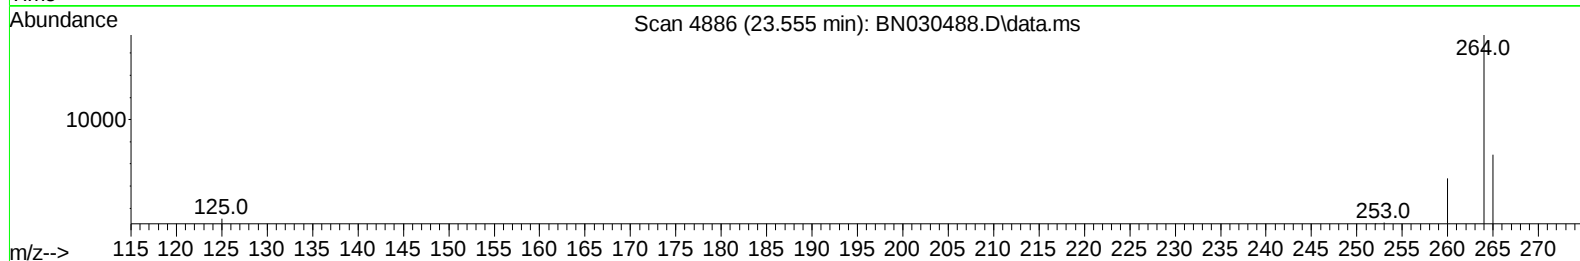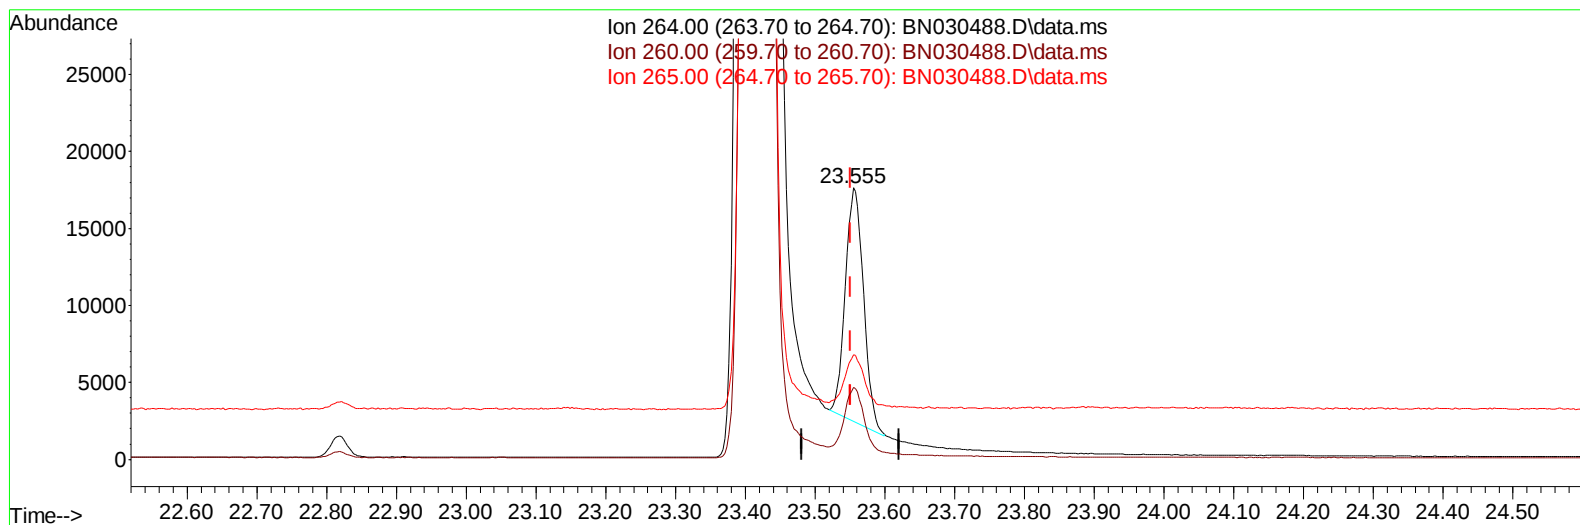

TIC: BN030488.D\data.ms

(23) Perylene-d12 (I)

23.555min (+ 0.004) 0.40 ng/ul m

response 27410

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.50
265.00	41.20	38.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030488.D
 Acq On : 25 Mar 2024 19:22
 Operator : MA/JU
 Sample : P1813-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LY2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	9936	0.400	ng/ul	0.00
4) Naphthalene-d8	10.512	136	31553	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.364	164	18745	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.113	188	43673	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	32701	0.400	ng/ul	0.00
23) Perylene-d12	23.555	264	27410m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	48920	4.190	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152	12597	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.142	212	34933	0.342	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030488.D
Acq On : 25 Mar 2024 19:22
Operator : MA/JU
Sample : P1813-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LY2

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

