




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030490.D
Acq On : 25 Mar 2024 20:35
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

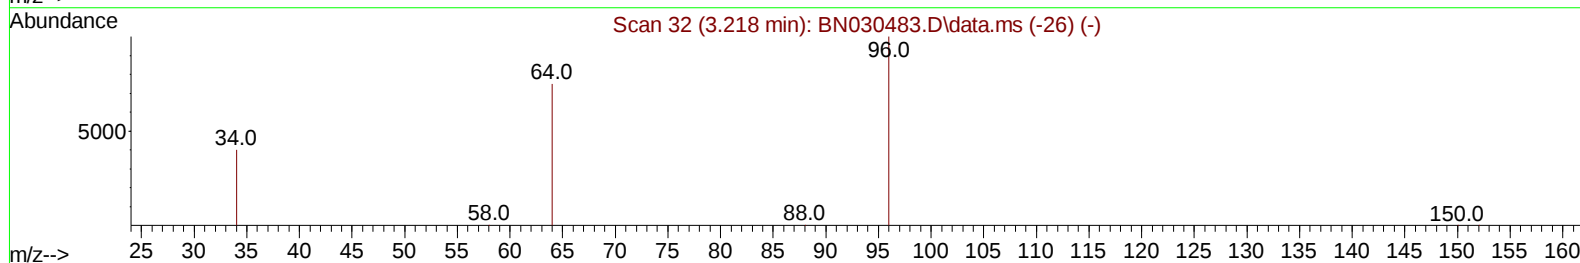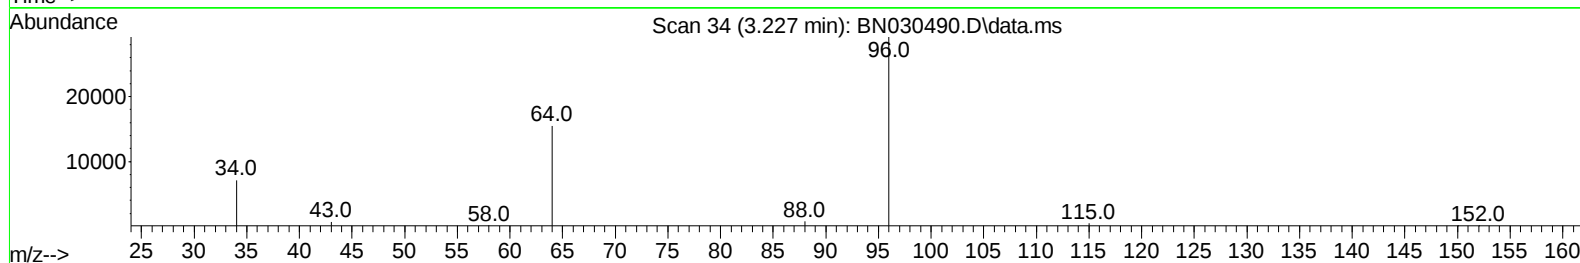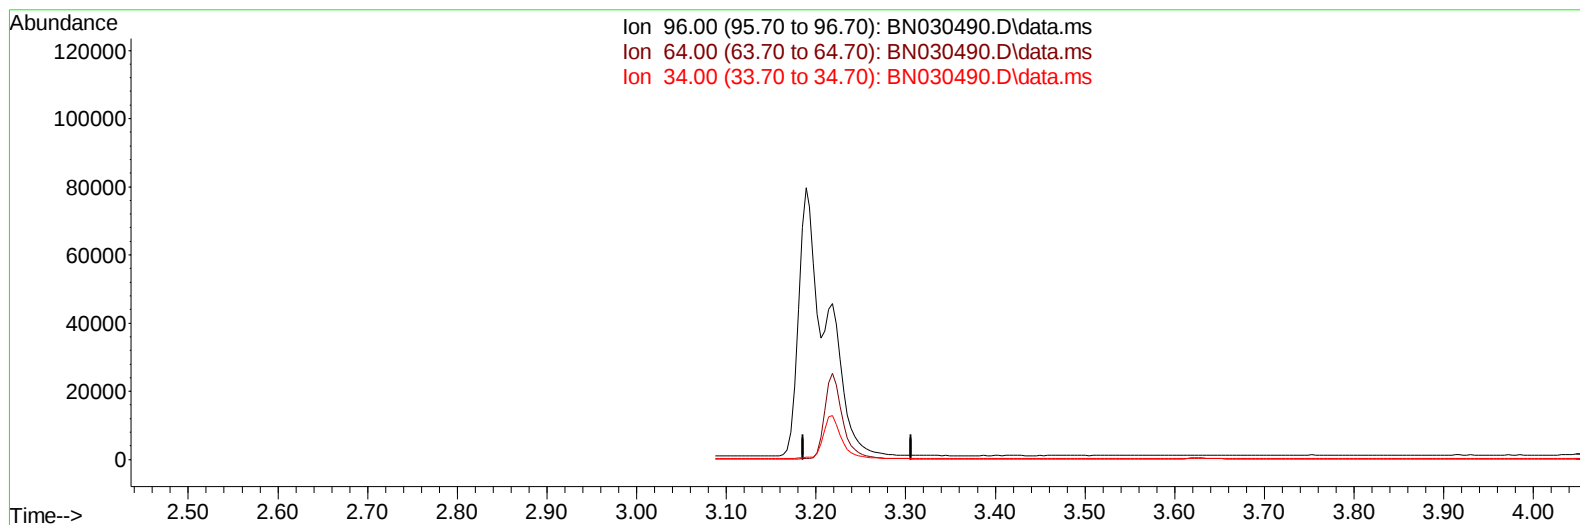

TIC: BN030490.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.226min (-3.226) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	60.00	0.00#
34.00	35.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030490.D
Acq On : 25 Mar 2024 20:35
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

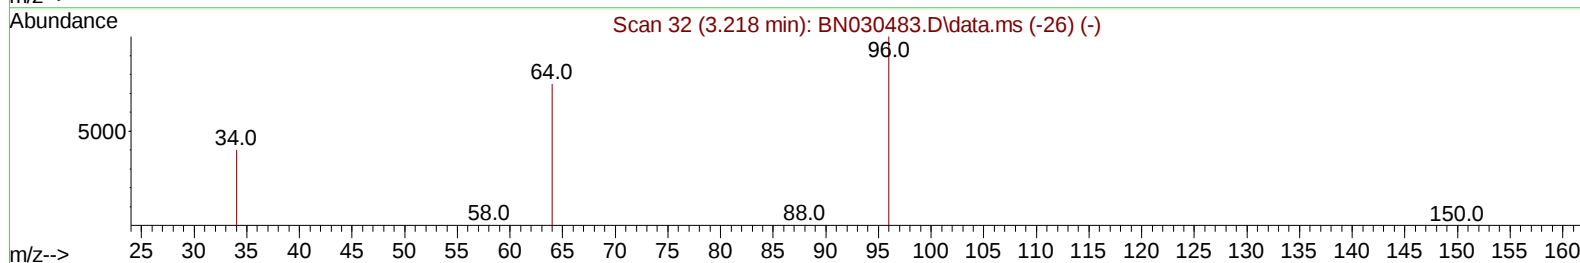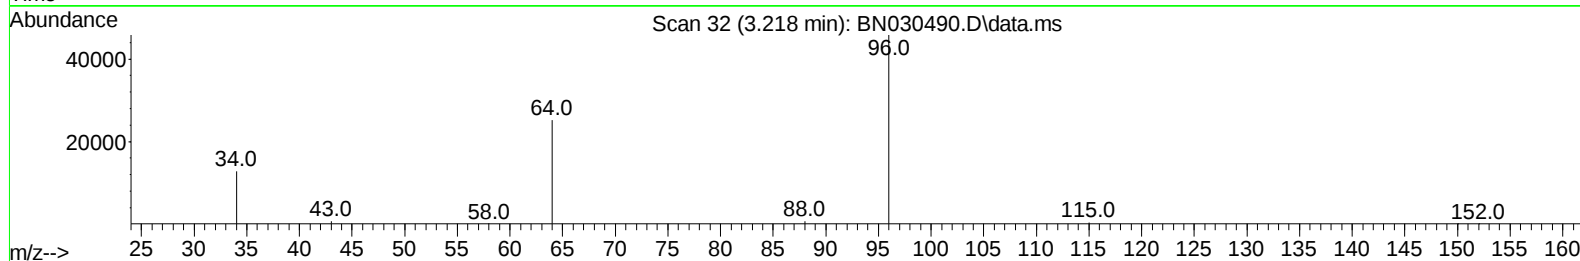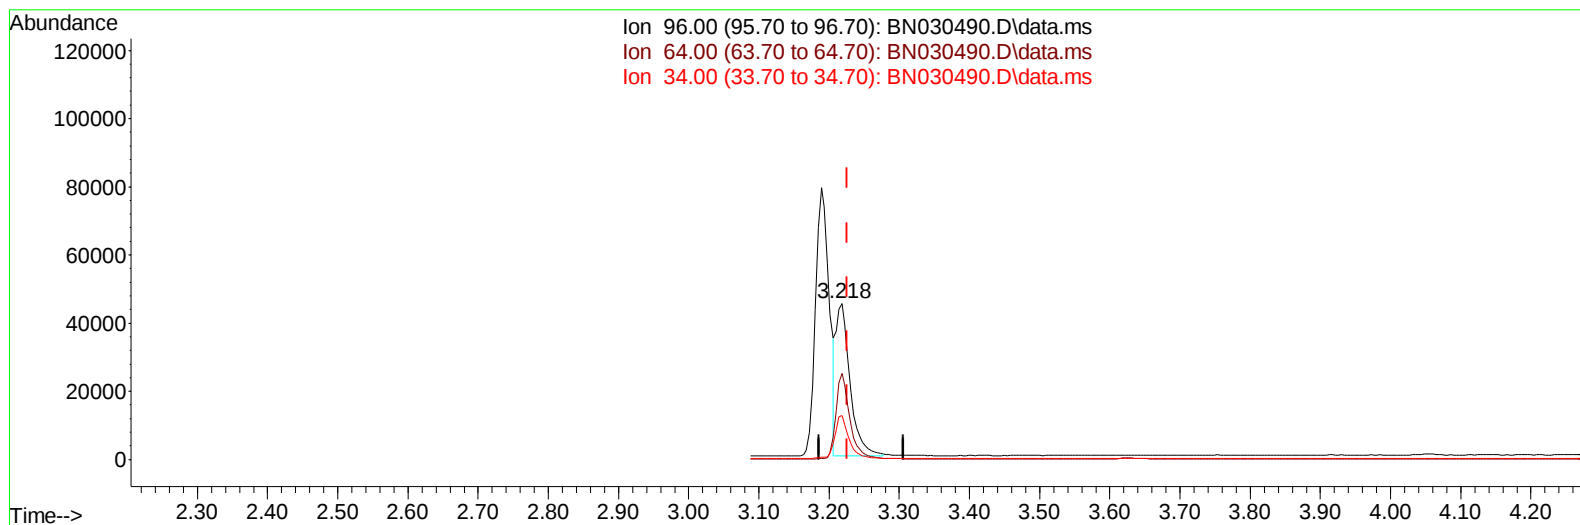

TIC: BN030490.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.218min (-0.008) 5.91 ng/ul m

response 63293

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	60.00	55.15
34.00	35.00	27.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030490.D
Acq On : 25 Mar 2024 20:35
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

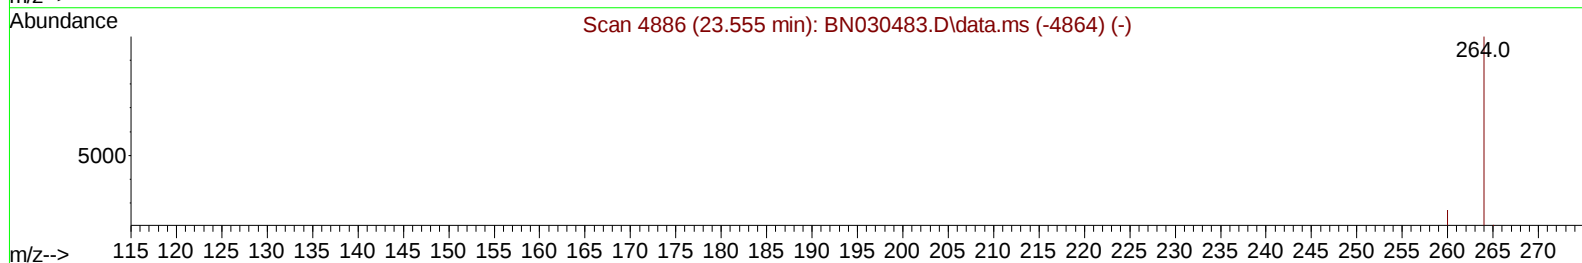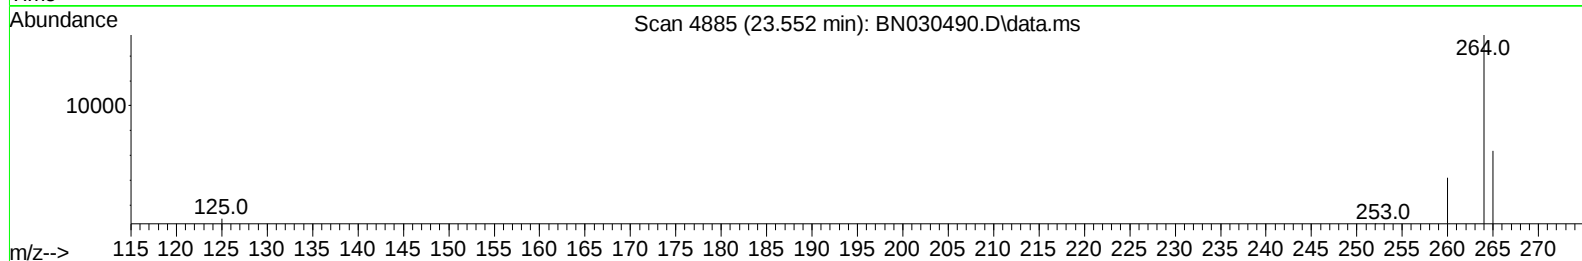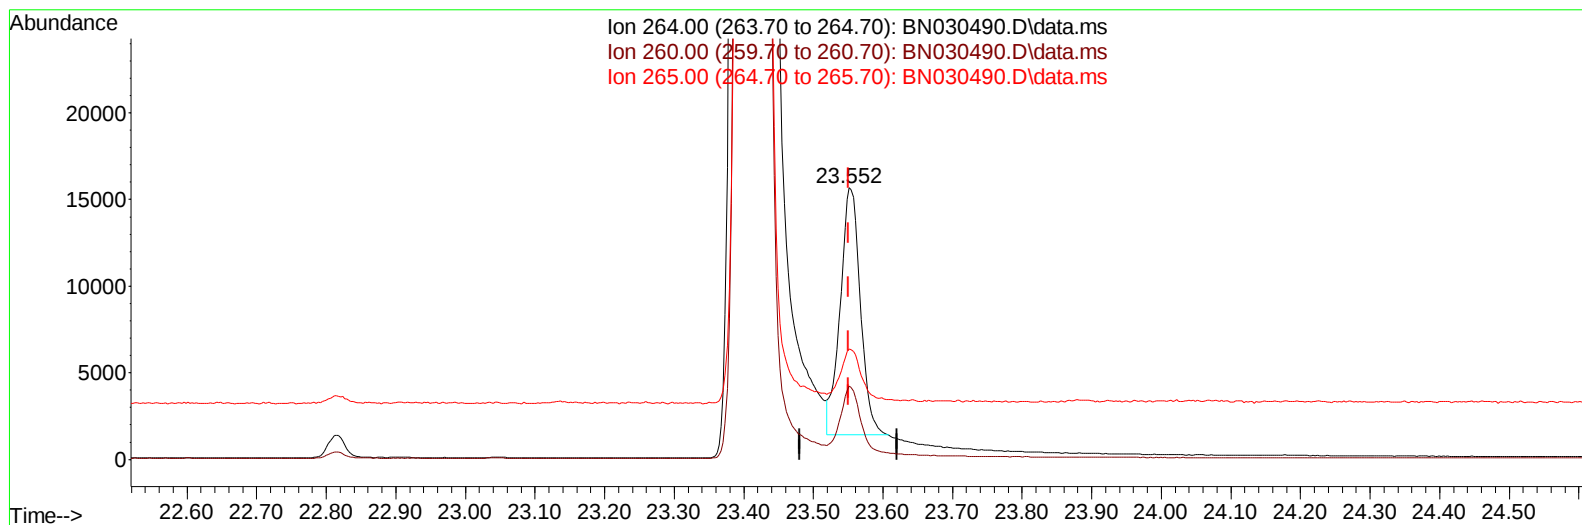

TIC: BN030490.D\data.ms

(23) Perylene-d12 (I)

23.552min (+ 0.000) 0.40 ng/u1

response 28740

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.98
265.00	41.20	40.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030490.D
Acq On : 25 Mar 2024 20:35
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

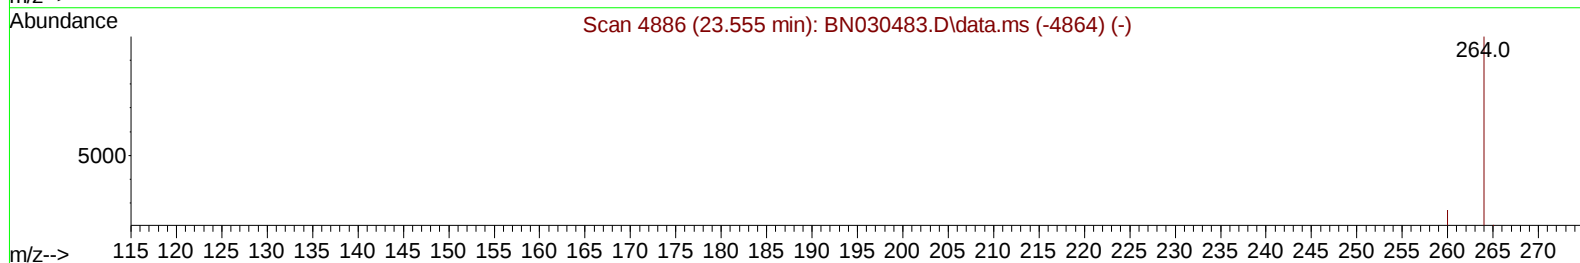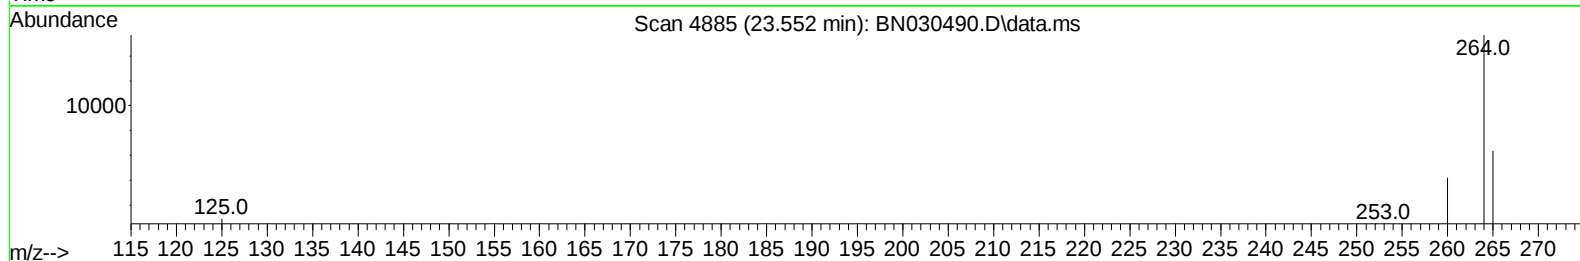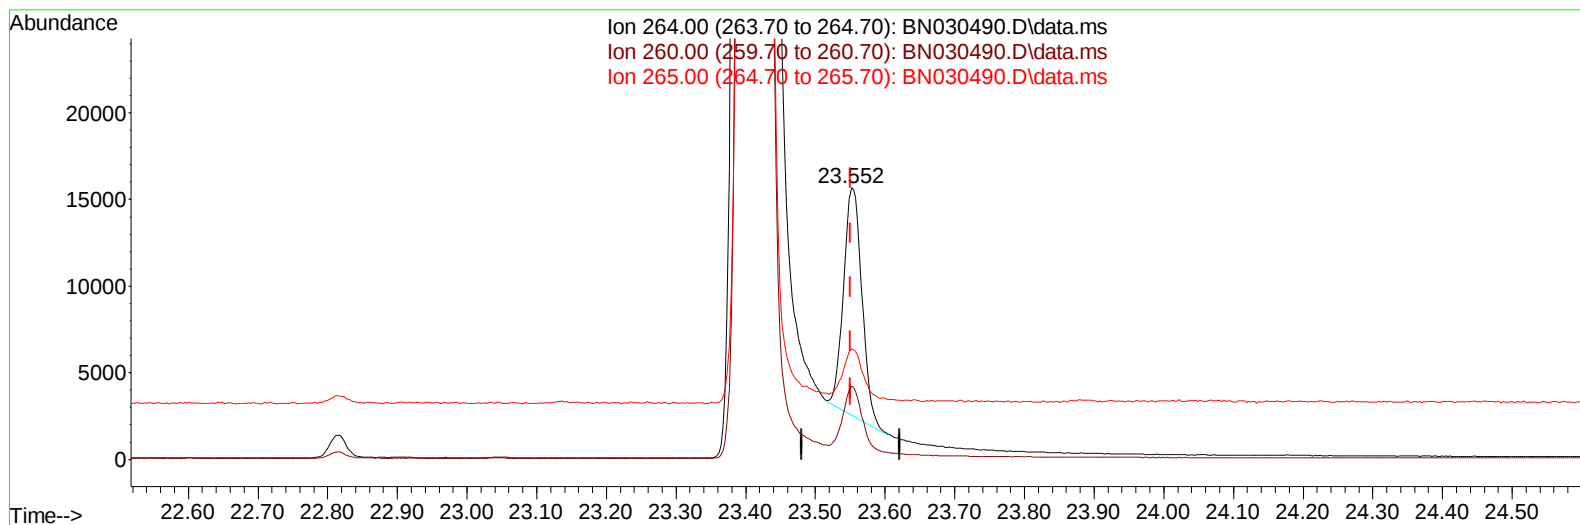

TIC: BN030490.D\data.ms

(23) Perylene-d12 (I)

23.552min (+ 0.000) 0.40 ng/ul m

response 24041

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.98
265.00	41.20	40.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030490.D
 Acq On : 25 Mar 2024 20:35
 Operator : MA/JU
 Sample : P1841-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.729	152		9107	0.400	ng/ul	0.00
4) Naphthalene-d8	10.513	136		28534	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.363	164		17145	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.108	188		39930	0.400	ng/ul	0.00
17) Chrysene-d12	21.301	240		27654	0.400	ng/ul	0.00
23) Perylene-d12	23.552	264		24041m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.218	96		63293m	5.915	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152		13240	0.329	ng/ul	0.00
18) Fluoranthene-d10	19.142	212		34701	0.402	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.252	88		14050	1.270	ng/ul	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030490.D
Acq On : 25 Mar 2024 20:35
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK3

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

